

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL031519\
 Data File : VL033336.D
 Acq On : 15 Mar 2019 18:22
 Operator : SY/AP
 Sample : OC031319 CAN 10265
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC031319 CAN 10265

Quant Time: Mar 16 04:09:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL031519AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Mar 15 14:52:14 2019
 QLast Update : Fri Mar 15 14:52:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.76	49	813260	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.29	114	1845577	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.25	117	1960046	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.58	95	1473887	10.15	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.50%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL031519\
Data File : VL033336.D
Acq On : 15 Mar 2019 18:22
Operator : SY/AP
Sample : OC031319 CAN 10265
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC031319 CAN 10265

Quant Time: Mar 16 04:09:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL031519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Mar 15 14:52:14 2019
QLast Update : Fri Mar 15 14:52:14 2019
Response via : Initial Calibration

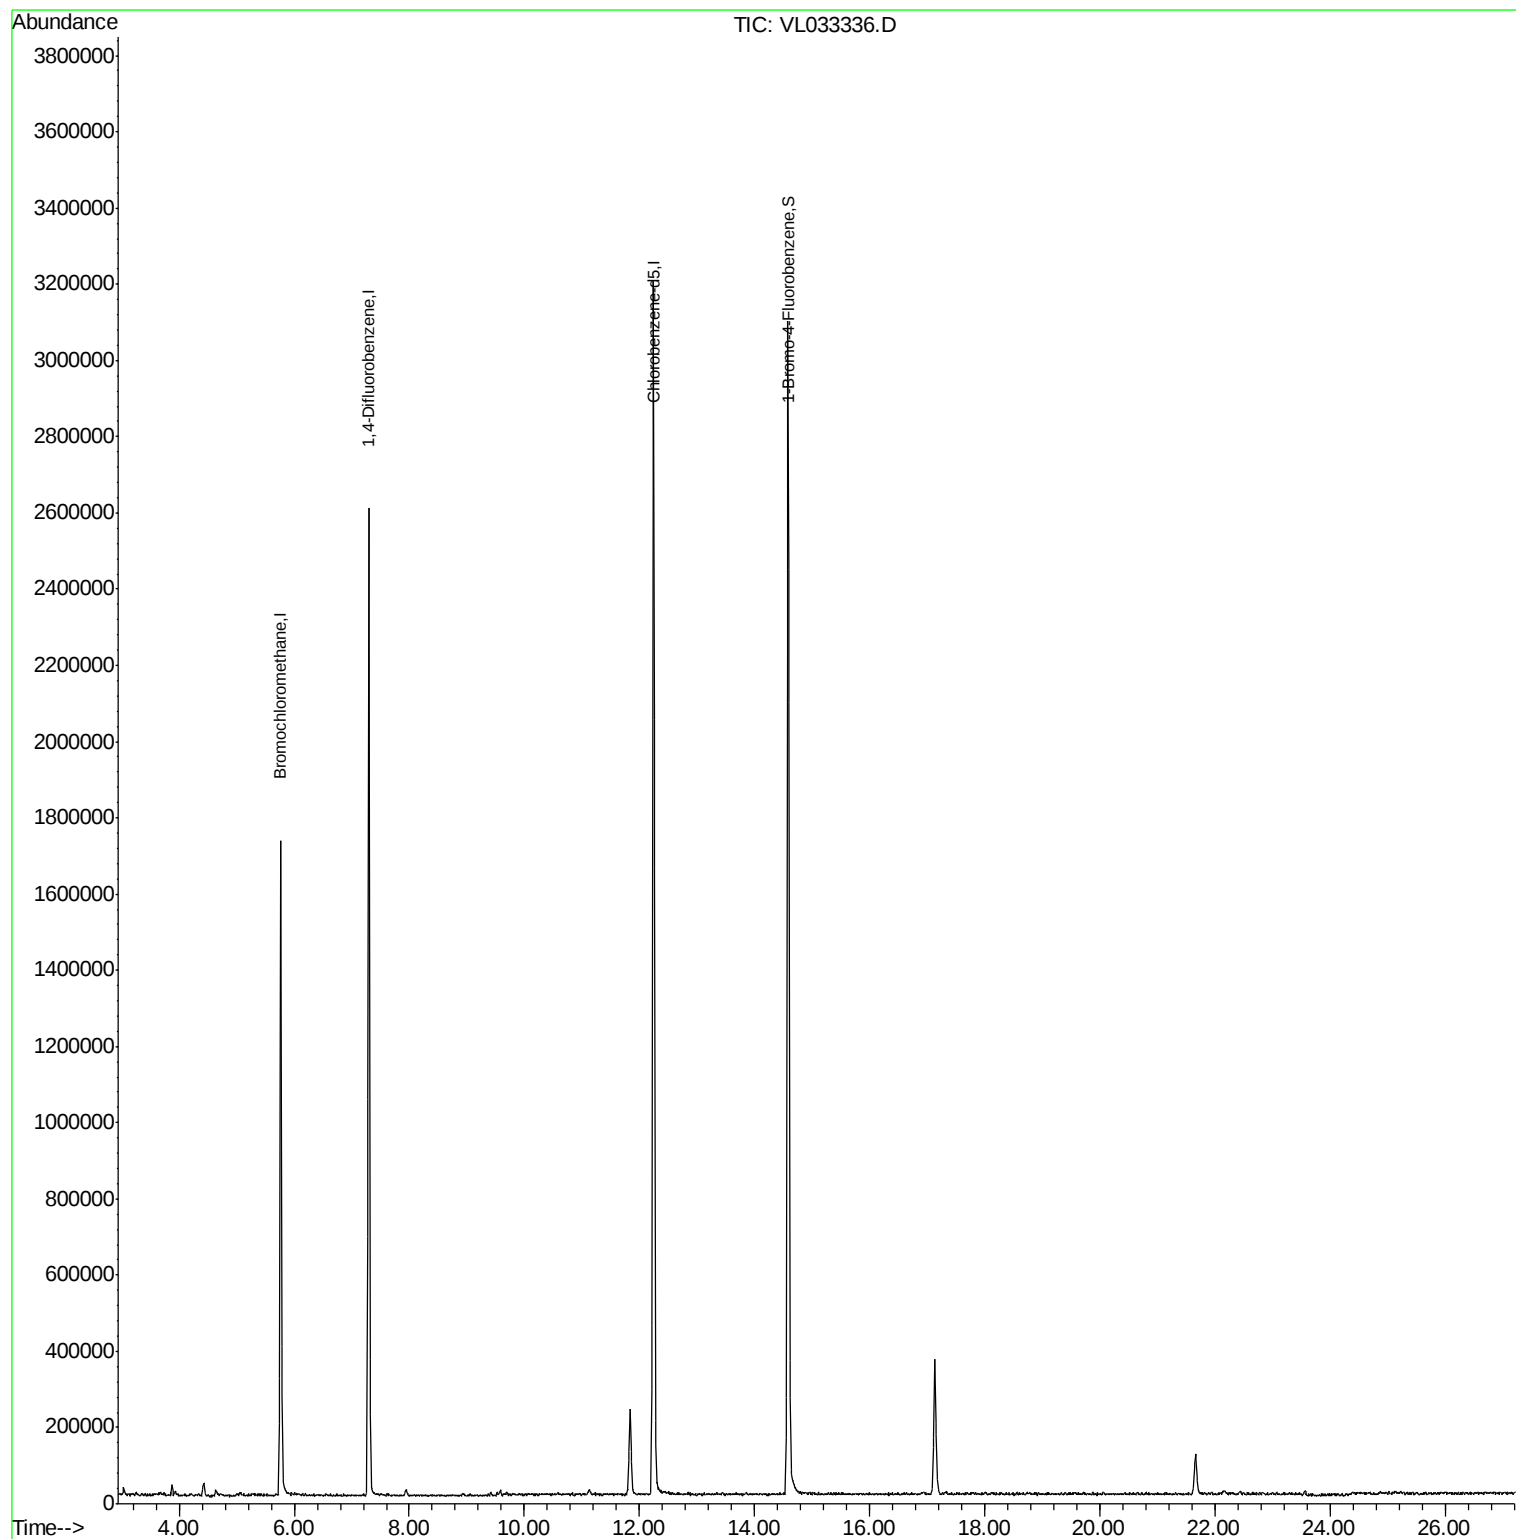

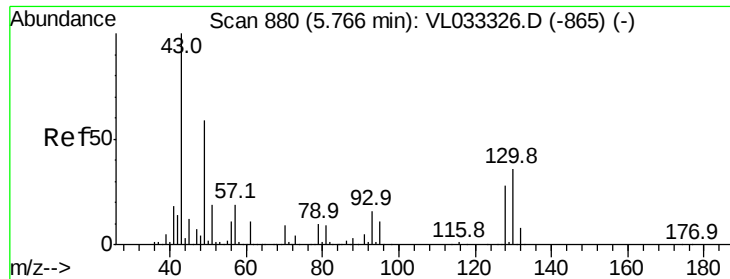

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.76 min Scan# 879

Delta R.T. -0.00 min

Lab File: VL033336.D

Acq: 15 Mar 2019 18:22

Instrument :

MSVOA_L

ClientSampleId :

QC031319 CAN 10265


Tot Ion: 49 Resp: 813260

Ion Ratio Lower Upper

49 100

128 46.6 23.5 70.6




130 61.0 30.1 90.3

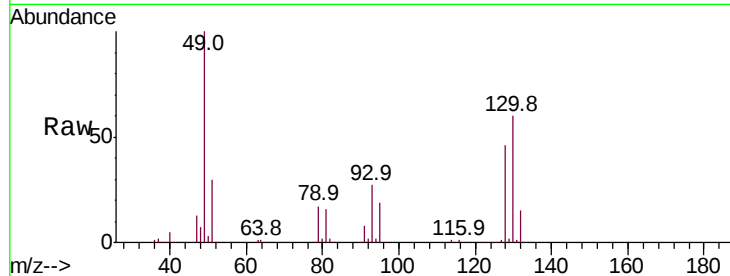

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

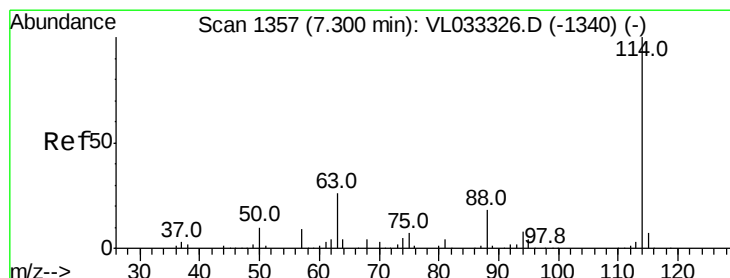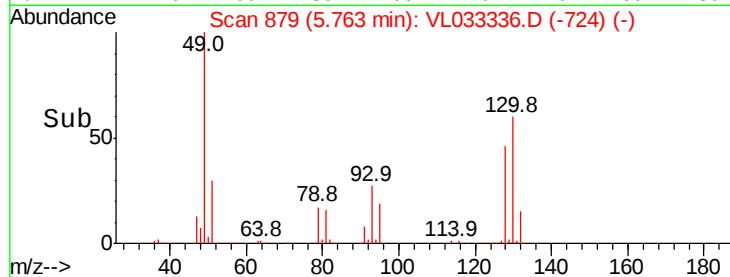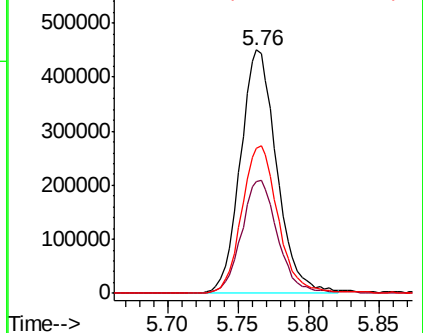

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.29 min Scan# 1355

Delta R.T. -0.01 min

Lab File: VL033336.D

Acq: 15 Mar 2019 18:22


Tgt Ion:114 Resp: 1845577

Ion Ratio Lower Upper

114 100

63 26.4 21.4 32.2



88 17.9 14.5 21.7

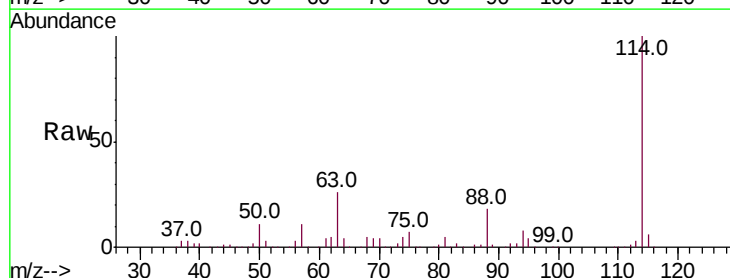


Abundance Ion 114.10 (113.80 to 114.80): V

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

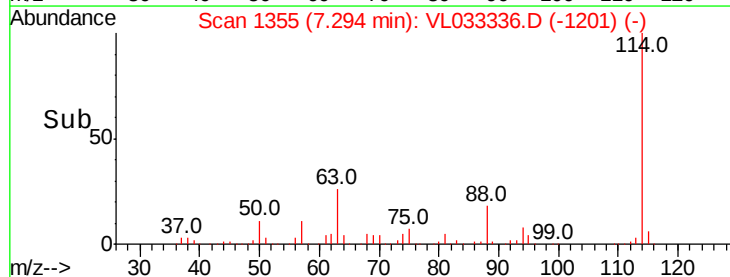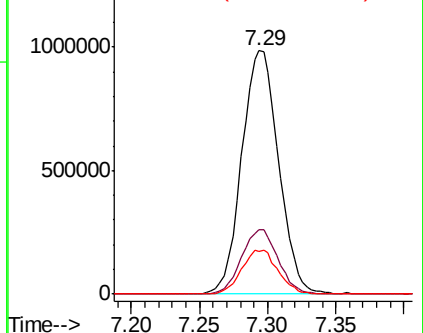


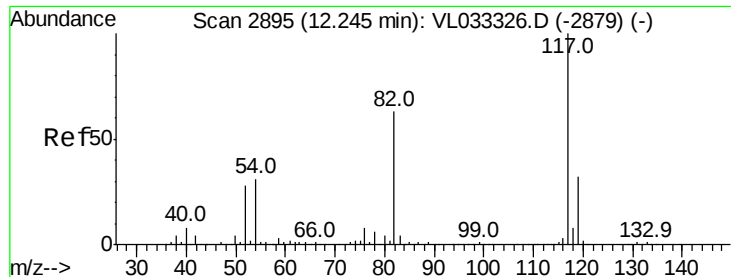




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.25 min Scan# 2895
Delta R.T. -0.00 min
Lab File: VL033336.D
Acq: 15 Mar 2019 18:22

Instrument :
MSVOA_L
ClientSampleId :
QC031319 CAN 10265

Tot Ion:117 Resp: 1960046
Ion Ratio Lower Upper
117 100
82 68.1 53.4 80.2
119 32.2 27.3 40.9

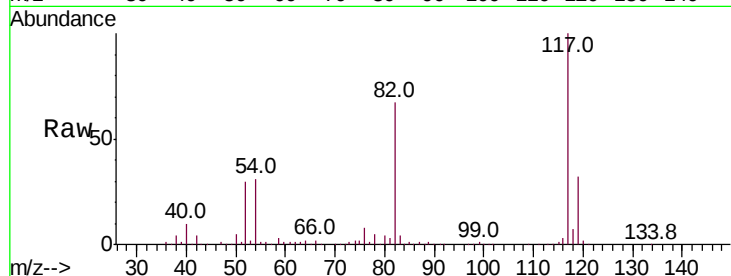


Abundance Ion 117.10 (116.80 to 117.80): V
Ion 82.10 (81.80 to 82.80): VL0
Ion 119.10 (118.80 to 119.80): V

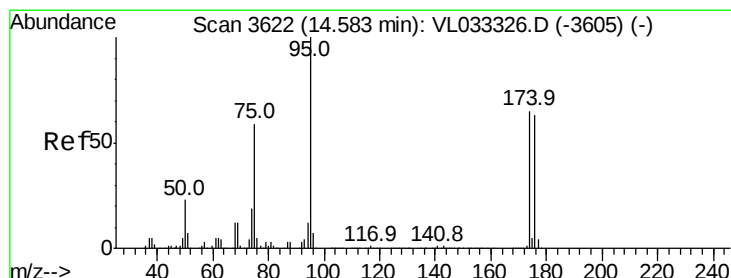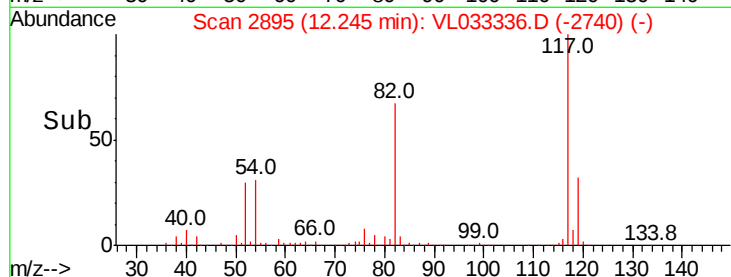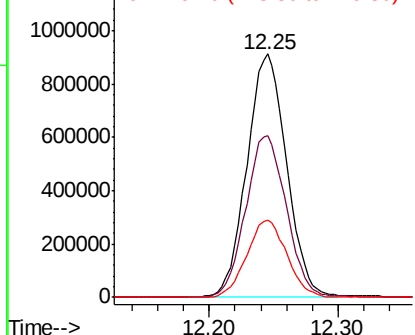

#68
1-Bromo-4-Fluorobenzene
Concen: 10.148 ppbv
RT: 14.58 min Scan# 3622
Delta R.T. -0.00 min
Lab File: VL033336.D
Acq: 15 Mar 2019 18:22

Tgt Ion: 95 Resp: 1473887
Ion Ratio Lower Upper
95 100
174 64.7 51.5 77.3
175 4.7 3.8 5.6

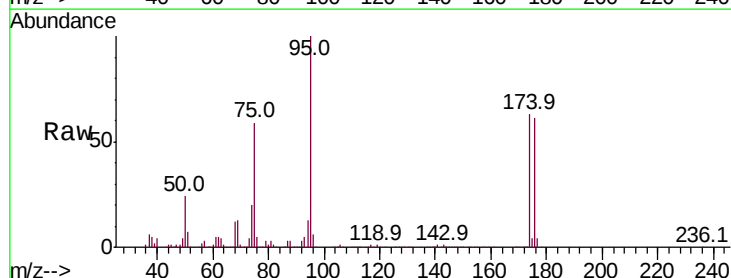

Abundance Ion 95.10 (94.80 to 95.80): VL0
Ion 174.00 (173.70 to 174.70): V
Ion 175.00 (174.70 to 175.70): V

