


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL031519\
Data File : VL033316.D
Acq On : 15 Mar 2019 2:16
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL031419AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Mar 15 08:43:32 2019
Last Update : Fri Mar 15 08:43:32 2019

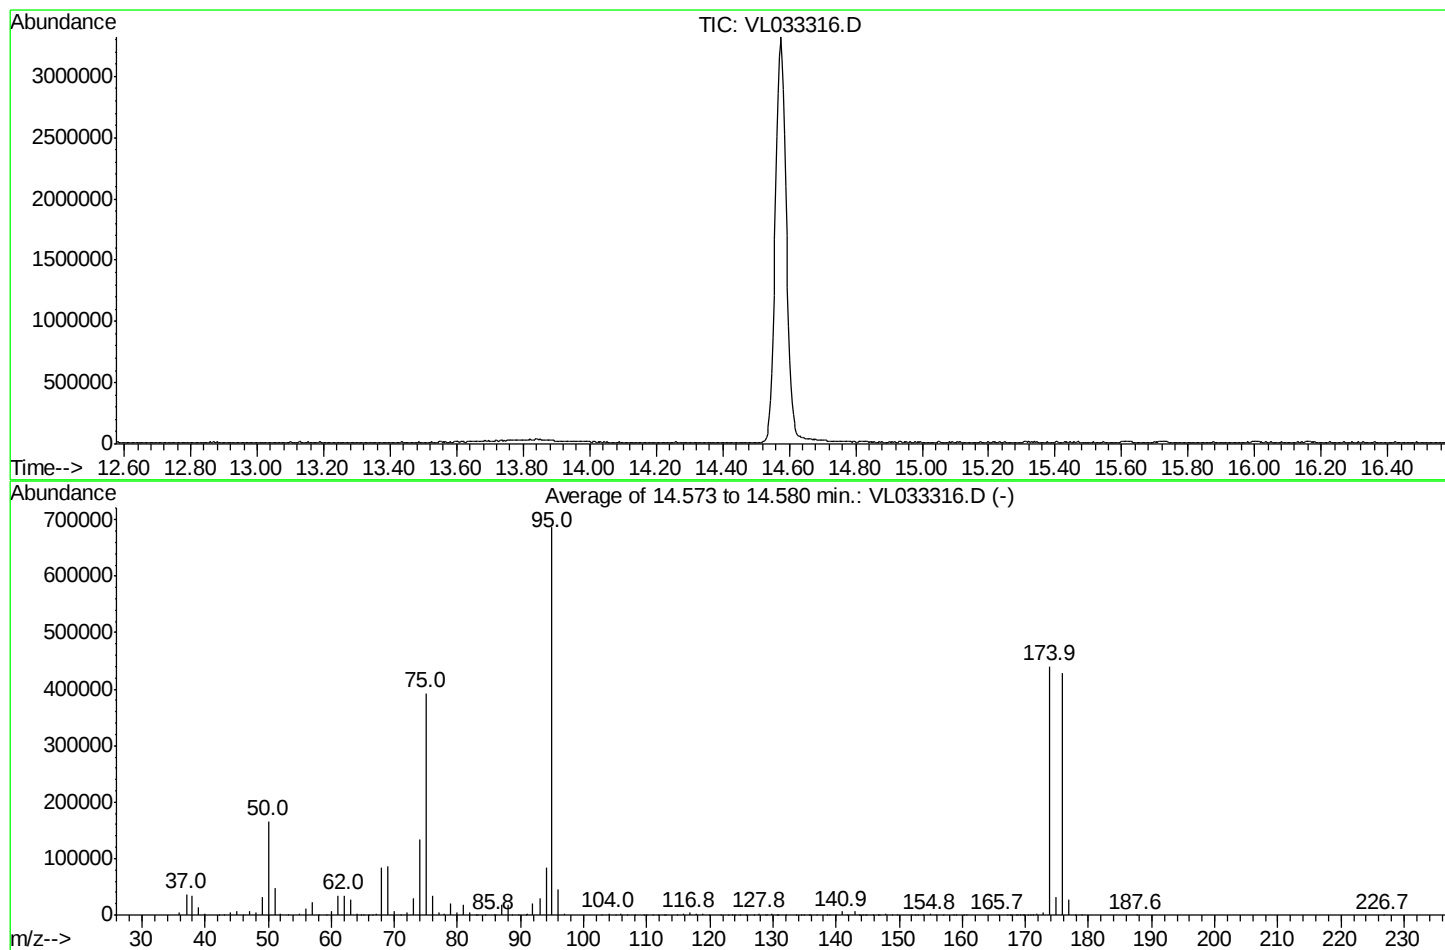

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	165568	PASS
75	95	30	66	57.2	393002	PASS
95	95	100	100	100.0	686656	PASS
96	95	5	9	6.7	46154	PASS
173	174	0.00	2	0.9	3796	PASS
174	95	50	120	64.1	439936	PASS
175	174	4	9	7.1	31117	PASS
176	174	93	101	97.3	428032	PASS
177	176	5	9	6.4	27208	PASS