


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL031519\
 Data File : VL033325.D
 Acq On : 15 Mar 2019 9:47
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL031419AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Mar 15 08:43:32 2019
 Last Update : Fri Mar 15 08:43:32 2019

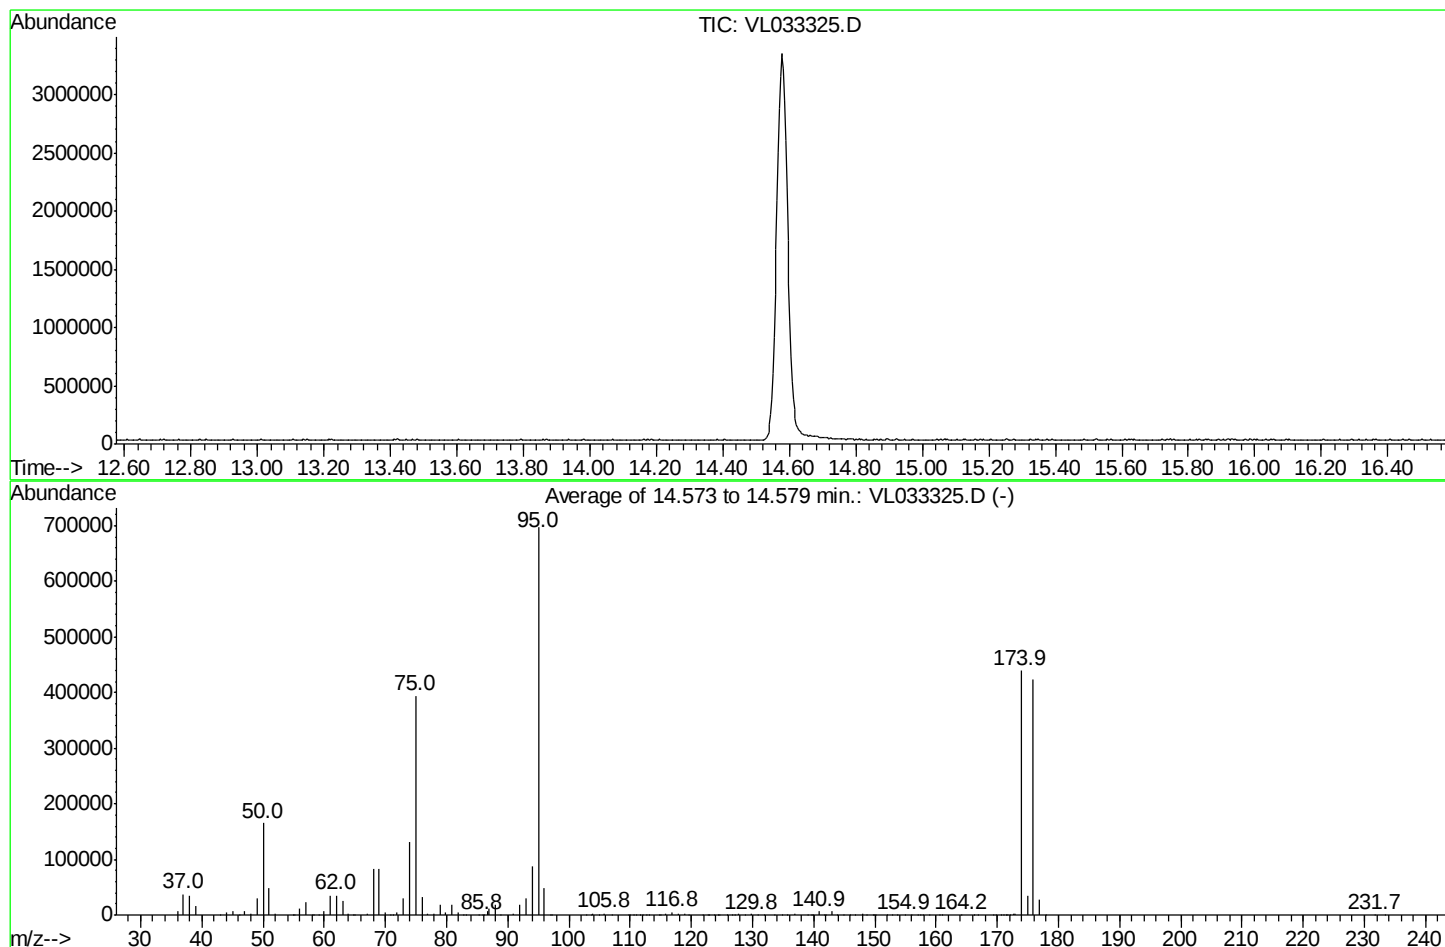

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.7	165418	PASS
75	95	30	66	56.6	394837	PASS
95	95	100	100	100.0	697280	PASS
96	95	5	9	7.0	48541	PASS
173	174	0.00	2	0.6	2784	PASS
174	95	50	120	63.0	439616	PASS
175	174	4	9	7.8	34445	PASS
176	174	93	101	96.4	423957	PASS
177	176	5	9	6.5	27410	PASS