



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031523\
Data File : VL040278.D
Acq On : 15 Mar 2023 10:49
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Mar 15 16:14:43 2023

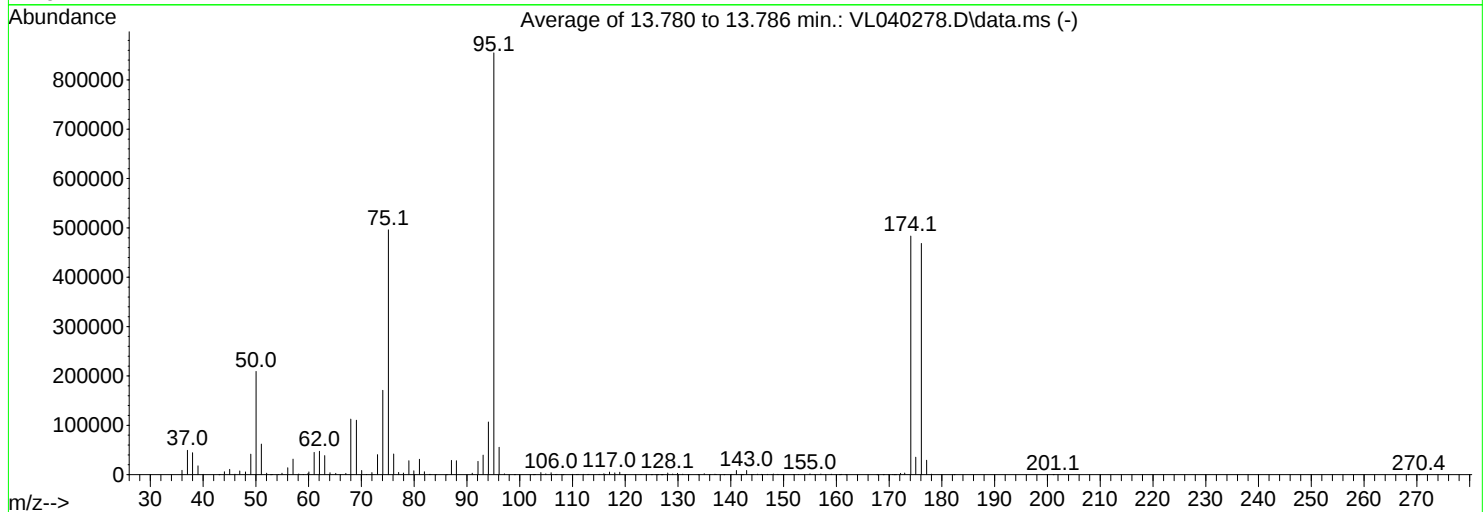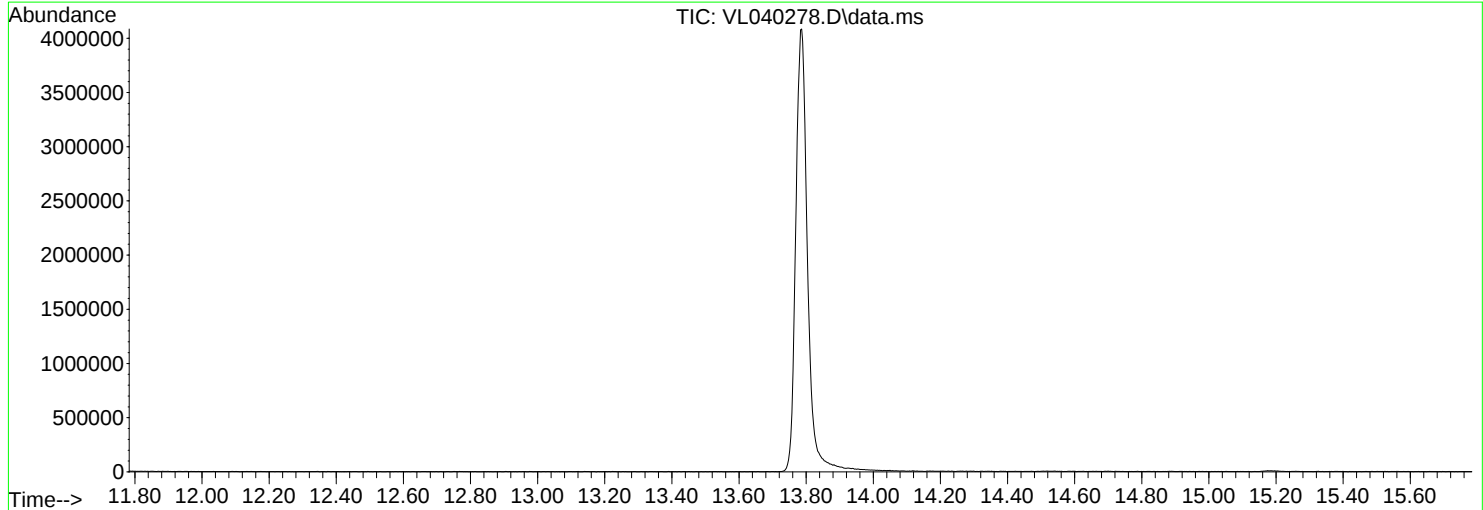

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.5	209024	PASS
75	95	30	66	58.0	495936	PASS
95	95	100	100	100.0	854763	PASS
96	95	5	9	6.5	55491	PASS
173	174	0.00	2	0.7	3189	PASS
174	95	50	120	56.6	483541	PASS
175	174	4	9	7.3	35320	PASS
176	174	93	101	96.9	468672	PASS
177	176	5	9	6.2	29253	PASS

Average of 13.780 to 13.786 min.: VL040278.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8703	48.05	5569	58.15	1173	68.00	11263
37.05	49456	49.05	41531	59.00	405	69.05	11025
38.00	44517	50.05	209024	59.90	2590	70.05	858
39.05	17731	51.05	61896	60.05	5573	70.95	21
40.00	705	52.05	3026	61.05	45237	72.00	4181
43.00	152	52.80	180	62.05	47229	73.05	40683
43.15	458	53.15	202	63.05	38704	74.05	171051
44.05	5756	54.30	193	64.05	3769	75.10	495936
45.05	10560	54.95	2985	65.15	2615	76.10	41883
46.05	945	56.05	13810	66.05	263	77.05	4519
46.95	7433	57.05	31435	67.05	2657	77.95	3220

Average of 13.780 to 13.786 min.: VL040278.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.00	28149	92.10	27013	105.95	3906	115.05	806
79.95	7875	93.05	39472	106.80	393	115.95	2086
81.00	31040	94.05	106597	107.05	520	116.20	747
81.95	5725	95.10	854763	107.95	200	117.00	5297
82.90	585	96.10	55491	108.20	62	118.00	3489
83.15	556	97.10	1583	110.00	810	118.95	4764
84.00	77	99.00	65	110.80	385	120.10	254
86.10	153	102.60	136	111.05	518	121.90	194
87.05	28997	102.95	212	112.10	750	123.00	439
88.00	28235	104.00	4338	112.90	372	124.00	638
91.00	2862	104.95	1548	113.10	630	124.95	179

Average of 13.780 to 13.786 min.: VL040278.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.85	325	136.05	302	145.05	1065	152.05	310
126.10	116	137.00	1037	145.80	562	152.85	417
126.80	92	137.20	491	146.00	434	153.95	386
127.00	137	138.70	155	146.95	634	155.00	1773
128.05	3318	140.05	821	147.80	460	155.90	361
129.00	1317	141.05	8387	148.05	1198	157.05	1336
129.90	2782	141.95	614	148.80	522	157.95	335
130.90	974	142.20	182	149.10	282	159.05	1077
131.90	61	143.00	8511	149.70	196	160.60	136
133.80	56	143.95	385	150.05	720	161.00	521
134.95	1963	144.20	272	151.90	202	161.80	154

Average of 13.780 to 13.786 min.: VL040278.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
167.70	155	177.10	29253				
168.90	85	178.05	1140				
169.95	294	182.30	52				
170.65	412	201.10	93				
170.90	124	268.30	54				
171.20	144	270.40	92				
172.15	2494						
172.95	3189						
174.10	483541						
175.05	35320						
176.10	468672						