


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031623\
Data File : VL040287.D
Acq On : 16 Mar 2023 8:33
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Mar 15 16:14:43 2023

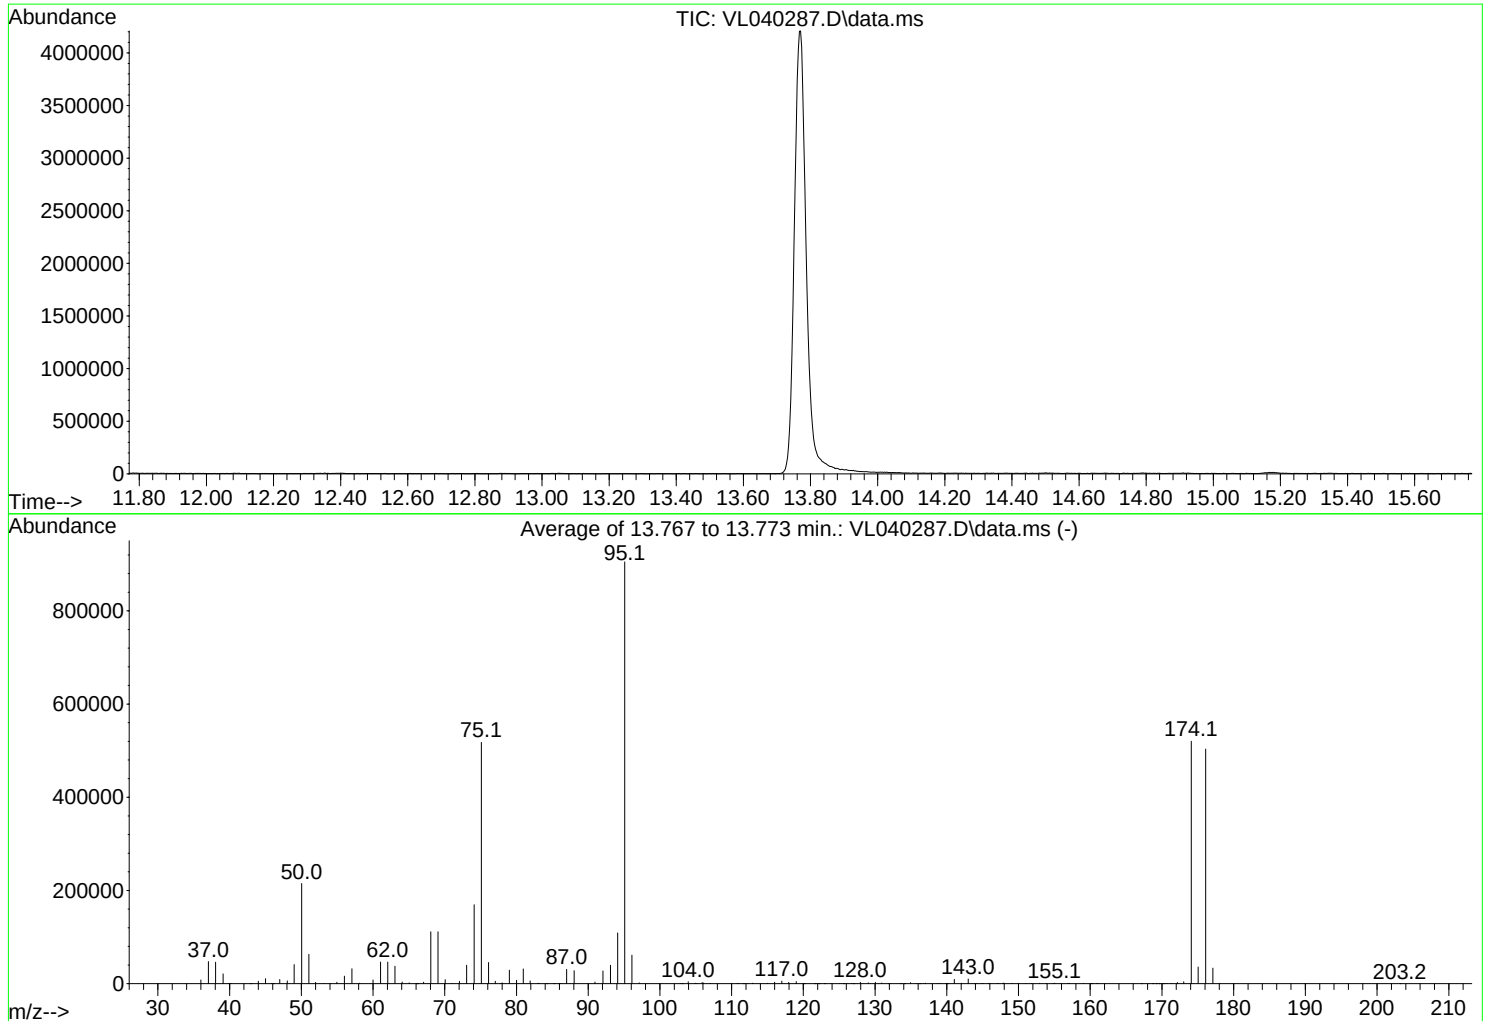

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	214997	PASS
75	95	30	66	57.2	517952	PASS
95	95	100	100	100.0	905195	PASS
96	95	5	9	6.8	61120	PASS
173	174	0.00	2	0.8	4222	PASS
174	95	50	120	57.5	520107	PASS
175	174	4	9	6.8	35555	PASS
176	174	93	101	96.8	503360	PASS
177	176	5	9	6.6	33224	PASS

Average of 13.767 to 13.773 min.: VL040287.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7906	46.10	174	57.05	31813	68.05	11114
37.05	47384	47.00	8812	58.15	911	69.05	11112
38.05	46056	48.05	5873	60.00	7885	70.05	876
39.10	20923	49.00	40819	61.05	46400	71.05	40
39.85	277	50.05	214997	62.05	46464	72.05	4700
40.20	559	51.05	62741	63.05	37587	73.05	39667
42.90	123	52.00	2935	64.05	3597	74.10	169131
43.10	398	53.15	346	65.05	1592	75.10	517952
44.00	5200	54.05	310	66.00	92	76.10	45219
45.00	10758	54.95	3016	66.20	111	77.05	5243
45.85	317	56.00	16076	67.05	3210	77.80	480

Average of 13.767 to 13.773 min.: VL040287.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.00	1919	87.00	30600	103.95	3998	112.95	900
79.00	28923	88.05	27981	104.90	966	115.00	610
80.00	7420	90.95	3476	105.10	238	116.00	3045
80.95	31677	92.05	27232	105.90	2436	117.00	5501
81.90	6023	93.10	39661	106.10	1240	117.95	2707
83.00	954	94.10	108755	107.05	863	119.00	4574
83.20	283	95.10	905195	109.95	594	120.10	155
84.25	153	96.10	61120	110.70	321	121.60	57
85.20	107	97.10	1579	111.00	692	121.90	64
85.90	109	102.85	214	111.65	153	122.20	61
86.20	483	103.10	115	112.20	522	122.95	156

Average of 13.767 to 13.773 min.: VL040287.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.95	469	133.55	185	141.05	9121	147.80	356
125.10	345	134.10	143	142.05	925	147.95	1388
125.60	74	134.95	2067	143.00	9932	149.10	678
126.05	205	135.85	330	143.85	215	150.00	725
126.70	221	136.20	110	144.10	192	151.00	299
127.00	68	136.80	411	144.85	464	151.80	381
127.95	2818	137.05	1123	145.10	336	152.95	620
129.05	1793	138.70	195	145.80	599	153.90	578
130.05	2778	139.05	586	146.05	748	154.90	419
130.95	1239	139.90	566	147.00	333	155.05	1146
131.90	61	140.10	158	147.20	355	155.90	408

Average of 13.767 to 13.773 min.: VL040287.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.90	717	170.70	346				
157.10	548	171.30	192				
159.10	774	172.15	2396				
160.20	62	173.05	4222				
160.90	744	174.10	520107				
161.10	249	175.05	35555				
167.10	68	176.10	503360				
168.70	117	177.10	33224				
169.20	171	178.05	807				
169.60	97	203.20	69				
170.20	68						