


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL031720\
 Data File : VL034913.D
 Acq On : 17 Mar 2020 10:14
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030920AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Mar 09 16:42:53 2020
 Last Update : Mon Mar 09 16:42:53 2020

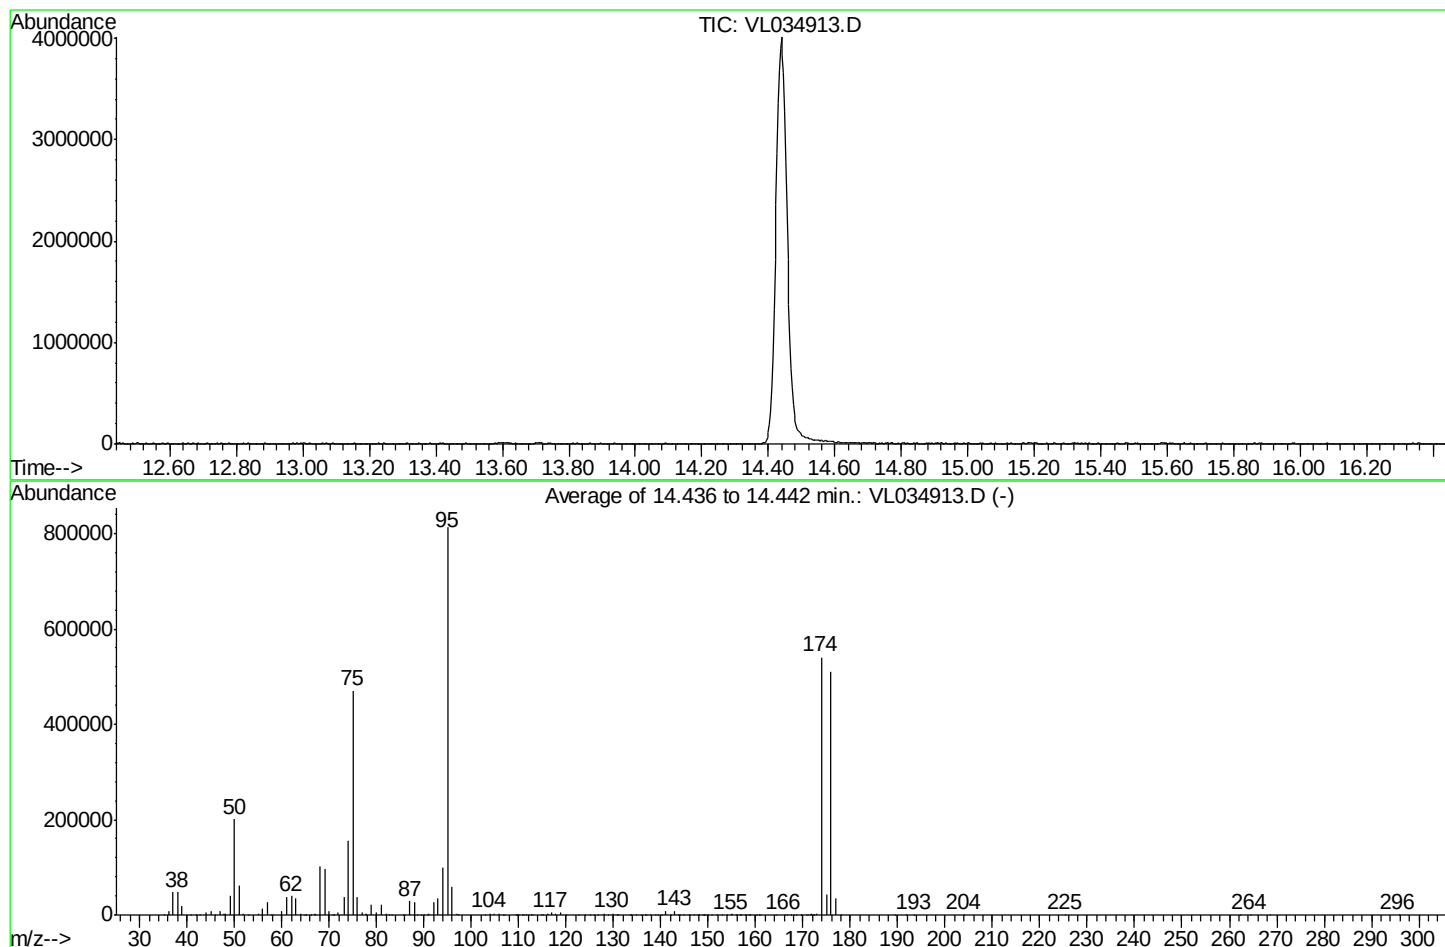

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.7	200682	PASS
75	95	30	66	57.8	469888	PASS
95	95	100	100	100.0	813162	PASS
96	95	5	9	7.2	58642	PASS
173	174	0.00	2	0.3	1532	PASS
174	95	50	120	66.5	540416	PASS
175	174	4	9	7.8	42117	PASS
176	174	93	101	94.2	508970	PASS
177	176	5	9	7.1	36149	PASS