


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031722\
 Data File : VL038623.D
 Acq On : 17 Mar 2022 11:17
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030822AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Mar 08 21:18:44 2022
 Last Update : Tue Mar 08 21:18:44 2022

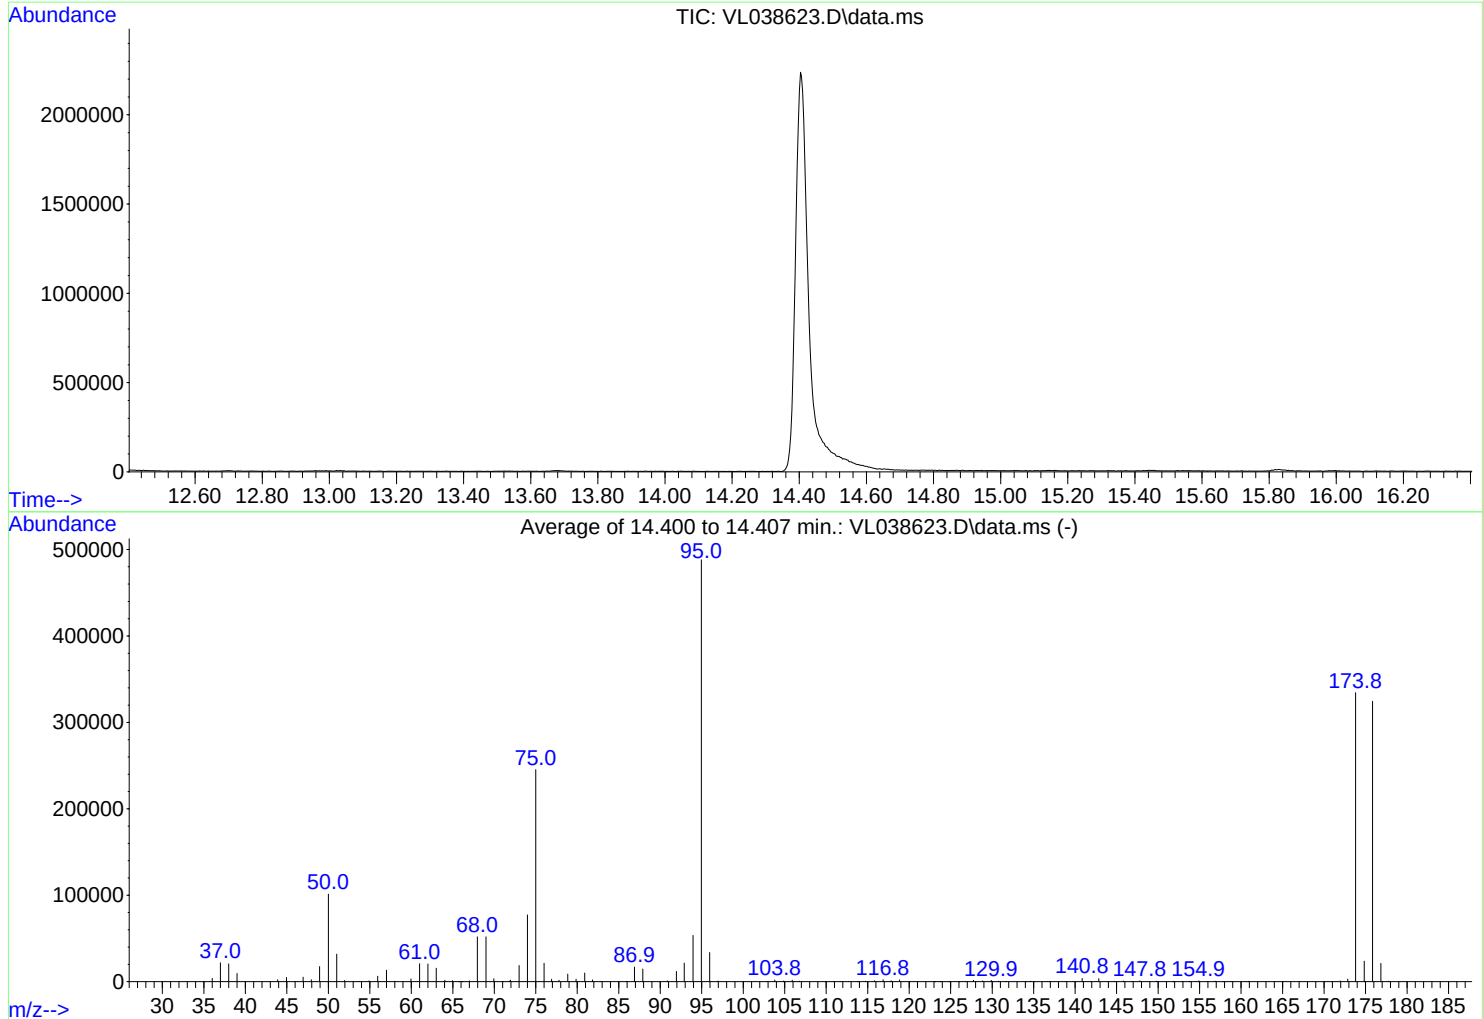

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.8	101328	PASS
75	95	30	66	50.3	245333	PASS
95	95	100	100	100.0	488085	PASS
96	95	5	9	6.9	33771	PASS
173	174	0.00	2	0.9	3070	PASS
174	95	50	120	68.5	334336	PASS
175	174	4	9	7.1	23755	PASS
176	174	93	101	97.0	324373	PASS
177	176	5	9	6.5	21173	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	3675	48.95	17381	61.00	20709	71.10	111
37.00	21939	50.00	101328	62.00	20301	71.80	741
38.00	20651	51.00	31771	63.00	15506	71.95	162
39.00	9364	51.95	1306	64.05	1703	73.00	1866
43.00	164	53.00	121	64.95	1053	74.00	77243
43.90	2148	53.70	133	65.70	59	75.00	245333
44.95	4866	54.90	1037	66.10	61	76.00	21339
45.95	220	55.95	6359	67.00	1010	76.90	2826
46.30	125	57.00	13175	67.95	51947	77.80	1626
46.95	5110	58.00	546	69.00	51856	78.85	8647
47.95	2240	59.95	3239	69.95	3350	79.85	2812

Average of 14.400 to 14.407 min.: VL038623.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	10059	95.95	33771	112.70	278	124.80	56
81.85	1960	96.95	745	113.80	66	126.00	62
82.85	377	102.80	146	114.75	502	126.80	323
85.90	452	103.80	1942	115.80	1157	127.75	1452
86.90	16935	104.85	702	116.85	2213	128.85	854
87.90	14611	105.90	1697	117.70	383	129.90	1471
90.85	980	106.75	508	117.85	877	130.80	560
91.95	11932	109.90	59	118.85	2110	131.60	57
92.90	21485	110.90	284	123.10	80	134.00	51
93.95	53536	111.70	134	123.70	83	134.65	537
94.95	488085	111.95	202	124.00	183	136.60	164

Average of 14.400 to 14.407 min.: VL038623.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
136.90	341	148.90	203	158.80	388		
138.80	112	149.80	542	160.60	150		
139.75	252	151.80	57	160.90	347		
140.85	3776	152.90	350	170.90	131		
141.80	429	153.70	86	171.95	966		
142.85	3576	153.85	233	172.85	3070		
143.85	226	154.90	1033	173.80	334336		
144.75	447	155.90	265	174.85	23755		
145.85	823	156.70	246	175.85	324373		
146.85	324	156.95	523	176.85	21173		
147.80	978	157.90	54	177.80	632		