
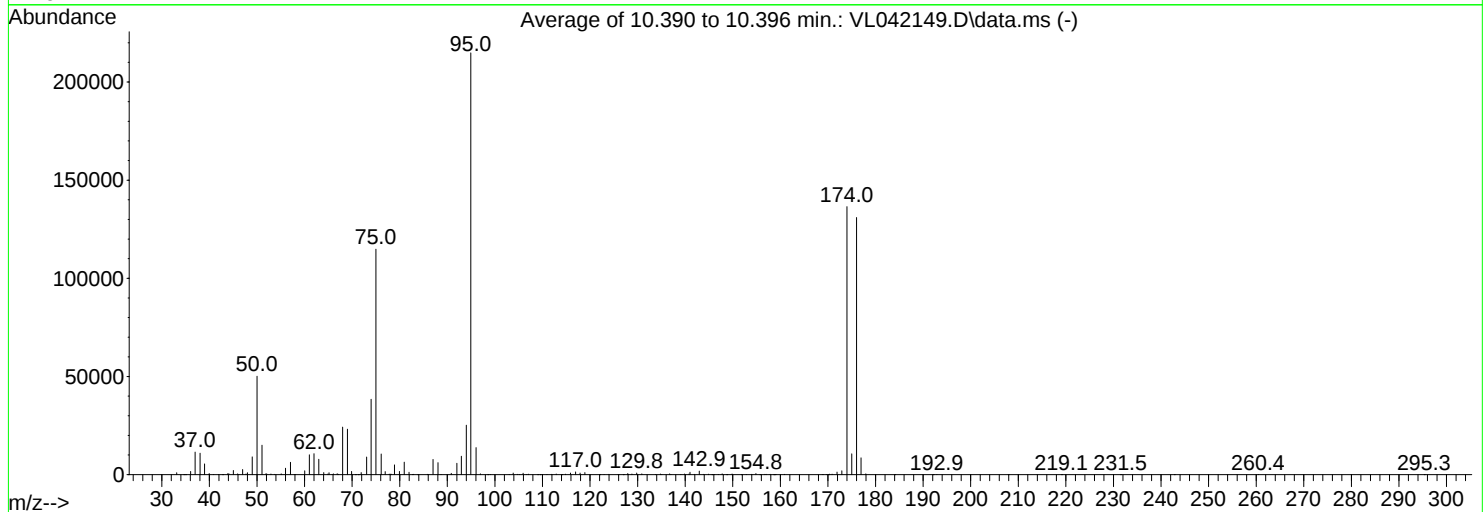


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031725\
Data File : VL042149.D
Acq On : 17 Mar 2025 09:09
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Feb 26 01:08:36 2025

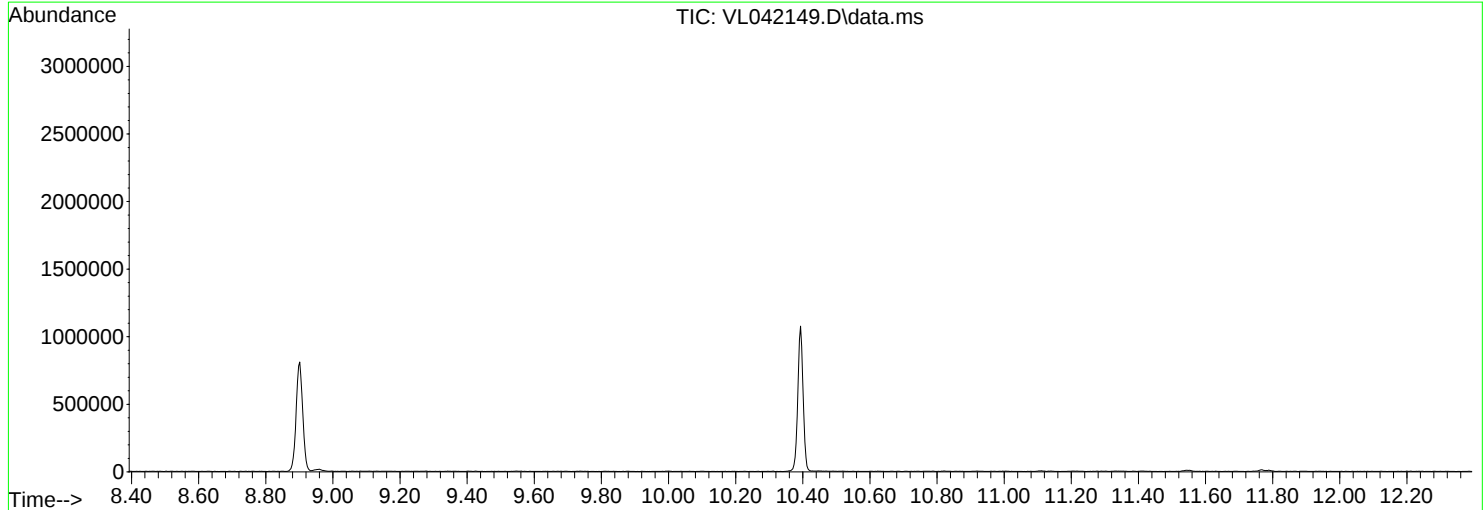

AutoFind: Scans 3183, 3184, 3185; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.3	50096	PASS
75	95	30	66	53.5	114875	PASS
95	95	100	100	100.0	214863	PASS
96	95	5	9	6.4	13812	PASS
173	174	0.00	2	1.4	1941	PASS
174	95	50	120	63.5	136544	PASS
175	174	4	9	7.7	10561	PASS
176	174	93	101	96.0	131021	PASS
177	176	5	9	6.6	8603	PASS

Average of 10.390 to 10.396 min.: VL042149.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	956	43.85	532	51.90	525	62.00	1065
34.60	19	44.10	512	52.05	348	63.00	782
35.00	32	45.05	2152	52.95	314	64.05	107
36.05	1619	45.95	382	53.75	155	64.90	30
37.00	11470	46.20	67	55.10	409	65.15	998
38.05	10914	47.00	2620	56.00	3300	65.80	92
39.00	5467	47.70	364	57.05	6318	66.05	391
39.95	580	48.00	968	57.90	87	66.85	518
40.90	75	49.00	9019	58.10	91	67.10	153
41.95	122	50.00	50096	60.05	1936	68.00	24232
42.80	38	51.05	15036	61.00	10110	69.00	23121

Average of 10.390 to 10.396 min.: VL042149.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
69.90	1617	78.20	287	87.00	7751	99.05	56
70.70	19	78.90	5007	88.05	6097	103.00	80
71.30	24	79.95	1637	88.70	90	103.85	791
71.90	1043	80.95	6320	90.85	691	104.80	174
73.05	8935	81.95	1233	92.00	5753	105.20	65
74.00	38429	82.70	56	92.95	9387	105.95	780
75.00	114875	82.80	90	94.00	25184	106.70	93
76.10	10501	82.95	189	94.95	214863	107.05	230
76.95	1575	83.80	26	96.05	13812	109.00	20
77.80	230	85.85	157	96.95	419	109.50	22
78.00	227	86.10	114	98.50	22	110.05	82

Average of 10.390 to 10.396 min.: VL042149.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
110.95	127	123.95	129	136.75	404	145.90	96
111.95	184	125.90	26	137.00	65	146.10	64
112.90	353	127.00	17	139.10	104	146.95	66
114.05	38	127.90	519	139.85	289	147.75	391
114.85	234	128.10	228	140.80	375	148.70	34
115.90	794	128.80	358	141.00	1196	148.90	78
116.95	1382	129.80	841	141.95	200	149.85	292
117.90	850	130.90	441	142.95	1785	151.80	21
118.90	1034	133.75	113	143.90	175	152.85	88
122.00	33	134.80	374	144.90	284	154.00	188
122.95	75	135.10	82	145.60	44	154.85	549

Average of 10.390 to 10.396 min.: VL042149.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.70	43	170.10	22	192.10	38		
156.75	186	170.35	226	192.90	60		
157.00	177	170.85	278	207.90	21		
157.85	142	171.90	1336	219.10	32		
158.60	42	172.90	1941	231.50	26		
158.80	42	174.00	136544	242.80	26		
159.10	66	175.00	10561	260.45	73		
160.85	166	176.00	131021	295.30	24		
168.80	68	176.95	8603				
169.00	50	177.95	393				
169.65	117	184.00	29				