


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL032019\
Data File : VL033389.D
Acq On : 20 Mar 2019 13:24
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL031519AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Mar 15 14:52:14 2019
Last Update : Fri Mar 15 14:52:14 2019

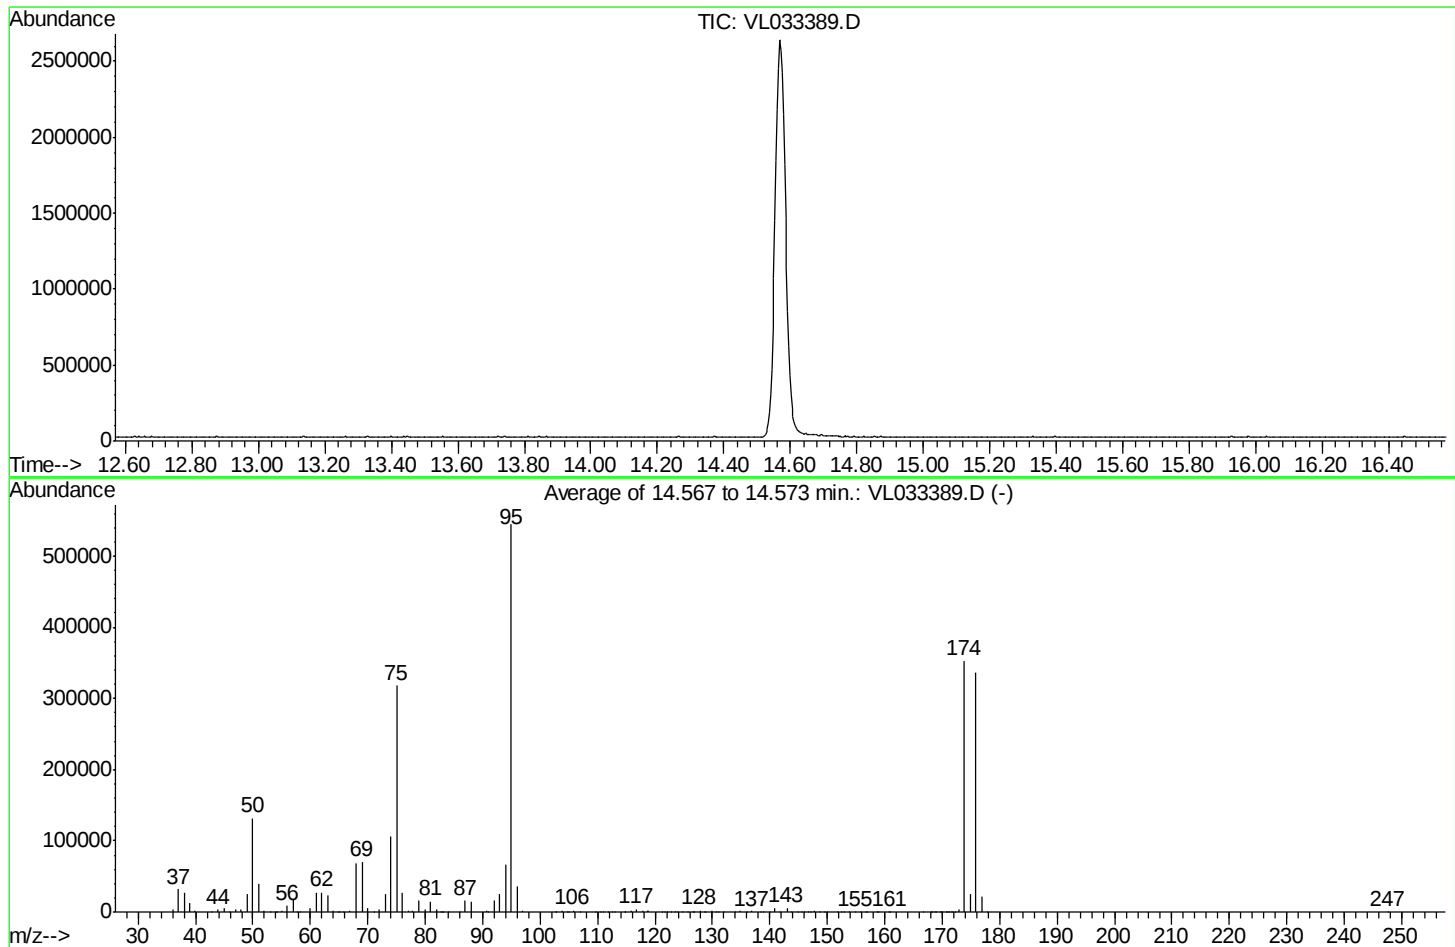

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	131392	PASS
75	95	30	66	58.3	317461	PASS
95	95	100	100	100.0	544448	PASS
96	95	5	9	6.5	35277	PASS
173	174	0.00	2	0.9	3270	PASS
174	95	50	120	64.8	352704	PASS
175	174	4	9	7.4	26013	PASS
176	174	93	101	95.1	335445	PASS
177	176	5	9	6.3	21037	PASS