


Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_L\DATA\VL032322\  
 Data File : VL038714.D  
 Acq On : 23 Mar 2022 12:47  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 400mL/MSVOA\_L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL032122AIR.M  
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Mon Mar 21 17:09:26 2022  
 Last Update : Mon Mar 21 17:09:26 2022

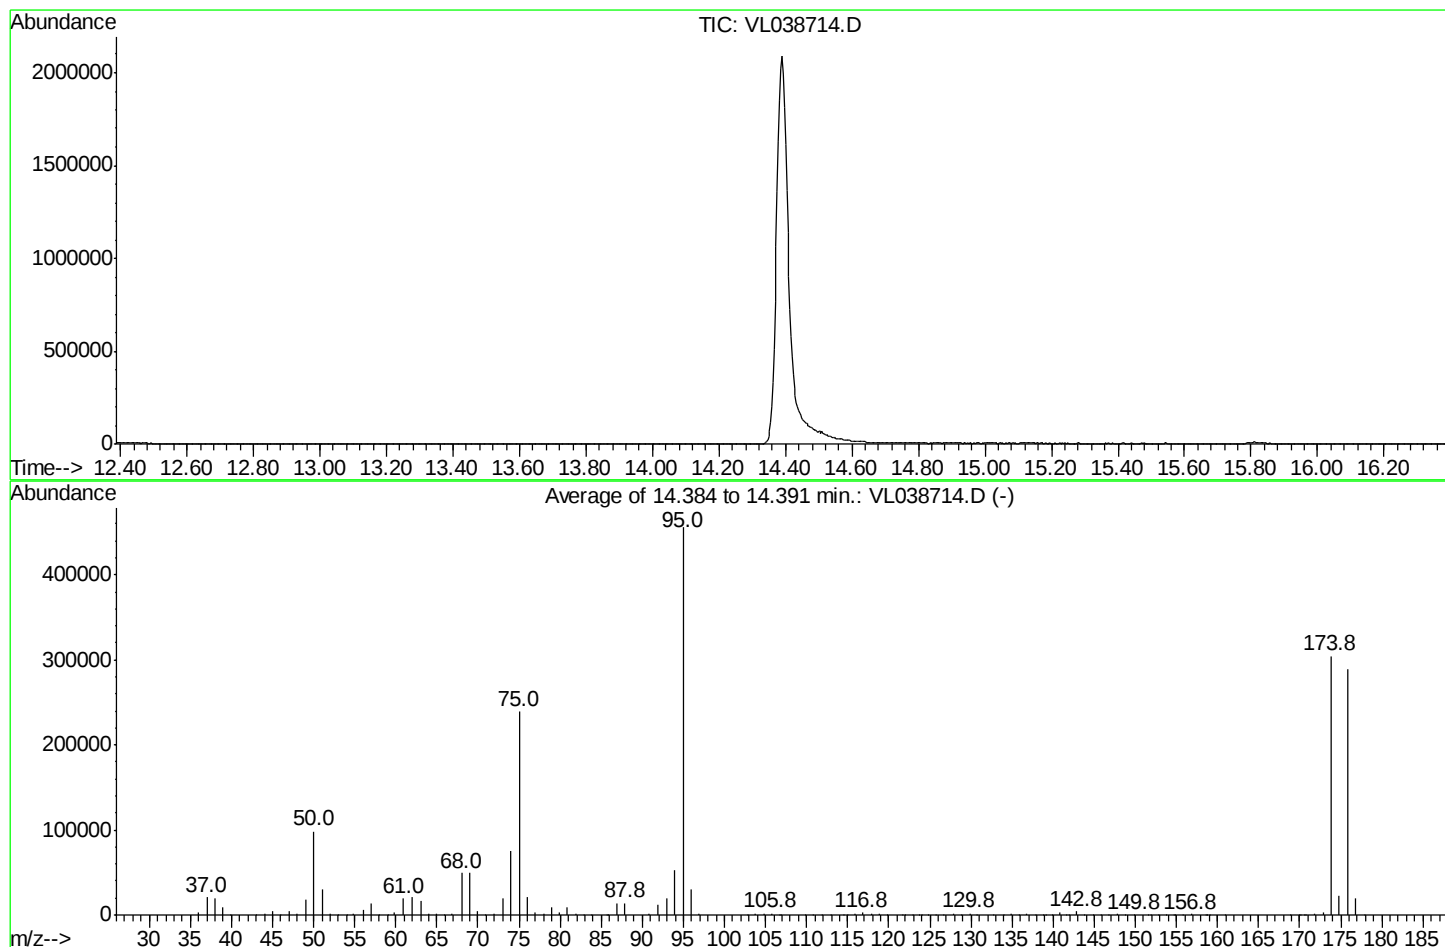

AutoFind: Scans 3607, 3608, 3609; Background Corrected with Scan 3585

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 21.5      | 98149   | PASS             |
| 75          | 95           | 30           | 66           | 52.4      | 238805  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 455829  | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 30797   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 2861    | PASS             |
| 174         | 95           | 50           | 120          | 66.8      | 304618  | PASS             |
| 175         | 174          | 4            | 9            | 7.4       | 22549   | PASS             |
| 176         | 174          | 93           | 101          | 95.0      | 289450  | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 19176   | PASS             |