


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL032421\
 Data File : VL036460.D
 Acq On : 24 Mar 2021 8:40
 Operator :
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030321AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Mar 03 14:18:24 2021
 Last Update : Wed Mar 03 14:18:24 2021

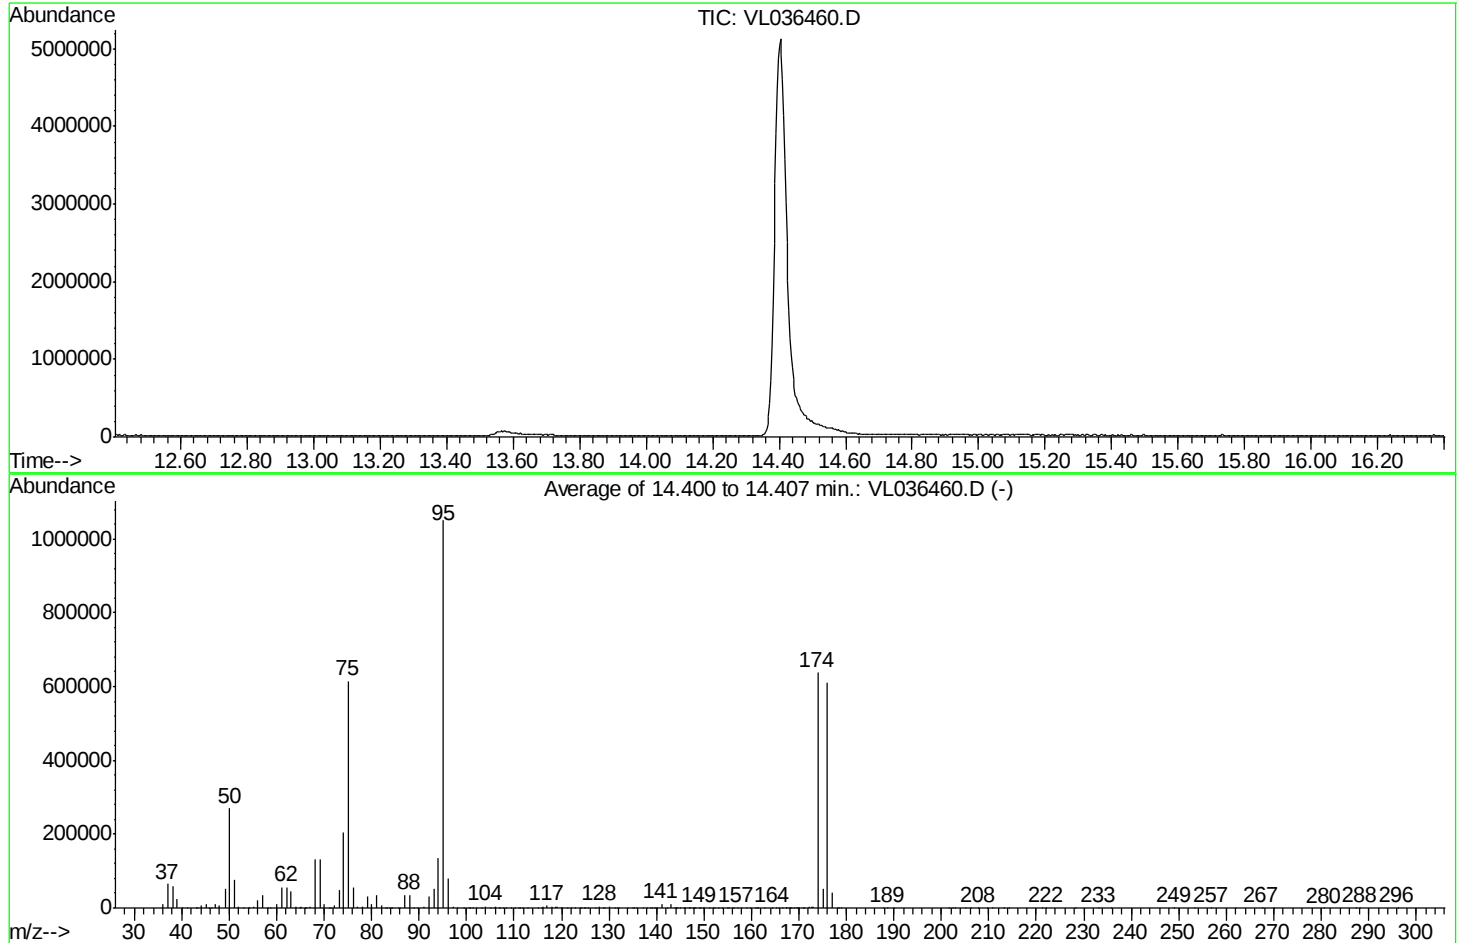

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.7	269525	PASS
75	95	30	66	58.5	613802	PASS
95	95	100	100	100.0	1050048	PASS
96	95	5	9	7.5	78493	PASS
173	174	0.00	2	0.5	3209	PASS
174	95	50	120	60.8	637909	PASS
175	174	4	9	8.1	51690	PASS
176	174	93	101	95.8	611178	PASS
177	176	5	9	6.6	40144	PASS