


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL032422\
 Data File : VL038748.D
 Acq On : 24 Mar 2022 13:51
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032122AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Mar 21 17:09:26 2022
 Last Update : Mon Mar 21 17:09:26 2022

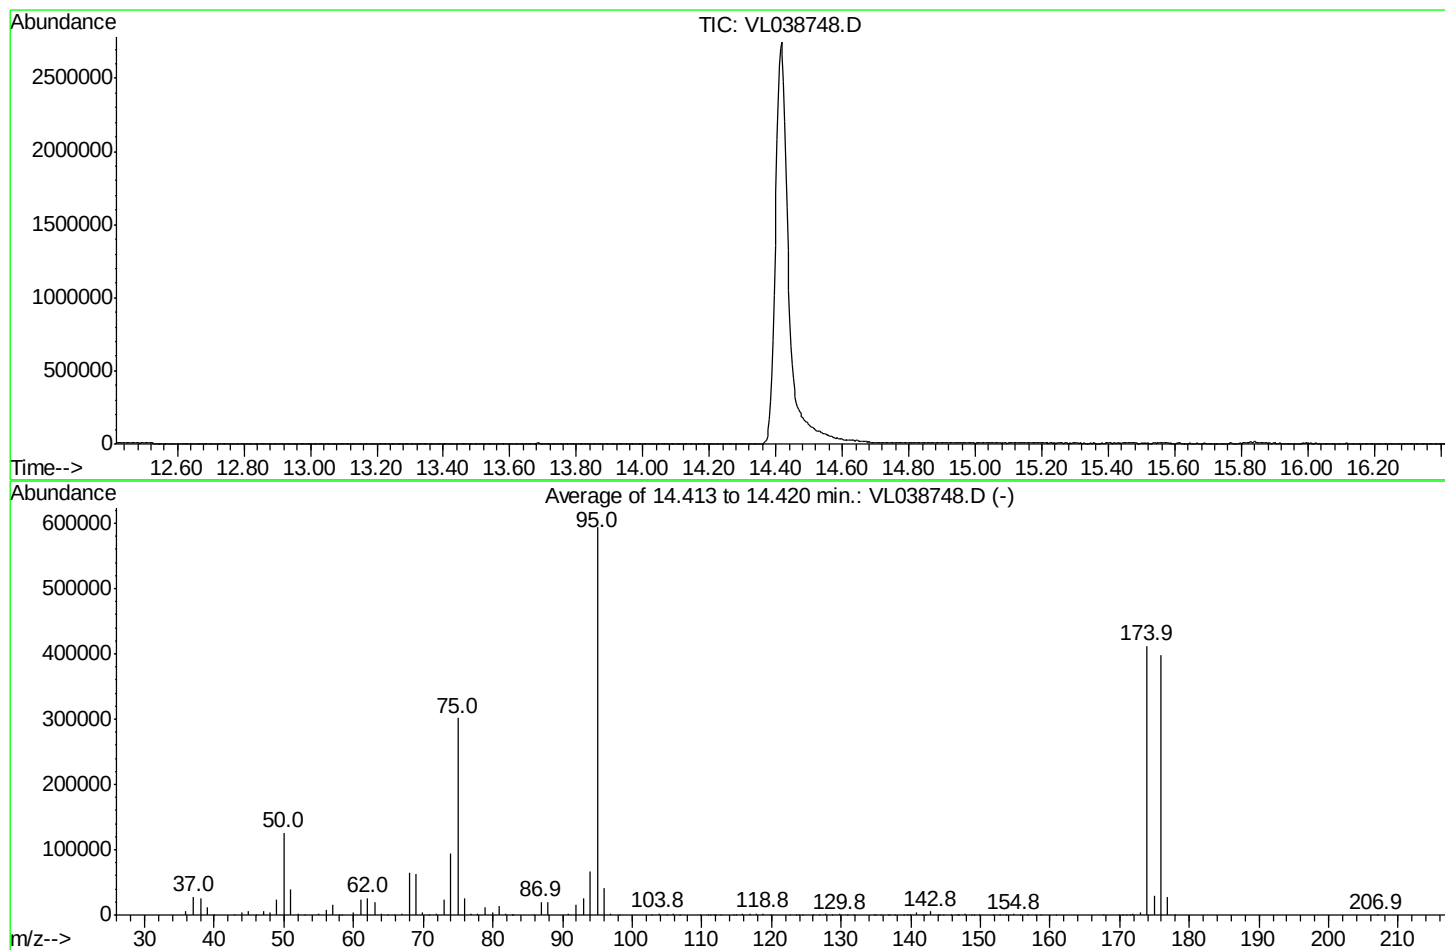

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.2	125874	PASS
75	95	30	66	50.8	301717	PASS
95	95	100	100	100.0	593621	PASS
96	95	5	9	6.8	40376	PASS
173	174	0.00	2	0.9	3722	PASS
174	95	50	120	69.4	411925	PASS
175	174	4	9	7.4	30333	PASS
176	174	93	101	96.8	398720	PASS
177	176	5	9	6.7	26906	PASS