


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL032621\
 Data File : VL036503.D
 Acq On : 26 Mar 2021 5:13
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032521AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Mar 25 09:42:40 2021
 Last Update : Thu Mar 25 09:42:40 2021

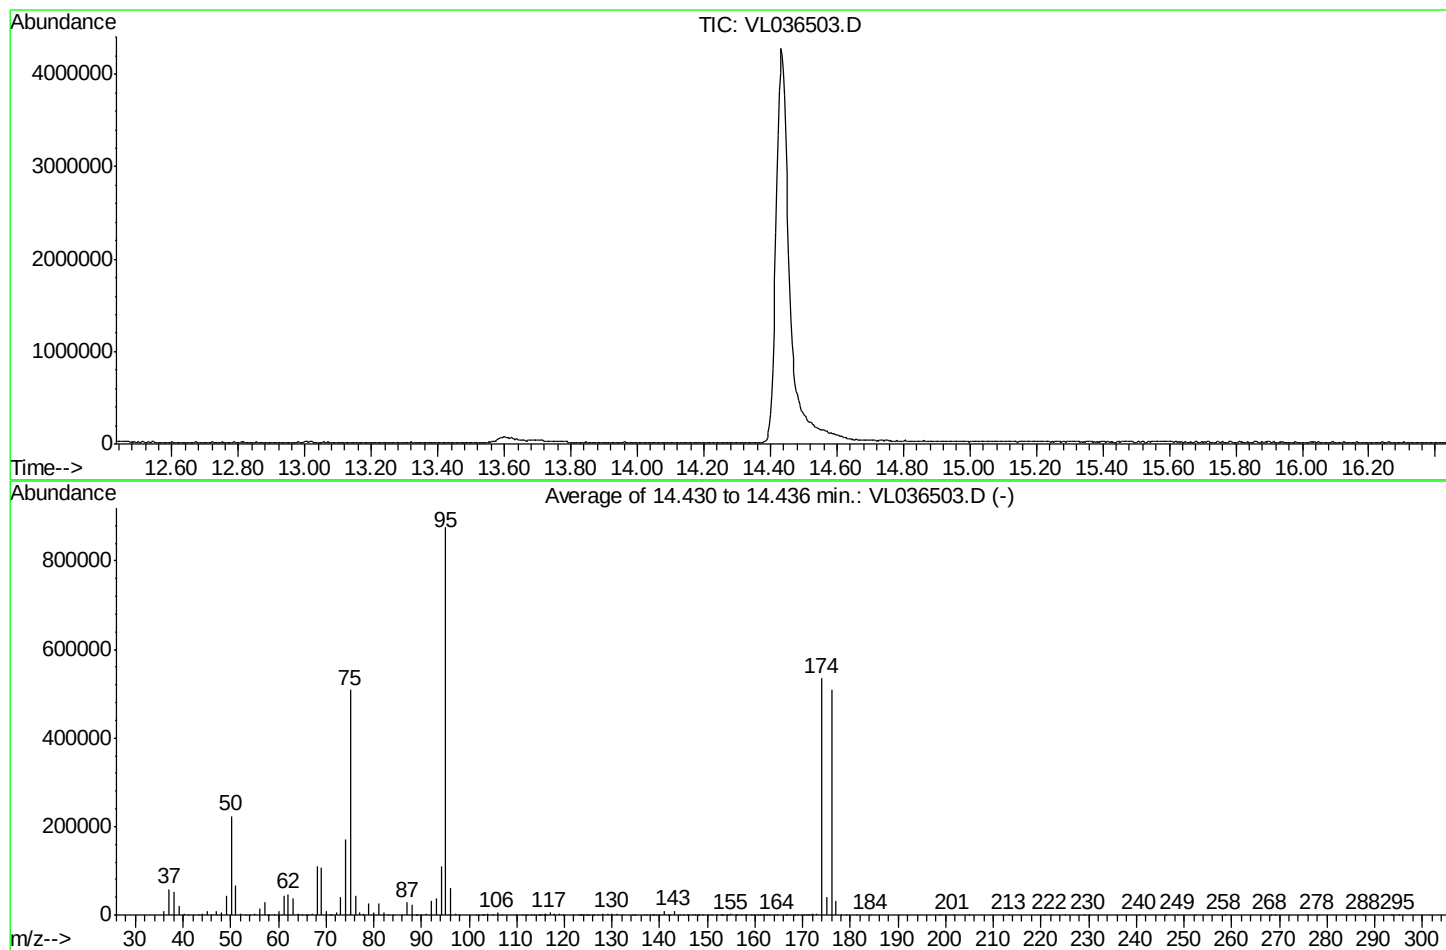

AutoFind: Scans 3621, 3622, 3623; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.5	223466	PASS
75	95	30	66	58.0	507788	PASS
95	95	100	100	100.0	876096	PASS
96	95	5	9	6.9	60682	PASS
173	174	0.00	2	0.7	3897	PASS
174	95	50	120	61.0	534080	PASS
175	174	4	9	7.7	41106	PASS
176	174	93	101	95.4	509383	PASS
177	176	5	9	6.4	32418	PASS