


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL032919\
 Data File : VL033495.D
 Acq On : 29 Mar 2019 9:18
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032519AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019
 Last Update : Tue Mar 26 16:00:50 2019

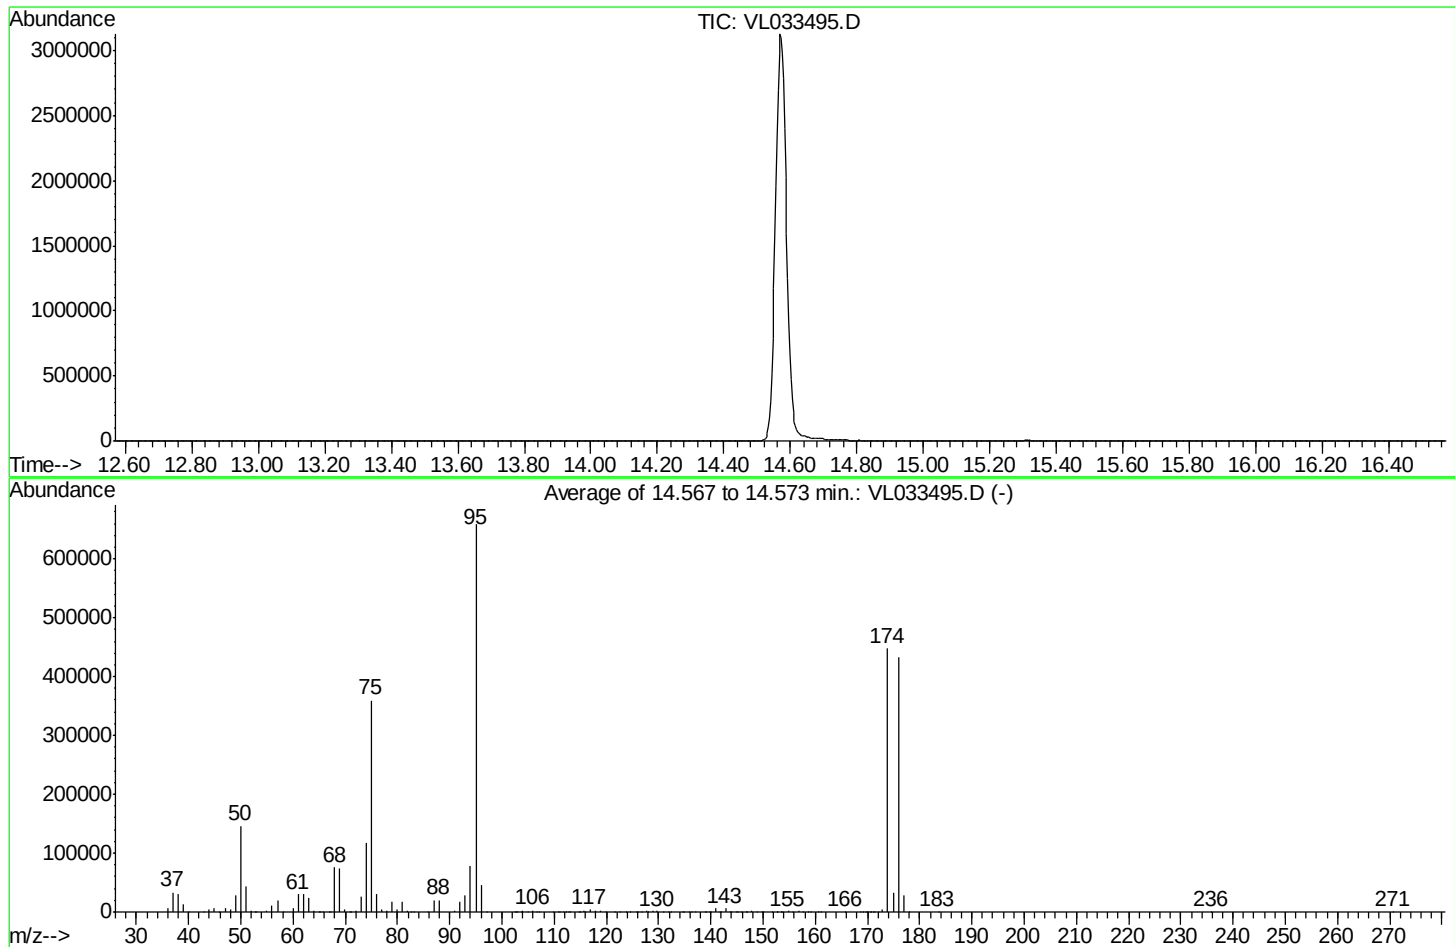

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.2	145920	PASS
75	95	30	66	54.5	358869	PASS
95	95	100	100	100.0	658645	PASS
96	95	5	9	7.1	46648	PASS
173	174	0.00	2	1.0	4305	PASS
174	95	50	120	68.0	447872	PASS
175	174	4	9	7.5	33752	PASS
176	174	93	101	96.8	433408	PASS
177	176	5	9	6.6	28802	PASS