


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL032921\
 Data File : VL036535.D
 Acq On : 29 Mar 2021 10:19
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032521AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Mar 25 09:42:40 2021
 Last Update : Thu Mar 25 09:42:40 2021

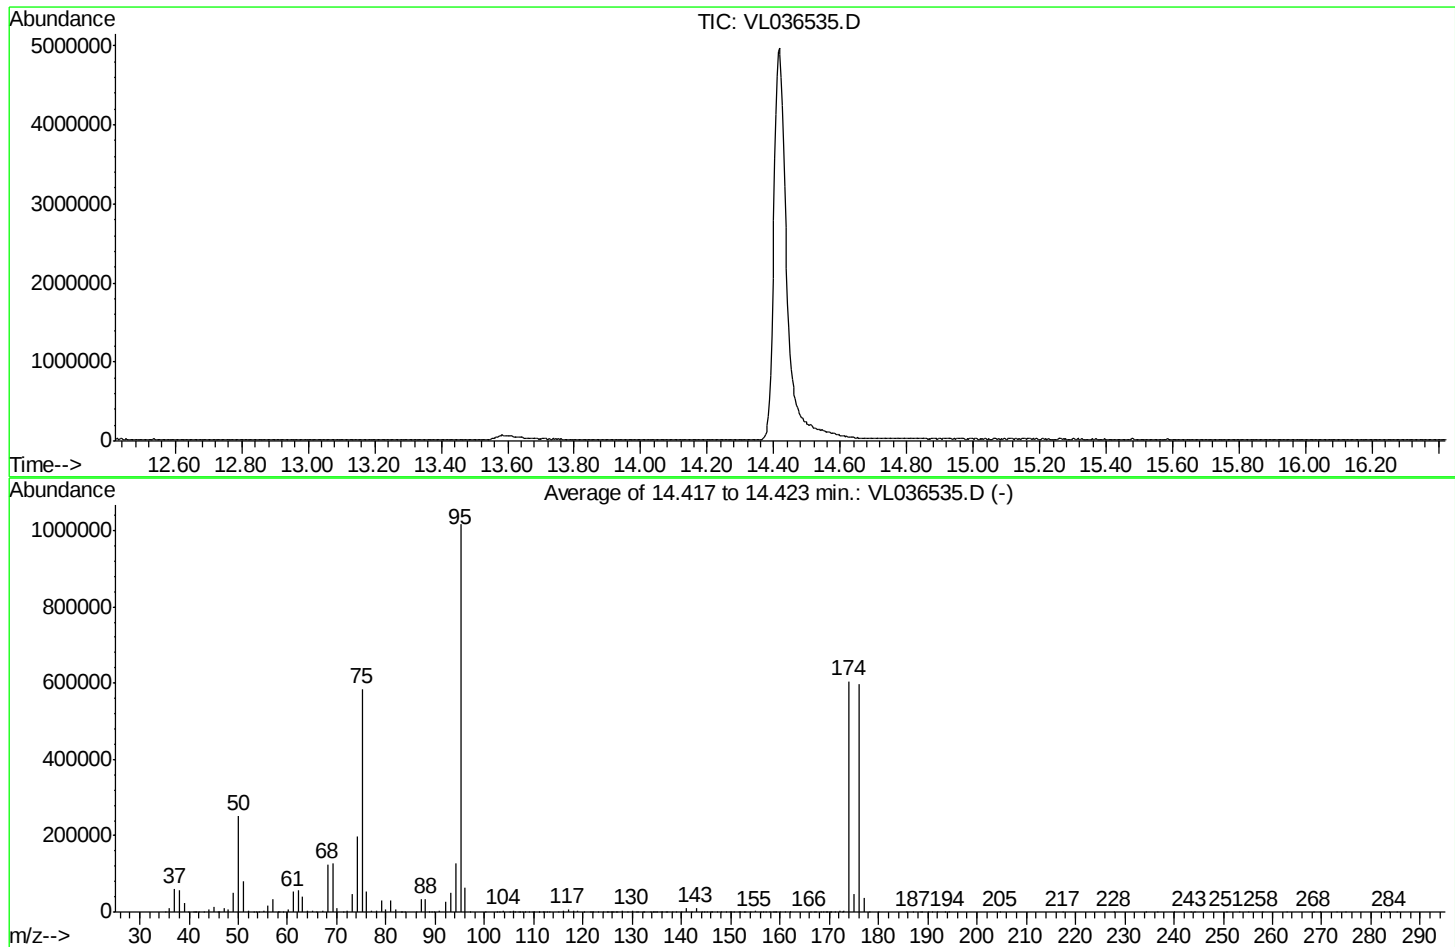

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	252928	PASS
75	95	30	66	57.5	584554	PASS
95	95	100	100	100.0	1016388	PASS
96	95	5	9	6.4	65525	PASS
173	174	0.00	2	0.8	4738	PASS
174	95	50	120	59.6	605440	PASS
175	174	4	9	7.8	47389	PASS
176	174	93	101	98.5	596245	PASS
177	176	5	9	6.2	37216	PASS