


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL033121\
 Data File : VL036590.D
 Acq On : 31 Mar 2021 5:11
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032521AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Mar 25 09:42:40 2021
 Last Update : Thu Mar 25 09:42:40 2021

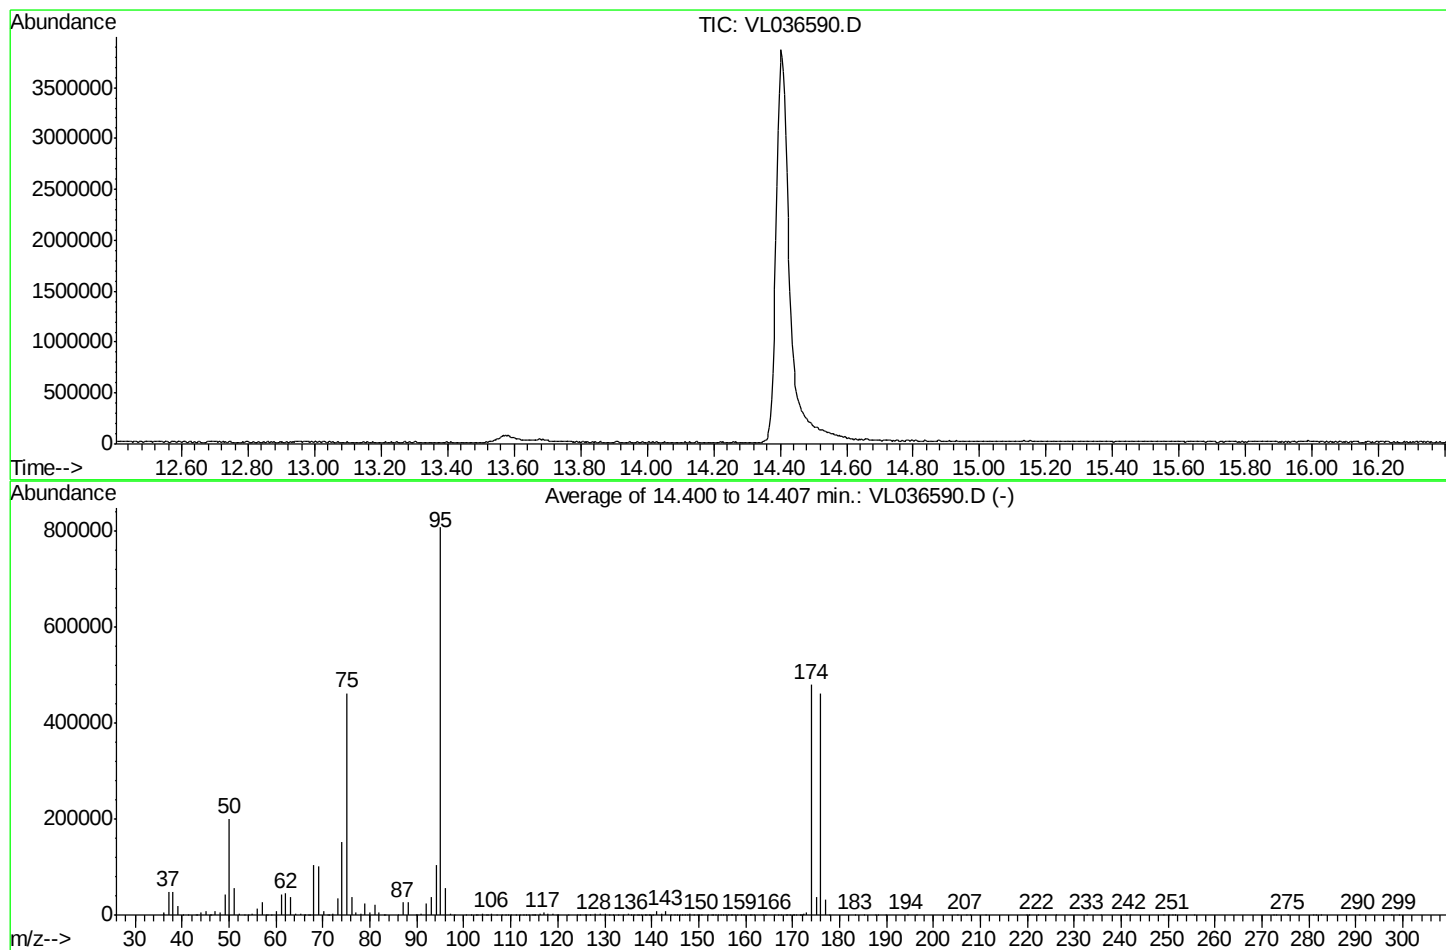

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	200898	PASS
75	95	30	66	57.3	462250	PASS
95	95	100	100	100.0	806869	PASS
96	95	5	9	7.0	56416	PASS
173	174	0.00	2	1.3	6112	PASS
174	95	50	120	59.3	478656	PASS
175	174	4	9	7.6	36586	PASS
176	174	93	101	96.4	461333	PASS
177	176	5	9	7.0	32330	PASS