

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL033125\
 Data File : VL042209.D
 Acq On : 31 Mar 2025 14:07
 Operator : SY/MD
 Sample : VIBLK
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VIBLK

Quant Time: Apr 01 01:40:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.807	49	183601	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	3.988	114	531049	10.000	ppbv	0.04
55) Chlorobenzene-d5	8.911	117	471191	10.000	ppbv	0.04

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.400	95	377111	9.746	ppbv	0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL033125\
Data File : VL042209.D
Acq On : 31 Mar 2025 14:07
Operator : SY/MD
Sample : VIBLK
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Apr 01 01:40:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration




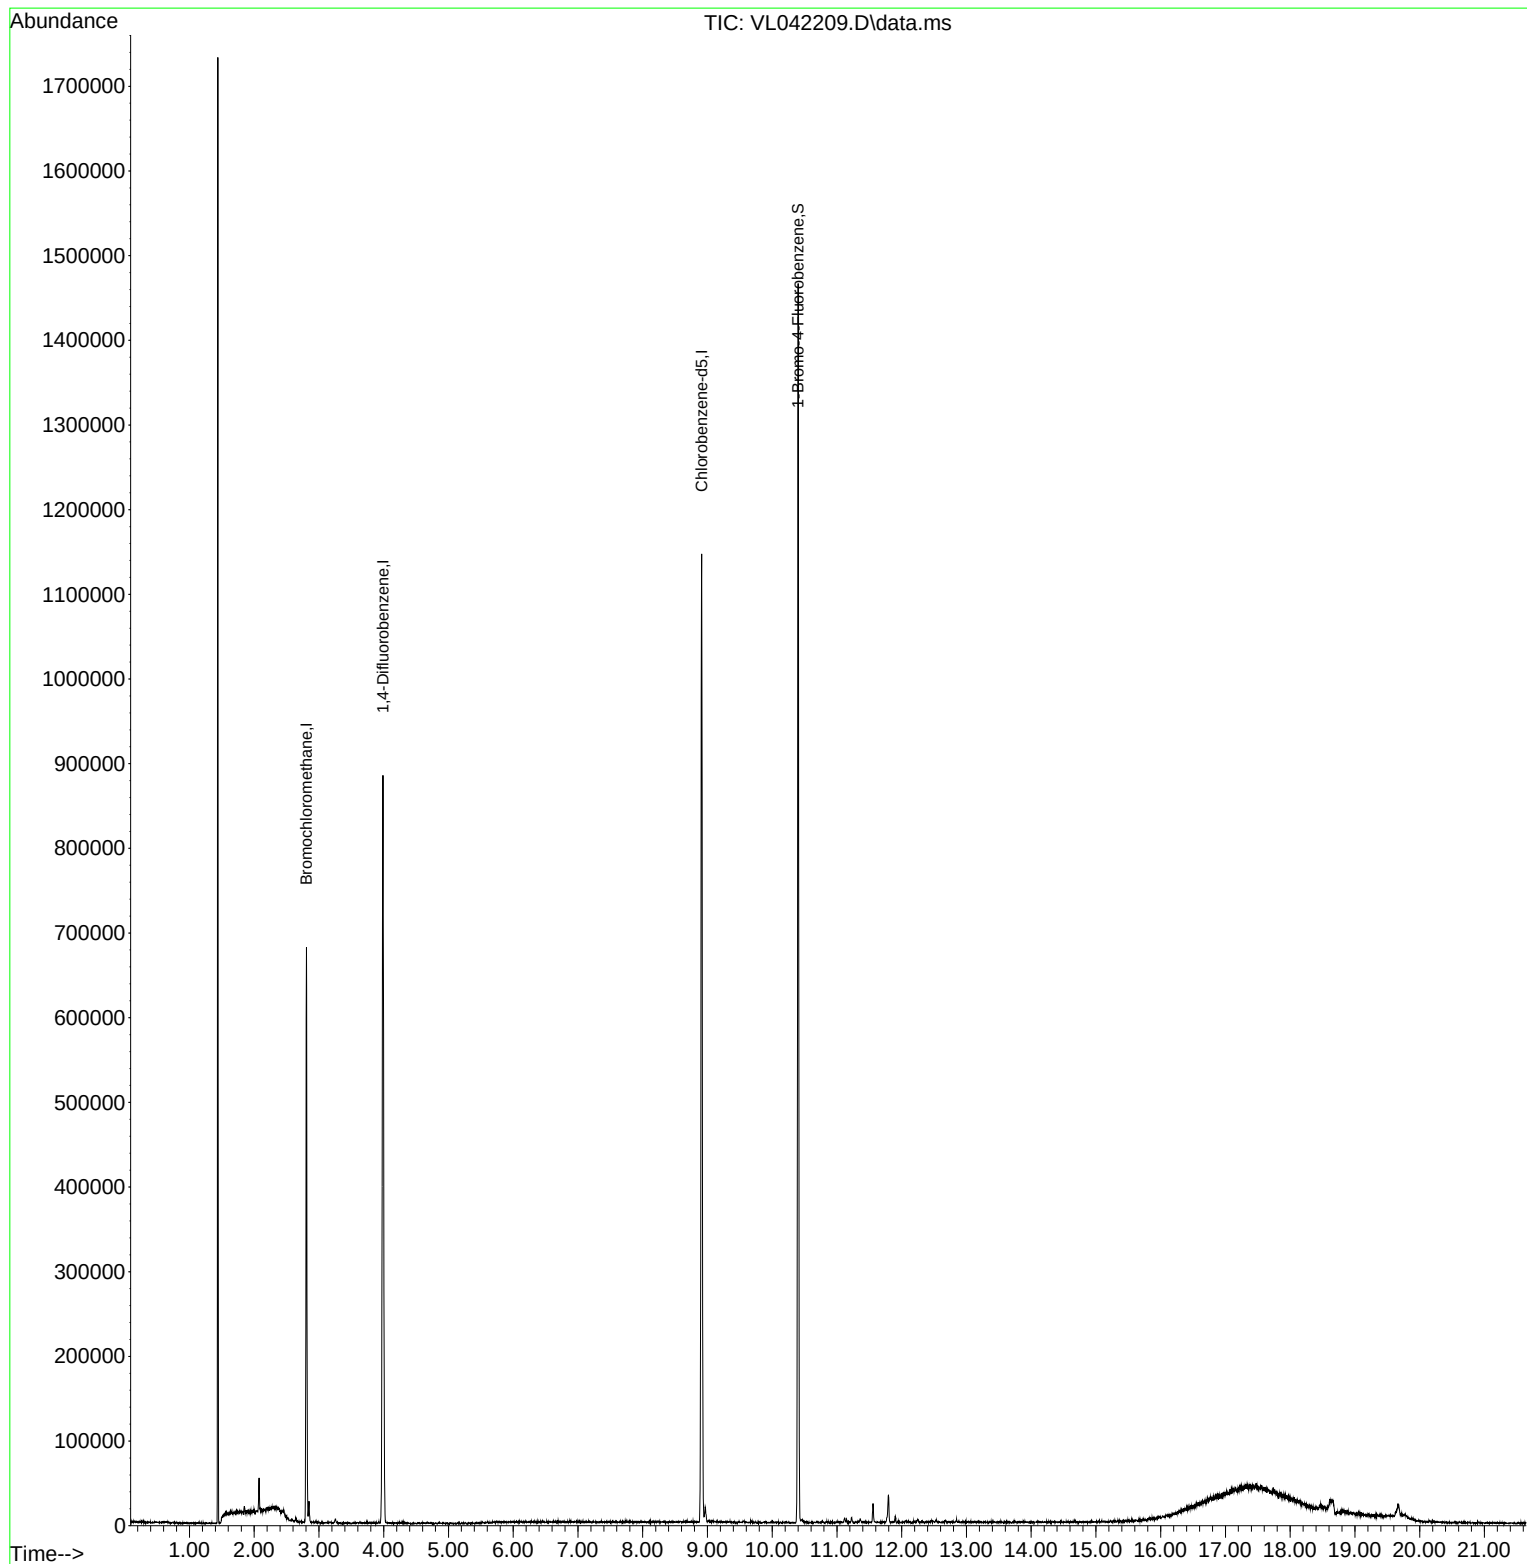


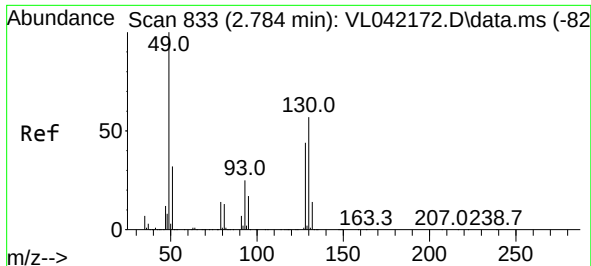

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.807 min Scan# 84
Delta R.T. 0.023 min
Lab File: VL042209.D
Acq: 31 Mar 2025 14:07




Instrument :
MSVOA_L
ClientSampleId :
VIBLK


Tgt Ion: 49 Resp: 183601
Ion Ratio Lower Upper
49 100
128 46.4 22.9 68.5
130 59.6 28.8 86.4

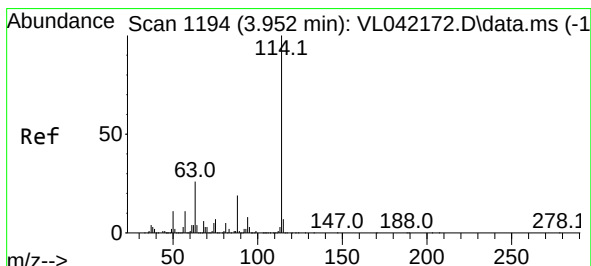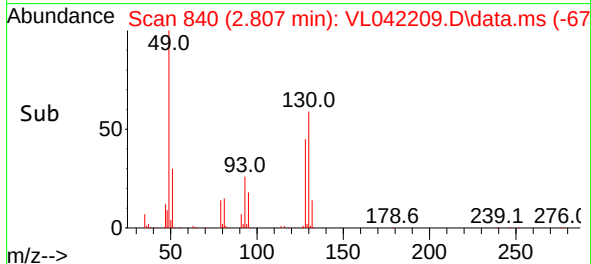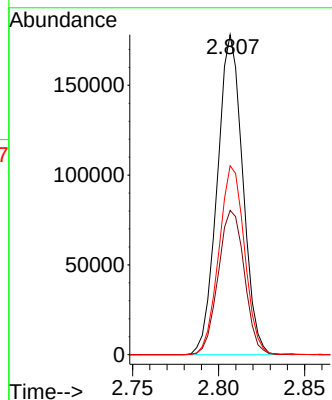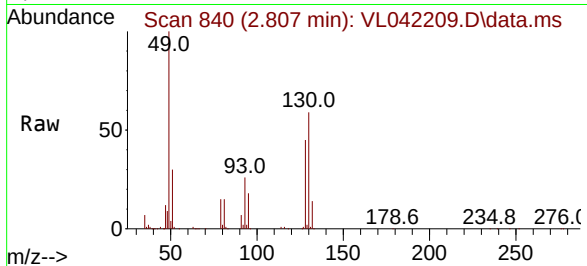

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.988 min Scan# 1205
Delta R.T. 0.036 min
Lab File: VL042209.D
Acq: 31 Mar 2025 14:07

Tgt Ion: 114 Resp: 531049
Ion Ratio Lower Upper
114 100
63 25.0 20.7 31.1
88 17.5 15.0 22.4


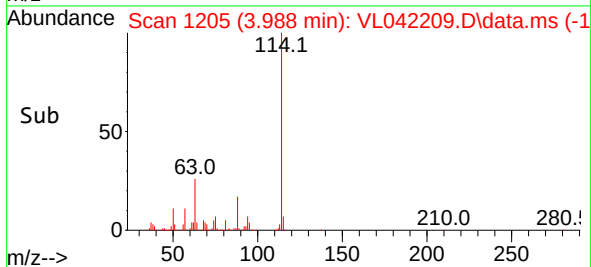
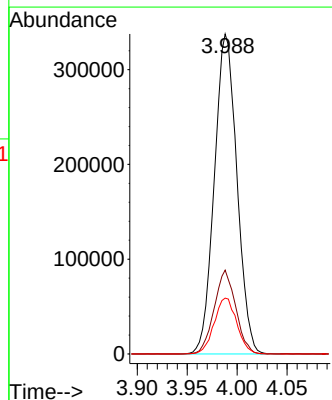
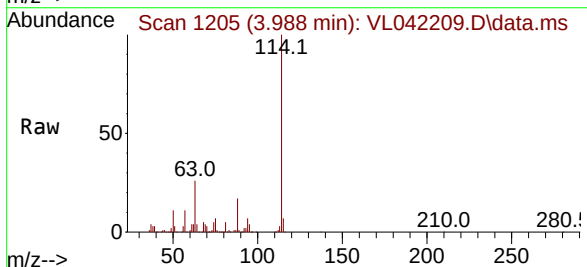


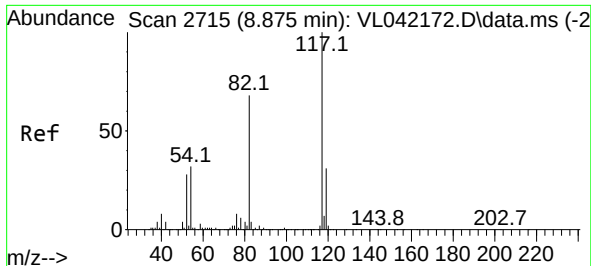

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.911 min Scan# 21
Delta R.T. 0.036 min
Lab File: VL042209.D
Acq: 31 Mar 2025 14:07

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 471191
Ion Ratio Lower Upper
117 100
82 64.2 55.8 83.6
119 31.9 25.5 38.3

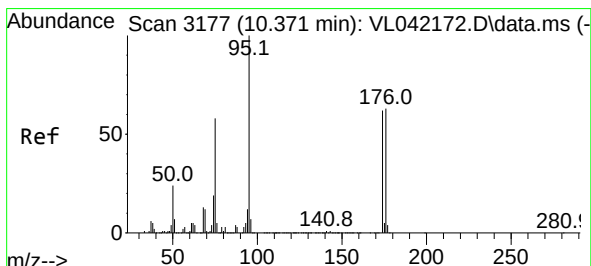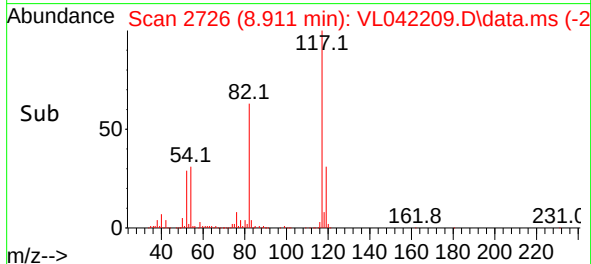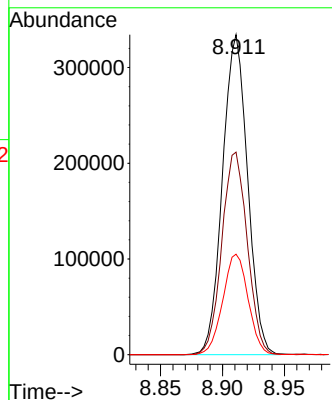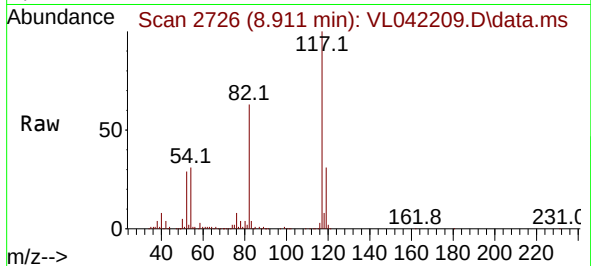

#68
1-Bromo-4-Fluorobenzene
Concen: 9.746 ppbv
RT: 10.400 min Scan# 3186
Delta R.T. 0.029 min
Lab File: VL042209.D
Acq: 31 Mar 2025 14:07

Tgt Ion: 95 Resp: 377111
Ion Ratio Lower Upper
95 100
174 60.4 50.6 76.0
175 4.4 3.8 5.6

