
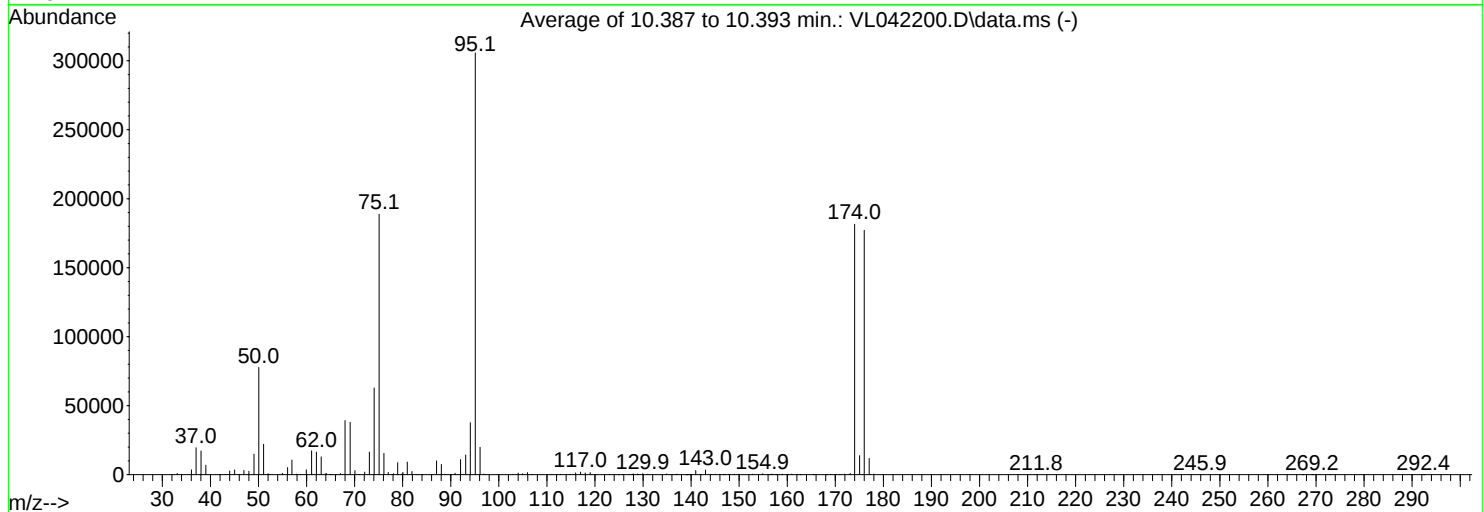


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL033125\
Data File : VL042200.D
Acq On : 31 Mar 2025 08:09
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

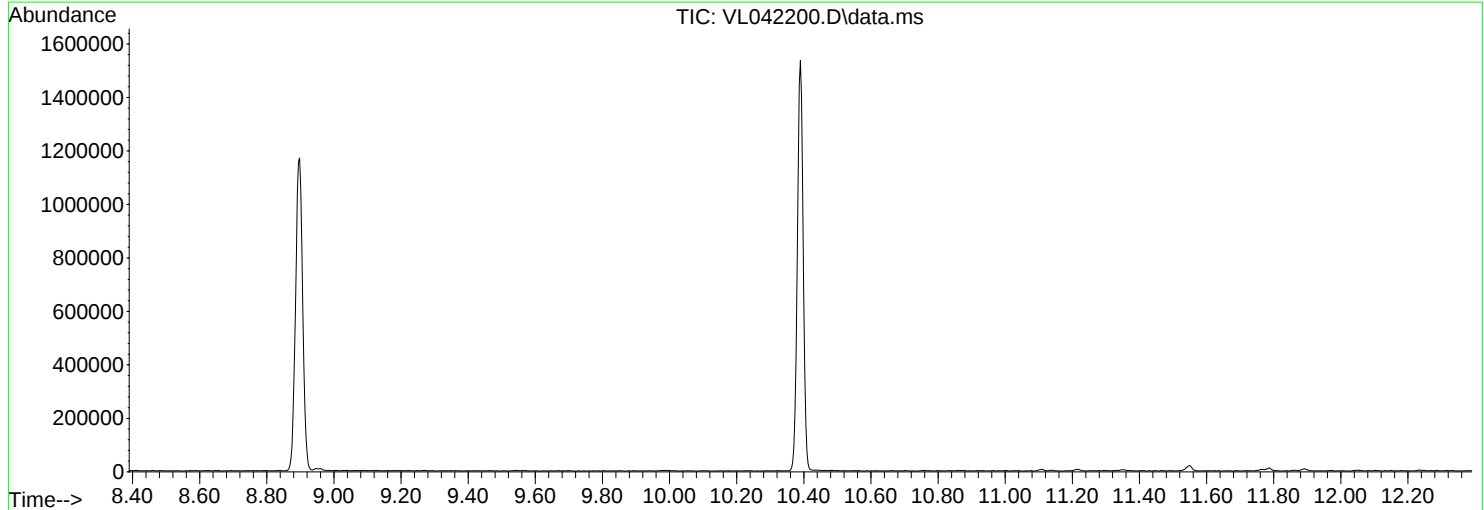

AutoFind: Scans 3182, 3183, 3184; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	77685	PASS
75	95	30	66	61.8	188843	PASS
95	95	100	100	100.0	305749	PASS
96	95	5	9	6.5	19795	PASS
173	174	0.00	2	0.5	913	PASS
174	95	50	120	59.4	181483	PASS
175	174	4	9	7.6	13787	PASS
176	174	93	101	97.6	177067	PASS
177	176	5	9	6.6	11740	PASS

Average of 10.387 to 10.393 min.: VL042200.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	975	46.00	208	57.95	385	67.05	874
36.05	3507	46.95	3045	58.75	124	68.00	3919
37.00	19484	48.00	2455	59.95	3488	69.05	3797
38.05	17138	49.05	14857	61.05	17269	70.05	305
39.05	6803	50.05	77685	62.05	16376	70.90	171
41.10	109	51.05	22030	63.05	12891	72.10	1817
41.90	98	52.00	703	63.90	548	73.05	16309
42.15	86	52.20	275	64.10	956	74.05	62893
43.15	299	54.95	1071	64.95	279	75.10	188843
44.00	2694	56.05	5087	65.20	156	76.10	15437
45.05	3400	56.95	10540	66.00	24	77.00	1630

Average of 10.387 to 10.393 min.: VL042200.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.80	264	87.05	9968	99.80	70	112.80	254
78.10	661	88.05	7479	102.85	137	114.90	236
78.95	8711	88.80	77	104.00	1139	115.95	1319
79.90	820	89.85	36	104.90	600	117.00	1833
80.05	1619	90.90	1038	105.95	1509	117.95	1303
80.95	9196	92.05	10949	106.75	143	119.00	1558
81.90	2322	93.10	14323	107.05	182	120.10	43
82.80	113	94.05	37717	109.95	218	123.05	82
83.15	178	95.10	305749	111.05	232	123.75	138
84.00	18	96.10	19795	111.90	136	124.90	24
85.80	205	96.90	427	112.15	129	125.80	143

Average of 10.387 to 10.393 min.: VL042200.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.10	157	135.70	87	143.00	3359	152.80	320
127.70	373	136.60	94	144.15	224	153.95	264
127.95	605	136.90	211	145.00	397	154.90	748
128.85	484	137.10	389	145.95	323	155.85	174
129.10	132	138.90	26	146.70	31	156.10	43
129.80	224	139.15	60	147.10	158	156.60	104
129.95	745	139.70	33	147.80	201	156.85	500
131.00	393	140.00	56	148.05	393	157.10	137
132.00	99	140.95	3083	148.95	316	157.60	31
133.95	133	141.85	346	149.95	357	158.00	87
134.95	655	142.20	120	151.85	168	158.80	88

Average of 10.387 to 10.393 min.: VL042200.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
159.00	240	171.85	485	269.20	29		
160.00	23	172.10	118	272.90	28		
160.85	327	173.10	913	292.40	20		
161.10	136	174.00	181483				
162.00	35	175.05	13787				
162.65	44	176.00	177067				
165.40	19	177.05	11740				
168.10	38	178.00	473				
169.10	98	211.80	30				
170.20	167	245.90	22				
170.95	120	267.20	22				