


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL040121\
 Data File : VL036624.D
 Acq On : 1 Apr 2021 6:17
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032521AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Mar 25 09:42:40 2021
 Last Update : Thu Mar 25 09:42:40 2021

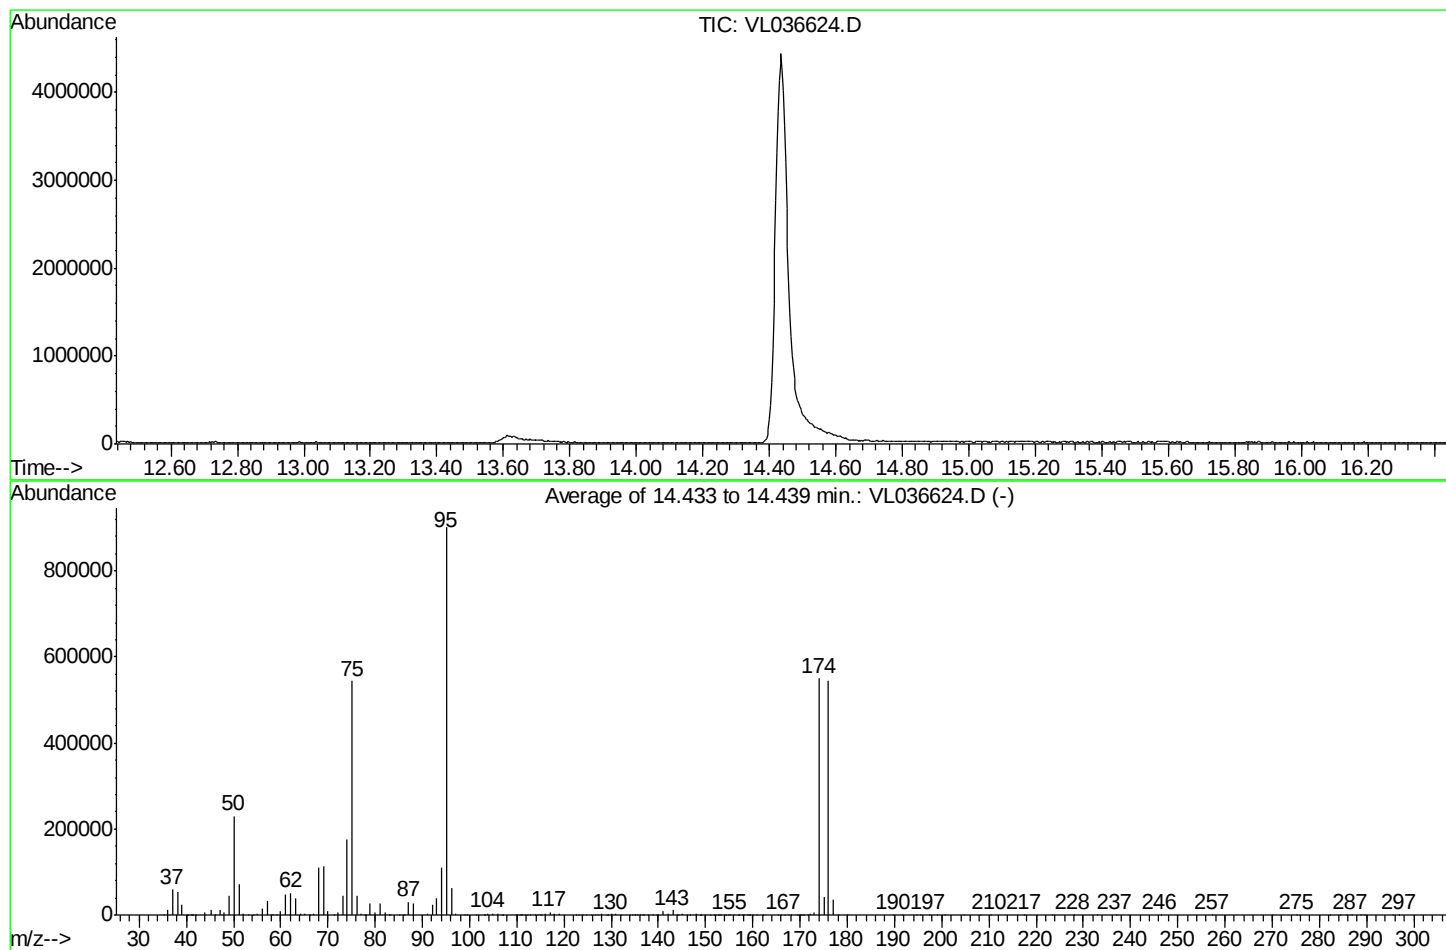

AutoFind: Scans 3622, 3623, 3624; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.5	229973	PASS
75	95	30	66	60.3	543829	PASS
95	95	100	100	100.0	901546	PASS
96	95	5	9	7.1	63773	PASS
173	174	0.00	2	1.3	6907	PASS
174	95	50	120	61.0	549994	PASS
175	174	4	9	7.6	41701	PASS
176	174	93	101	99.0	544725	PASS
177	176	5	9	6.6	35816	PASS