

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL040221\
 Data File : VL036655.D
 Acq On : 2 Apr 2021 21:41
 Operator : SY/AP
 Sample : M1853-04
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Apr 03 02:58:55 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Mar 25 09:42:40 2021
 QLast Update : Thu Mar 25 09:42:40 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.65	49	1187591	10.00	ppbv	-0.02
33) 1,4-Difluorobenzene	7.16	114	3117094	10.00	ppbv	-0.02
55) Chlorobenzene-d5	12.06	117	2791943	10.00	ppbv	-0.03

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
68) 1-Bromo-4-Fluorobenzene	14.39	95	2211637	9.94	ppbv	-0.03	
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.40%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.03	85	41924	0.216	ppbv	89
3) Chlorodifluoromethane	2.98	51	324597	1.463	ppbv	96
4) Chloromethane	3.13	50	9639	0.123	ppbv #	87
9) Propene	3.01	41	13647	0.193	ppbv #	72
10) Heptane	8.10	43	11643	0.065	ppbv #	28
11) Trichlorofluoromethane	3.94	101	24981	0.127	ppbv	95
12) 1,1,2-Trichlorotrifluoroet	4.47	101	5630	0.045	ppbv #	43
13) Ethanol	3.60	45	2018089	239.578	ppbv	93
15) Acetone	3.83	43	1308485	11.194	ppbv	96
16) 1,3-Butadiene	3.31	39	1880	0.023	ppbv	94
19) Isopropyl Alcohol	3.97	45	390119	6.067	ppbv #	1
20) Methylene Chloride	4.33	84	1728324	31.581	ppbv	94
23) Vinyl Acetate	5.05	43	16040	0.080	ppbv #	72
25) Ethyl Acetate	5.67	43	1054290	3.794	ppbv #	78
26) Hexane	5.66	57	1441604	11.179	ppbv #	47
27) Carbon Disulfide	4.53	76	6349	0.050	ppbv #	64
30) Cyclohexane	7.10	84	4458	0.043	ppbv #	1
34) 2-Butanone	5.23	43	60326	0.396	ppbv #	81
36) Benzene	6.86	78	29873	0.104	ppbv #	93
39) 1,2-Dichloropropane	7.15	63	818693	7.020	ppbv #	24
41) Tetrahydrofuran	6.04	42	8322	0.119	ppbv #	67
44) 2,2,4-Trimethylpentane	7.85	57	54691	0.108	ppbv #	60
52) Tetrachloroethene	11.20	164	2342	0.022	ppbv #	45
53) Toluene	9.78	91	86574	0.283	ppbv #	20
58) Ethyl Benzene	12.69	91	57638	0.142	ppbv	91
59) m/p-Xylene	12.95	91	116452	0.329	ppbv #	32
60) o-Xylene	13.67	91	82206	0.240	ppbv	97
69) p-Isopropyltoluene	17.63	119	61015	0.138	ppbv #	46
72) 4-Ethyltoluene	15.82	105	42465	0.113	ppbv #	95
73) 1,3,5-Trimethylbenzene	15.98	105	20361	0.058	ppbv	99
74) 1,2,4-Trimethylbenzene	16.74	105	128030	0.341	ppbv #	65
80) Naphthalene,2-methyl-	24.95	142	1429	0.033	ppbv #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL040221\
Data File : VL036655.D
Acq On : 2 Apr 2021 21:41
Operator : SY/AP
Sample : M1853-04
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :

Quant Time: Apr 03 02:58:55 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Mar 25 09:42:40 2021
QLast Update : Thu Mar 25 09:42:40 2021
Response via : Initial Calibration

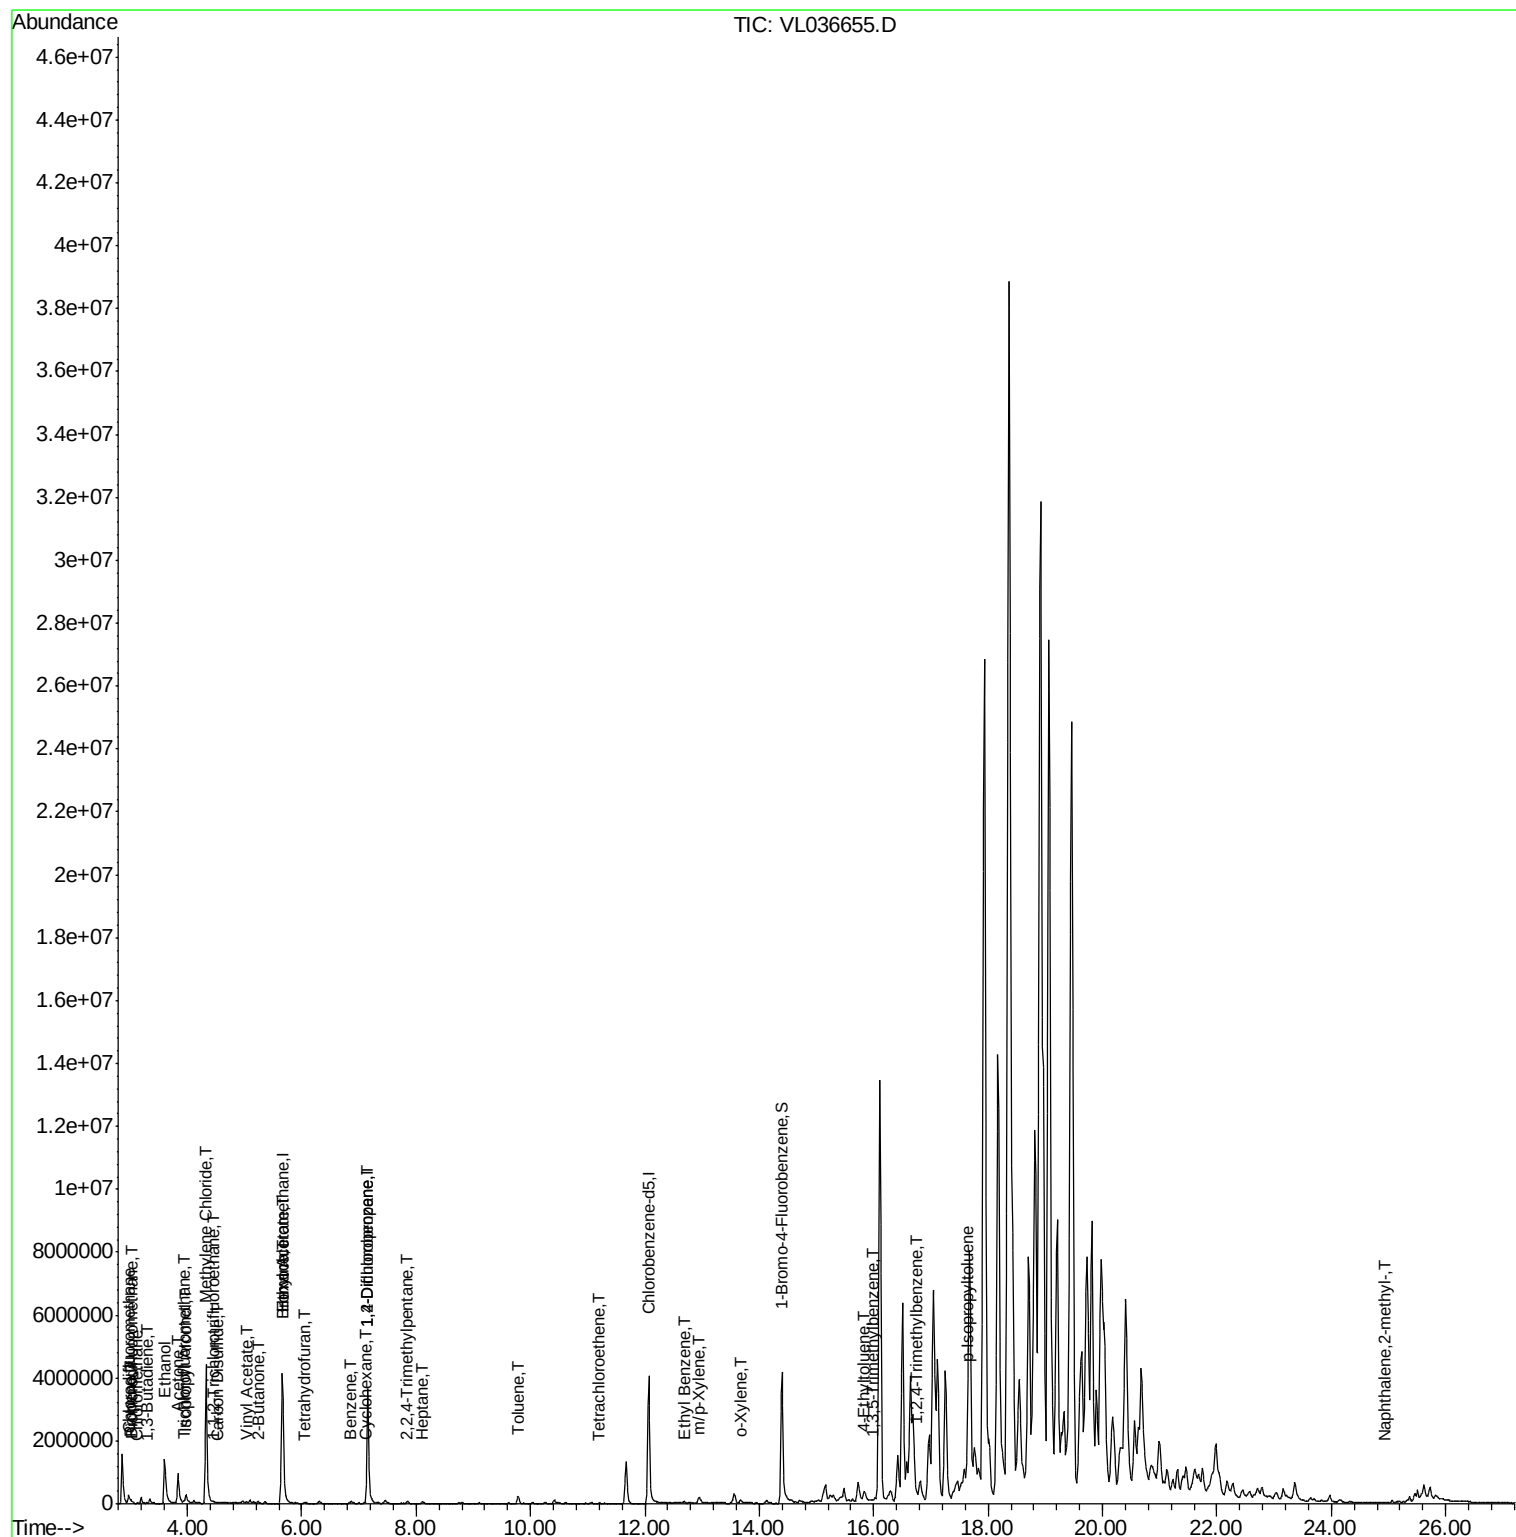

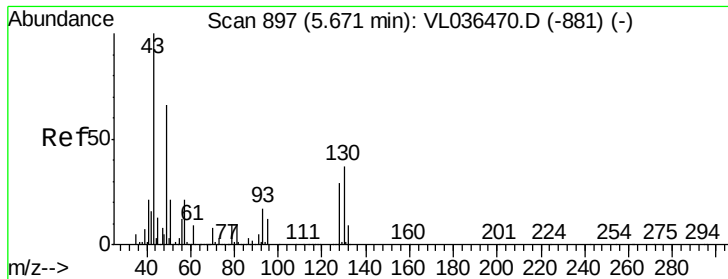

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.65 min Scan# 890

Delta R.T. -0.02 min

Lab File: VL036655.D

Acq: 2 Apr 2021 21:41

Instrument :

MSVOA_L

ClientSampleId :


Tot Ion: 49 Resp: 1187591

Ion Ratio Lower Upper

49 100

128 49.3 23.5 70.6




130 63.6 29.1 87.4

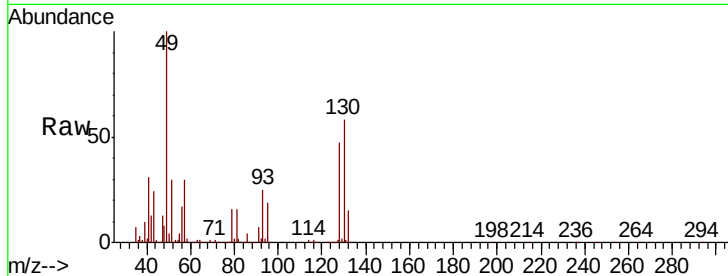

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

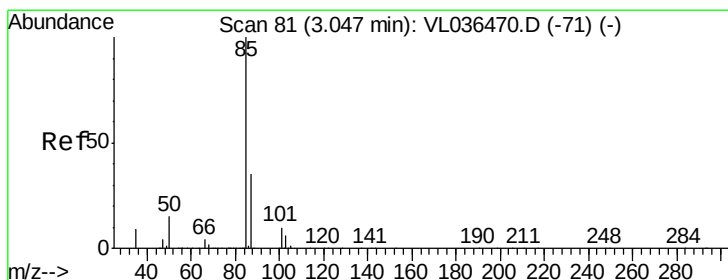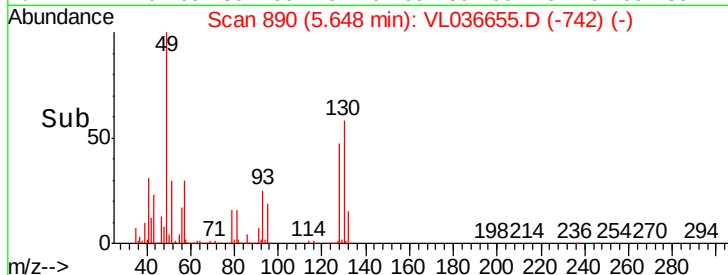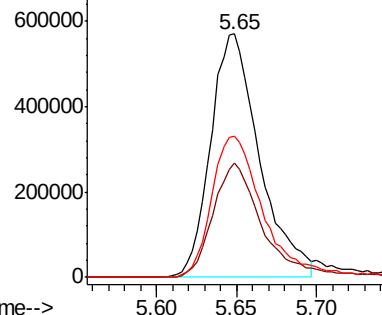

#2

Dichlorodifluoromethane

Concen: 0.216 ppbv

RT: 3.03 min Scan# 77

Delta R.T. -0.01 min

Lab File: VL036655.D


Acq: 2 Apr 2021 21:41

Tgt Ion: 85 Resp: 41924

Ion Ratio Lower Upper



85 100


87 41.5 27.8 41.8

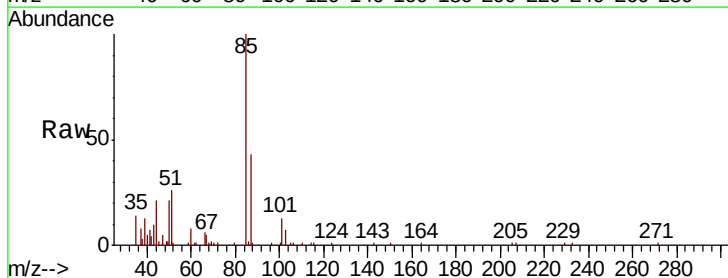

Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

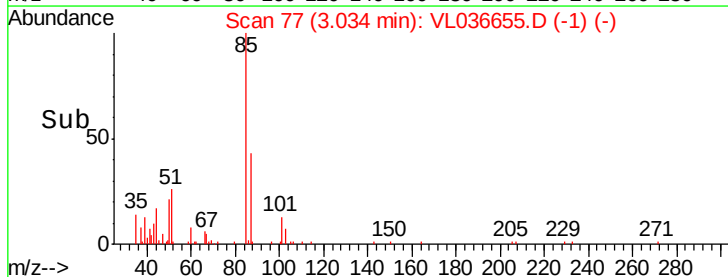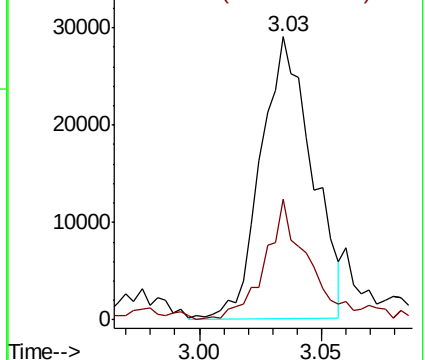



#3

Chlorodifluoromethane

Concen: 1.463 ppbv

RT: 2.98 min Scan# 59

Delta R.T. -0.01 min

Lab File: VL036655.D

Acq: 2 Apr 2021 21:41

Instrument :

MSVOA_L


ClientSampleId :

Tot Ion: 51 Resp: 324597

Ion Ratio Lower Upper

51 100

67 16.7 14.7 22.1

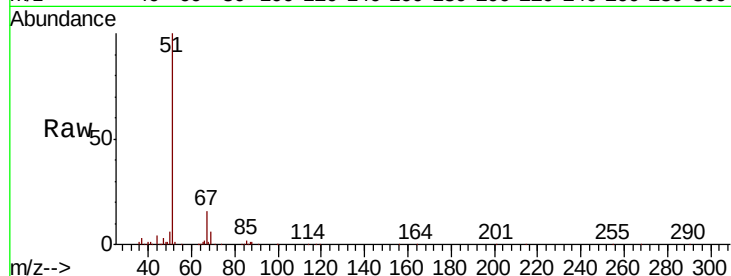

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

200000

150000



100000

50000

0

2.80 3.00 3.20

Time-->



#4

Chloromethane

Concen: 0.123 ppbv

RT: 3.13 min Scan# 107

Delta R.T. -0.01 min

Lab File: VL036655.D


Acq: 2 Apr 2021 21:41

Tgt Ion: 50 Resp: 9639

Ion Ratio Lower Upper

50 100

52 26.4 27.0 40.6#



Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

10000

8000

6000


4000


2000

0

3.12 3.14 3.16

Time-->





#9

Propene

Concen: 0.193 ppbv

RT: 3.01 min Scan# 69

Delta R.T. -0.00 min

Lab File: VL036655.D

Acq: 2 Apr 2021 21:41

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 41 Resp: 13647

Ion Ratio Lower Upper

41 100

42 94.6 57.0 85.4#

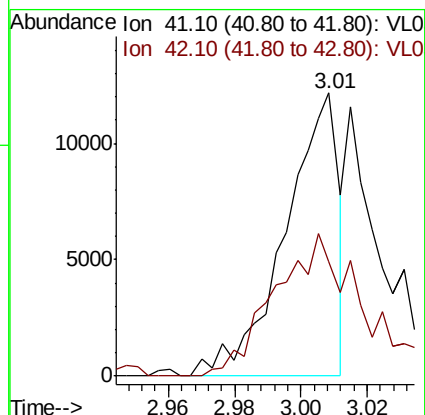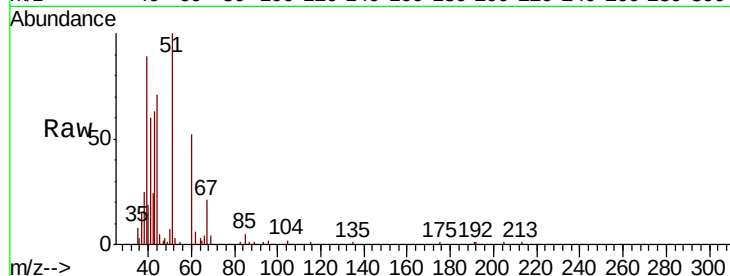

#10

Heptane

Concen: 0.065 ppbv

RT: 8.10 min Scan# 1652

Delta R.T. -0.03 min

Lab File: VL036655.D




Acq: 2 Apr 2021 21:41


Tgt Ion: 43 Resp: 11643

Ion Ratio Lower Upper

43 100

57 0.0 39.0 58.6#


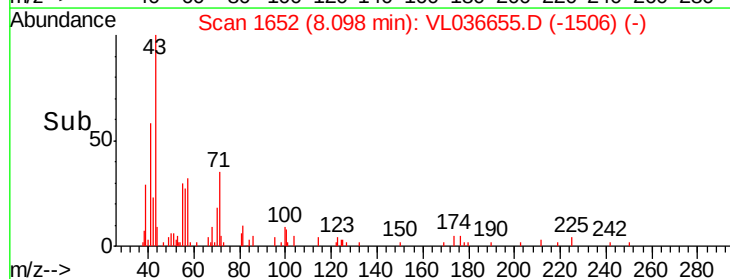
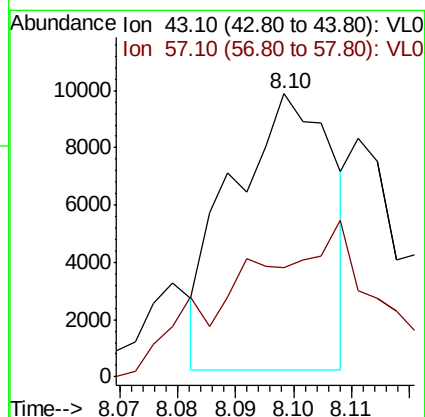





#11
 Trichlorofluoromethane
 Concen: 0.127 ppbv
 RT: 3.94 min Scan# 358
 Delta R.T. -0.01 min
 Lab File: VL036655.D
 Acq: 2 Apr 2021 21:41




Instrument :
 MSVOA_L
 ClientSampled :


Tot Ion:101 Resp: 24981
 Ion Ratio Lower Upper
 101 100
 103 62.0 52.5 78.7

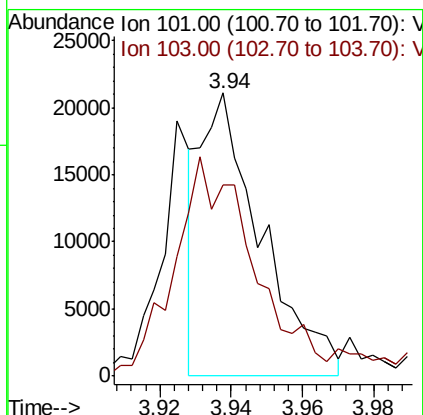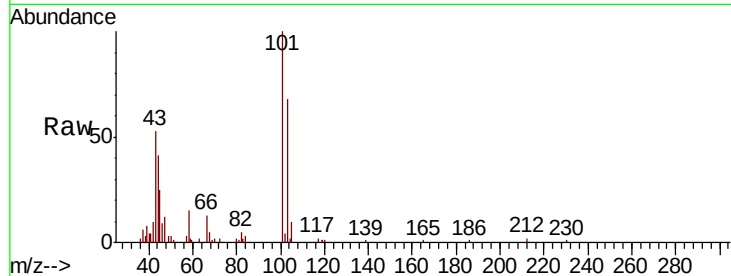

#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.045 ppbv
 RT: 4.47 min Scan# 523
 Delta R.T. -0.02 min
 Lab File: VL036655.D
 Acq: 2 Apr 2021 21:41

Tgt Ion:101 Resp: 5630
 Ion Ratio Lower Upper
 101 100
 151 124.7 60.9 91.3#









#13
Ethanol
Concen: 239.578 ppbv
RT: 3.60 min Scan# 254
Delta R.T. -0.00 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 45 Resp: 2018089
Ion Ratio Lower Upper
45 100
46 37.1 16.6 66.2

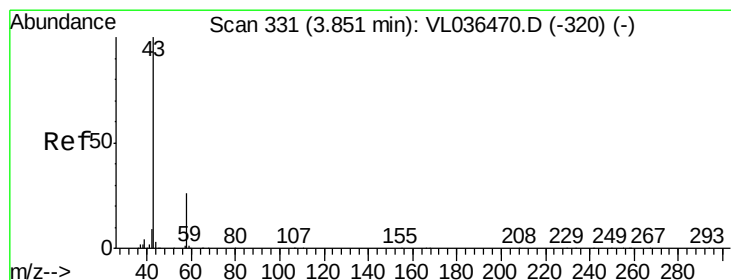

#15
Acetone
Concen: 11.194 ppbv
RT: 3.83 min Scan# 326
Delta R.T. -0.02 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Tgt Ion: 43 Resp: 1308485
Ion Ratio Lower Upper
43 100
58 24.2 21.2 31.8




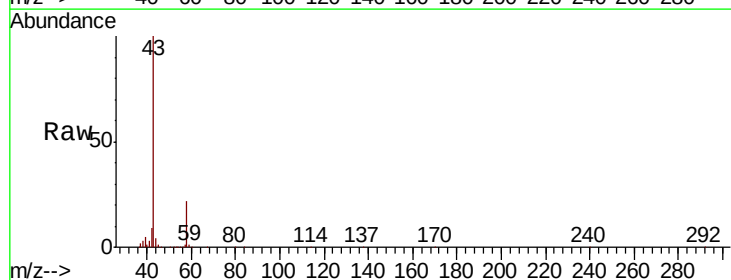




#16
 1,3-Butadiene
 Concen: 0.023 ppbv
 RT: 3.31 min Scan# 162
 Delta R.T. -0.02 min
 Lab File: VL036655.D
 Acq: 2 Apr 2021 21:41




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion: 39 Resp: 1880
 Ion Ratio Lower Upper
 39 100
 54 68.1 58.8 88.2

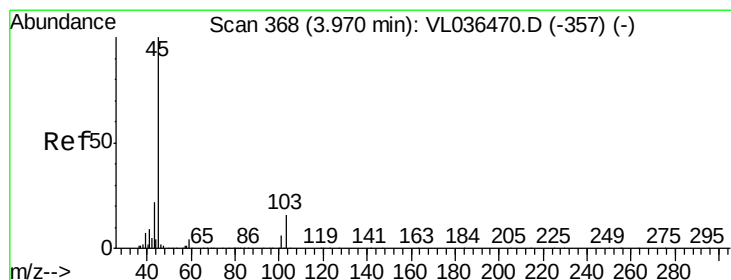

#19
 Isopropyl Alcohol
 Concen: 6.067 ppbv
 RT: 3.97 min Scan# 367
 Delta R.T. -0.00 min
 Lab File: VL036655.D
 Acq: 2 Apr 2021 21:41

Tgt Ion: 45 Resp: 390119
 Ion Ratio Lower Upper
 45 100
 58 81.8 2.9 4.3#

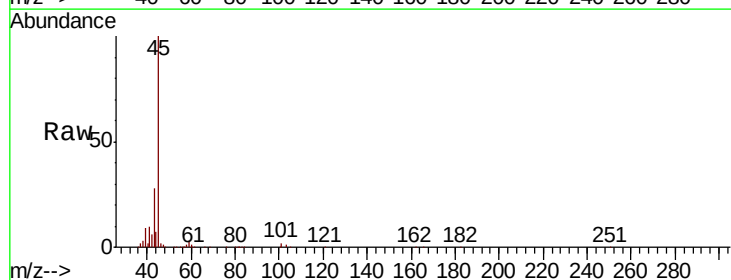







#20
Methvlene Chloride
Concen: 31.581 ppbv
RT: 4.33 min Scan# 479
Delta R.T. -0.02 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Instrument :
MSVOA_L
ClientSampleId :

Tot Ion: 84 Resp: 1728324




Ion	Ratio	Lower	Upper
84	100		
49	162.4	122.9	184.3
51	51.7	36.9	55.3
86	62.5	48.2	72.4

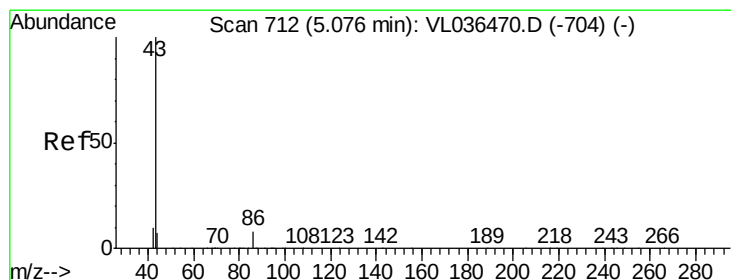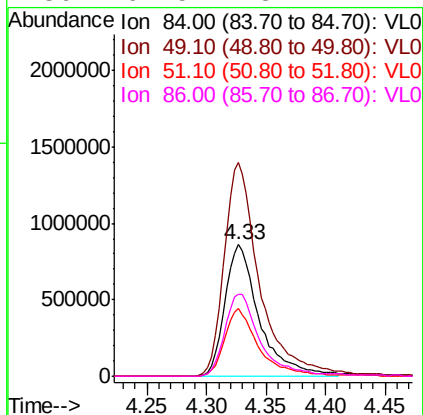


#23
Vinyl Acetate
Concen: 0.080 ppbv
RT: 5.05 min Scan# 703
Delta R.T. -0.03 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Tgt Ion: 43 Resp: 16040

Ion	Ratio	Lower	Upper
43	100		
86	9.4	5.4	8.0#
42	24.1	8.5	12.7#
44	18.5	4.6	7.0#

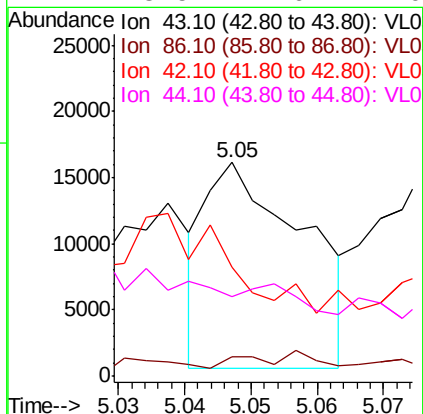







#25
Ethyl Acetate
Concen: 3.794 ppbv
RT: 5.67 min Scan# 896
Delta R.T. -0.02 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Instrument :
MSVOA_L
ClientSampleId :

Tot Ion: 43 Resp: 1054290




Ion	Ratio	Lower	Upper
43	100		
45	0.4	7.9	11.9#
61	0.3	7.4	11.2#
70	1.6	5.1	7.7#

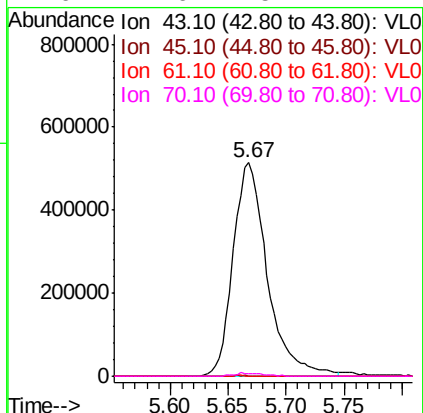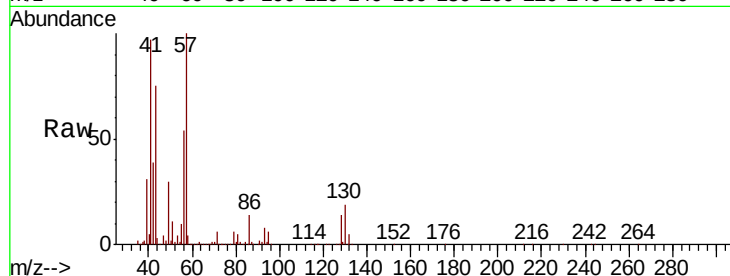


#26
Hexane
Concen: 11.179 ppbv
RT: 5.66 min Scan# 895
Delta R.T. -0.02 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Tgt Ion: 57 Resp: 1441604

Ion	Ratio	Lower	Upper
57	100		
41	98.5	77.2	115.8
43	74.4	173.8	260.6#
56	54.7	43.8	65.6

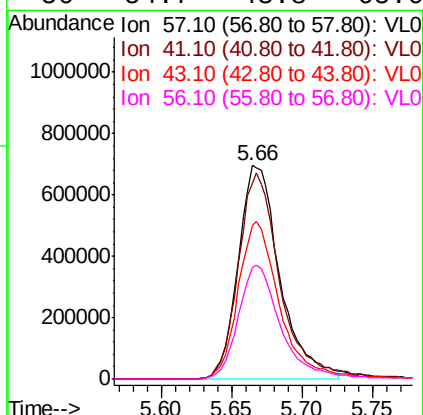



#27

Carbon Disulfide

Concen: 0.050 ppbv

RT: 4.53 min Scan# 543

Delta R.T. -0.02 min

Lab File: VL036655.D

Acq: 2 Apr 2021 21:41

Instrument :

MSVOA_L

ClientSampleId :


Tot Ion: 76 Resp: 6349

Ion Ratio Lower Upper


76 100

44 0.0 17.5 26.3#



78 16.3 8.6 13.0#



Abundance Ion 76.00 (75.70 to 76.70): VL0
Ion 44.10 (43.80 to 44.80): VL0
Ion 78.00 (77.70 to 78.70): VL0

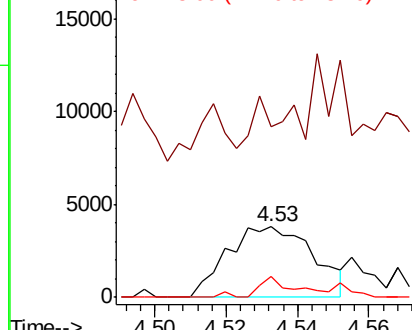

Time-->



#30

Cyclohexane

Concen: 0.043 ppbv

RT: 7.10 min Scan# 1343

Delta R.T. -0.03 min

Lab File: VL036655.D

Acq: 2 Apr 2021 21:41


Tgt Ion: 84 Resp: 4458

Ion Ratio Lower Upper


84 100

56 0.0 114.6 171.8#


41 0.0 75.3 112.9#




Abundance Ion 84.20 (83.90 to 84.90): VL0
Ion 56.10 (55.80 to 56.80): VL0
Ion 41.10 (40.80 to 41.80): VL0

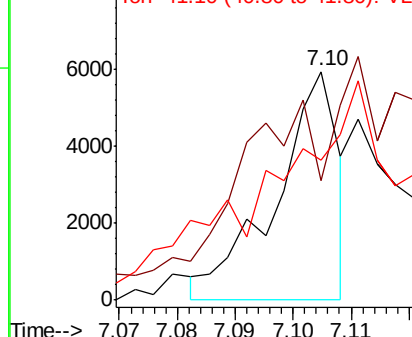

Time-->






#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.16 min Scan# 1359
 Delta R.T. -0.02 min
 Lab File: VL036655.D
 Acq: 2 Apr 2021 21:41




Instrument :
 MSVOA_L
 ClientSampleId :

Tot Ion:114 Resp: 3117094

Ion	Ratio	Lower	Upper
114	100		
63	27.0	22.4	33.6
88	18.8	15.4	23.0

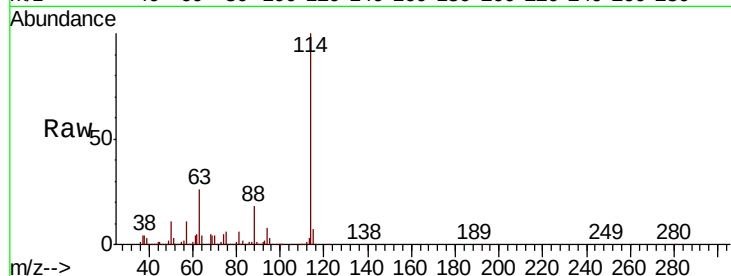


Abundance Ion 114.10 (113.80 to 114.80): VL0
 Ion 63.10 (62.80 to 63.80): VL0
 Ion 88.10 (87.80 to 88.80): VL0

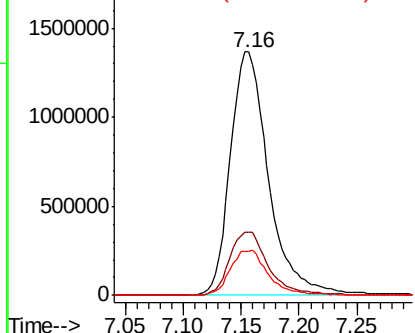



#34
 2-Butanone
 Concen: 0.396 ppbv
 RT: 5.23 min Scan# 761
 Delta R.T. -0.02 min
 Lab File: VL036655.D
 Acq: 2 Apr 2021 21:41


Tgt Ion: 43 Resp: 60326

Ion	Ratio	Lower	Upper
43	100		
72	30.1	17.0	25.6#



Abundance Ion 43.10 (42.80 to 43.80): VL0
 Ion 72.10 (71.80 to 72.80): VL0




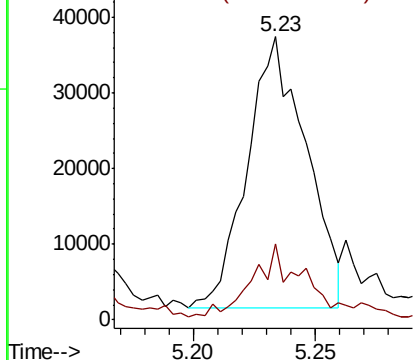




#36
Benzene
Concen: 0.104 ppbv
RT: 6.86 min Scan# 1268
Delta R.T. -0.03 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 78 Resp: 29873
Ion Ratio Lower Upper
78 100
77 22.3 18.0 27.0
50 13.6 16.5 24.7#

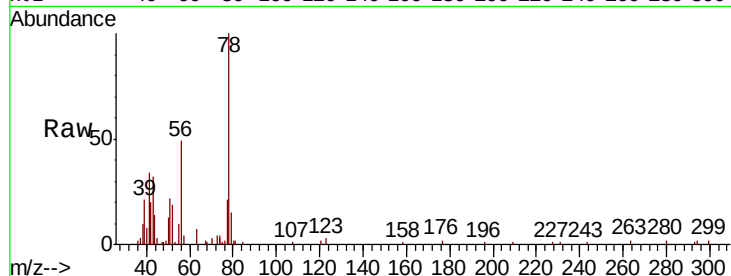

#39
1,2-Dichloropropane
Concen: 7.020 ppbv
RT: 7.15 min Scan# 1358
Delta R.T. -0.47 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Tgt Ion: 63 Resp: 818693
Ion Ratio Lower Upper
63 100
41 0.0 62.4 93.6#
62 17.8 52.8 79.2#









#41
Tetrahydrofuran
Concen: 0.119 ppbv
RT: 6.04 min Scan# 1013
Delta R.T. -0.01 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 42 Resp: 8322
Ion Ratio Lower Upper
42 100
72 49.6 27.6 41.4#
71 56.9 27.0 40.4#

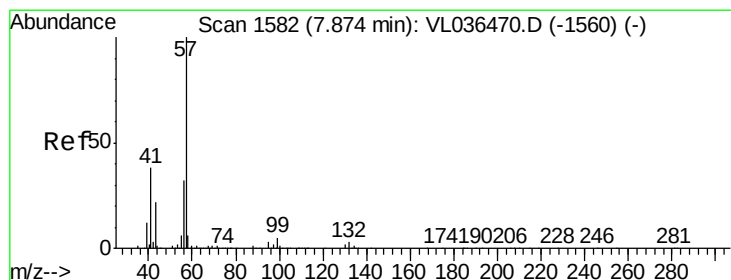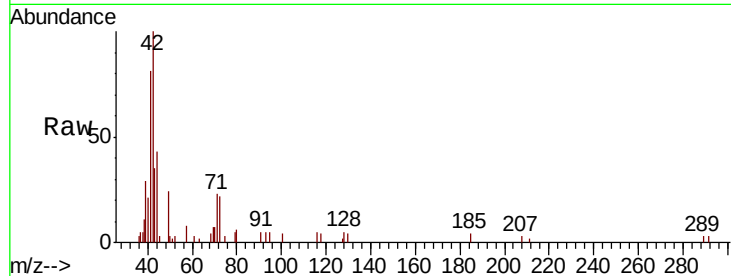

#44
2,2,4-Trimethylpentane
Concen: 0.108 ppbv
RT: 7.85 min Scan# 1574
Delta R.T. -0.03 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Tgt Ion: 57 Resp: 54691
Ion Ratio Lower Upper
57 100
41 63.4 28.8 43.2#
56 51.4 26.1 39.1#



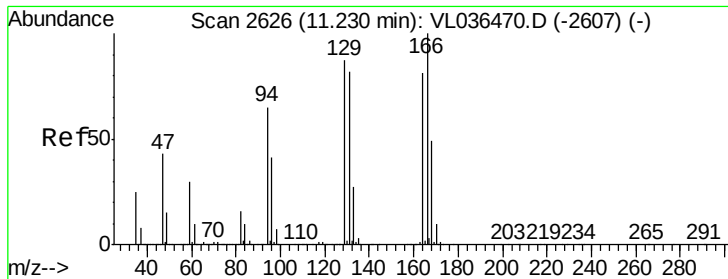

#52

Tetrachloroethene

Concen: 0.022 ppbv

RT: 11.20 min Scan# 2616

Delta R.T. -0.03 min

Lab File: VL036655.D

Acq: 2 Apr 2021 21:41

Instrument :

MSVOA_L

ClientSampled :

Tot Ion:164 Resp: 2342





Ion Ratio Lower Upper

164 100

166 59.0 98.3 147.5#

129 55.4 85.8 128.8#

131 43.7 80.9 121.3#

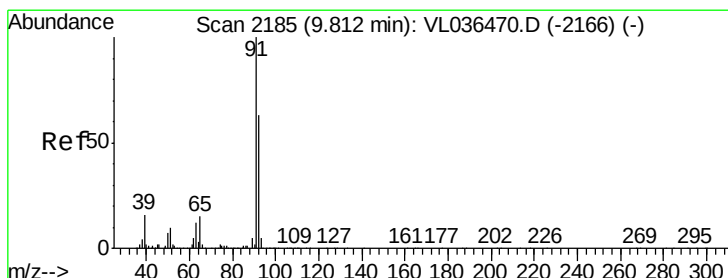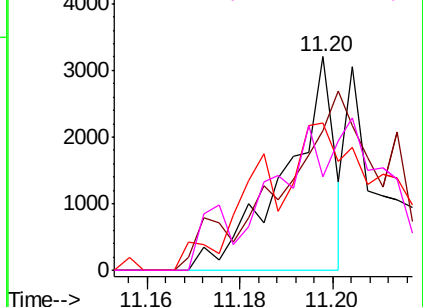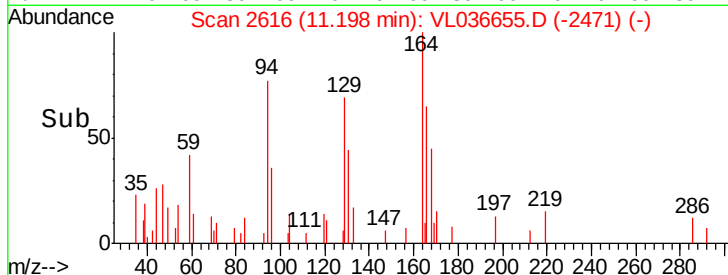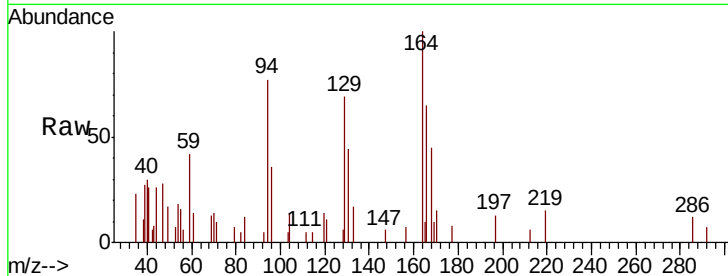

#53

Toluene

Concen: 0.283 ppbv

RT: 9.78 min Scan# 2175

Delta R.T. -0.03 min

Lab File: VL036655.D





Acq: 2 Apr 2021 21:41


Tgt Ion: 91 Resp: 86574

Ion Ratio Lower Upper

91 100

92 0.0 48.8 73.2#

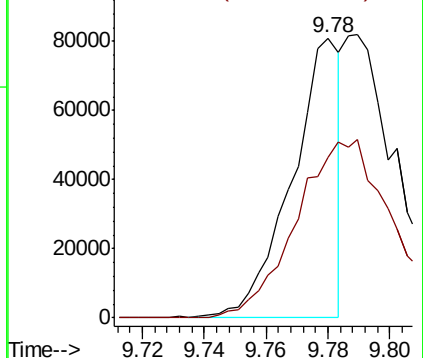
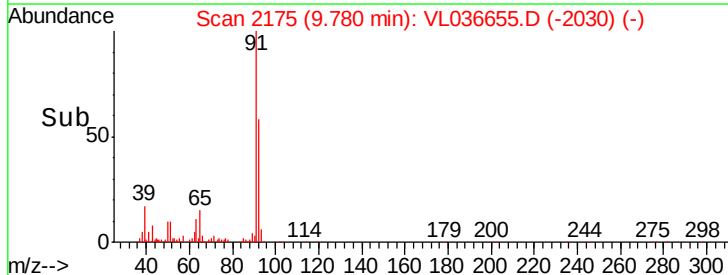

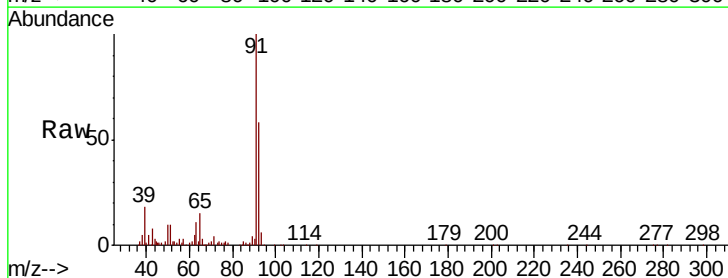




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.06 min Scan# 2885
Delta R.T. -0.03 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41




Instrument :
MSVOA_L
ClientSampled :


Tot Ion:117 Resp: 2791943
Ion Ratio Lower Upper
117 100
82 66.4 57.4 86.0
119 32.8 47.4 71.0#

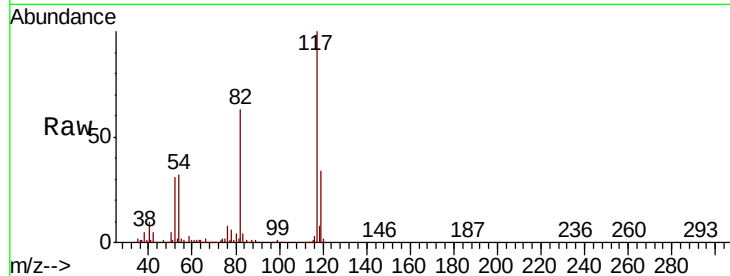

#58
Ethyl Benzene
Concen: 0.142 ppbv
RT: 12.69 min Scan# 3079
Delta R.T. -0.03 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Tgt Ion: 91 Resp: 57638
Ion Ratio Lower Upper
91 100
106 26.6 25.3 37.9









#59
m/p-Xylene
Concen: 0.329 ppbv
RT: 12.95 min Scan# 3162
Delta R.T. -0.05 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 91 Resp: 116452
Ion Ratio Lower Upper
91 100
106 0.0 35.3 52.9#

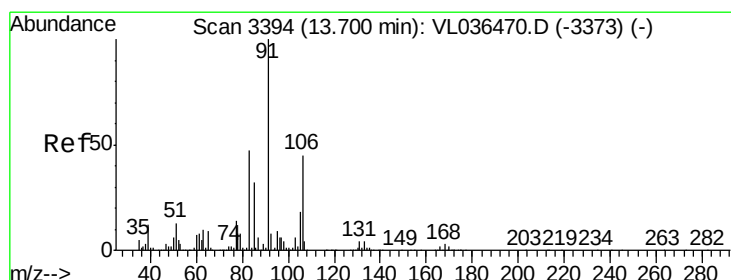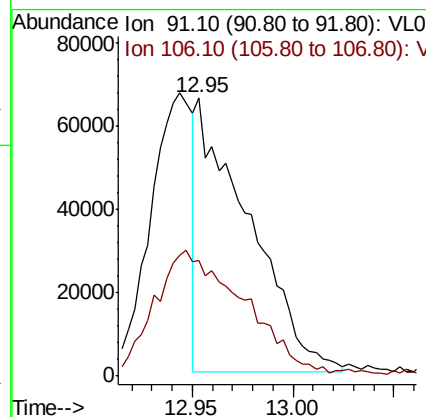

#60
o-Xylene
Concen: 0.240 ppbv
RT: 13.67 min Scan# 3384
Delta R.T. -0.03 min
Lab File: VL036655.D
Acq: 2 Apr 2021 21:41

Tgt Ion: 91 Resp: 82206
Ion Ratio Lower Upper
91 100
106 46.4 22.3 66.9



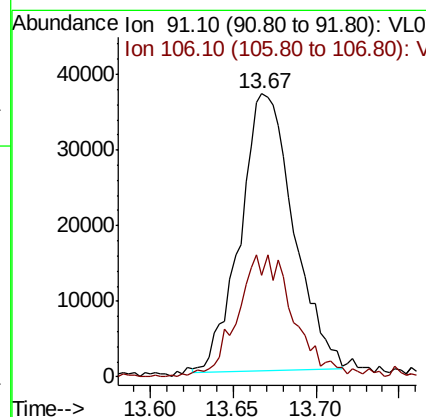



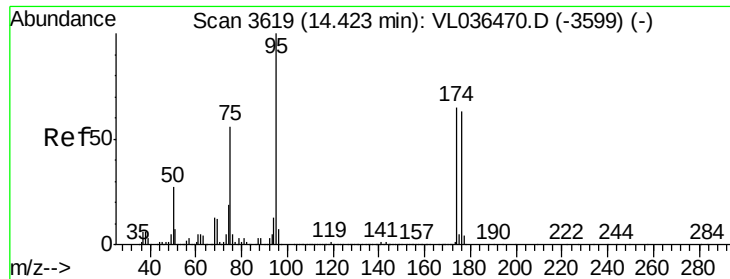

#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.939 ppbv
 RT: 14.39 min Scan# 3610
 Delta R.T. -0.03 min
 Lab File: VL036655.D
 Acq: 2 Apr 2021 21:41




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion: 95 Resp: 2211637
 Ion Ratio Lower Upper
 95 100
 174 69.9 51.0 76.6
 175 5.2 3.9 5.9

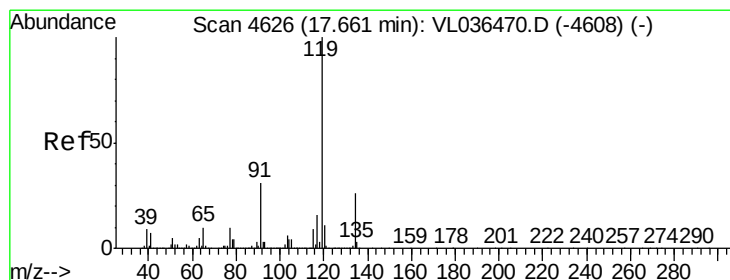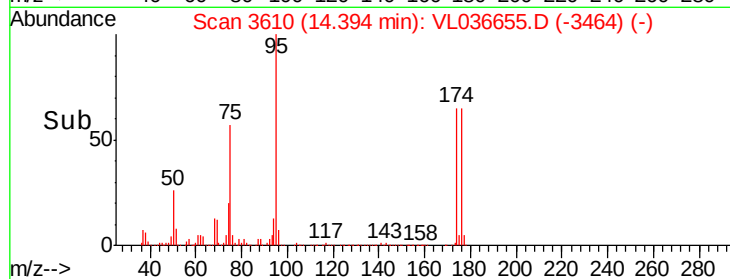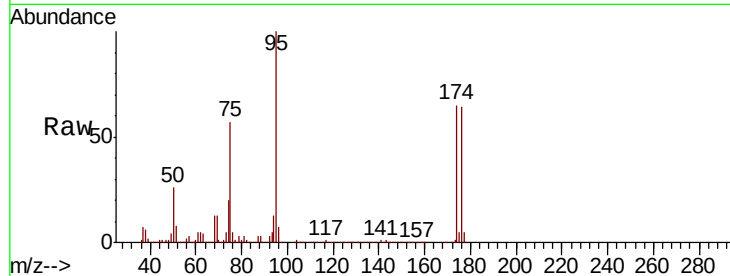

#69
 p-Isopropyltoluene
 Concen: 0.138 ppbv
 RT: 17.63 min Scan# 4616
 Delta R.T. -0.03 min
 Lab File: VL036655.D
 Acq: 2 Apr 2021 21:41

Tgt Ion: 119 Resp: 61015
 Ion Ratio Lower Upper
 119 100
 134 0.0 20.6 30.8#
 91 0.0 25.0 37.6#

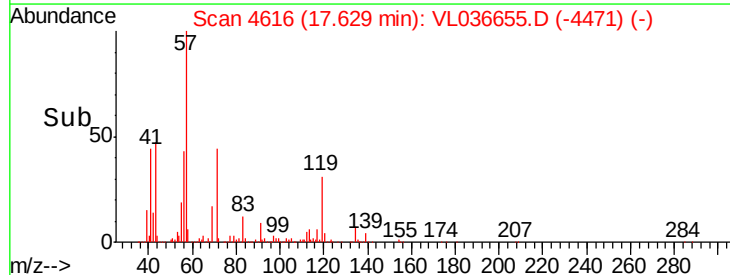



#72

4-Ethyltoluene

Concen: 0.113 ppbv

RT: 15.82 min Scan# 4052

Delta R.T. -0.03 min

Lab File: VL036655.D

Acq: 2 Apr 2021 21:41

Instrument :

MSVOA_L

ClientSampleId :

Tot Ion:105 Resp: 42465


Ion Ratio Lower Upper

105 100

120 31.5 24.0 36.0

91 13.9 11.0 16.4

77 20.9 11.7 17.5#






Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

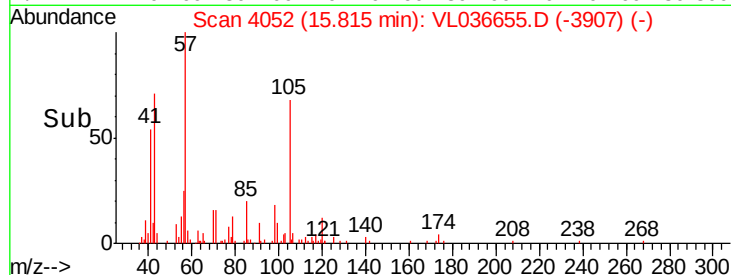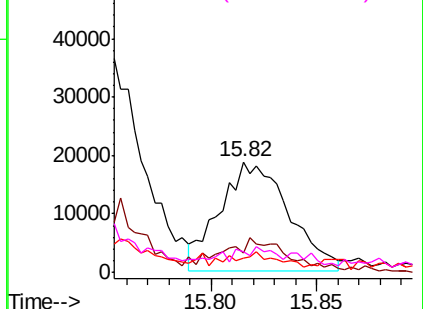

#73

1,3,5-Trimethylbenzene

Concen: 0.058 ppbv

RT: 15.98 min Scan# 4102

Delta R.T. -0.03 min

Lab File: VL036655.D


Acq: 2 Apr 2021 21:41

Tgt Ion:105 Resp: 20361

Ion Ratio Lower Upper



105 100


120 46.4 36.6 54.8



Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

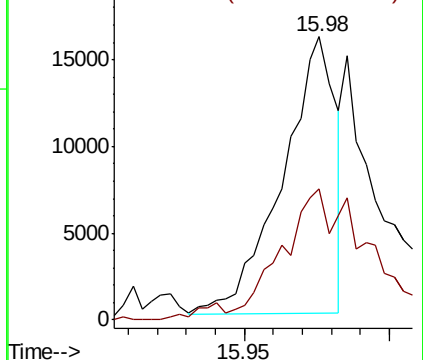

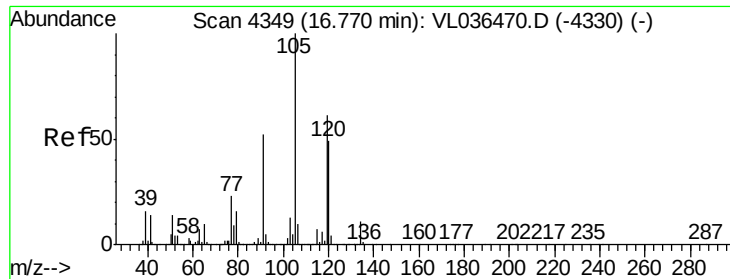

#74

1,2,4-Trimethylbenzene

Concen: 0.341 ppbv

RT: 16.74 min Scan# 4341

Delta R.T. -0.03 min

Lab File: VL036655.D





Acq: 2 Apr 2021 21:41

Instrument :

MSVOA_L

ClientSampleId :

Tot Ion:	105	Resp:	128030
Ion	Ratio	Lower	Upper
105	100		
120	39.4	39.2	58.8
91	11.0	42.6	64.0#
77	11.0	18.6	28.0#

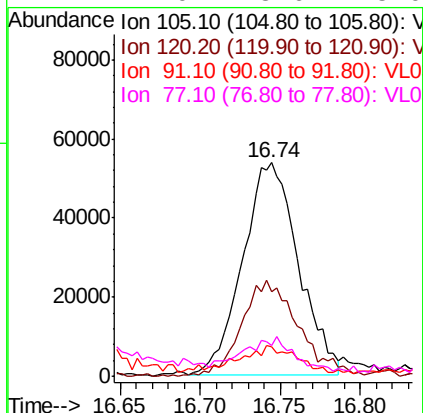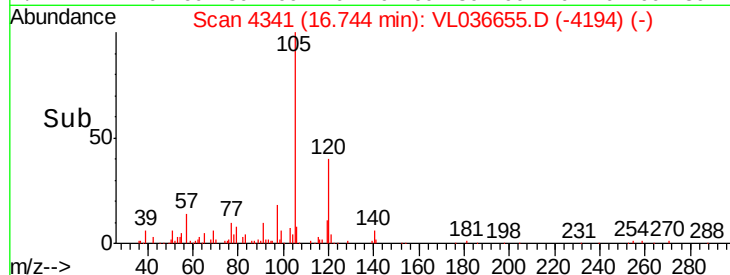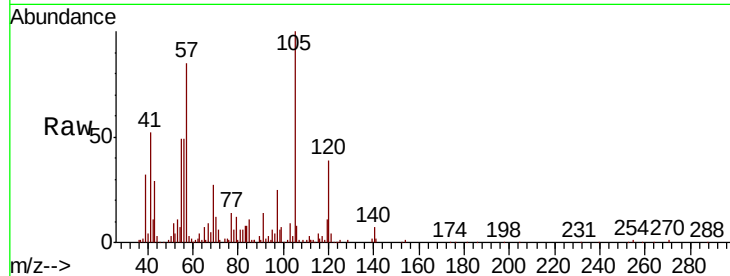

#80

Naphthalene, 2-methyl-

Concen: 0.033 ppbv

RT: 24.95 min Scan# 6893

Delta R.T. -0.03 min

Lab File: VL036655.D

Acq: 2 Apr 2021 21:41

Tgt Ion:	142	Resp:	1429
Ion	Ratio	Lower	Upper
142	100		
141	45.1	67.8	101.8#
115	23.9	34.0	51.0#

