
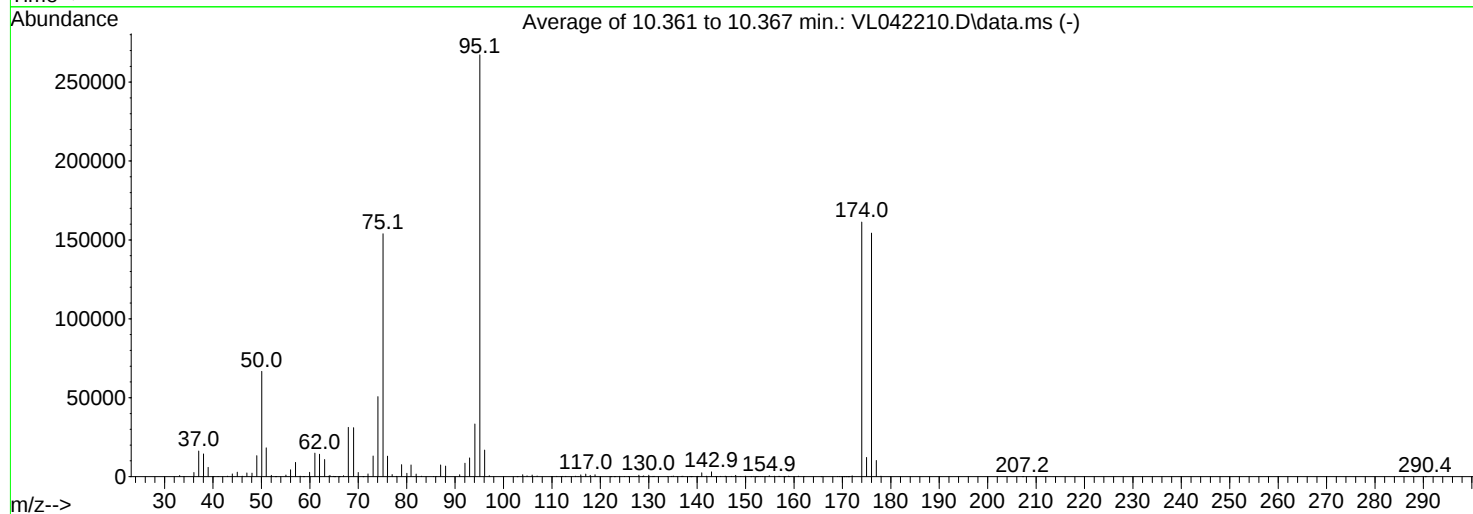


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040225\
Data File : VL042210.D
Acq On : 02 Apr 2025 07:54
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

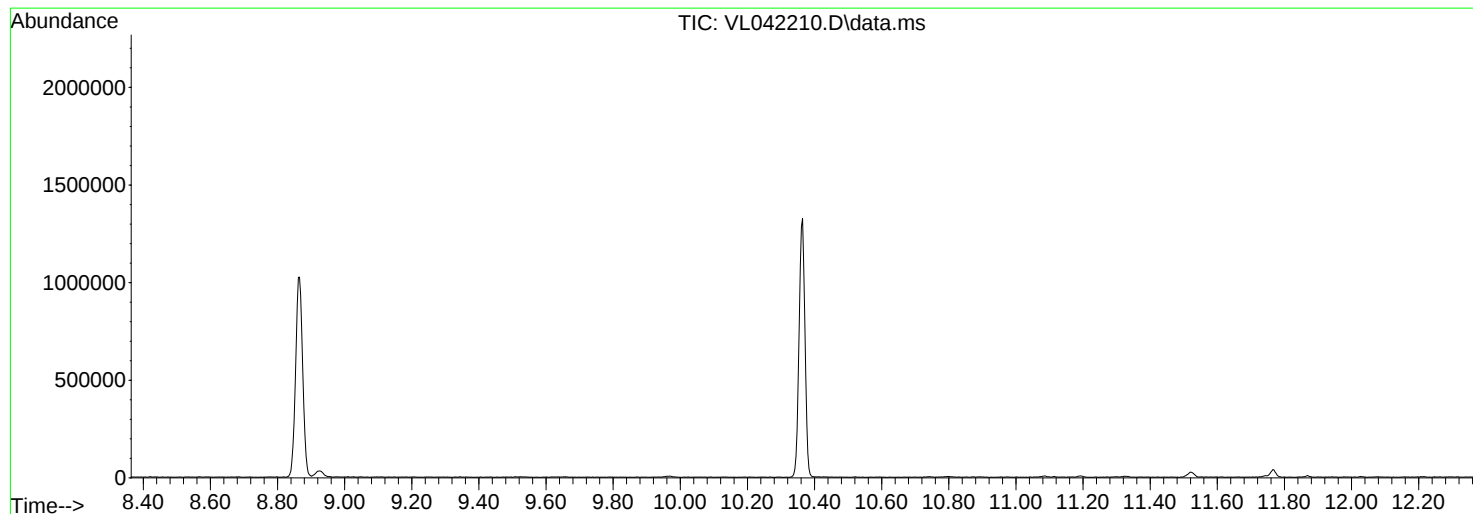

AutoFind: Scans 3174, 3175, 3176; Background Corrected with Scan 3159

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.9	66685	PASS
75	95	30	66	57.6	153963	PASS
95	95	100	100	100.0	267285	PASS
96	95	5	9	6.3	16820	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	60.4	161365	PASS
175	174	4	9	7.6	12193	PASS
176	174	93	101	95.6	154304	PASS
177	176	5	9	6.6	10247	PASS

Average of 10.361 to 10.367 min.: VL042210.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	690	46.05	272	58.00	355	66.95	64
34.00	133	47.00	2346	58.70	39	67.95	3126
36.05	2701	48.05	2235	59.95	2771	69.05	3104
37.05	16190	49.05	13279	61.05	14948	70.00	269
38.05	14355	50.05	66685	62.00	14189	71.00	38
39.00	5854	51.00	18247	63.05	10850	72.00	1773
40.00	57	52.05	773	63.90	296	73.05	13062
41.05	77	52.90	20	64.15	768	74.05	50745
43.00	337	55.05	1047	64.85	230	75.10	153963
44.00	1681	56.00	4382	65.10	49	76.05	13023
45.00	2851	57.05	9053	66.05	55	77.00	1331

Average of 10.361 to 10.367 min.: VL042210.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.90	212	92.05	8508	109.90	52	118.90	1256
78.95	7612	93.00	11882	110.05	91	122.10	28
80.05	2123	94.10	33373	111.00	164	122.90	22
80.90	7453	95.10	267285	111.90	81	123.95	225
81.95	1667	96.10	16820	112.10	170	125.00	82
83.05	314	97.05	599	112.85	262	125.85	64
85.55	67	102.80	57	114.90	341	127.95	919
86.10	154	103.95	1216	115.40	86	128.70	192
87.00	7390	104.85	502	115.95	1141	128.95	486
88.05	6659	105.90	1014	117.00	1642	130.00	958
90.95	1241	106.95	412	117.90	795	130.85	243

Average of 10.361 to 10.367 min.: VL042210.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
131.10	183	140.20	94	149.00	145	156.90	343
133.85	154	140.95	2421	149.95	280	157.10	135
134.70	164	141.90	292	151.10	33	157.90	20
135.05	424	142.95	3072	151.70	160	158.10	30
135.85	107	143.90	171	152.20	30	158.85	294
136.80	174	144.10	99	152.70	85	159.10	130
137.05	311	144.85	215	153.05	152	160.90	299
138.50	64	145.80	300	153.45	102	162.10	93
138.70	34	146.00	138	154.05	95	165.60	20
139.10	85	147.05	199	154.90	608	169.00	93
140.00	215	147.95	770	156.00	281	169.40	116

Average of 10.361 to 10.367 min.: VL042210.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
169.90	21	207.20	21				
170.30	57	290.40	19				
170.70	17						
171.10	63						
171.30	50						
172.00	572						
174.00	161365						
175.00	12193						
176.00	154304						
177.00	10247						
177.95	353						

Instrument :

MSVOA_L

ClientSampleId :

BFB