


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040423\
Data File : VL040300.D
Acq On : 4 Apr 2023 8:39
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Mar 15 16:14:43 2023

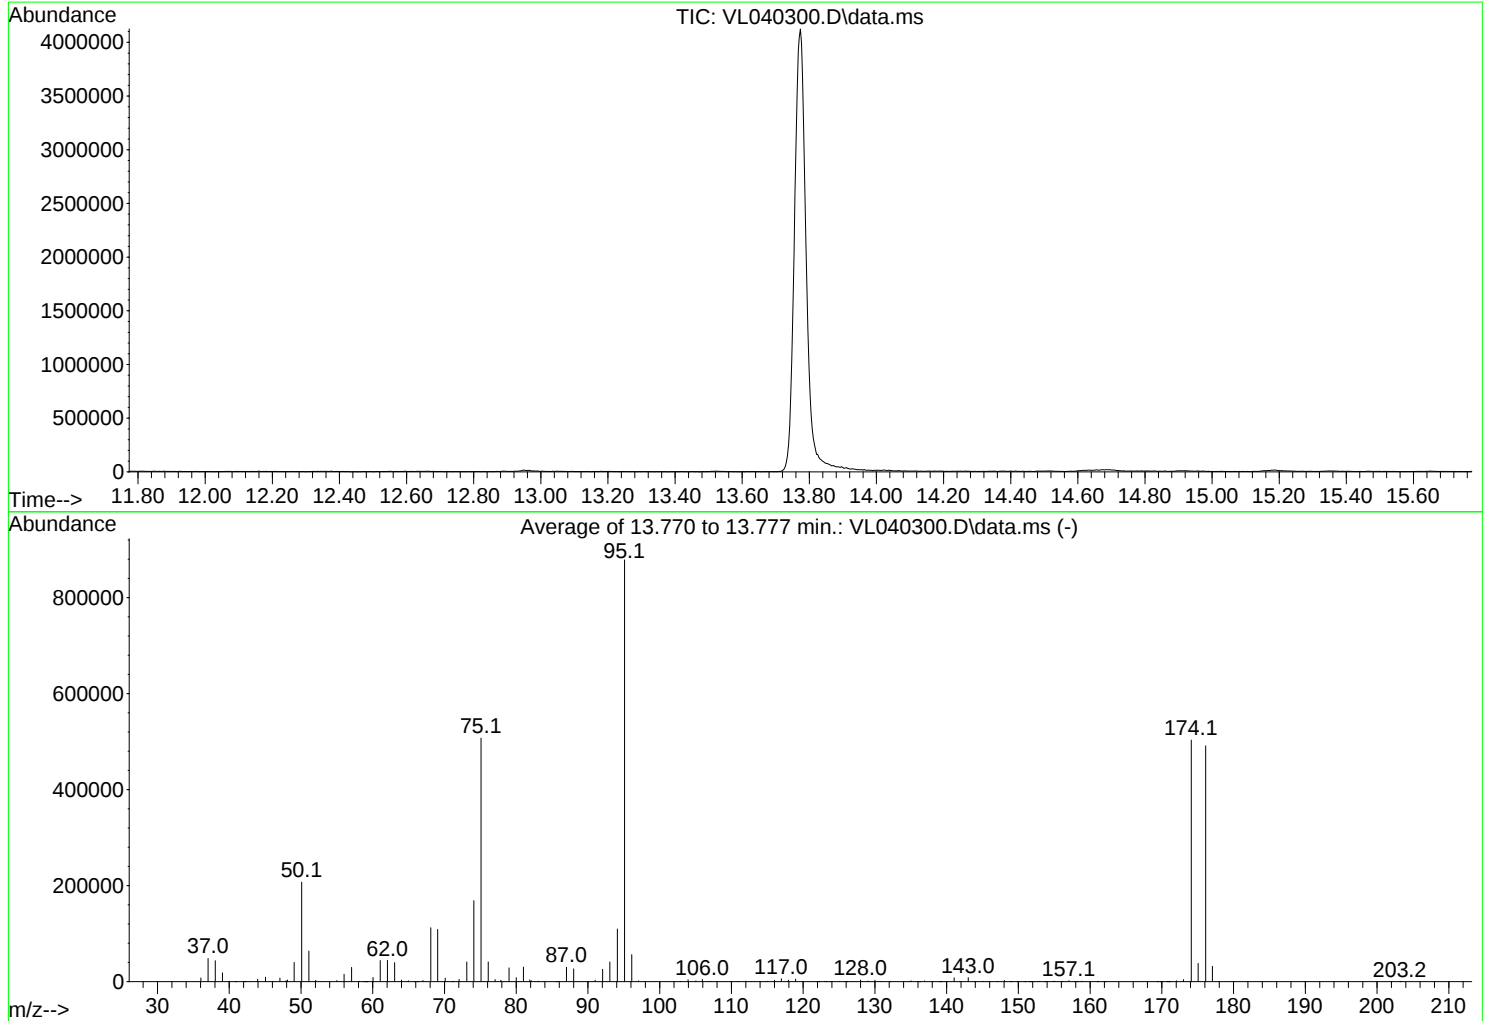

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	207168	PASS
75	95	30	66	57.7	507435	PASS
95	95	100	100	100.0	878699	PASS
96	95	5	9	6.4	56424	PASS
173	174	0.00	2	0.8	4219	PASS
174	95	50	120	57.3	503211	PASS
175	174	4	9	7.5	37899	PASS
176	174	93	101	97.7	491435	PASS
177	176	5	9	6.5	32072	PASS

Average of 13.770 to 13.777 min.: VL040300.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7581	47.05	7411	58.10	1097	66.20	111
37.05	48453	47.90	1976	58.70	69	67.00	233
38.05	43792	48.10	3508	59.00	87	68.10	11249
39.05	18440	49.05	40099	59.20	92	69.05	10856
40.05	1036	50.10	207168	60.05	8621	70.10	7502
40.90	67	51.10	63629	61.05	43971	71.10	166
42.20	149	52.05	2577	62.05	44205	72.05	4555
42.95	343	52.95	482	63.05	39771	73.10	41160
43.95	4957	55.00	2499	64.00	3512	74.10	168640
45.05	9238	56.00	15205	65.00	1822	75.10	507435
46.10	609	57.05	29760	65.80	51	76.10	40907

Average of 13.770 to 13.777 min.: VL040300.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	4409	88.00	26840	105.05	1575	113.25	388
77.85	3085	90.00	55	105.95	4517	114.00	75
79.00	28773	91.00	3153	106.75	707	114.80	314
80.00	8218	92.05	25816	107.15	624	115.05	627
81.00	30397	93.05	40901	108.00	372	116.00	2845
81.90	3772	94.10	109565	109.80	335	116.95	5861
82.10	1943	95.10	878699	110.15	309	117.95	3005
83.05	933	96.10	56424	110.90	371	118.95	5253
85.60	93	97.05	1632	111.05	432	121.90	86
85.95	579	102.90	532	112.00	1034	122.20	60
87.00	29995	103.95	4064	112.85	438	122.95	267

Average of 13.770 to 13.777 min.: VL040300.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.20	62	132.10	55	141.05	8021	148.05	2446
123.80	190	134.00	242	141.85	514	148.90	56
124.05	434	134.80	518	142.10	363	149.15	355
125.05	306	135.05	1658	143.00	8293	149.85	771
125.75	216	135.95	244	143.90	103	150.10	408
126.10	122	136.20	112	144.05	285	150.90	56
126.85	212	136.95	1563	144.95	600	151.50	59
128.00	3510	138.00	73	145.20	274	151.80	188
129.05	1527	139.00	116	145.70	393	152.20	249
130.00	3139	139.20	109	146.05	736	152.70	208
130.85	837	139.90	259	147.10	686	152.95	363

Average of 13.770 to 13.777 min.: VL040300.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.70	93	162.10	58	176.10	491435		
154.05	315	169.40	65	177.05	32072		
154.80	539	169.80	102	177.90	317		
155.05	936	170.00	73	178.05	782		
156.00	191	170.70	112	203.20	172		
157.05	1870	170.90	184				
157.80	93	171.10	172				
158.20	110	172.05	1671				
158.85	972	173.00	4219				
161.00	123	174.10	503211				
161.15	750	175.05	37899				