
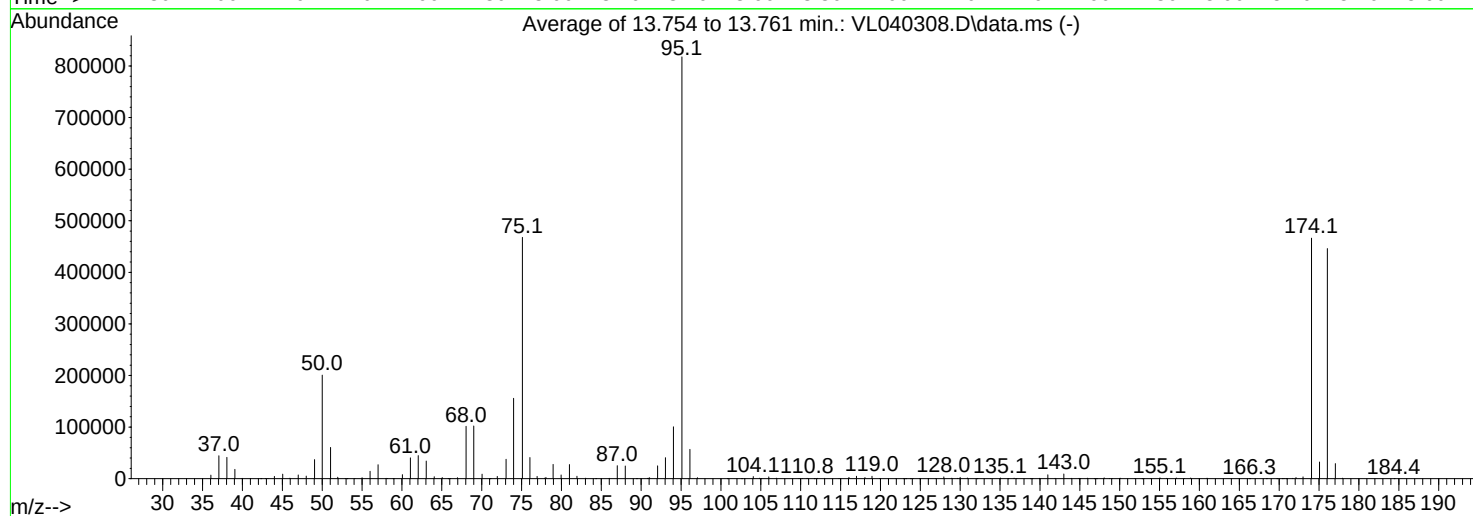


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040523\
 Data File : VL040308.D
 Acq On : 5 Apr 2023 8:58
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031523AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Wed Mar 15 16:14:43 2023

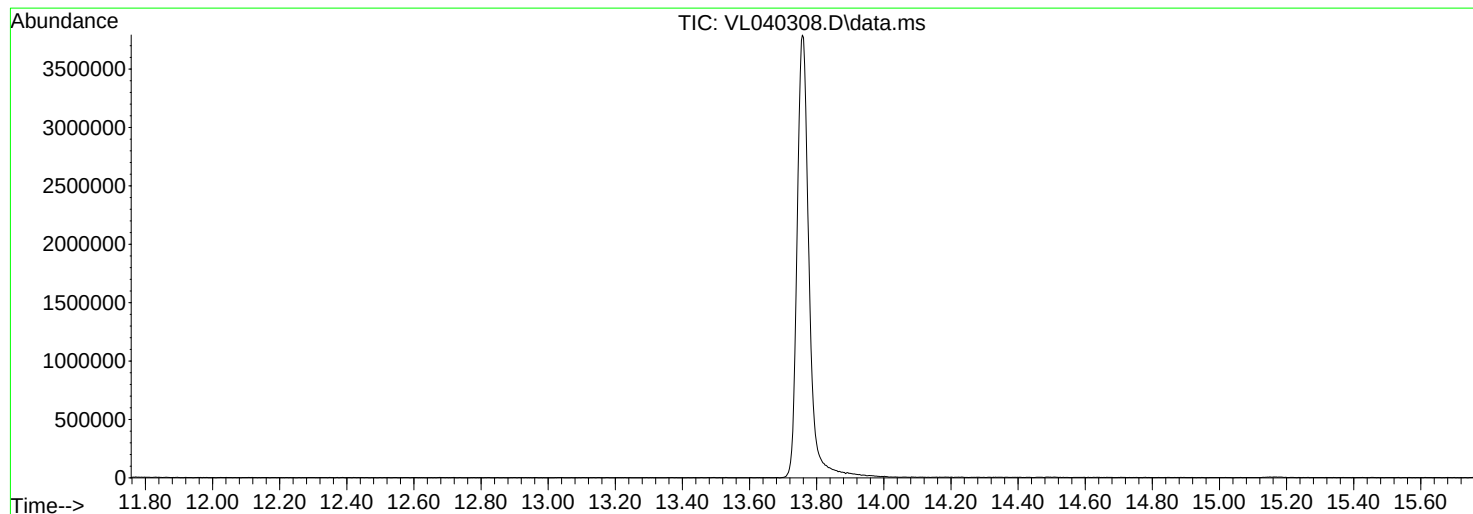

AutoFind: Scans 3468, 3469, 3470; Background Corrected with Scan 3444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.5	200659	PASS
75	95	30	66	57.2	467669	PASS
95	95	100	100	100.0	817749	PASS
96	95	5	9	7.0	56880	PASS
173	174	0.00	2	0.8	3524	PASS
174	95	50	120	57.0	466325	PASS
175	174	4	9	6.9	32176	PASS
176	174	93	101	95.6	445995	PASS
177	176	5	9	6.6	29317	PASS

Average of 13.754 to 13.761 min.: VL040308.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6988	45.95	806	56.00	14151	65.80	91
37.05	44421	47.00	7244	57.00	27005	66.10	44
38.05	41133	48.00	5002	58.00	754	66.95	189
39.05	18040	49.05	36984	58.20	396	68.05	10138
39.95	649	50.00	200659	58.90	67	69.00	102077
41.00	219	51.05	60363	60.05	7774	70.05	8838
42.30	82	51.95	2843	61.05	40264	71.05	189
42.90	284	52.90	281	62.05	44677	71.95	4349
43.20	200	53.10	97	63.05	34088	73.05	37469
44.00	4360	54.10	206	64.05	3696	74.00	155648
45.05	8603	55.00	1744	65.05	2181	75.10	467669

Average of 13.754 to 13.761 min.: VL040308.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	41093	87.00	25213	97.05	2004	110.80	713
76.95	4486	88.00	24592	100.80	100	111.70	138
77.90	827	89.40	109	102.60	191	112.10	619
78.05	2394	90.80	695	103.00	404	113.00	771
78.95	27724	90.90	1058	104.05	4156	114.80	262
79.95	7101	91.05	1851	104.85	888	115.00	440
81.00	27285	92.05	24869	105.10	413	116.05	2634
81.95	4658	93.05	40563	106.00	3348	117.00	4658
83.05	818	94.05	100549	106.95	1013	118.05	2365
84.30	94	95.10	817749	109.80	479	118.95	4760
86.00	501	96.10	56880	110.20	209	119.90	207

Average of 13.754 to 13.761 min.: VL040308.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.95	271	130.00	2534	141.00	7524	149.05	357
122.90	72	130.90	1382	141.90	739	150.05	935
123.15	149	132.10	79	143.00	9164	151.90	300
123.75	179	133.80	341	143.95	566	152.80	171
124.10	325	135.05	1360	144.90	518	153.05	315
124.95	267	136.00	73	145.10	345	153.90	434
126.00	294	136.75	908	145.95	1109	155.05	1573
126.95	278	137.10	413	146.80	99	155.90	639
127.95	3334	138.80	151	147.10	95	157.10	1153
128.95	1014	139.00	142	148.05	1421	158.10	289
129.70	618	139.95	527	148.75	283	158.90	1328

Average of 13.754 to 13.761 min.: VL040308.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.95	815	175.05	32176				
166.30	66	176.05	445995				
168.40	70	177.05	29317				
169.70	189	177.95	1007				
170.40	69	184.40	54				
170.70	378						
170.90	135						
171.70	628						
172.10	2258						
173.00	3524						
174.05	466325						