

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040721\
 Data File : VL036730.D
 Acq On : 7 Apr 2021 17:23
 Operator : SY/AP
 Sample : M1929-02
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampled :
 FS-SV-04

Manual Integrations
 APPROVED

MMDadoda
 4/12/2021 11:15:50 AM

Quant Time: Apr 08 02:41:35 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032521AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Apr 08 01:58:43 2021
 QLast Update : Thu Apr 08 01:58:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.668	49	1266089	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.182	114	3181412	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.092	117	2769795	10.00	ppbv	# 0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.426	95	2242936	10.16	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.60%
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	3.051	85	36306	0.18	ppbv	94
3) Chlorodifluoromethane	2.989	51	34181m	0.14	ppbv	
4) Chloromethane	3.141	50	21610m	0.26	ppbv	
9) Propene	3.012	41	124010	1.64	ppbv	92
10) Heptane	8.124	43	24835m	0.13	ppbv	
11) Trichlorofluoromethane	3.948	101	122693	0.58	ppbv	90
13) Ethanol	3.613	45	105415	11.74	ppbv	98
15) Acetone	3.851	43	1162733	9.33	ppbv	98
19) Isopropyl Alcohol	3.989	45	194960m	2.84	ppbv	
20) Methylene Chloride	4.343	84	841863	14.43	ppbv	95
24) 1,1-Dichloroethane	5.012	63	34770m	0.22	ppbv	
26) Hexane	5.687	57	613330	4.46	ppbv #	47
27) Carbon Disulfide	4.555	76	38616m	0.29	ppbv	
29) Chloroform	5.755	83	415959	1.89	ppbv	98
32) 1,1,1-Trichloroethane	6.510	97	86296	0.39	ppbv	93
34) 2-Butanone	5.250	43	137289	0.88	ppbv #	71
35) Carbon Tetrachloride	7.025	117	8397m	0.03	ppbv	
36) Benzene	6.893	78	7318928	24.94	ppbv	95
37) 1,2-Dichloroethane	6.311	62	51703	0.30	ppbv #	96
52) Tetrachloroethene	11.230	164	2412642	22.33	ppbv	100
53) Toluene	9.812	91	3049043	9.76	ppbv	99
58) Ethyl Benzene	12.716	91	2093139	5.19	ppbv	95
59) m/p-Xylene	13.005	91	2753976	7.84	ppbv	96
60) o-Xylene	13.700	91	1323152	3.89	ppbv	100
61) Styrene	13.539	104	23232m	0.14	ppbv	
62) Isopropylbenzene	14.674	105	47156	0.10	ppbv	96
64) n-propylbenzene	15.565	120	30728m	0.27	ppbv	
72) 4-Ethyltoluene	15.847	105	267256	0.72	ppbv #	96
73) 1,3,5-Trimethylbenzene	16.002	105	523468	1.51	ppbv	94
74) 1,2,4-Trimethylbenzene	16.767	105	1362300	3.66	ppbv #	68
79) Naphthalene	22.214	128	511273	2.36	ppbv #	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040721\
Data File : VL036730.D
Acq On : 7 Apr 2021 17:23
Operator : SY/AP
Sample : M1929-02
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:50 AM


Quant Time: Apr 08 02:41:35 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032521AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Apr 08 01:58:43 2021
QLast Update : Thu Apr 08 01:58:43 2021
Response via : Initial Calibration

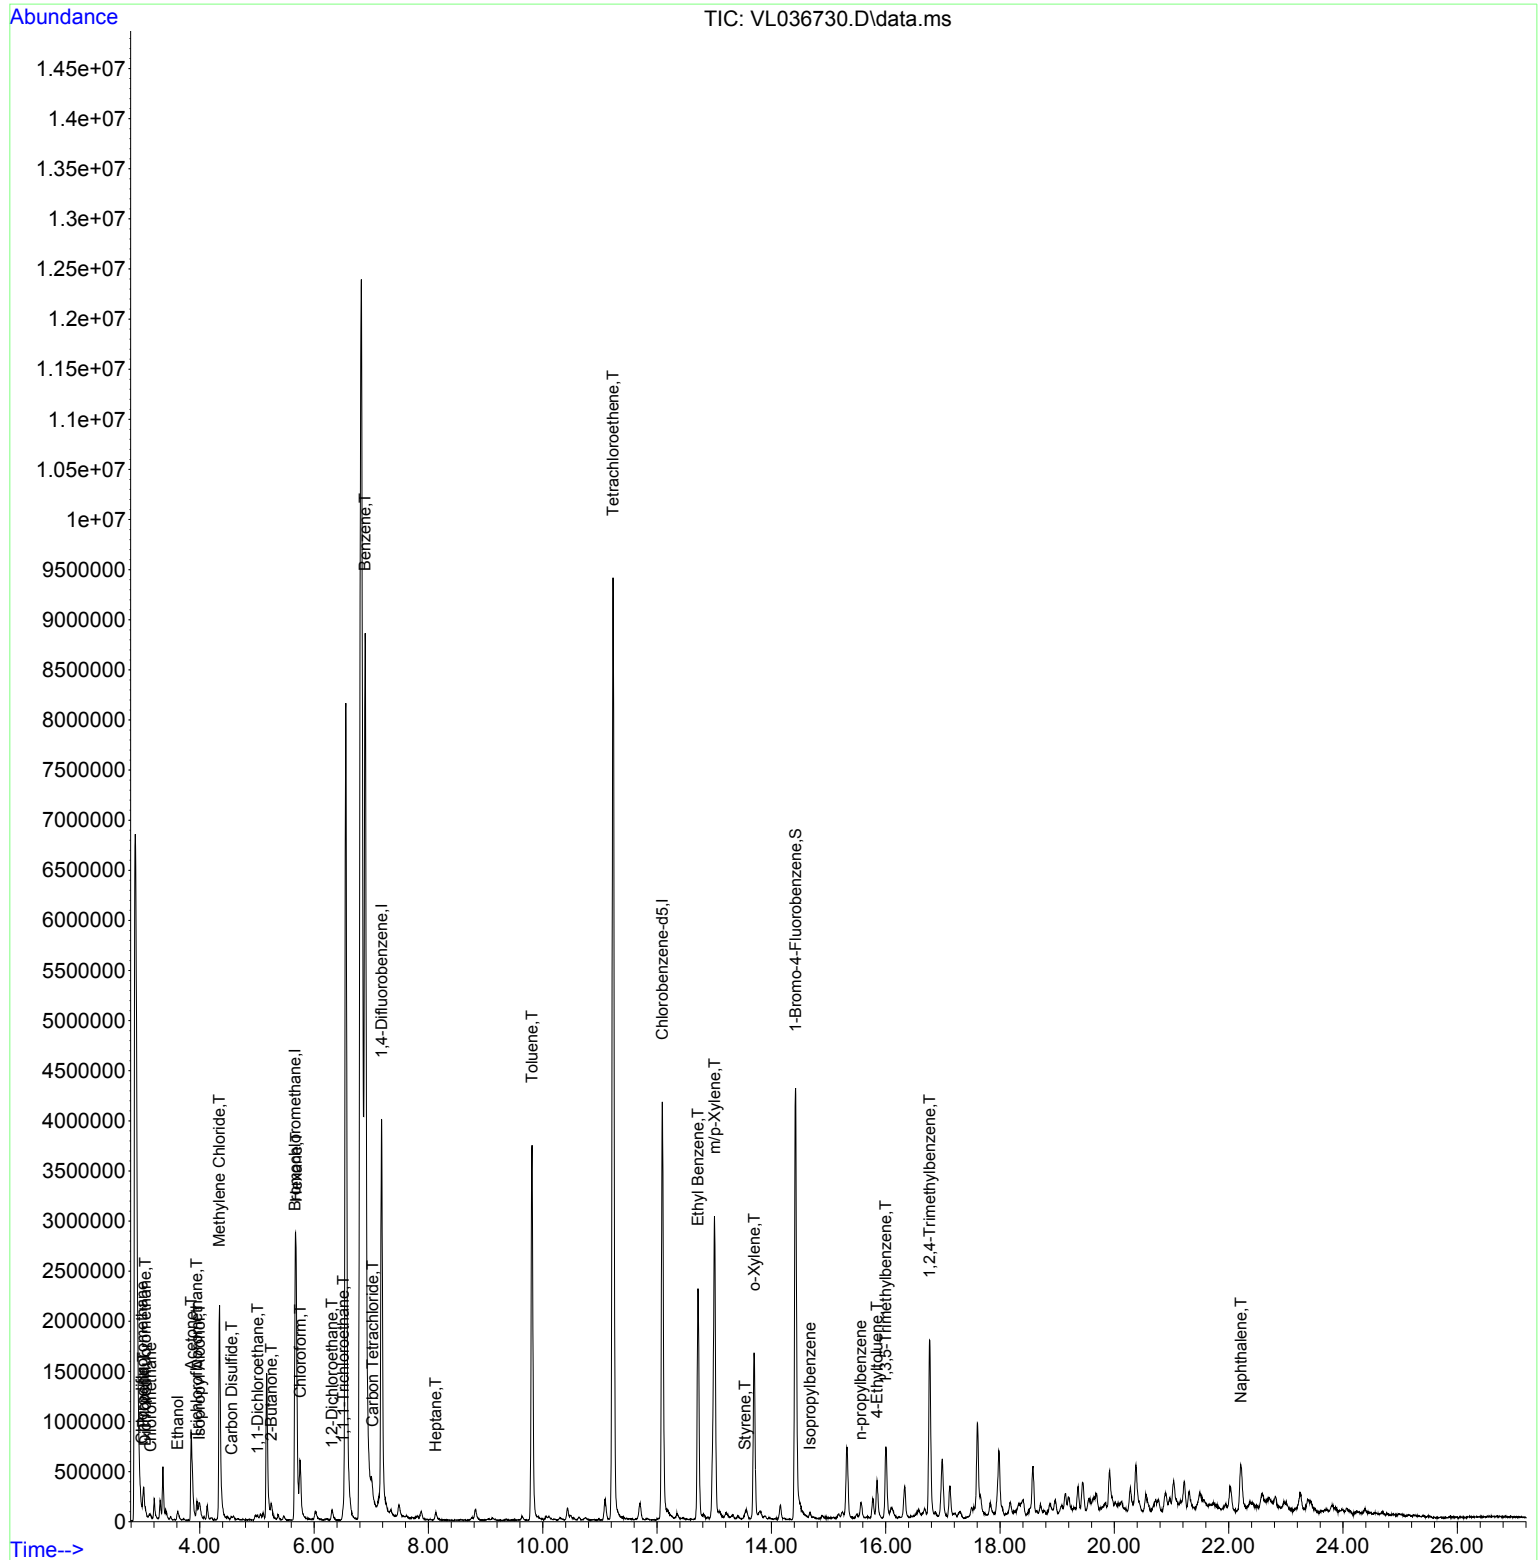

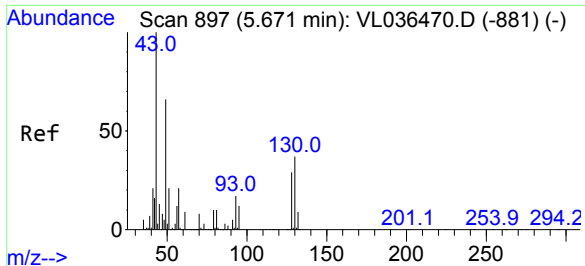

#1
Bromochloromethane
Concen: 10.00 ppbv
RT: 5.668 min Scan# 896
Delta R.T. -0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23




Instrument :
MSVOA_L
ClientSampled :
FS-SV-04

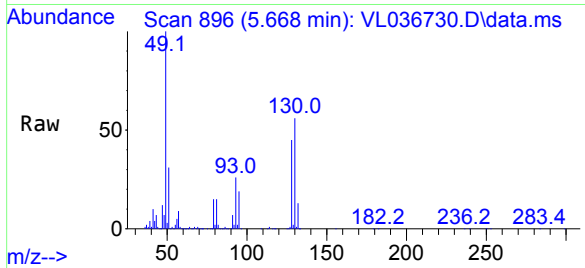


Tgt Ion: 49 Resp: 1266089
Ion Ratio Lower Upper
49 100
128 46.8 23.5 70.6
130 59.8 29.1 87.4

Manual Integrations
APPROVED



MMDadoda
4/12/2021 11:15:50 AM

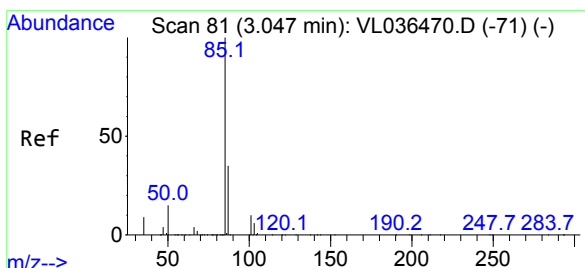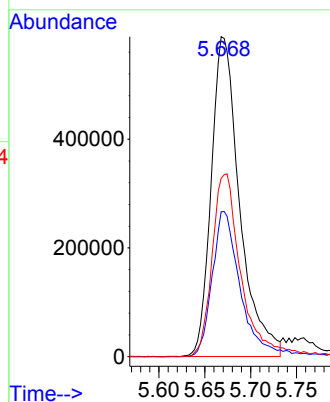


#2
Dichlorodifluoromethane
Concen: 0.18 ppbv
RT: 3.051 min Scan# 82
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

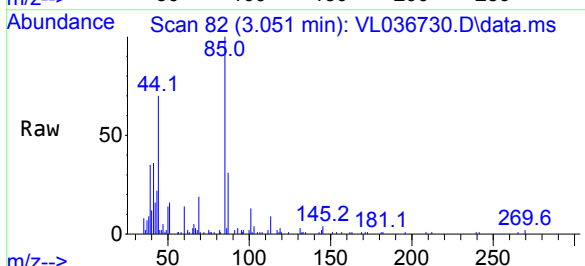

Tgt Ion: 85 Resp: 36306
Ion Ratio Lower Upper
85 100
87 31.2 27.8 41.8

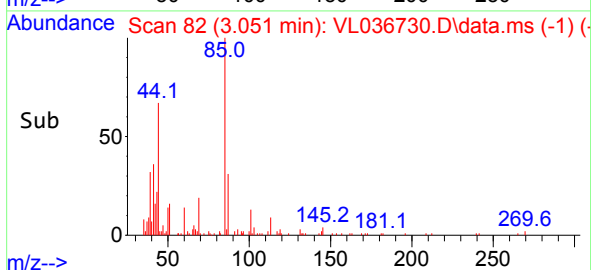

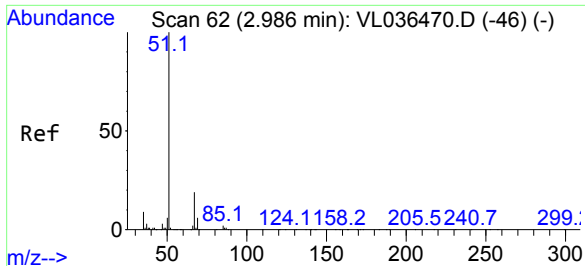





#3
Chlorodifluoromethane
Concen: 0.14 ppbv m
RT: 2.989 min Scan# 63
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Tgt Ion: 51 Resp: 34181
Ion Ratio Lower Upper
51 100
67 1.1 14.7 22.1#

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM

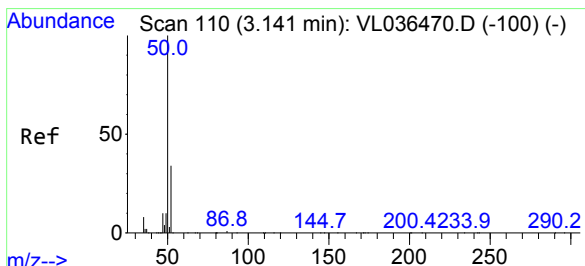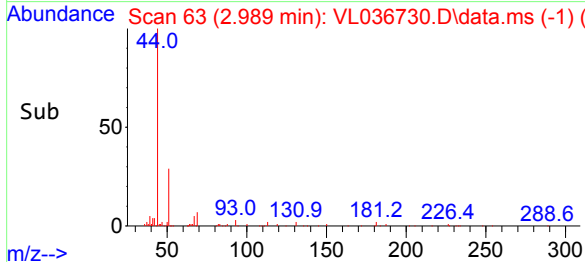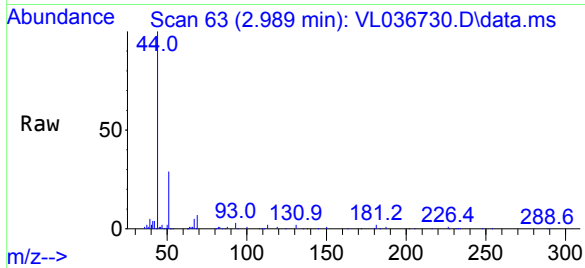

#4
Chloromethane
Concen: 0.26 ppbv m
RT: 3.141 min Scan# 110
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Tgt Ion: 50 Resp: 21610
Ion Ratio Lower Upper
50 100
52 32.5 27.0 40.6

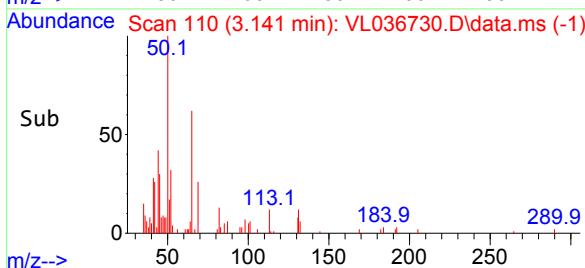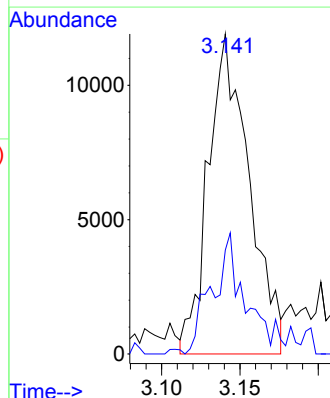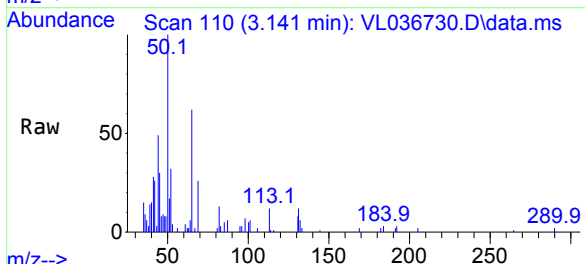

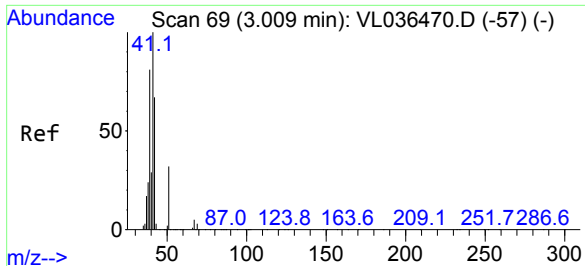





#9
Propene
Concen: 1.64 ppbv
RT: 3.012 min Scan# 70
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Tgt Ion: 41 Resp: 124010
Ion Ratio Lower Upper
41 100
42 64.6 57.0 85.4

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM

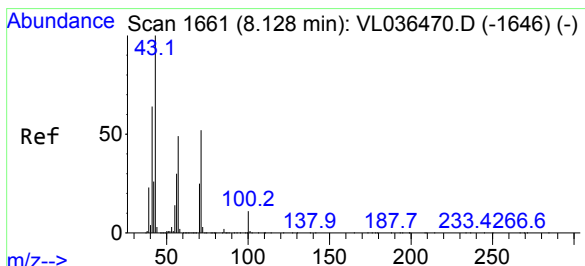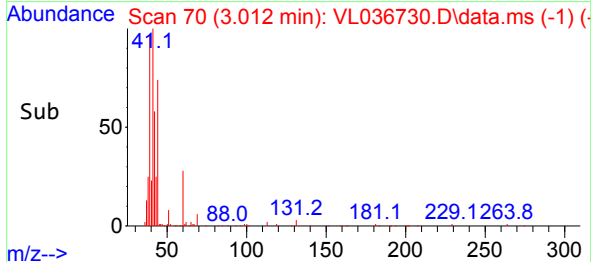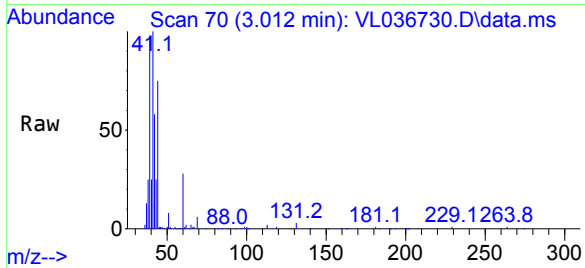

#10
Heptane
Concen: 0.13 ppbv m
RT: 8.124 min Scan# 1660
Delta R.T. -0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23


Tgt Ion: 43 Resp: 24835
Ion Ratio Lower Upper
43 100
57 57.4 39.0 58.6

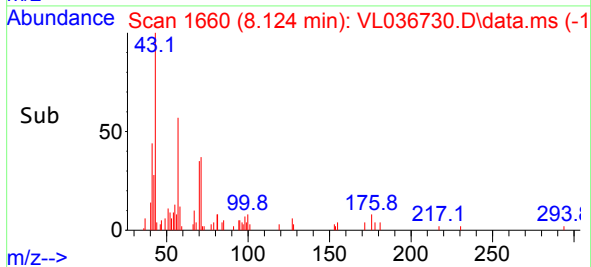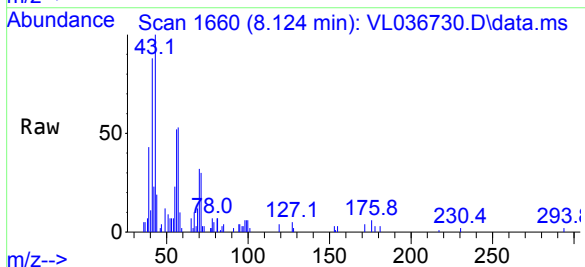



#11
Trichlorofluoromethane
Concen: 0.58 ppbv
RT: 3.948 min Scan# 361
Delta R.T. -0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23




Instrument :
MSVOA_L
ClientSampled :
FS-SV-04




Tgt Ion:101 Resp: 122693
Ion Ratio Lower Upper
101 100
103 57.8 52.5 78.7

Manual Integrations
APPROVED



MMDadoda
4/12/2021 11:15:50 AM

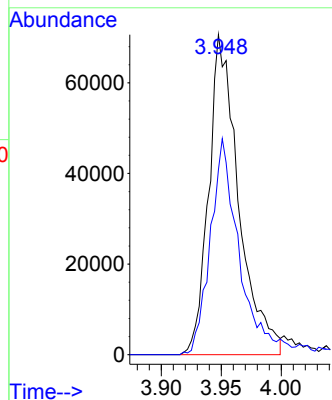


#13
Ethanol
Concen: 11.74 ppbv
RT: 3.613 min Scan# 257
Delta R.T. 0.006 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

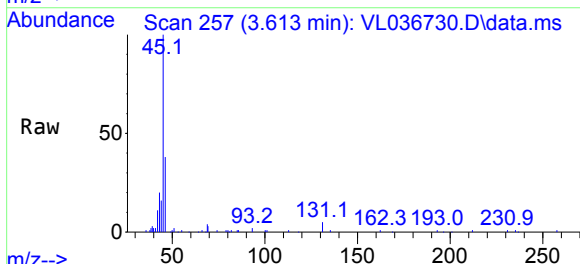

Tgt Ion: 45 Resp: 105415
Ion Ratio Lower Upper
45 100
46 39.9 16.6 66.2

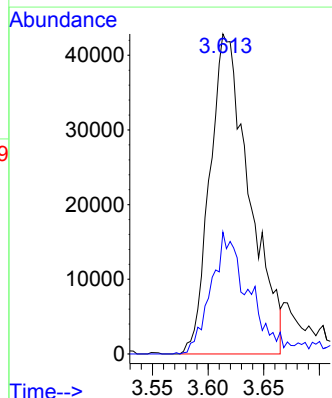







#15
Acetone
Concen: 9.33 ppbv
RT: 3.851 min Scan# 331
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04

Tgt Ion: 43 Resp: 1162733
Ion Ratio Lower Upper
43 100
58 25.6 21.2 31.8




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM

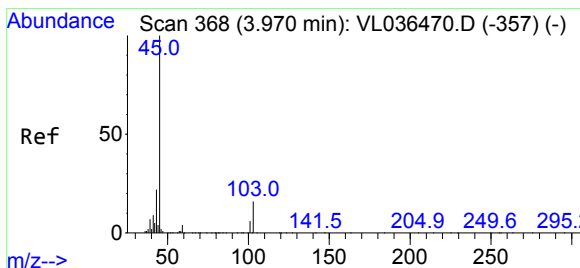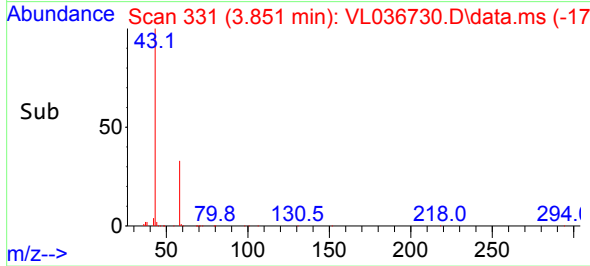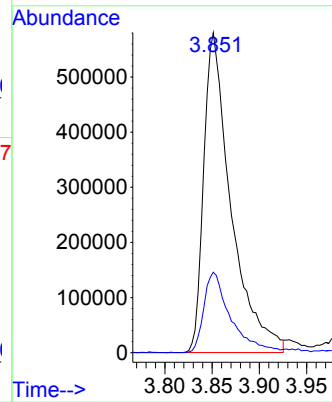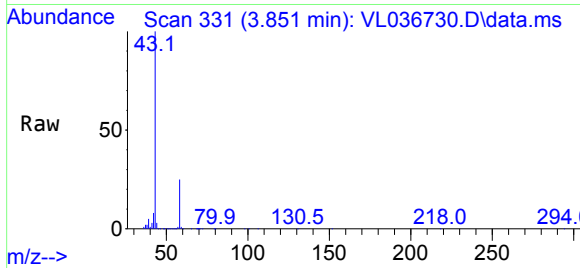

#19
Isopropyl Alcohol
Concen: 2.84 ppbv m
RT: 3.989 min Scan# 374
Delta R.T. 0.019 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23


Tgt Ion: 45 Resp: 194960
Ion Ratio Lower Upper
45 100
58 6.3 2.9 4.3#

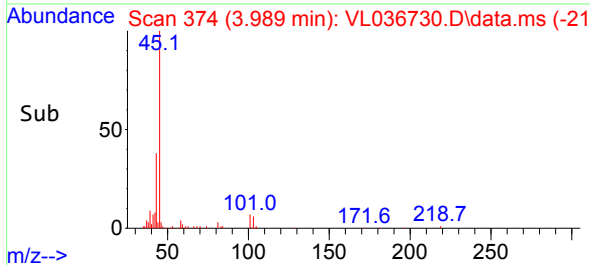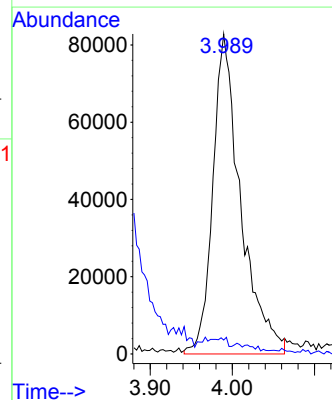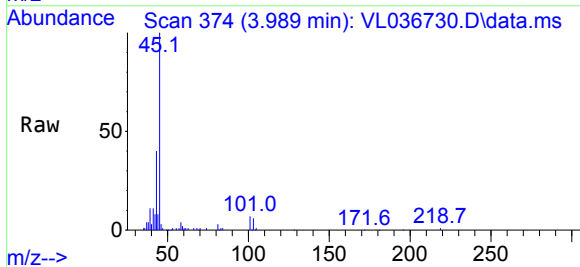



#20
Methylene Chloride
Concen: 14.43 ppbv
RT: 4.343 min Scan# 484
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Instrument :
MSVOA_L
ClientSampled :
FS-SV-04



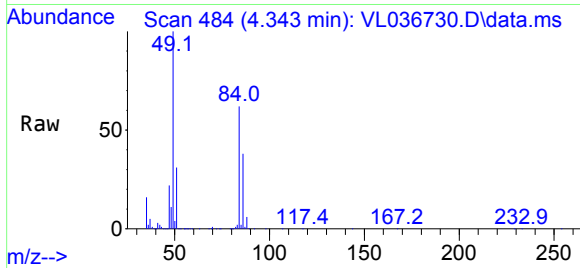


Tgt Ion: 84 Resp: 841863


Ion	Ratio	Lower	Upper
84	100		
49	161.2	122.9	184.3
51	50.0	36.9	55.3
86	61.7	48.2	72.4

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:50 AM

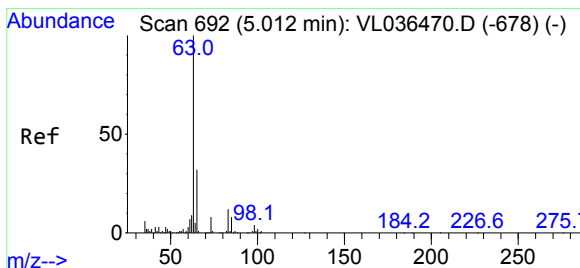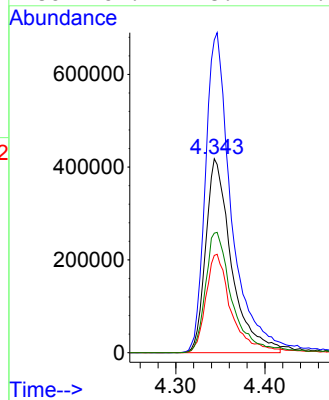
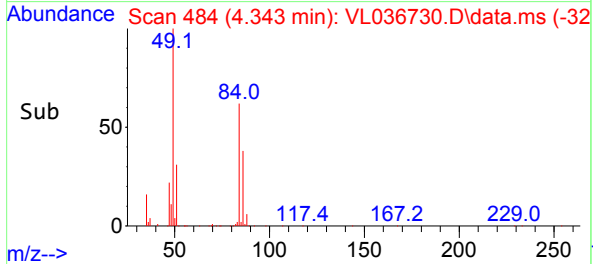



#24
1,1-Dichloroethane
Concen: 0.22 ppbv m
RT: 5.012 min Scan# 692
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

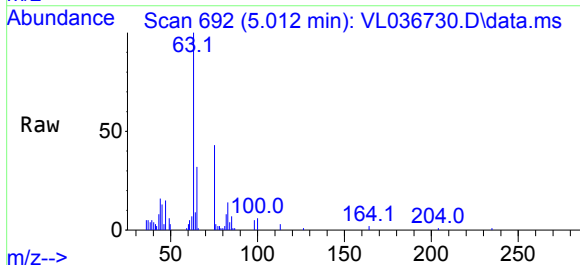

Tgt Ion: 63 Resp: 34770


Ion	Ratio	Lower	Upper
63	100		
98	4.6	2.1	6.2
100	5.6	0.9	2.8

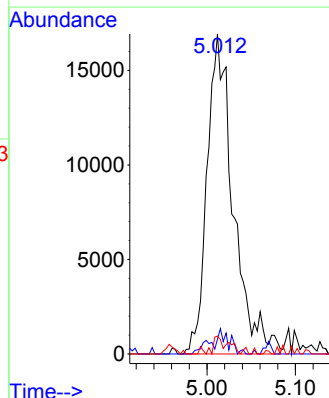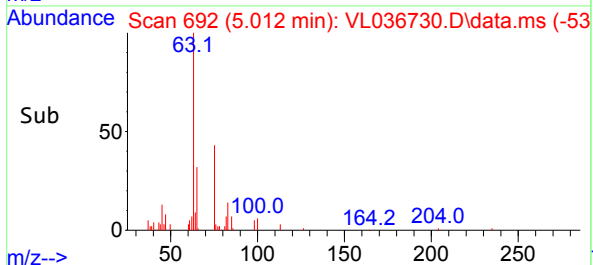

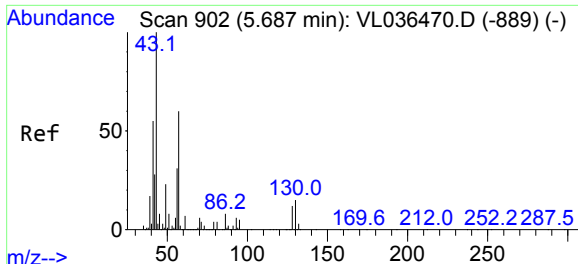

#26
Hexane
Concen: 4.46 ppbv
RT: 5.687 min Scan# 902
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23




Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04

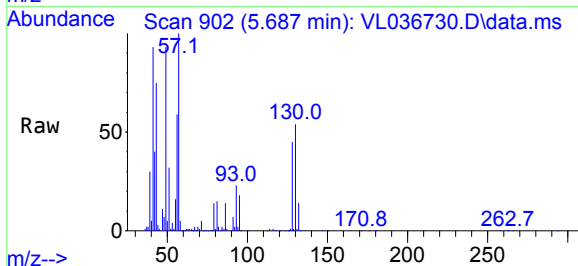


Tgt Ion: 57 Resp: 613330
Ion Ratio Lower Upper
57 100
41 96.5 77.2 115.8
43 75.0 173.8 260.6#
56 57.4 43.8 65.6

Manual Integrations
APPROVED



MMDadoda
4/12/2021 11:15:50 AM

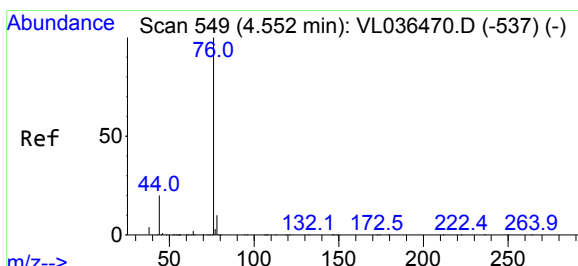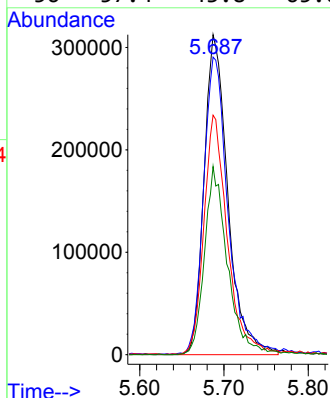


#27
Carbon Disulfide
Concen: 0.29 ppbv m
RT: 4.555 min Scan# 550
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

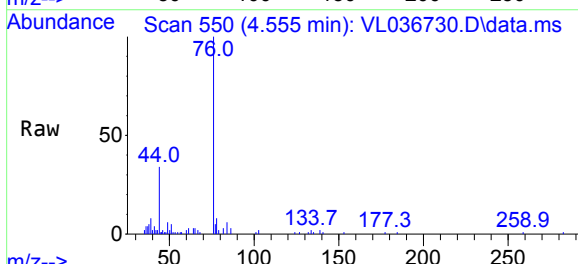

Tgt Ion: 76 Resp: 38616
Ion Ratio Lower Upper
76 100
44 45.6 17.5 26.3#
78 0.0 8.6 13.0#

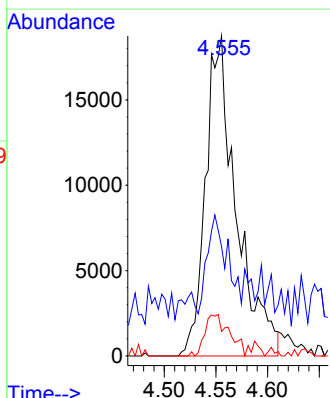

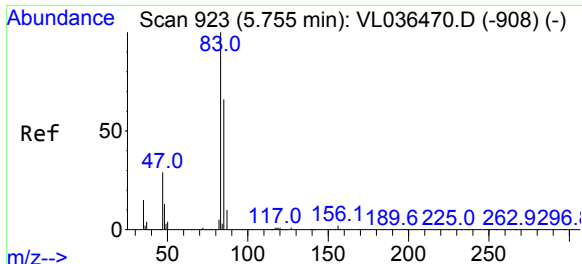





#29
Chloroform
Concen: 1.89 ppbv
RT: 5.755 min Scan# 923
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Instrument :
MSVOA_L
ClientSampled :
FS-SV-04

Tgt Ion: 83 Resp: 415959
Ion Ratio Lower Upper
83 100
85 64.4 52.6 78.8




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM

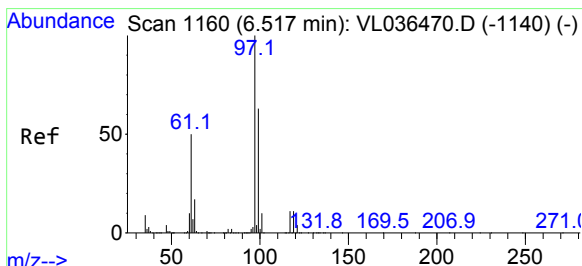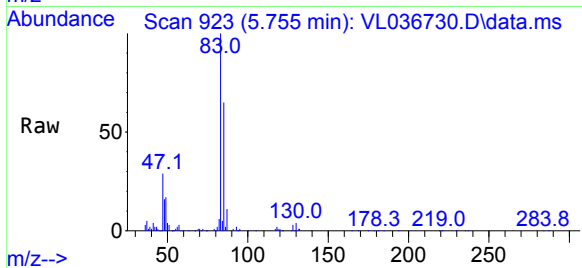

#32
1,1,1-Trichloroethane
Concen: 0.39 ppbv
RT: 6.510 min Scan# 1158
Delta R.T. -0.006 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23


Tgt Ion: 97 Resp: 86296
Ion Ratio Lower Upper
97 100
99 71.5 51.4 77.0
61 53.8 40.6 60.8

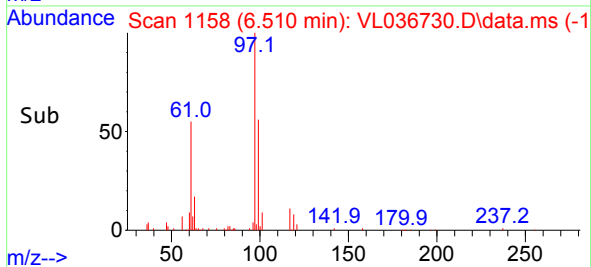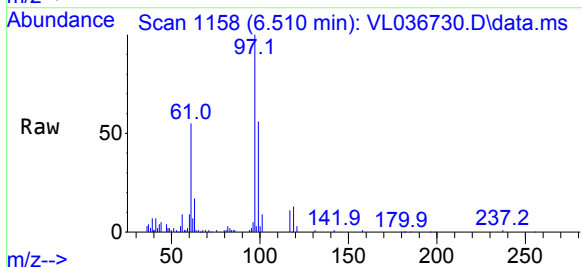



#33
1,4-Difluorobenzene
Concen: 10.00 ppbv
RT: 7.182 min Scan# 1367
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23




Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04




Tgt Ion:114 Resp: 3181412
Ion Ratio Lower Upper
114 100
63 26.9 22.4 33.6
88 18.3 15.4 23.0

Manual Integrations
APPROVED



MMDadoda
4/12/2021 11:15:50 AM

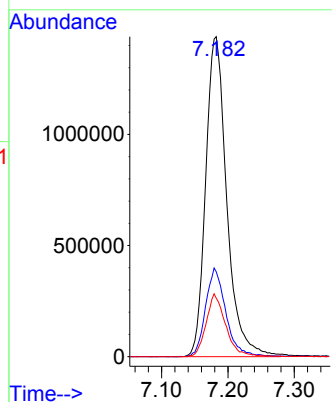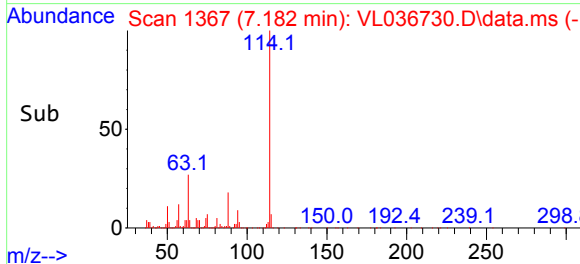


#34
2-Butanone
Concen: 0.88 ppbv
RT: 5.250 min Scan# 766
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

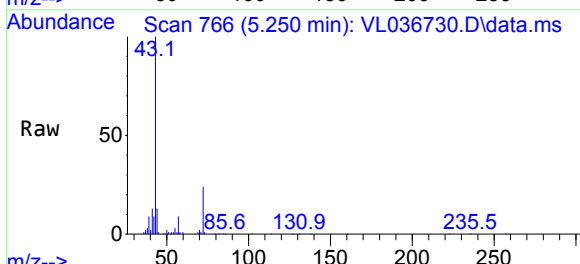

Tgt Ion: 43 Resp: 137289
Ion Ratio Lower Upper
43 100
72 35.1 17.0 25.6#

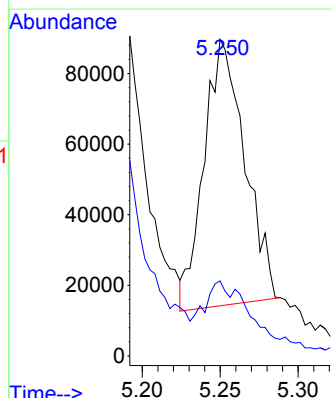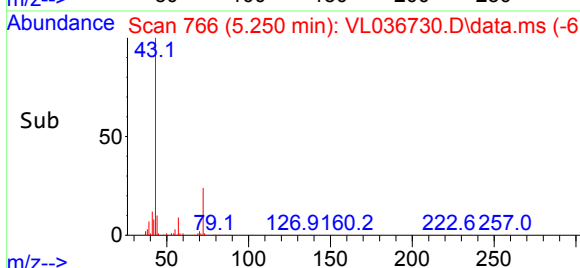







#35
Carbon Tetrachloride
Concen: 0.03 ppbv m
RT: 7.025 min Scan# 1318
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Instrument :
MSVOA_L
ClientSampled :
FS-SV-04

Tgt Ion:117 Resp: 8397
Ion Ratio Lower Upper
117 100
119 98.4 78.2 117.2
121 45.8 24.5 36.7#




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM

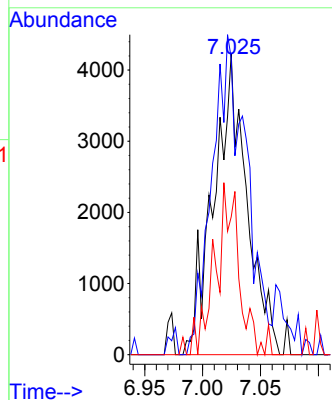

#36
Benzene
Concen: 24.94 ppbv
RT: 6.893 min Scan# 1277
Delta R.T. -0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23


Tgt Ion: 78 Resp: 7318928
Ion Ratio Lower Upper
78 100
77 25.5 18.0 27.0
50 22.6 16.5 24.7

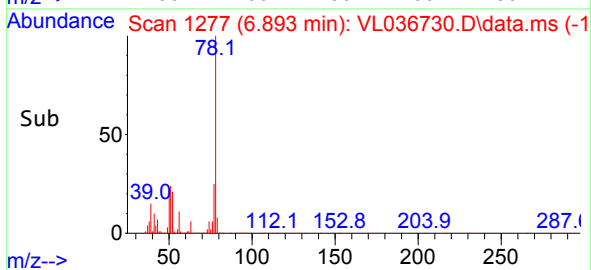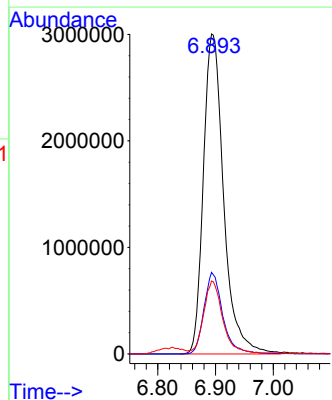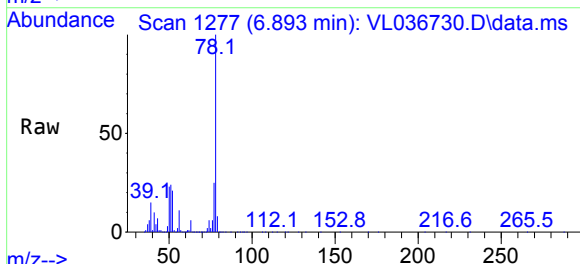



#37
1,2-Dichloroethane
Concen: 0.30 ppbv
RT: 6.311 min Scan# 1096
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23




Instrument :
MSVOA_L
ClientSampled :
FS-SV-04




Tgt Ion: 62 Resp: 51703
Ion Ratio Lower Upper
62 100
98 7.3 4.9 7.3#

Manual Integrations
APPROVED



MMDadoda
4/12/2021 11:15:50 AM




#52
Tetrachloroethene
Concen: 22.33 ppbv
RT: 11.230 min Scan# 2626
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

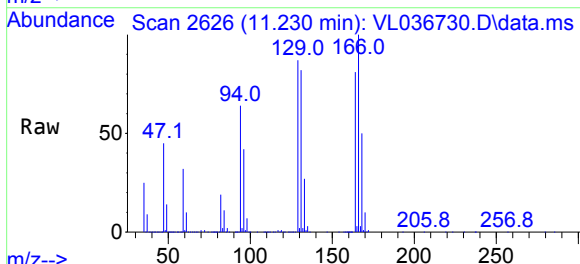

Tgt Ion: 164 Resp: 2412642
Ion Ratio Lower Upper
164 100
166 122.8 98.3 147.5
129 106.9 85.8 128.8
131 101.1 80.9 121.3

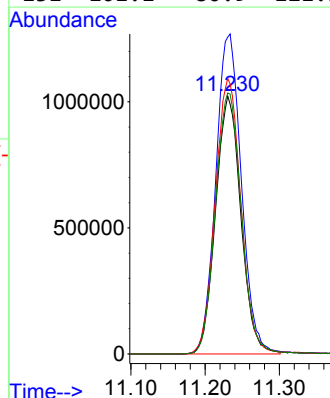







#53
Toluene
Concen: 9.76 ppbv
RT: 9.812 min Scan# 2185
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Tgt Ion: 91 Resp: 3049043
Ion Ratio Lower Upper
91 100
92 61.4 48.8 73.2

Instrument :
MSVOA_L
ClientSampled :
FS-SV-04




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM

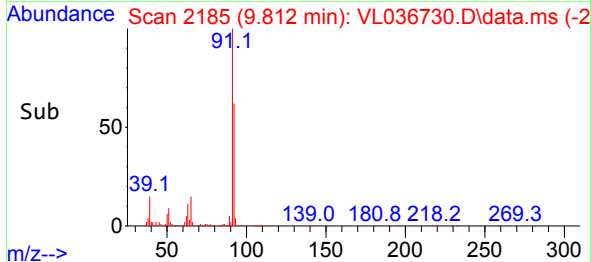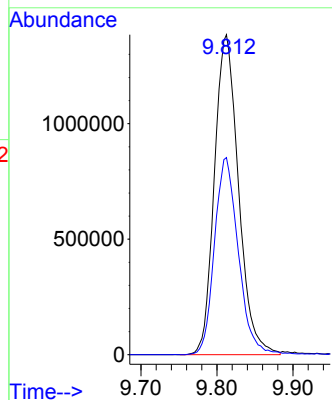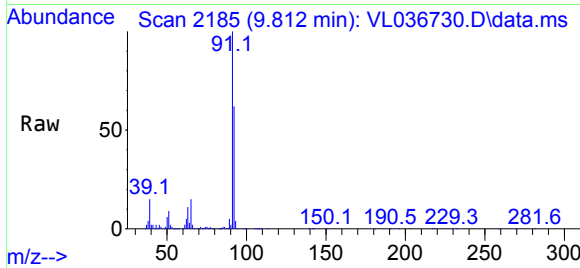

#55
Chlorobenzene-d5
Concen: 10.00 ppbv
RT: 12.092 min Scan# 2894
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Tgt Ion: 117 Resp: 2769795
Ion Ratio Lower Upper
117 100
82 66.0 57.4 86.0
119 32.6 47.4 71.0#

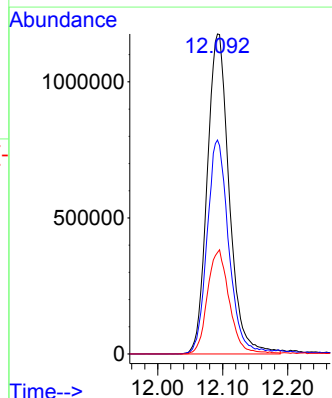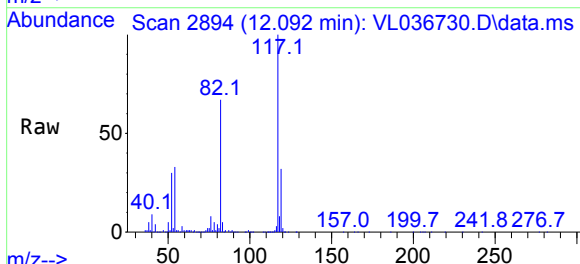







#58
Ethyl Benzene
Concen: 5.19 ppbv
RT: 12.716 min Scan# 3088
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Instrument :
MSVOA_L
ClientSampled :
FS-SV-04

Tgt Ion: 91 Resp: 2093139
Ion Ratio Lower Upper
91 100
106 28.8 25.3 37.9




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM



#59
m/p-Xylene
Concen: 7.84 ppbv
RT: 13.005 min Scan# 3178
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Tgt Ion: 91 Resp: 2753976
Ion Ratio Lower Upper
91 100
106 46.7 35.3 52.9

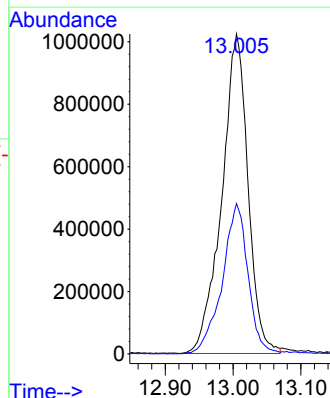







#60
o-Xylene
Concen: 3.89 ppbv
RT: 13.700 min Scan# 3394
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Instrument :
MSVOA_L
ClientSampled :
FS-SV-04

Tgt Ion: 91 Resp: 1323152
Ion Ratio Lower Upper
91 100
106 44.6 22.3 66.9




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM

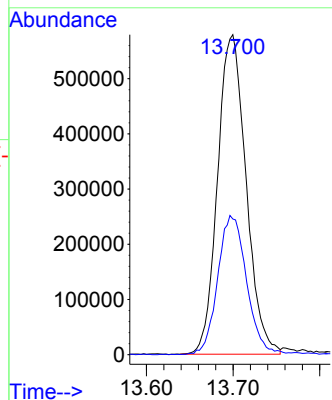

#61
Styrene
Concen: 0.14 ppbv m
RT: 13.539 min Scan# 3344
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23


Tgt Ion: 104 Resp: 23232
Ion Ratio Lower Upper
104 100
78 0.0 43.8 65.8#
103 50.7 38.3 57.5

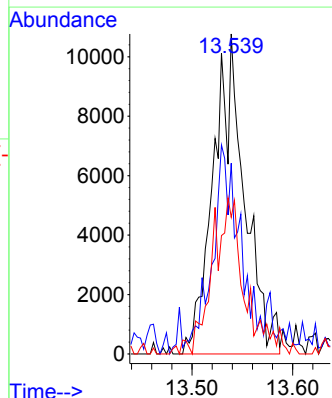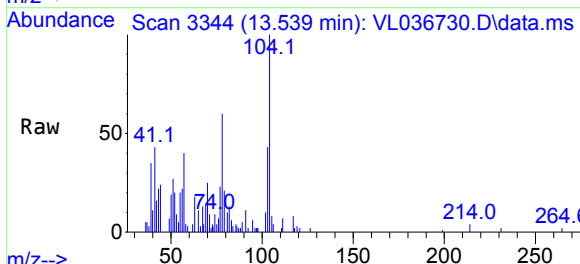



#62
Isopropylbenzene
Concen: 0.10 ppbv
RT: 14.674 min Scan# 3697
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23




Instrument :
MSVOA_L
ClientSampled :
FS-SV-04




Tgt Ion:105 Resp: 47156
Ion Ratio Lower Upper
105 100
120 23.9 20.6 31.0

Manual Integrations
APPROVED



MMDadoda
4/12/2021 11:15:50 AM

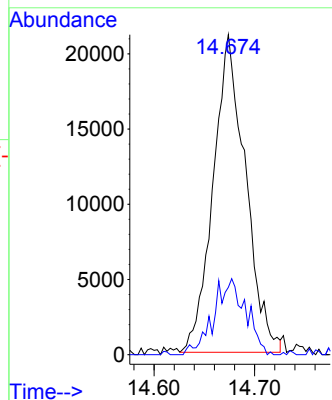


#64
n-propylbenzene
Concen: 0.27 ppbv m
RT: 15.565 min Scan# 3974
Delta R.T. -0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

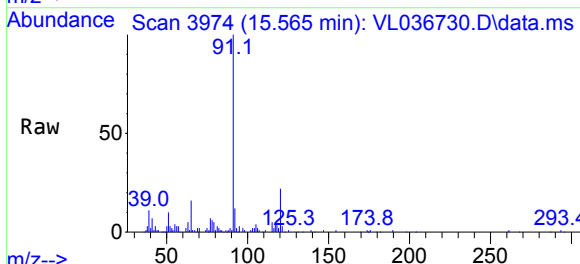


Tgt Ion:120 Resp: 30728
Ion Ratio Lower Upper
120 100
91 487.3 377.4 566.2

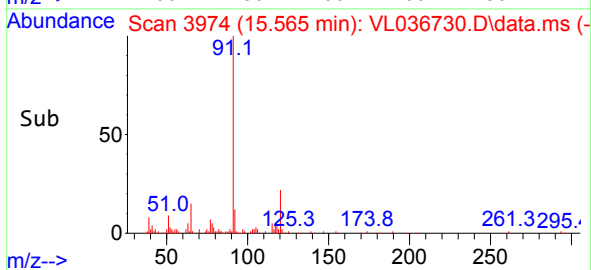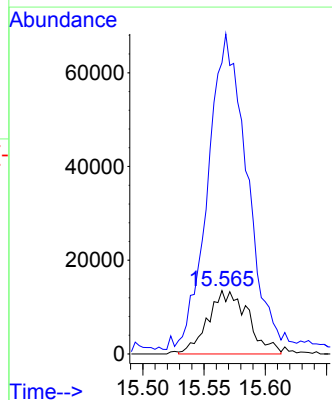



#68
1-Bromo-4-Fluorobenzene
Concen: 10.16 ppbv
RT: 14.426 min Scan# 3620
Delta R.T. 0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23




Instrument :
MSVOA_L
ClientSampled :
FS-SV-04




Tgt Ion: 95 Resp: 2242936
Ion Ratio Lower Upper
95 100
174 63.0 51.0 76.6
175 4.5 3.9 5.9

Manual Integrations
APPROVED



MMDadoda
4/12/2021 11:15:50 AM

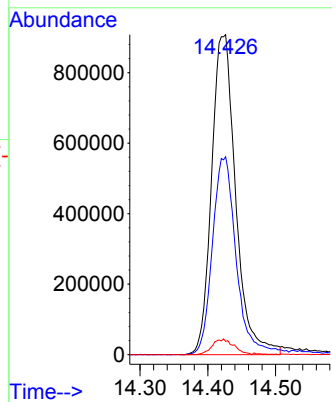


#72
4-Ethyltoluene
Concen: 0.72 ppbv
RT: 15.847 min Scan# 4062
Delta R.T. 0.000 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23



Tgt Ion: 105 Resp: 267256
Ion Ratio Lower Upper
105 100
120 31.3 24.0 36.0
91 16.9 11.0 16.4#
77 15.8 11.7 17.5

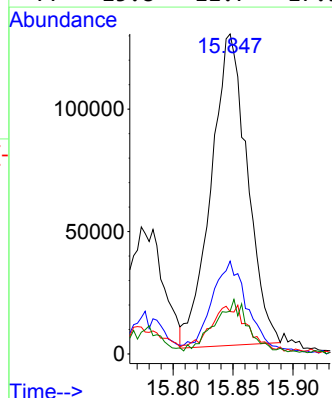







#73
1,3,5-Trimethylbenzene
Concen: 1.51 ppbv
RT: 16.002 min Scan# 4110
Delta R.T. -0.006 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Tgt Ion:105 Resp: 523468
Ion Ratio Lower Upper
105 100
120 41.8 36.6 54.8

Instrument :
MSVOA_L
ClientSampled :
FS-SV-04




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:50 AM



#74
1,2,4-Trimethylbenzene
Concen: 3.66 ppbv
RT: 16.767 min Scan# 4348
Delta R.T. -0.003 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23


Tgt Ion:105 Resp: 1362300
Ion Ratio Lower Upper
105 100
120 42.2 39.2 58.8
91 12.7 42.6 64.0#
77 14.0 18.6 28.0#

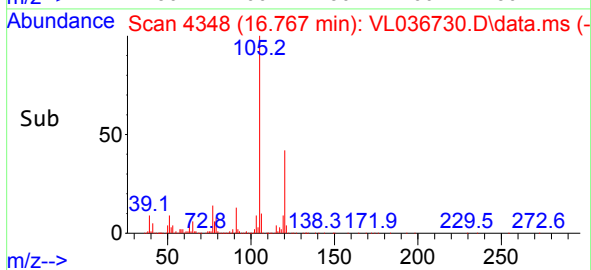



#79
Naphthalene
Concen: 2.36 ppbv
RT: 22.214 min Scan# 6042
Delta R.T. 0.010 min
Lab File: VL036730.D
Acq: 7 Apr 2021 17:23

Instrument :
MSVOA_L
ClientSampled :
FS-SV-04



Tgt Ion:128 Resp: 511273
Ion Ratio Lower Upper
128 100
127 10.4 10.9 16.3#
129 10.1 9.0 13.4

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:50 AM

