

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL040721\
 Data File : VL036731.D
 Acq On : 7 Apr 2021 18:04
 Operator : SY/AP
 Sample : M1929-02DUP
 Misc : 400mL/MSVOA L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 FS-SV-04DUP

Manual Integrations
 APPROVED

MMDadoda
 4/12/2021 11:15:54 AM

Quant Time: Apr 10 22:46:24 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Apr 08 01:58:43 2021
 QLast Update : Thu Apr 08 01:58:43 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	1271667	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.18	114	3227501	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.09	117	2730176	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.42	95	2216281	10.19	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.90%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.05	85	30155	0.145	ppbv	93
3) Chlorodifluoromethane	2.98	51	40144m	0.169	ppbv	
4) Chloromethane	3.14	50	22047m	0.263	ppbv	
9) Propene	3.01	41	124745	1.647	ppbv	93
10) Heptane	8.13	43	29622m	0.154	ppbv	
11) Trichlorofluoromethane	3.95	101	117448	0.556	ppbv	92
13) Ethanol	3.61	45	122300m	13.559	ppbv	
15) Acetone	3.85	43	1210585	9.672	ppbv	98
19) Isopropyl Alcohol	3.99	45	207356	3.012	ppbv #	1
20) Methylene Chloride	4.34	84	903044	15.410	ppbv	93
24) 1,1-Dichloroethane	5.01	63	30483	0.195	ppbv #	94
26) Hexane	5.69	57	653248	4.731	ppbv #	47
27) Carbon Disulfide	4.55	76	35091	0.258	ppbv #	91
29) Chloroform	5.75	83	374442	1.696	ppbv	95
30) Cyclohexane	7.13	84	46797m	0.418	ppbv	
32) 1,1,1-Trichloroethane	6.52	97	80293	0.361	ppbv	89
34) 2-Butanone	5.26	43	172142	1.093	ppbv #	77
35) Carbon Tetrachloride	7.02	117	10297m	0.042	ppbv	
36) Benzene	6.89	78	7019366	23.582	ppbv	96
37) 1,2-Dichloroethane	6.31	62	50632	0.289	ppbv #	95
52) Tetrachloroethene	11.23	164	2379331	21.707	ppbv	97
53) Toluene	9.81	91	2985818	9.419	ppbv	99
58) Ethyl Benzene	12.72	91	2049190	5.159	ppbv	98
59) m/p-Xylene	13.01	91	2687565	7.757	ppbv	96
60) o-Xylene	13.70	91	1308497	3.906	ppbv	100
61) Styrene	13.53	104	26303m	0.156	ppbv	
62) Isopropylbenzene	14.67	105	49176m	0.109	ppbv	
64) n-propylbenzene	15.57	120	33930m	0.308	ppbv	
72) 4-Ethyltoluene	15.84	105	277830	0.757	ppbv	98
73) 1,3,5-Trimethylbenzene	16.00	105	529103	1.544	ppbv	99
74) 1,2,4-Trimethylbenzene	16.77	105	1358453	3.705	ppbv #	69
79) Naphthalene	22.21	128	467300	2.184	ppbv #	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL040721\
Data File : VL036731.D
Acq On : 7 Apr 2021 18:04
Operator : SY/AP
Sample : M1929-02DUP
Misc : 400mL/MSVOA L
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:54 AM

Quant Time: Apr 10 22:46:24 2021
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Apr
QLast Update : Thu Apr 08 01:58:43 2021
Response via : Initial Calibration

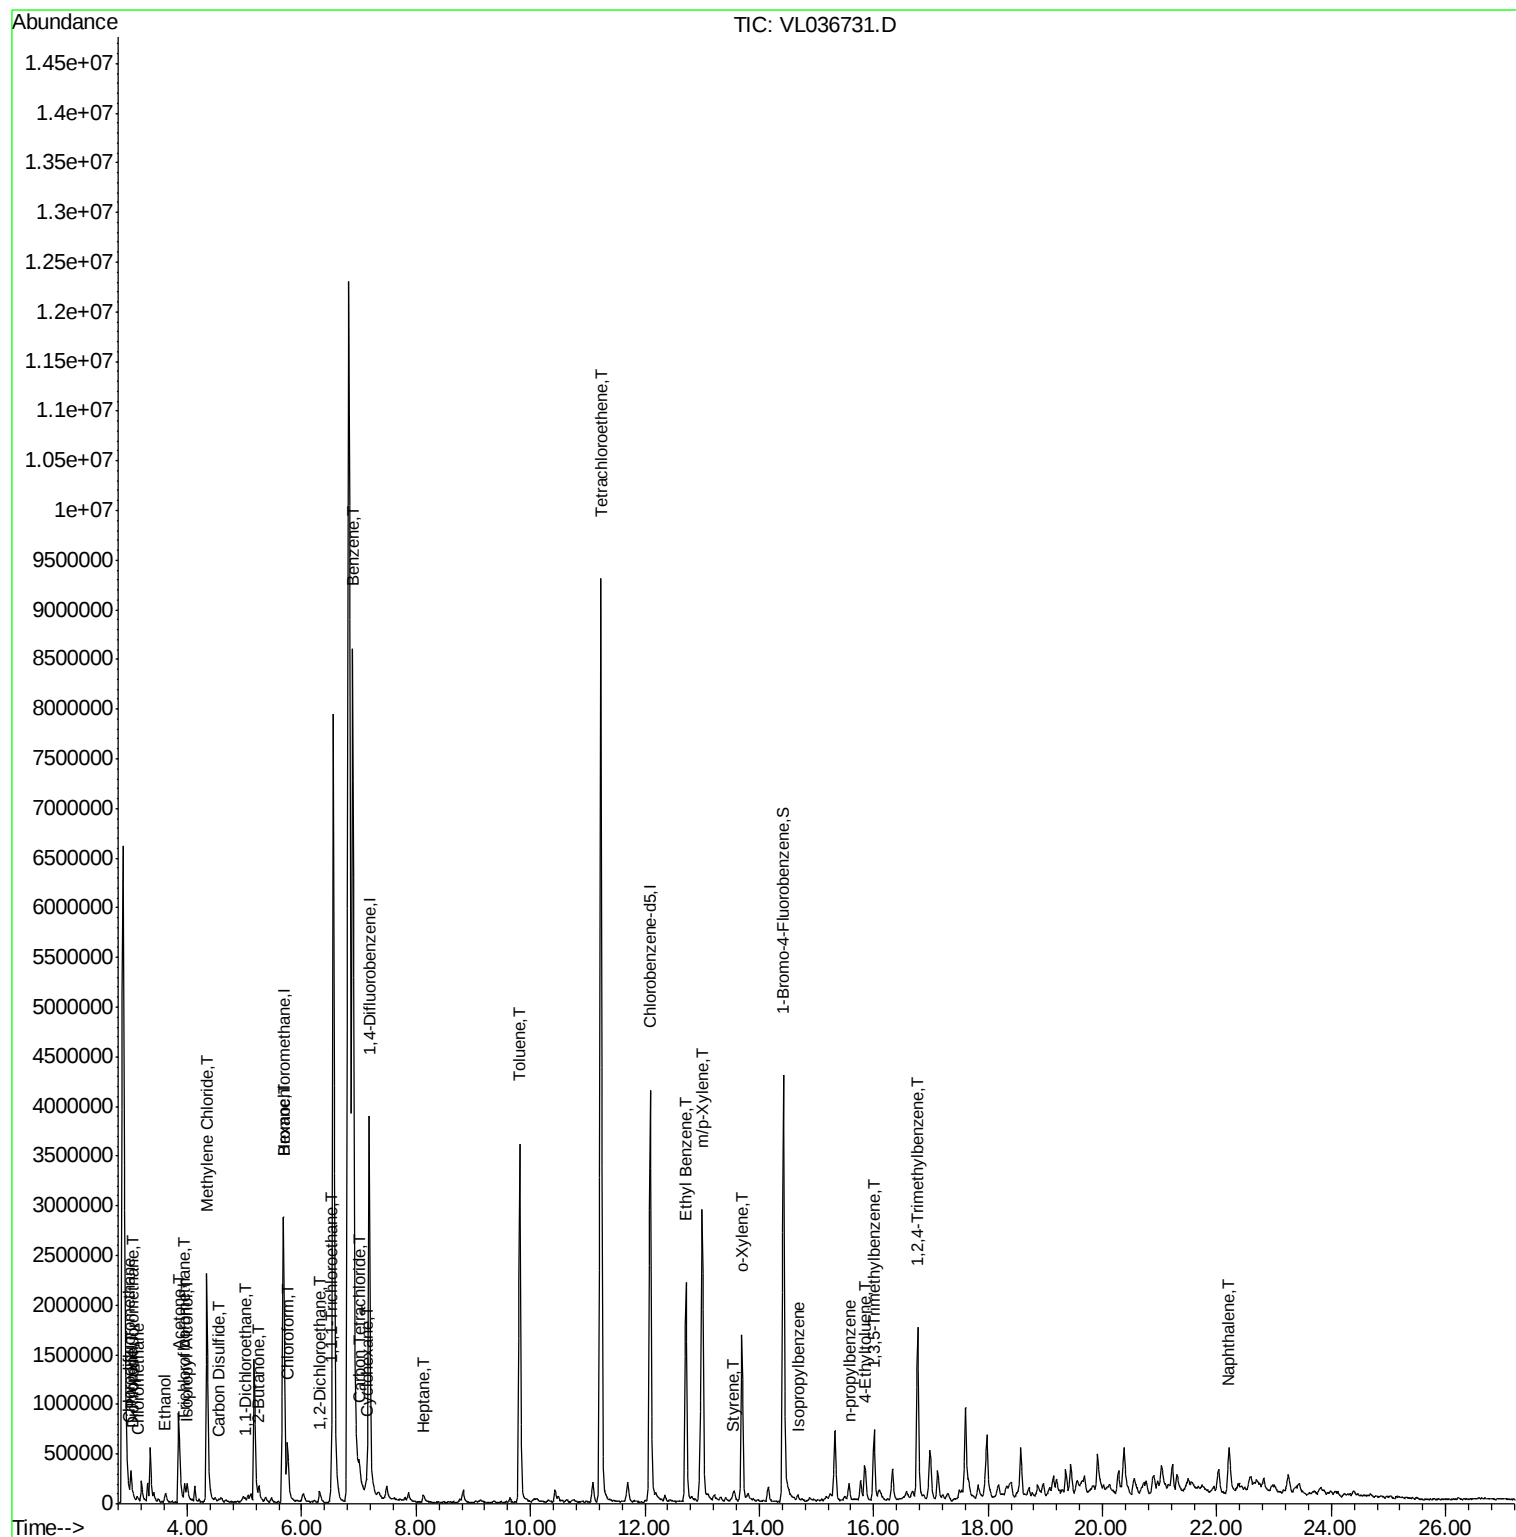

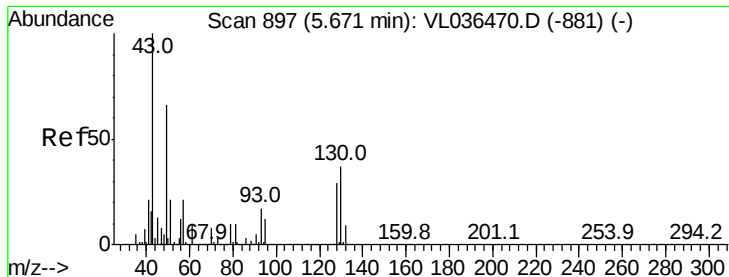

#1





Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.67 min Scan# 897
 Delta R.T. -0.00 min
 Lab File: VL036731.D
 Acq: 7 Apr 2021 18:04

Instrument :
 MSVOA_L
 ClientSampleId :
 FS-SV-04DUP

Tot Ion	Ratio	Lower	Upper
49	100		
128	47.1	23.5	70.6
130	61.0	29.1	87.4

Manual Integrations
 APPROVED




MMDadoda
 4/12/2021 11:15:54 AM

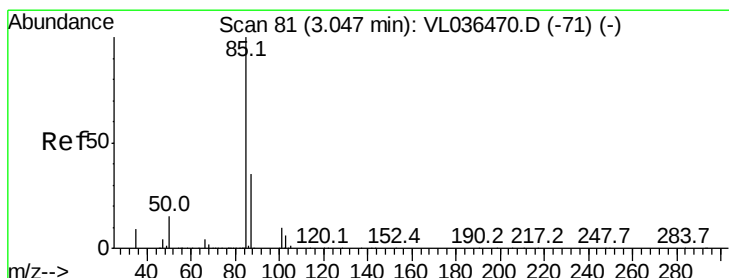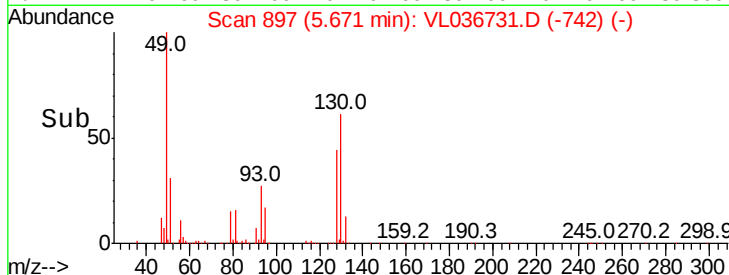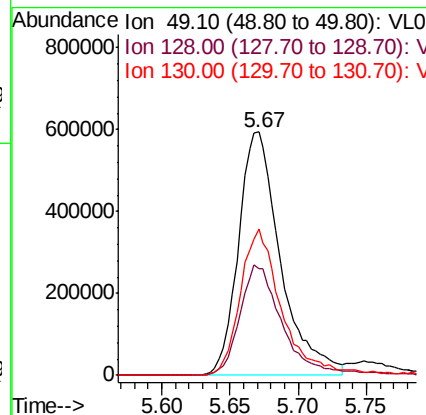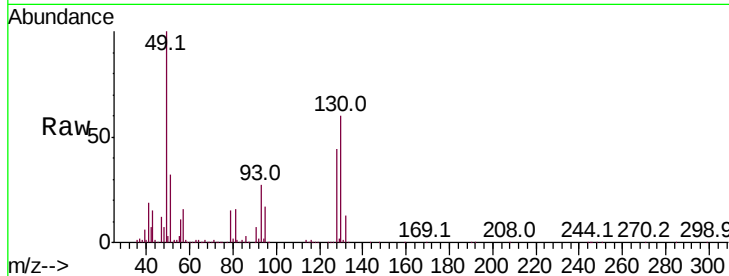


#2

Dichlorodifluoromethane
 Concen: 0.145 ppbv
 RT: 3.05 min Scan# 82
 Delta R.T. 0.00 min
 Lab File: VL036731.D
 Acq: 7 Apr 2021 18:04

Tgt Ion	Ratio	Lower	Upper
85	100		
87	30.6	27.8	41.8

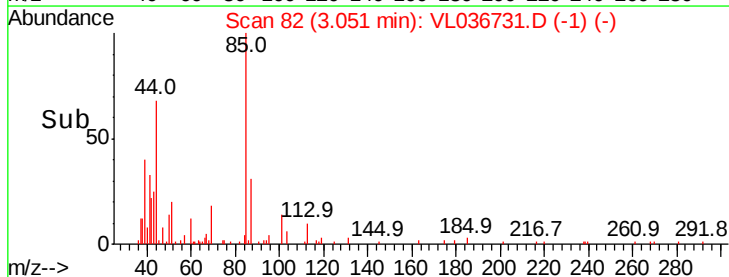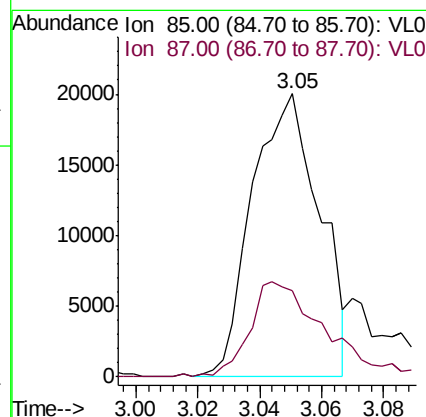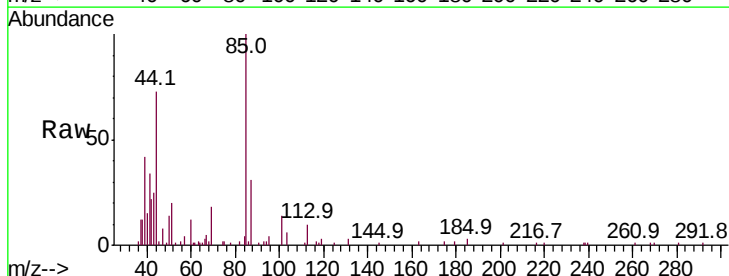

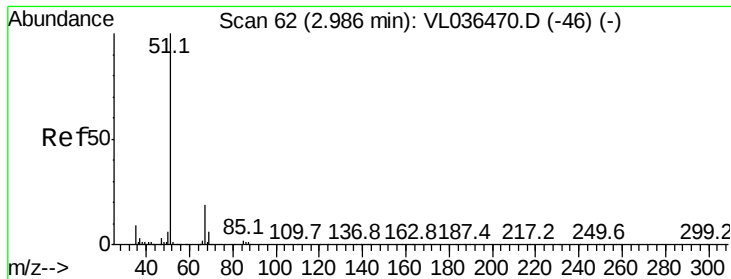





#3
Chlorodifluoromethane
Concen: 0.169 ppbv m
RT: 2.98 min Scan# 61
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Tot Ion: 51 Resp: 40144
Ion Ratio Lower Upper
51 100
67 15.5 14.7 22.1




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:54 AM

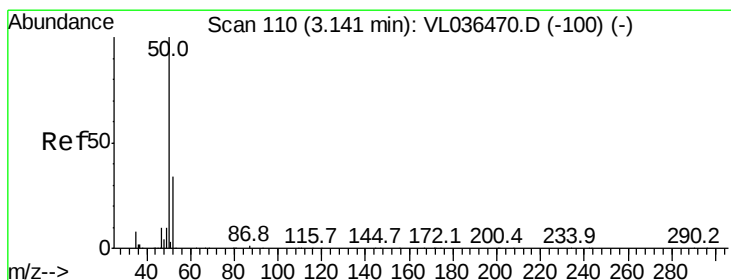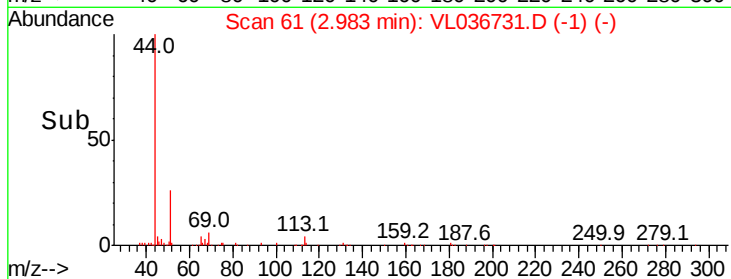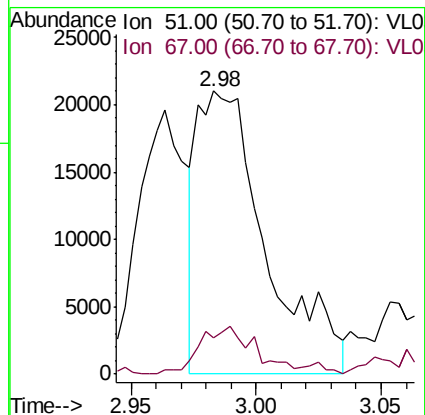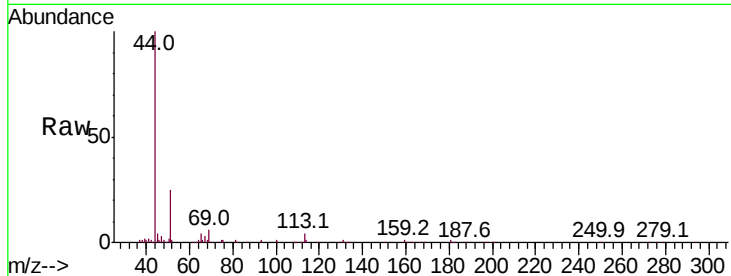

#4
Chloromethane
Concen: 0.263 ppbv m
RT: 3.14 min Scan# 109
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Tgt Ion: 50 Resp: 22047
Ion Ratio Lower Upper
50 100
52 24.0 27.0 40.6#

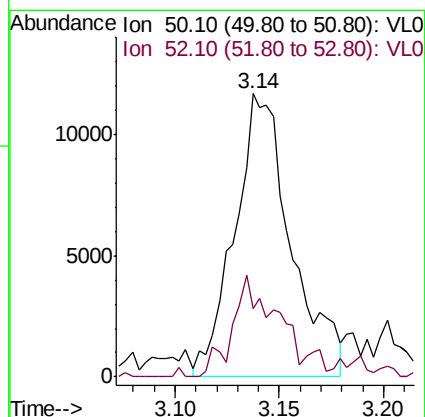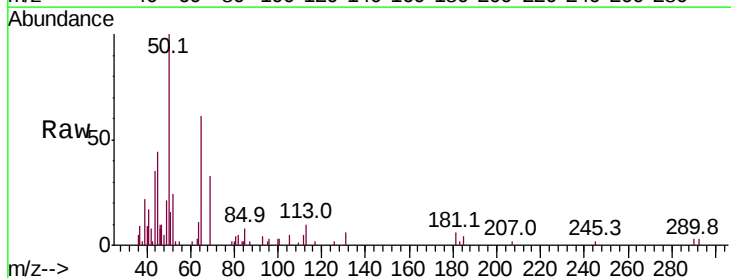

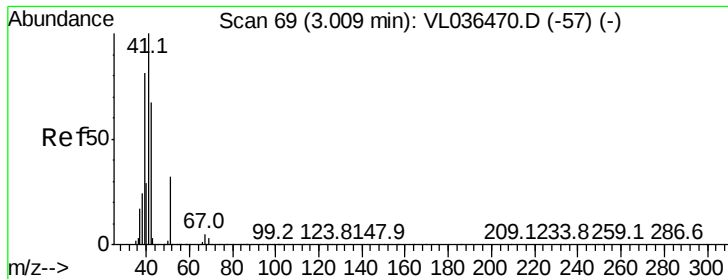

#9

Propene

Concen: 1.647 ppbv

RT: 3.01 min Scan# 69

Delta R.T. -0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Instrument :

MSVOA_L

ClientSampleId :

FS-SV-04DUP

Tot Ion: 41 Resp: 124745





Ion Ratio Lower Upper

41 100

42 65.1 57.0 85.4

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:54 AM

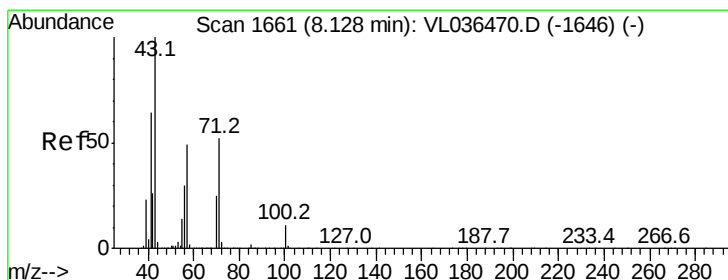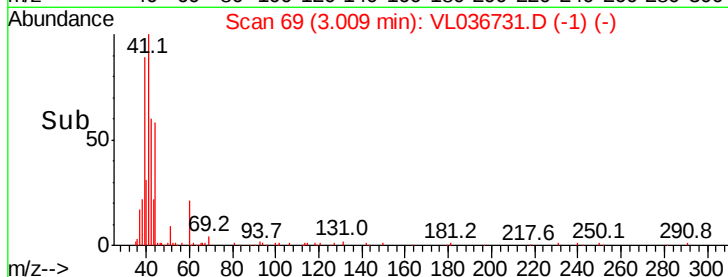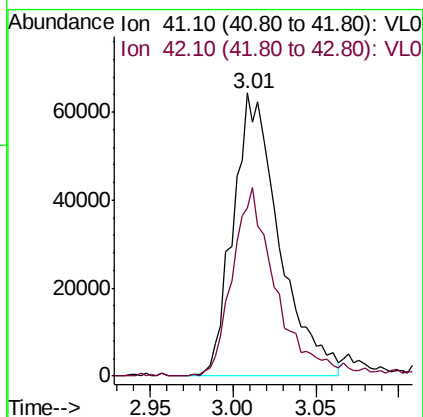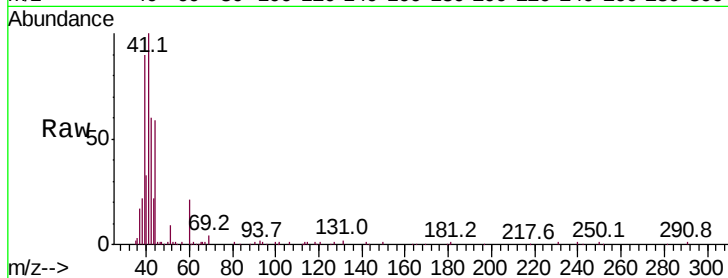

#10

Heptane

Concen: 0.154 ppbv m

RT: 8.13 min Scan# 1661

Delta R.T. -0.00 min

Lab File: VL036731.D




Acq: 7 Apr 2021 18:04


Tgt Ion: 43 Resp: 29622

Ion Ratio Lower Upper

43 100

57 49.5 39.0 58.6

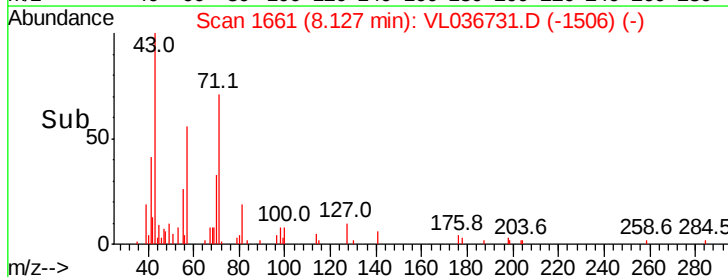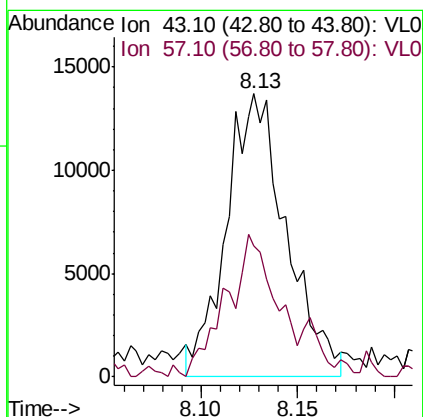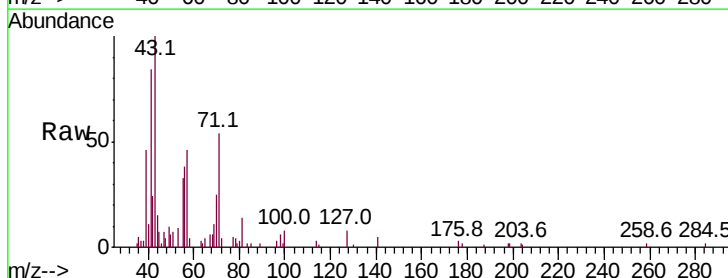

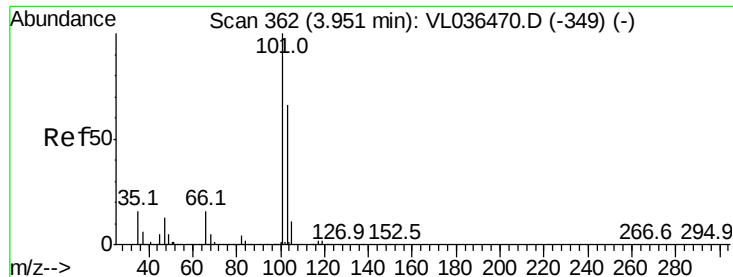





#11
 Trichlorofluoromethane
 Concen: 0.556 ppbv
 RT: 3.95 min Scan# 362
 Delta R.T. -0.00 min
 Lab File: VL036731.D
 Acq: 7 Apr 2021 18:04

Instrument :
 MSVOA_L
 ClientSampleId :
 FS-SV-04DUP

Tot Ion:101 Resp: 117448
 Ion Ratio Lower Upper
 101 100
 103 59.2 52.5 78.7




Manual Integrations
 APPROVED


MMDadoda
 4/12/2021 11:15:54 AM

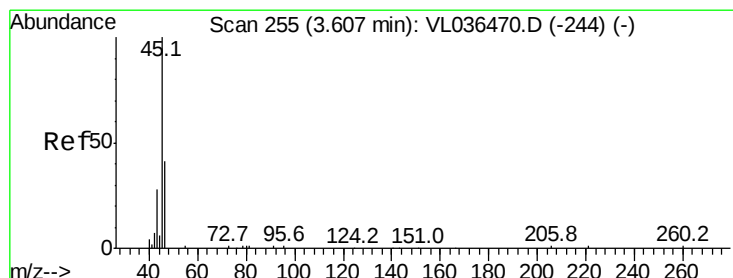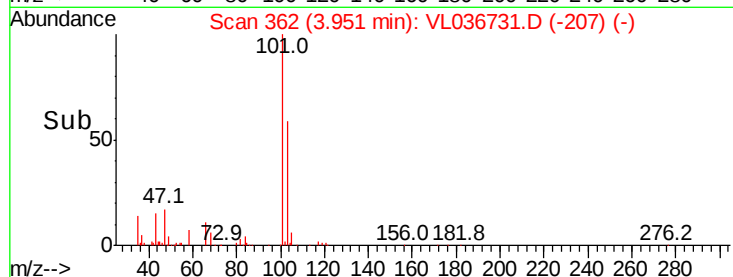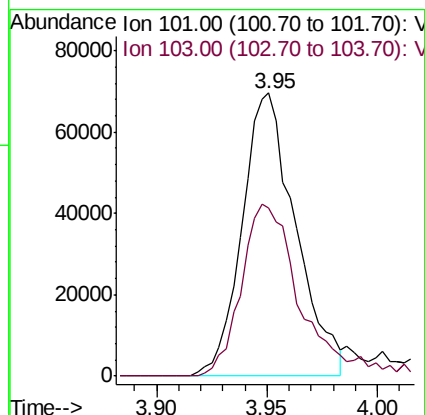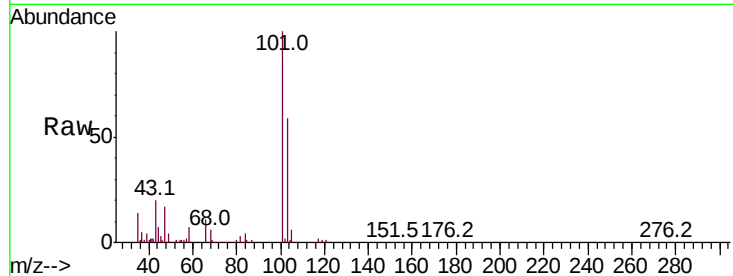

#13
 Ethanol
 Concen: 13.559 ppbv m
 RT: 3.61 min Scan# 257
 Delta R.T. 0.01 min
 Lab File: VL036731.D
 Acq: 7 Apr 2021 18:04

Tgt Ion: 45 Resp: 122300
 Ion Ratio Lower Upper
 45 100
 46 39.7 16.6 66.2

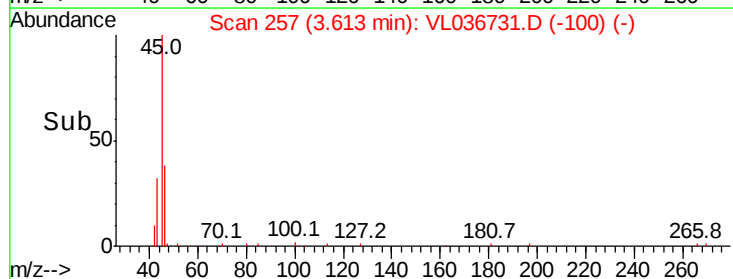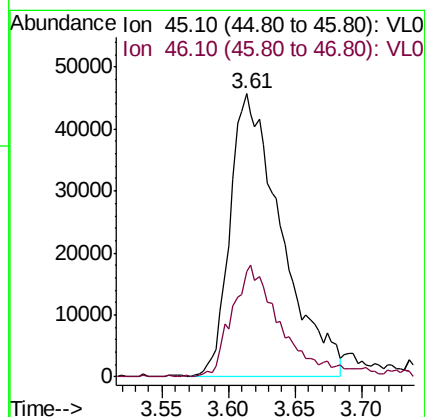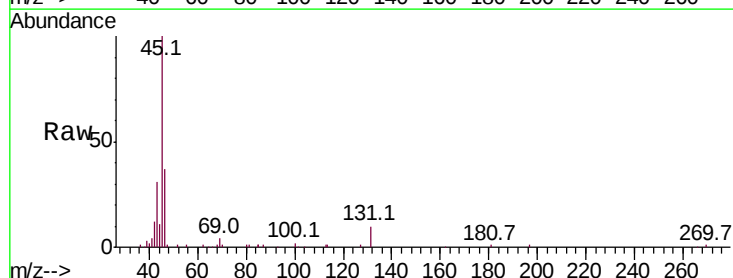

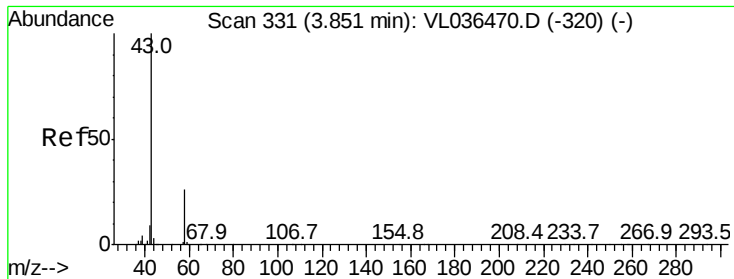

#15

Acetone

Concen: 9.672 ppbv

RT: 3.85 min Scan# 331

Delta R.T. -0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Instrument :

MSVOA_L

ClientSampleId :

FS-SV-04DUP

Tot Ion: 43 Resp: 1210585





Ion Ratio Lower Upper

43 100

58 25.3 21.2 31.8

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:54 AM

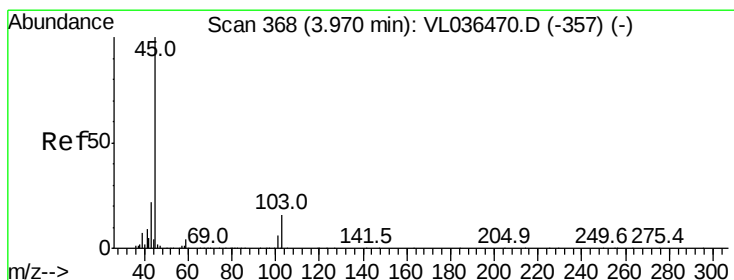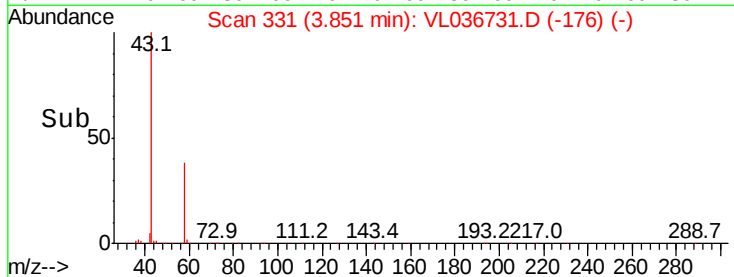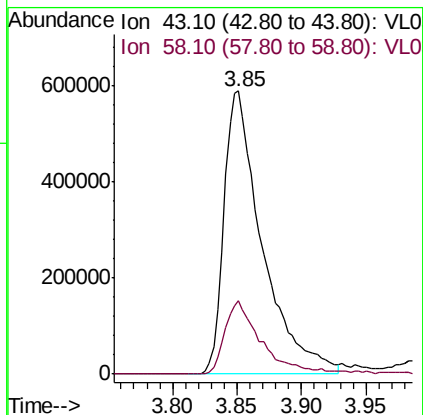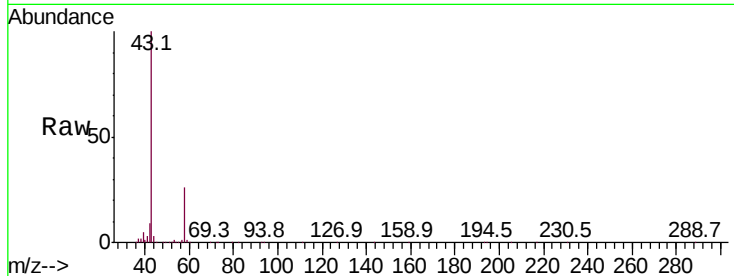

#19

Isopropyl Alcohol

Concen: 3.012 ppbv

RT: 3.99 min Scan# 374

Delta R.T. 0.02 min

Lab File: VL036731.D




Acq: 7 Apr 2021 18:04


Tgt Ion: 45 Resp: 207356

Ion Ratio Lower Upper

45 100

58 153.1 2.9 4.3#

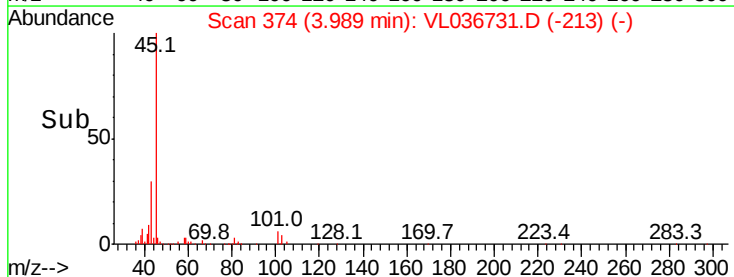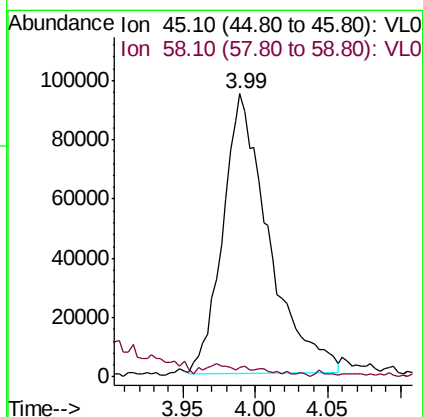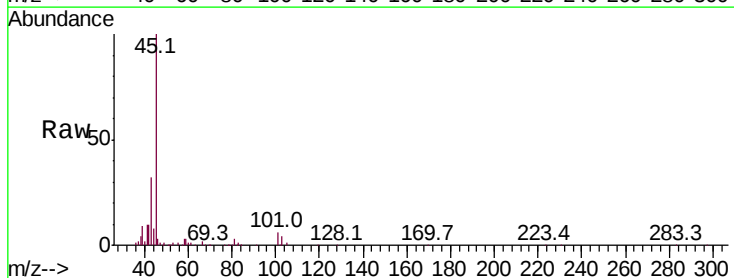

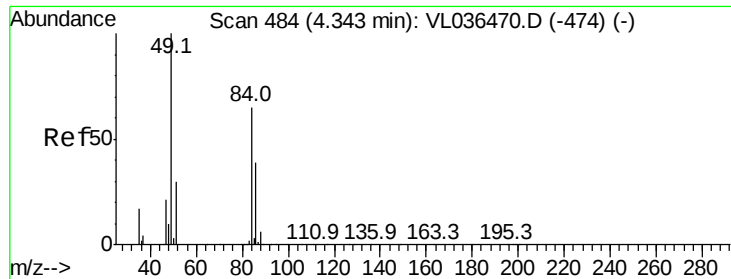





#20
Methylene Chloride
Concen: 15.410 ppbv
RT: 4.34 min Scan# 484
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Tot Ion	84	Resp	903044
Ion	Ratio	Lower	Upper
84	100		
49	164.6	122.9	184.3
51	49.6	36.9	55.3
86	62.9	48.2	72.4




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:54 AM

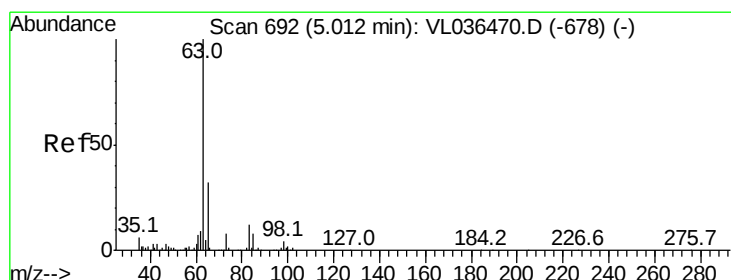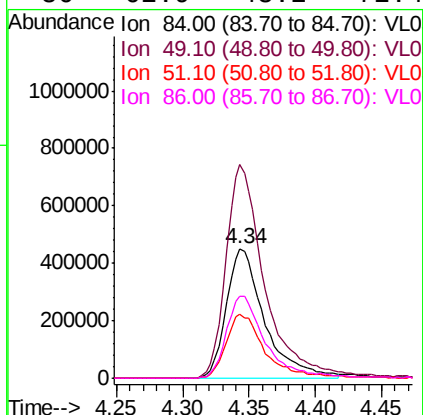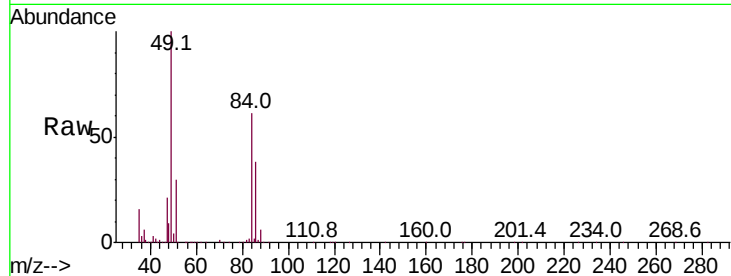

#24
1,1-Dichloroethane
Concen: 0.195 ppbv
RT: 5.01 min Scan# 692
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Tgt Ion	63	Resp	30483
Ion	Ratio	Lower	Upper
63	100		
98	6.6	2.1	6.2#
100	1.4	0.9	2.8

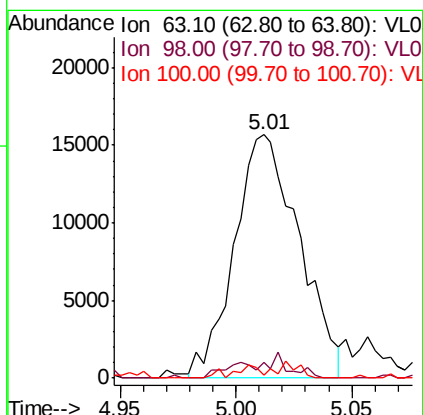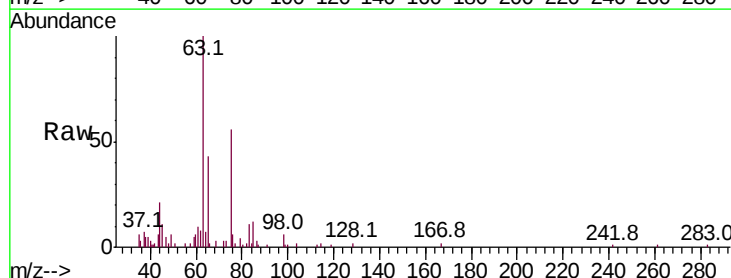

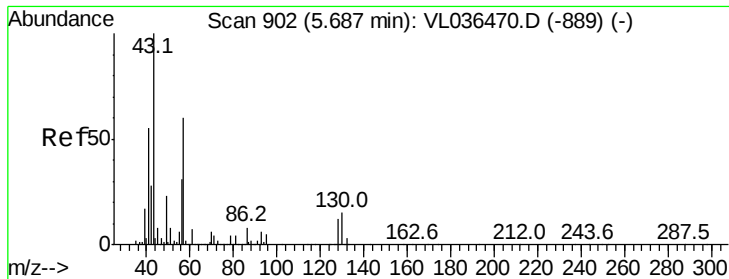





#26
Hexane
Concen: 4.731 ppbv
RT: 5.69 min Scan# 902
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Tot Ion	Ratio	Lower	Upper
57	100		
41	96.6	77.2	115.8
43	75.5	173.8	260.6#
56	55.7	43.8	65.6




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:54 AM

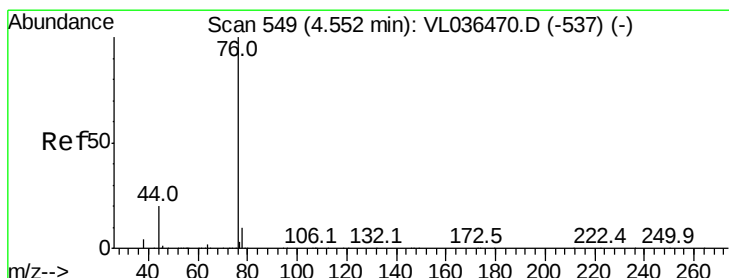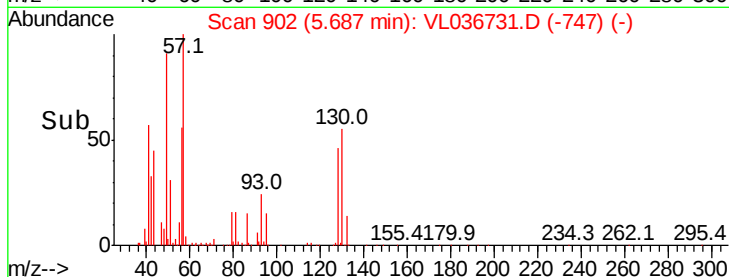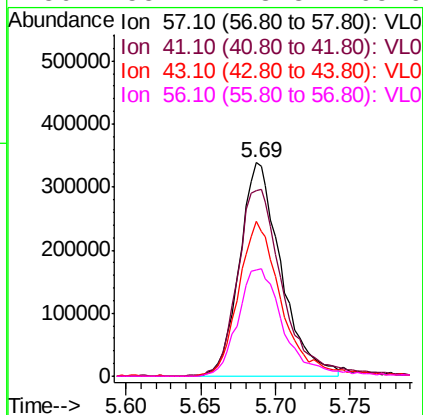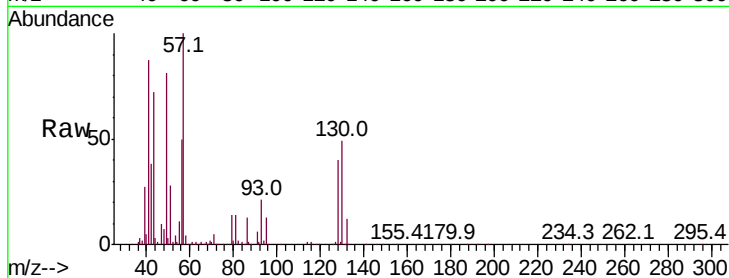

#27
Carbon Disulfide
Concen: 0.258 ppbv
RT: 4.55 min Scan# 548
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Tgt Ion	Ratio	Lower	Upper
76	100		
44	26.1	17.5	26.3
78	14.2	8.6	13.0#

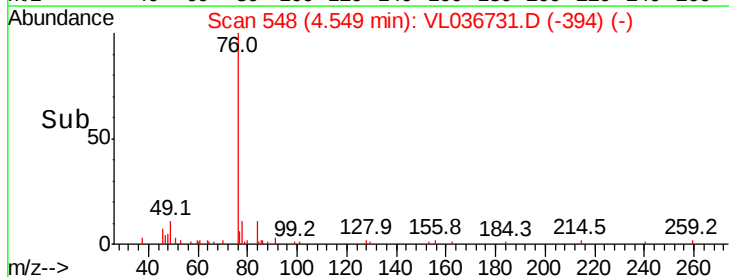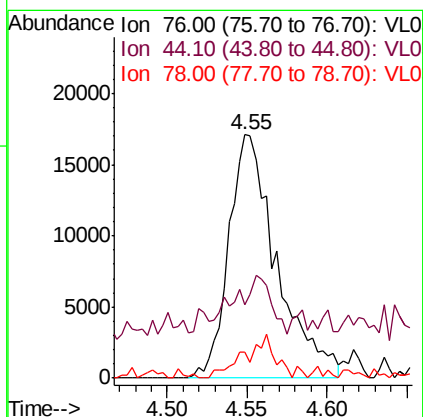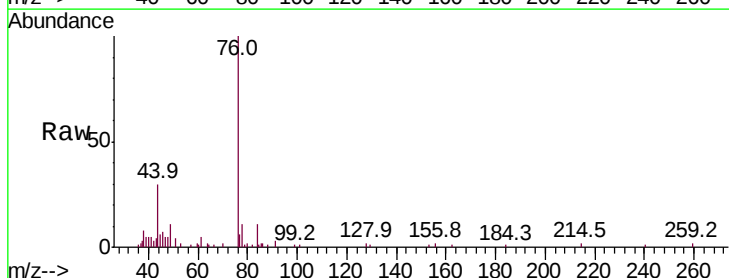

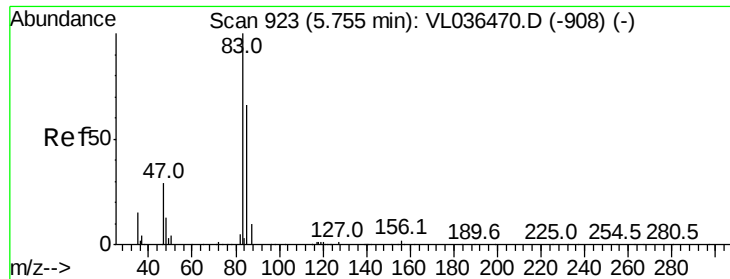





#29
Chloroform
Concen: 1.696 ppbv
RT: 5.75 min Scan# 923
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Tot Ion	83	Resp	374442
Ion Ratio	100	Lower	Upper
83	100		
85	61.4	52.6	78.8




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:54 AM

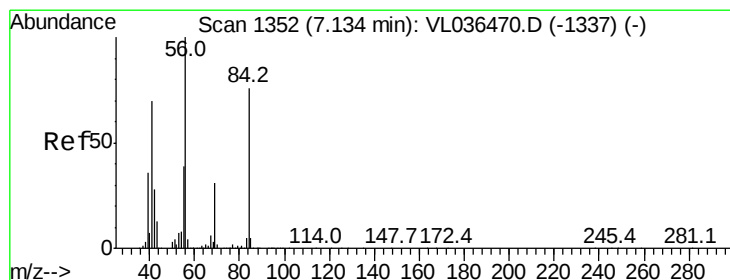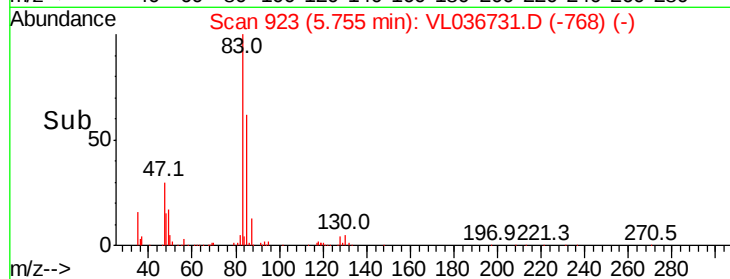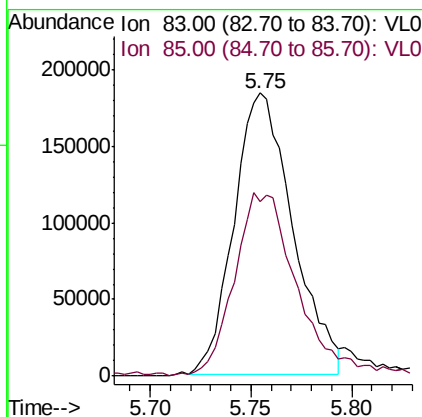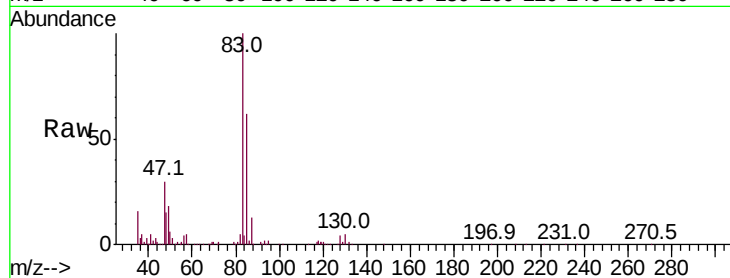

#30
Cyclohexane
Concen: 0.418 ppbv m
RT: 7.13 min Scan# 1351
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Tgt Ion	84	Resp	46797
Ion Ratio	100	Lower	Upper
84	100		
56	0.0	114.6	171.8#
41	0.0	75.3	112.9#

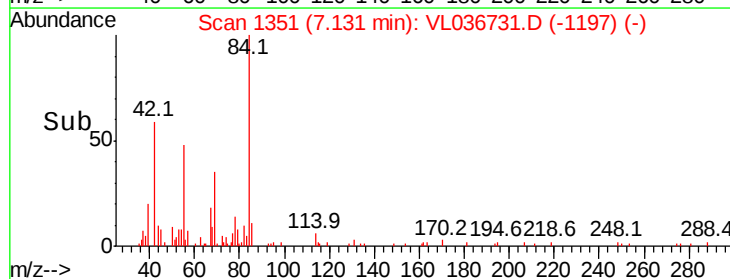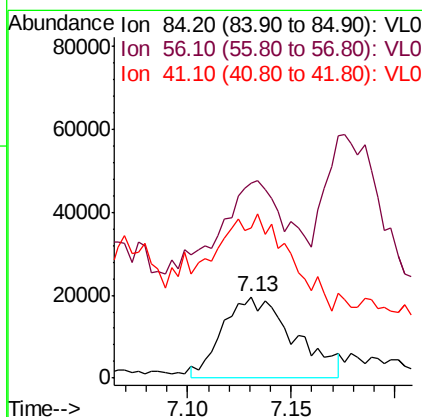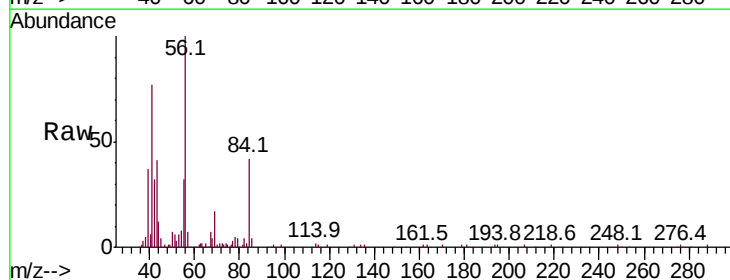

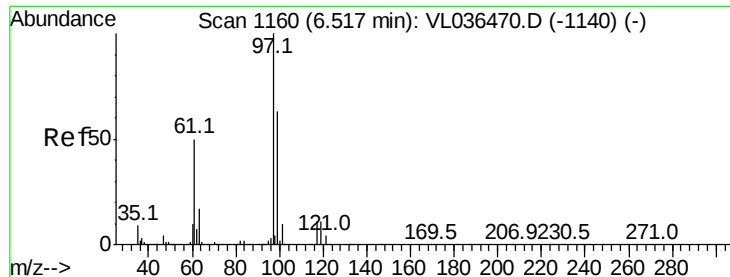

#32

1,1,1-Trichloroethane

Concen: 0.361 ppbv

RT: 6.52 min Scan# 1160

Delta R.T. -0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Instrument :

MSVOA_L





ClientSampleId :

FS-SV-04DUP

Tot Ion:	97	Resp:	80293
Ion	Ratio	Lower	Upper
97	100		
99	74.9	51.4	77.0
61	45.7	40.6	60.8

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:54 AM

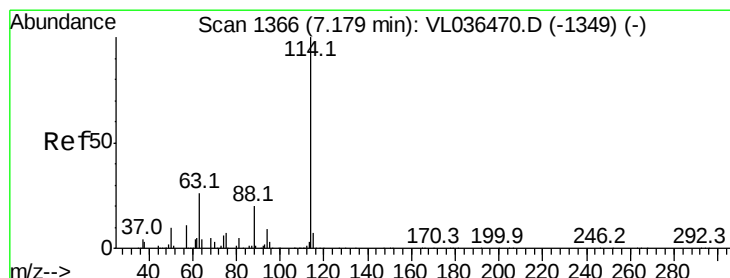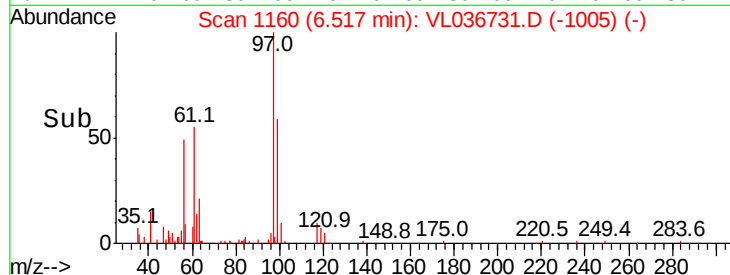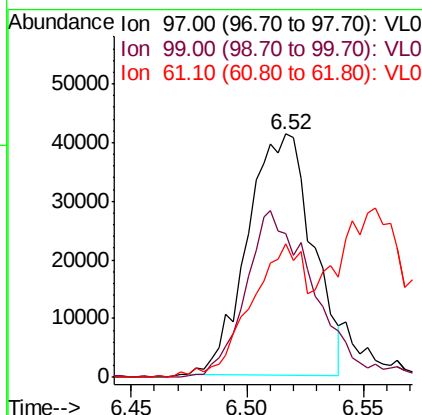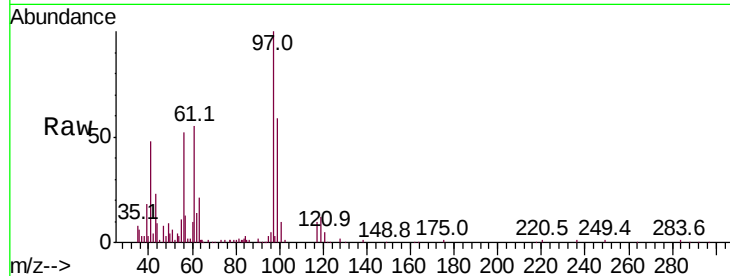

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv




RT: 7.18 min Scan# 1366


Delta R.T. -0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Tgt Ion:	114	Resp:	3227501
Ion	Ratio	Lower	Upper
114	100		
63	26.2	22.4	33.6
88	18.5	15.4	23.0

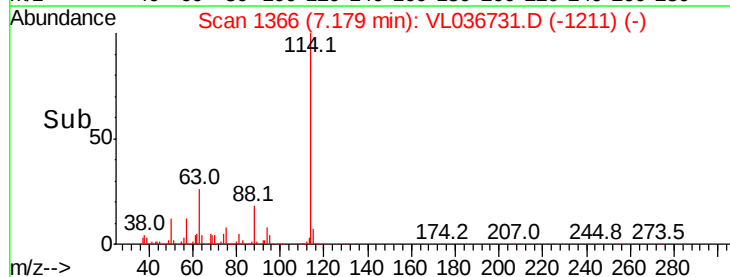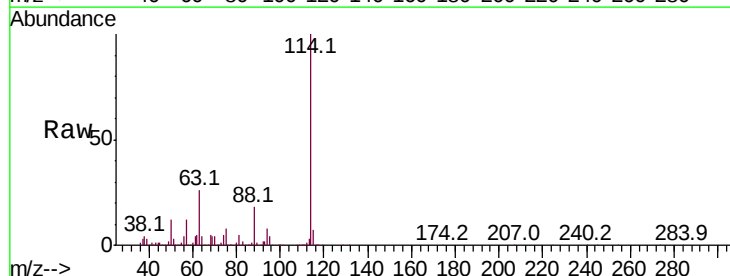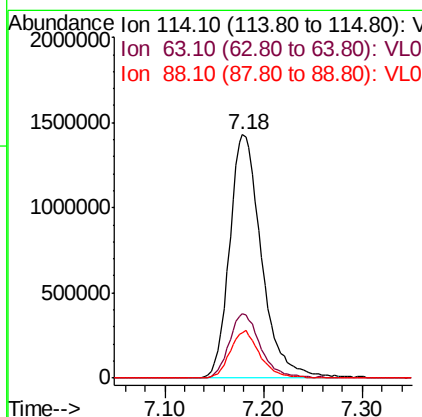

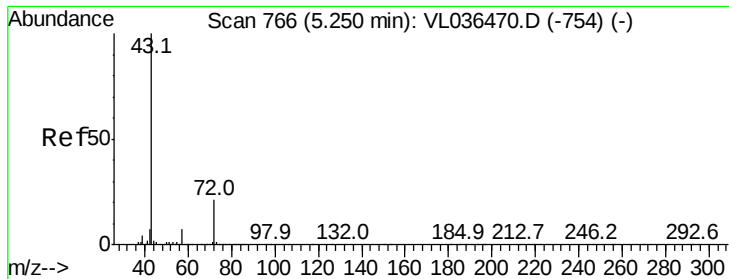

#34

2-Butanone

Concen: 1.093 ppbv

RT: 5.26 min Scan# 768

Delta R.T. 0.01 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Instrument :

MSVOA_L

ClientSampleId :

FS-SV-04DUP

Tot Ion: 43 Resp: 172142

Ion Ratio Lower Upper

43 100


72 32.3 17.0 25.6#

Manual Integrations

APPROVED

MMDadoda

4/12/2021 11:15:54 AM

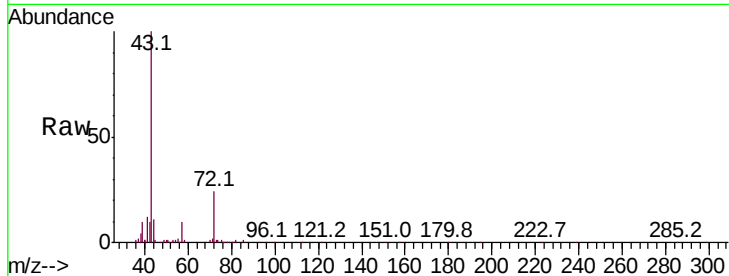

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 72.10 (71.80 to 72.80): VL0

150000



100000

50000

0

5.20 5.25 5.30

Time-->

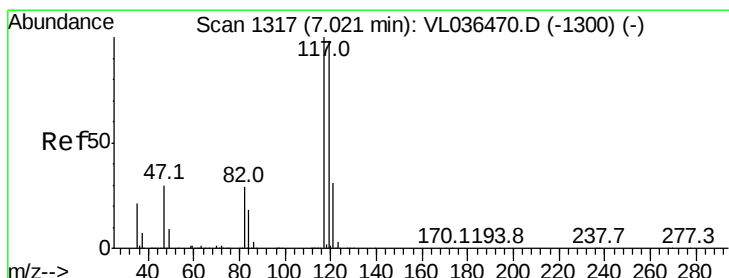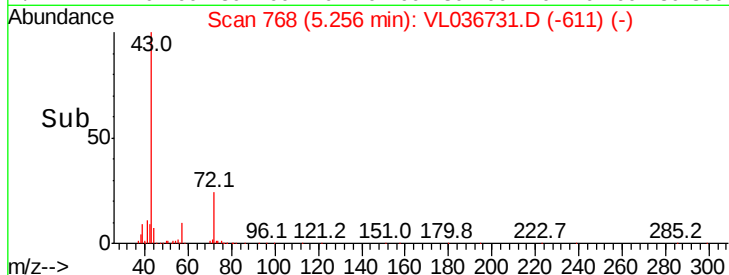

#35

Carbon Tetrachloride

Concen: 0.042 ppbv m

RT: 7.02 min Scan# 1318

Delta R.T. 0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04


Tgt Ion: 117 Resp: 10297

Ion Ratio Lower Upper

117 100

119 93.7 78.2 117.2

121 54.3 24.5 36.7#

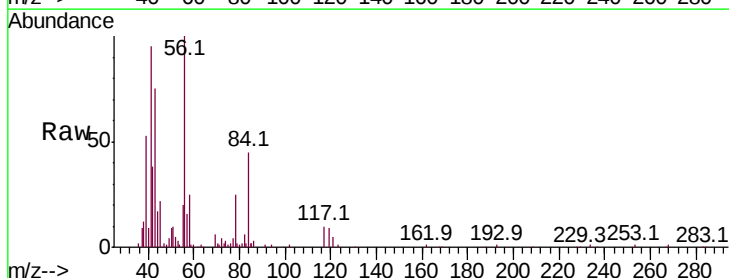

Abundance Ion 117.00 (116.70 to 117.70): V

Ion 119.00 (118.70 to 119.70): V

Ion 121.00 (120.70 to 121.70): V

6000

5000

4000

3000


2000


1000

0

6.95 7.00 7.05 7.10

Time-->

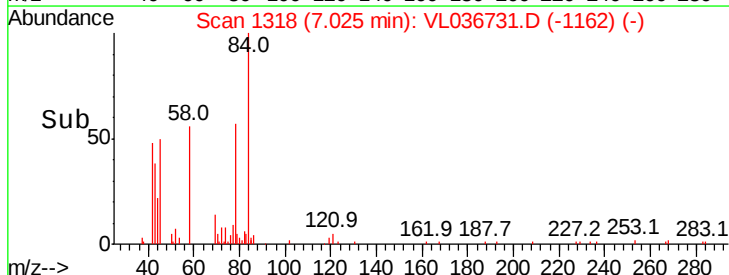

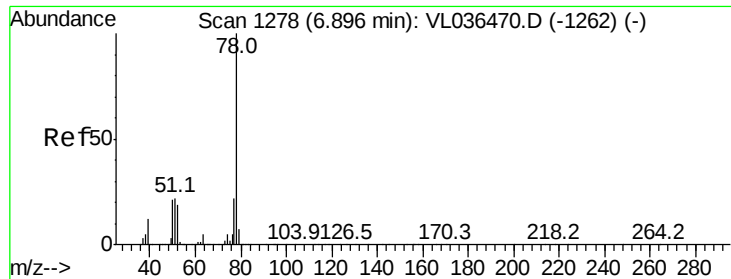





#36
Benzene
Concen: 23.582 ppbv
RT: 6.89 min Scan# 1277
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Tot Ion	Ratio	Lower	Upper
78	100		
77	24.5	18.0	27.0
50	22.6	16.5	24.7




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:54 AM

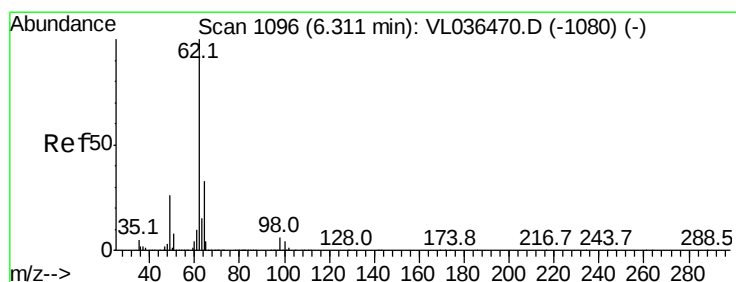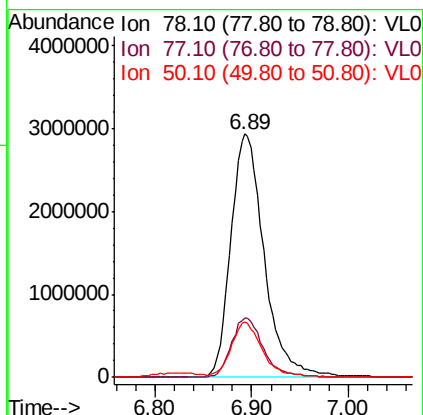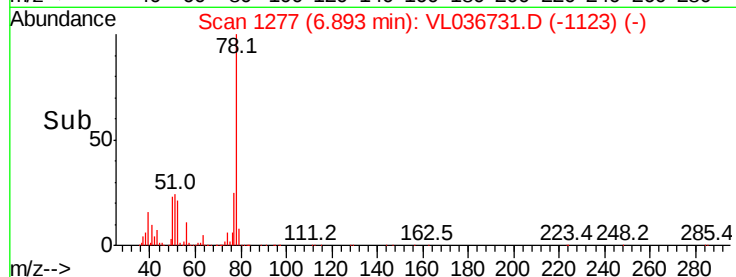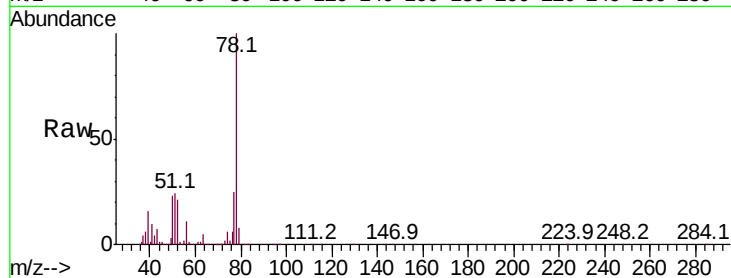

#37
1,2-Dichloroethane
Concen: 0.289 ppbv
RT: 6.31 min Scan# 1097
Delta R.T. 0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Tgt Ion	Ratio	Lower	Upper
62	100		
98	7.8	4.9	7.3#

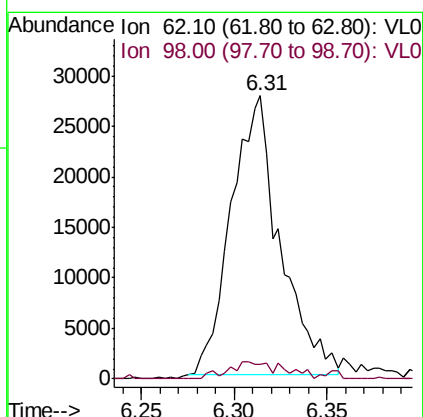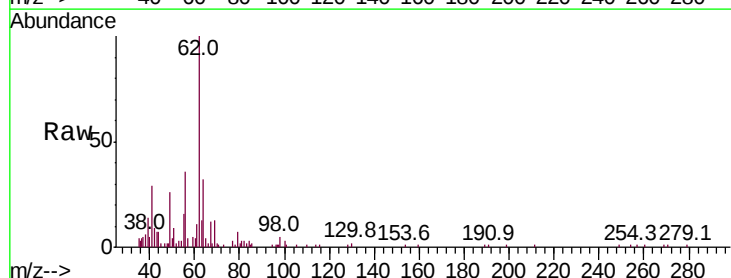

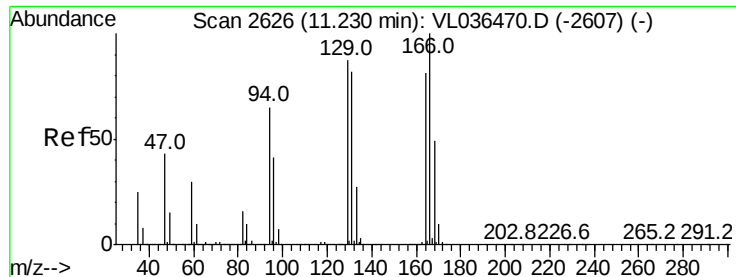

#52

Tetrachloroethene

Concen: 21.707 ppbv

RT: 11.23 min Scan# 2626

Delta R.T. -0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Instrument :

MSVOA_L

ClientSampleId :

FS-SV-04DUP

Tot Ion:164 Resp: 2379331

Ion Ratio Lower Upper

164 100

166 127.1 98.3 147.5


129 105.3 85.8 128.8

131 103.6 80.9 121.3




Manual Integrations
APPROVED

MMDadoda

4/12/2021 11:15:54 AM

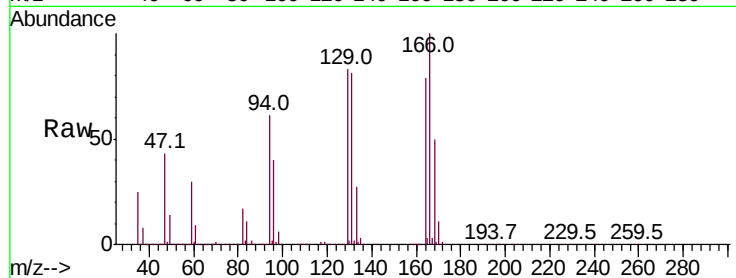

Abundance Ion 163.90 (163.60 to 164.60): V
2000000 Ion 165.90 (165.60 to 166.60): V
Ion 129.00 (128.70 to 129.70): V
Ion 131.00 (130.70 to 131.70): V

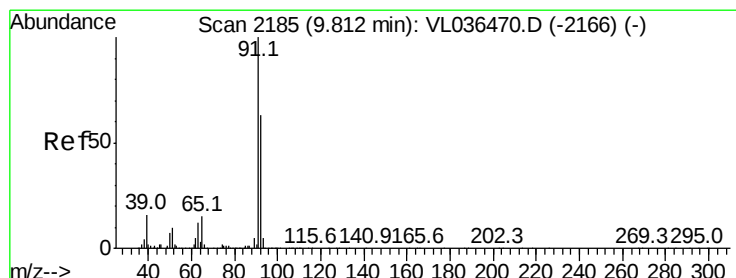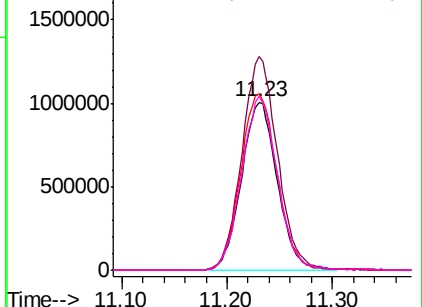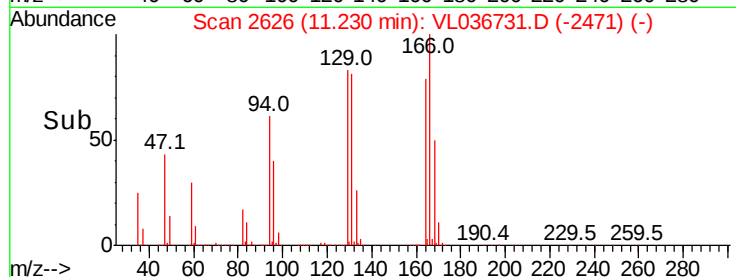

#53

Toluene

Concen: 9.419 ppbv

RT: 9.81 min Scan# 2184

Delta R.T. -0.00 min

Lab File: VL036731.D


Acq: 7 Apr 2021 18:04

Tgt Ion: 91 Resp: 2985818



Ion Ratio Lower Upper


91 100

92 61.8 48.8 73.2

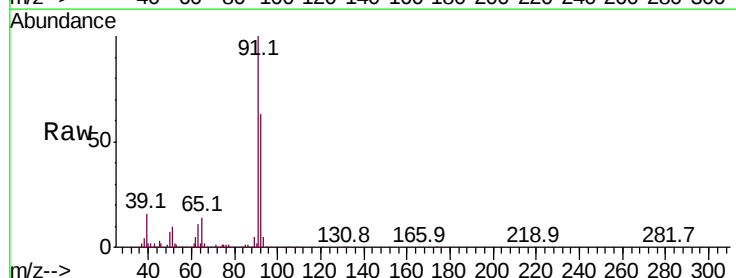

Abundance Ion 91.10 (90.80 to 91.80): VL0
1500000 Ion 92.10 (91.80 to 92.80): VL0

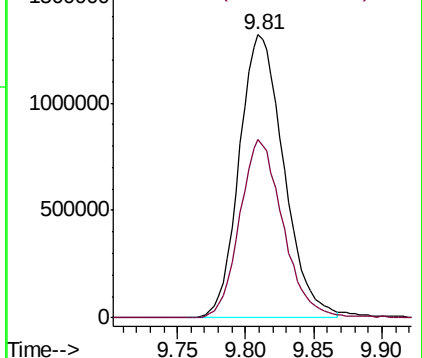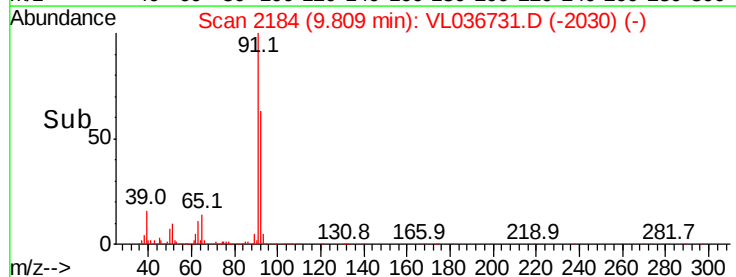

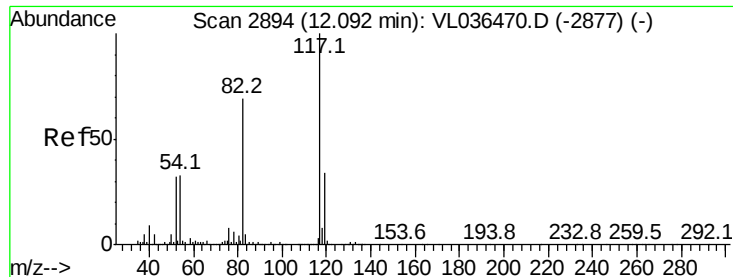





#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.09 min Scan# 2894
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Tot Ion	Ratio	Lower	Upper
117	100		
82	68.3	57.4	86.0
119	32.8	47.4	71.0#




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:54 AM

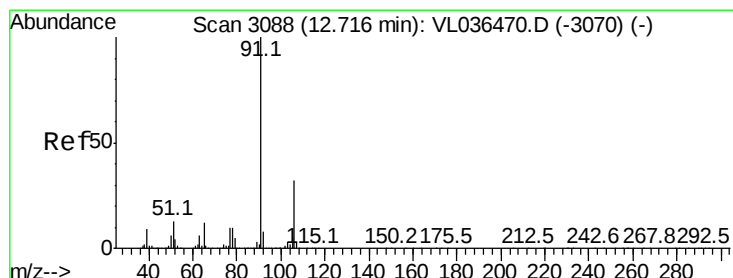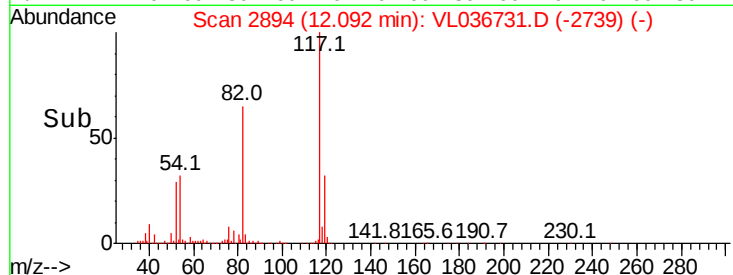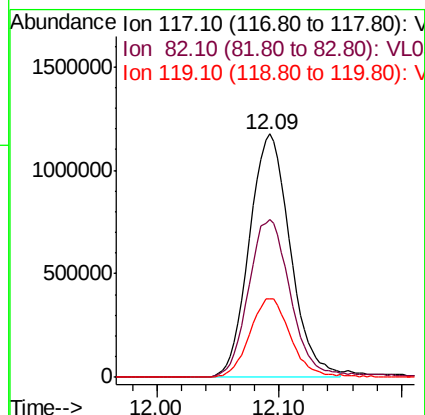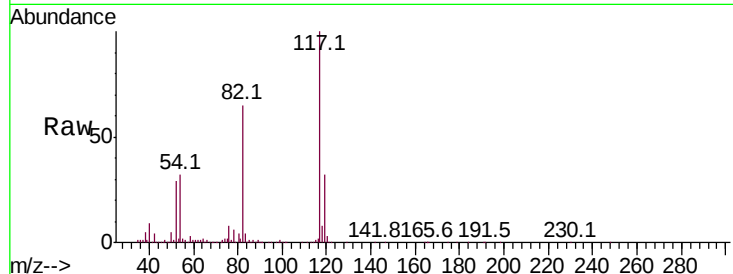

#58
Ethyl Benzene
Concen: 5.159 ppbv
RT: 12.72 min Scan# 3088
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Tgt Ion	Ratio	Lower	Upper
91	100		
106	30.3	25.3	37.9

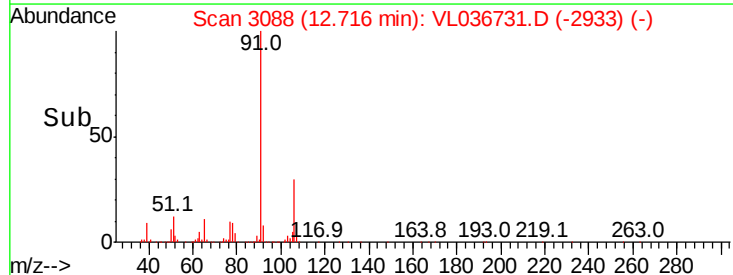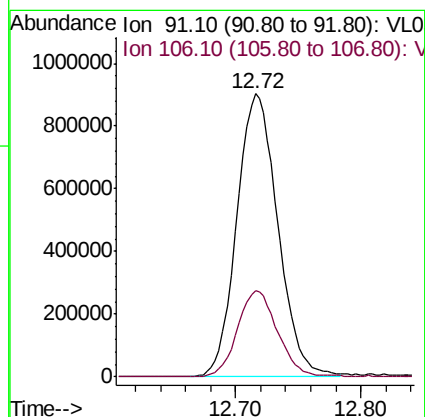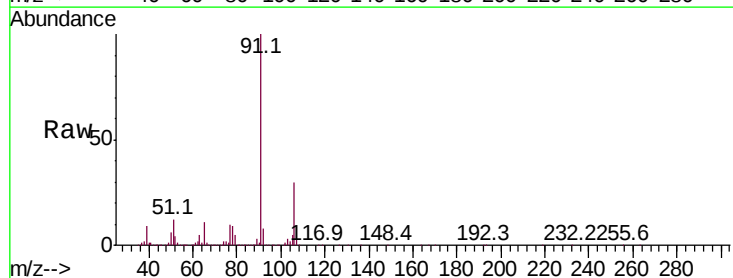







#59
m/p-Xylene
Concen: 7.757 ppbv
RT: 13.01 min Scan# 3178
Delta R.T. 0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Tot Ion: 91 Resp: 2687565
Ion Ratio Lower Upper
91 100
106 46.8 35.3 52.9




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:54 AM

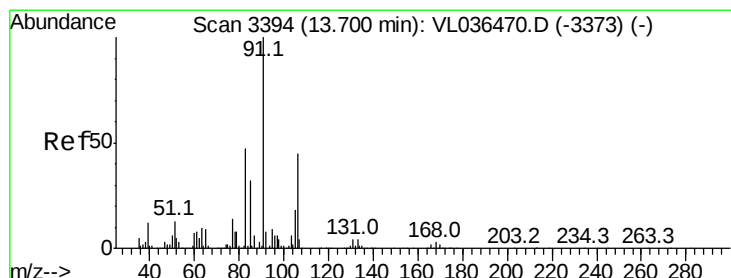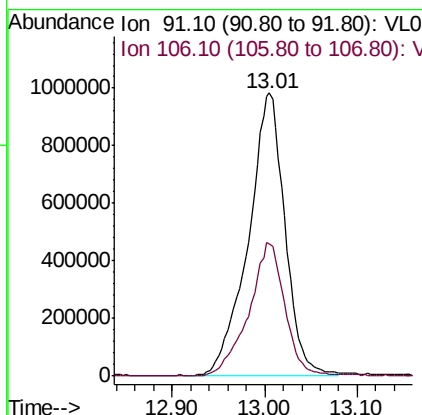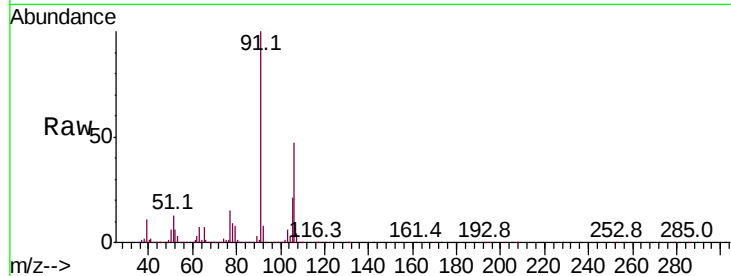

#60
o-Xylene
Concen: 3.906 ppbv
RT: 13.70 min Scan# 3393
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Tgt Ion: 91 Resp: 1308497
Ion Ratio Lower Upper
91 100
106 44.8 22.3 66.9

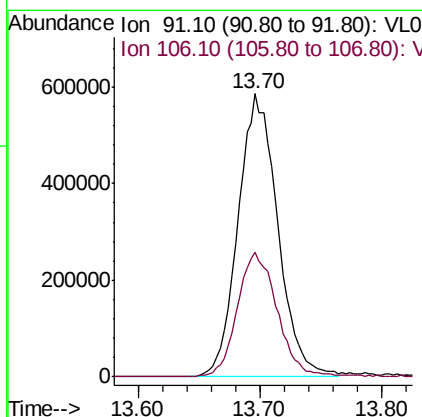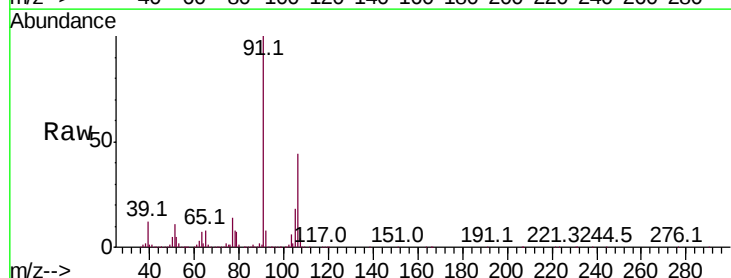







#61
Stvrene
Concen: 0.156 ppbv m
RT: 13.53 min Scan# 3342
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Instrument :
MSVOA_L
ClientSampleId :
FS-SV-04DUP

Tot Ion	Ratio	Lower	Upper
104	100		
78	66.6	43.8	65.8#
103	0.0	38.3	57.5#




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:15:54 AM

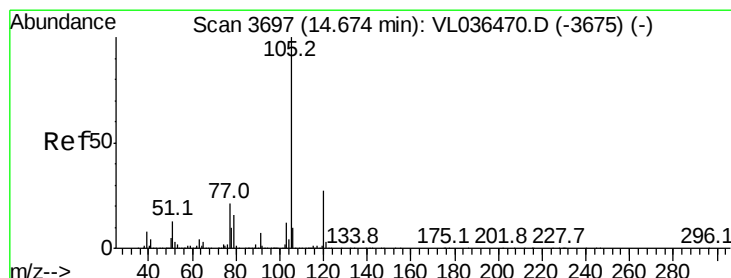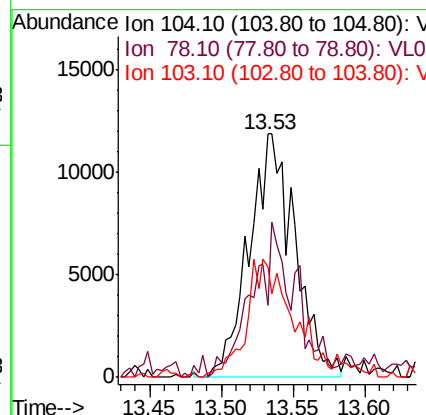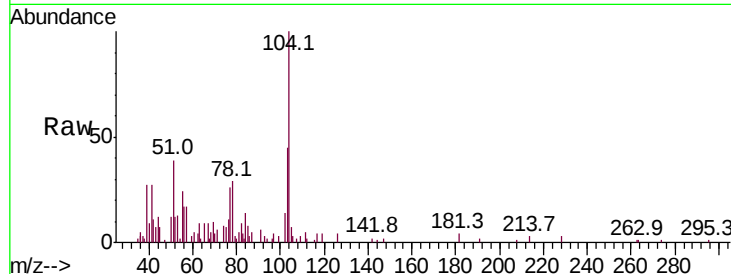

#62
Isopropylbenzene
Concen: 0.109 ppbv m
RT: 14.67 min Scan# 3697
Delta R.T. -0.00 min
Lab File: VL036731.D
Acq: 7 Apr 2021 18:04

Tgt Ion	Ratio	Lower	Upper
105	100		
120	26.7	20.6	31.0

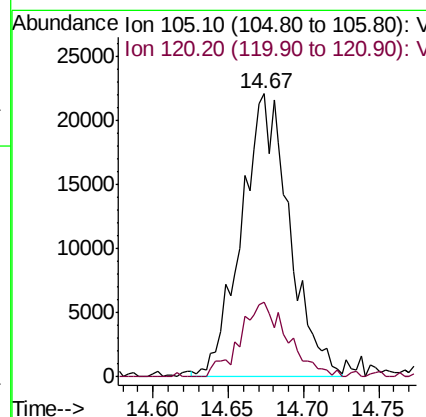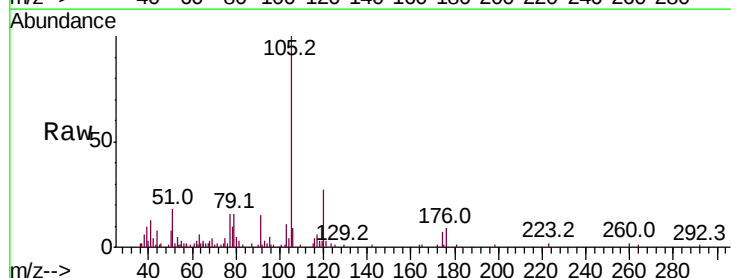

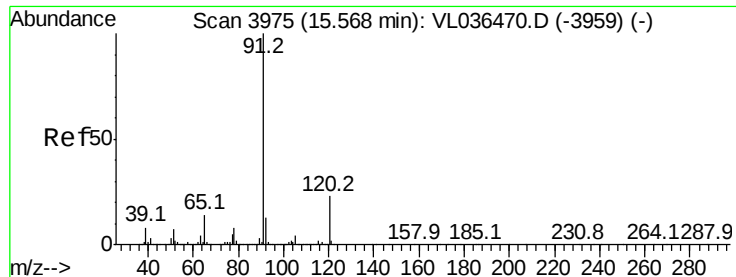

#64

n-propylbenzene

Concen: 0.308 ppbv m

RT: 15.57 min Scan# 3976

Delta R.T. 0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Instrument :

MSVOA_L

ClientSampleId :

FS-SV-04DUP

Tot Ion:120 Resp: 33930





Ion Ratio Lower Upper

120 100

91 484.2 377.4 566.2

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:54 AM

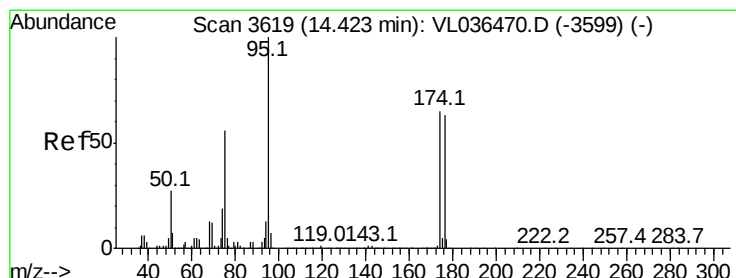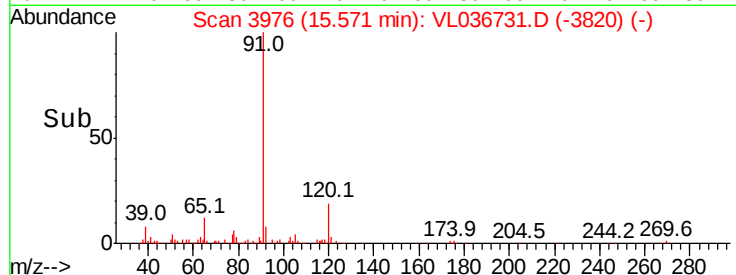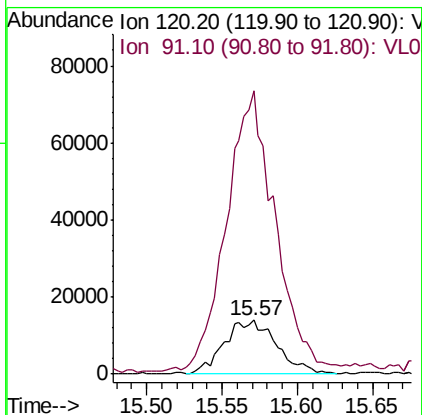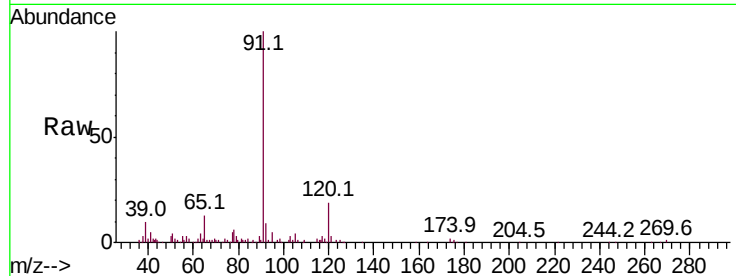

#68

1-Bromo-4-Fluorobenzene

Concen: 10.185 ppbv

RT: 14.42 min Scan# 3619

Delta R.T. -0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04




Tgt Ion: 95 Resp: 2216281


Ion Ratio Lower Upper

95 100

174 64.5 51.0 76.6

175 5.1 3.9 5.9

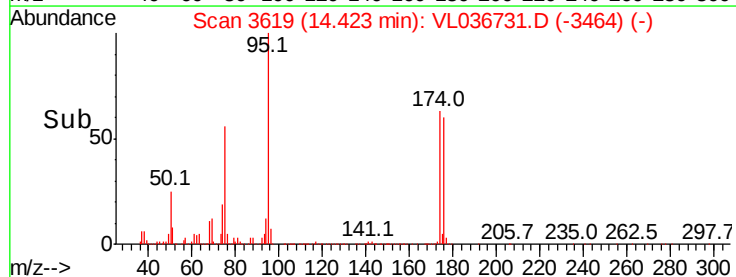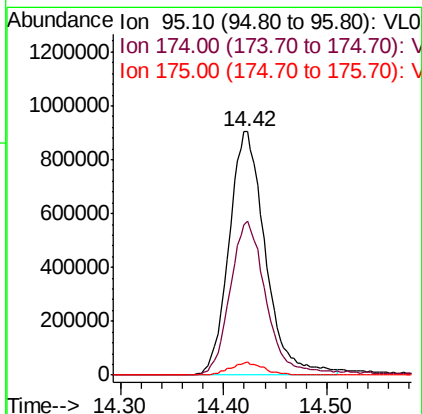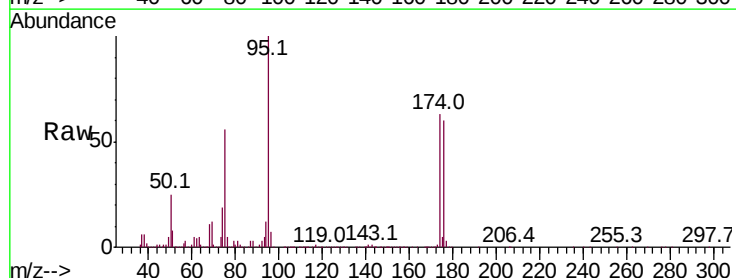

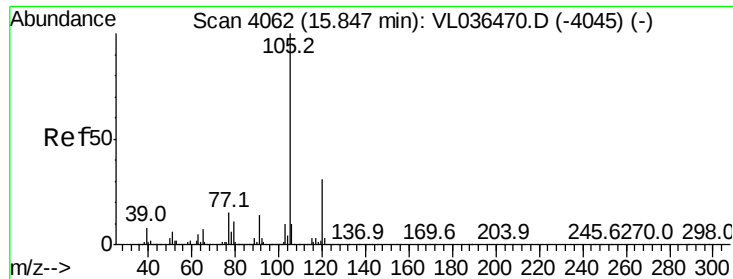

#72

4-Ethyltoluene

Concen: 0.757 ppbv

RT: 15.84 min Scan# 4061

Delta R.T. -0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Instrument :

MSVOA_L





ClientSampleId :

FS-SV-04DUP

Tot Ion	Ratio	Resp	Lower	Upper
105	100	277830		
120	29.5		24.0	36.0
91	15.2		11.0	16.4
77	13.9		11.7	17.5

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:54 AM

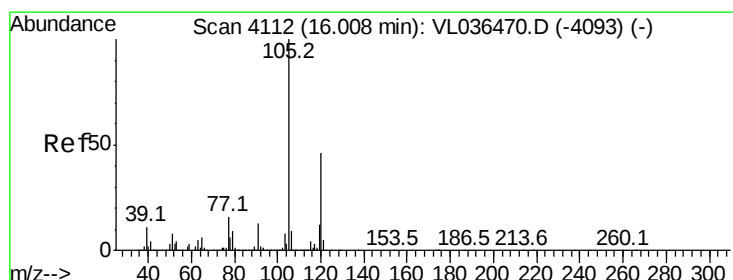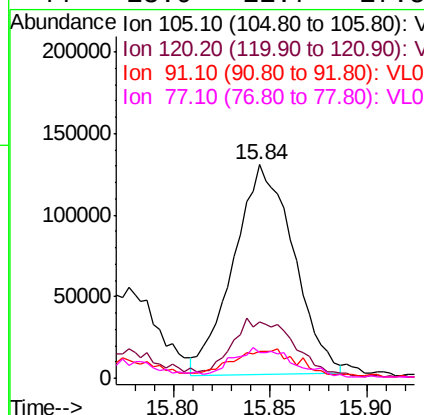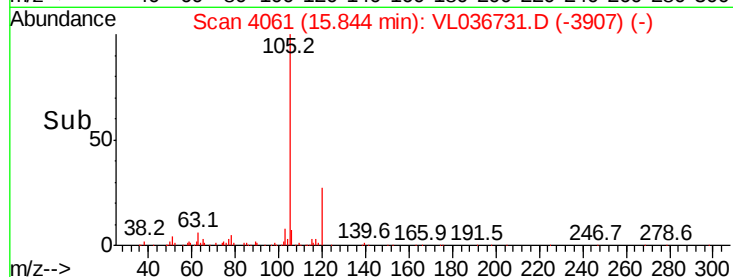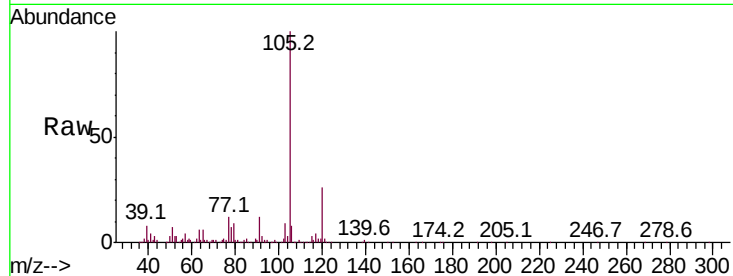

#73

1,3,5-Trimethylbenzene

Concen: 1.544 ppbv




RT: 16.00 min Scan# 4110


Delta R.T. -0.01 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Tgt Ion	Ratio	Resp	Lower	Upper
105	100	529103		
120	46.3		36.6	54.8

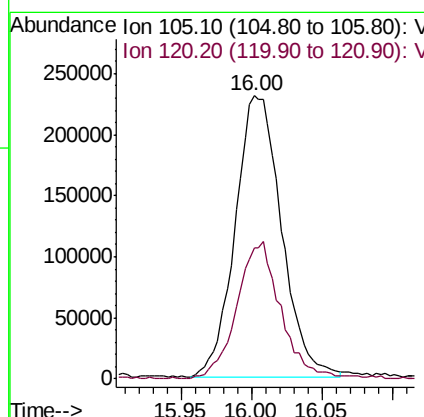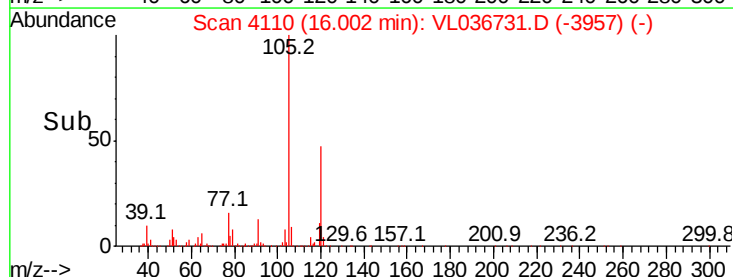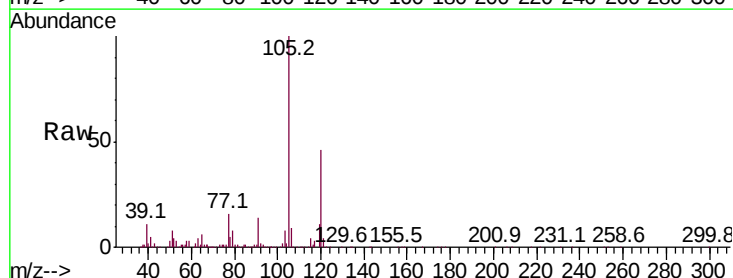

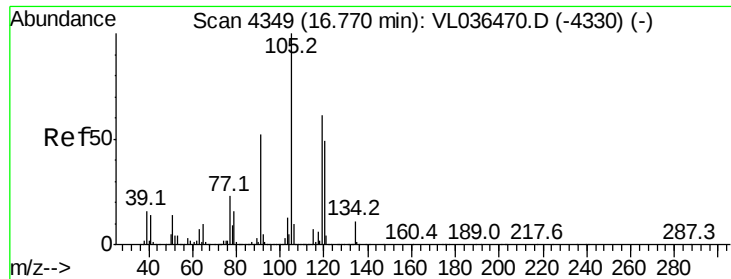

#74

1,2,4-Trimethylbenzene

Concen: 3.705 ppbv

RT: 16.77 min Scan# 4348

Delta R.T. -0.00 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Instrument :

MSVOA_L





ClientSampleId :

FS-SV-04DUP

Tot Ion	Ratio	Lower	Upper
105	100		
120	42.5	39.2	58.8
91	11.1	42.6	64.0#
77	16.8	18.6	28.0#

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:15:54 AM

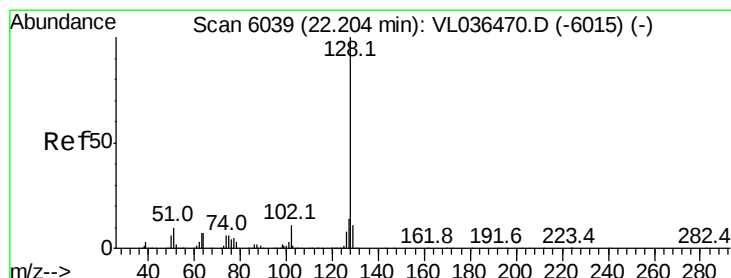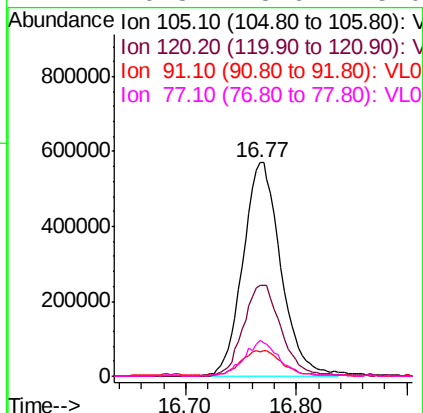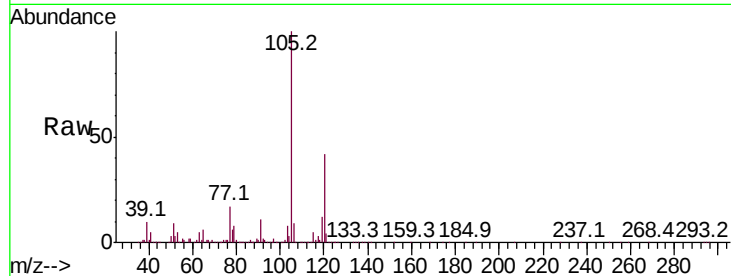

#79

Naphthalene

Concen: 2.184 ppbv

RT: 22.21 min Scan# 6041

Delta R.T. 0.01 min

Lab File: VL036731.D

Acq: 7 Apr 2021 18:04

Tgt Ion	Ratio	Lower	Upper
128	100		
127	10.4	10.9	16.3#
129	10.5	9.0	13.4

