

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL040721\
 Data File : VL036741.D
 Acq On : 8 Apr 2021 00:40
 Operator : SY/AP
 Sample : M1929-09
 Misc : 400mL/MSVOA L
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 FS-IA-03

Manual Integrations
 APPROVED

MMDadoda
 4/12/2021 11:16:36 AM

Quant Time: Apr 08 04:47:08 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Apr 08 2021
 QLast Update : Thu Apr 08 01:58:43 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.66	49	1277394	10.00	ppbv	-0.01
33) 1,4-Difluorobenzene	7.17	114	3038542	10.00	ppbv	-0.01
55) Chlorobenzene-d5	12.08	117	2727323	10.00	ppbv	-0.01

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.41	95	2112172	9.72	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.20%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.04	85	50332m	0.242	ppbv	
3) Chlorodifluoromethane	2.98	51	55897m	0.234	ppbv	
4) Chloromethane	3.13	50	35715	0.424	ppbv	100
9) Propene	3.01	41	151418	1.990	ppbv	87
10) Heptane	8.11	43	51616m	0.266	ppbv	
11) Trichlorofluoromethane	3.95	101	39900	0.188	ppbv	95
13) Ethanol	3.61	45	207442	22.895	ppbv	93
15) Acetone	3.84	43	1442896	11.477	ppbv	93
17) tert-Butyl alcohol	4.31	59	23203m	0.212	ppbv	
19) Isopropyl Alcohol	3.98	45	750099	10.846	ppbv #	97
20) Methylene Chloride	4.34	84	500484	8.502	ppbv	94
26) Hexane	5.68	57	390899	2.818	ppbv #	47
29) Chloroform	5.74	83	22163m	0.100	ppbv	
30) Cyclohexane	7.12	84	30079m	0.267	ppbv	
32) 1,1,1-Trichloroethane	6.50	97	25888m	0.116	ppbv	
34) 2-Butanone	5.24	43	180511	1.217	ppbv	95
35) Carbon Tetrachloride	7.01	117	12246m	0.052	ppbv	
36) Benzene	6.88	78	194898m	0.695	ppbv	
37) 1,2-Dichloroethane	6.29	62	17079m	0.104	ppbv	
41) Tetrahydrofuran	6.06	42	26364m	0.386	ppbv	
44) 2,2,4-Trimethylpentane	7.86	57	157753m	0.320	ppbv	
50) 4-Methyl-2-Pentanone	8.75	43	38523m	0.179	ppbv	
52) Tetrachloroethene	11.21	164	45651m	0.442	ppbv	
53) Toluene	9.80	91	2999774	10.052	ppbv	100
58) Ethyl Benzene	12.71	91	144589	0.364	ppbv	94
59) m/p-Xylene	12.96	91	549795	1.589	ppbv	94
60) o-Xylene	13.68	91	253175m	0.757	ppbv	
72) 4-Ethyltoluene	15.84	105	57264m	0.156	ppbv	
73) 1,3,5-Trimethylbenzene	15.99	105	61332m	0.179	ppbv	
74) 1,2,4-Trimethylbenzene	16.77	105	164434	0.449	ppbv #	65
79) Naphthalene	22.21	128	45645m	0.214	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL040721\
Data File : VL036741.D
Acq On : 8 Apr 2021 00:40
Operator : SY/AP
Sample : M1929-09
Misc : 400mL/MSVOA L
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
FS-IA-03

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:16:36 AM

Quant Time: Apr 08 04:47:08 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Apr
QLast Update : Thu Apr 08 01:58:43 2021
Response via : Initial Calibration

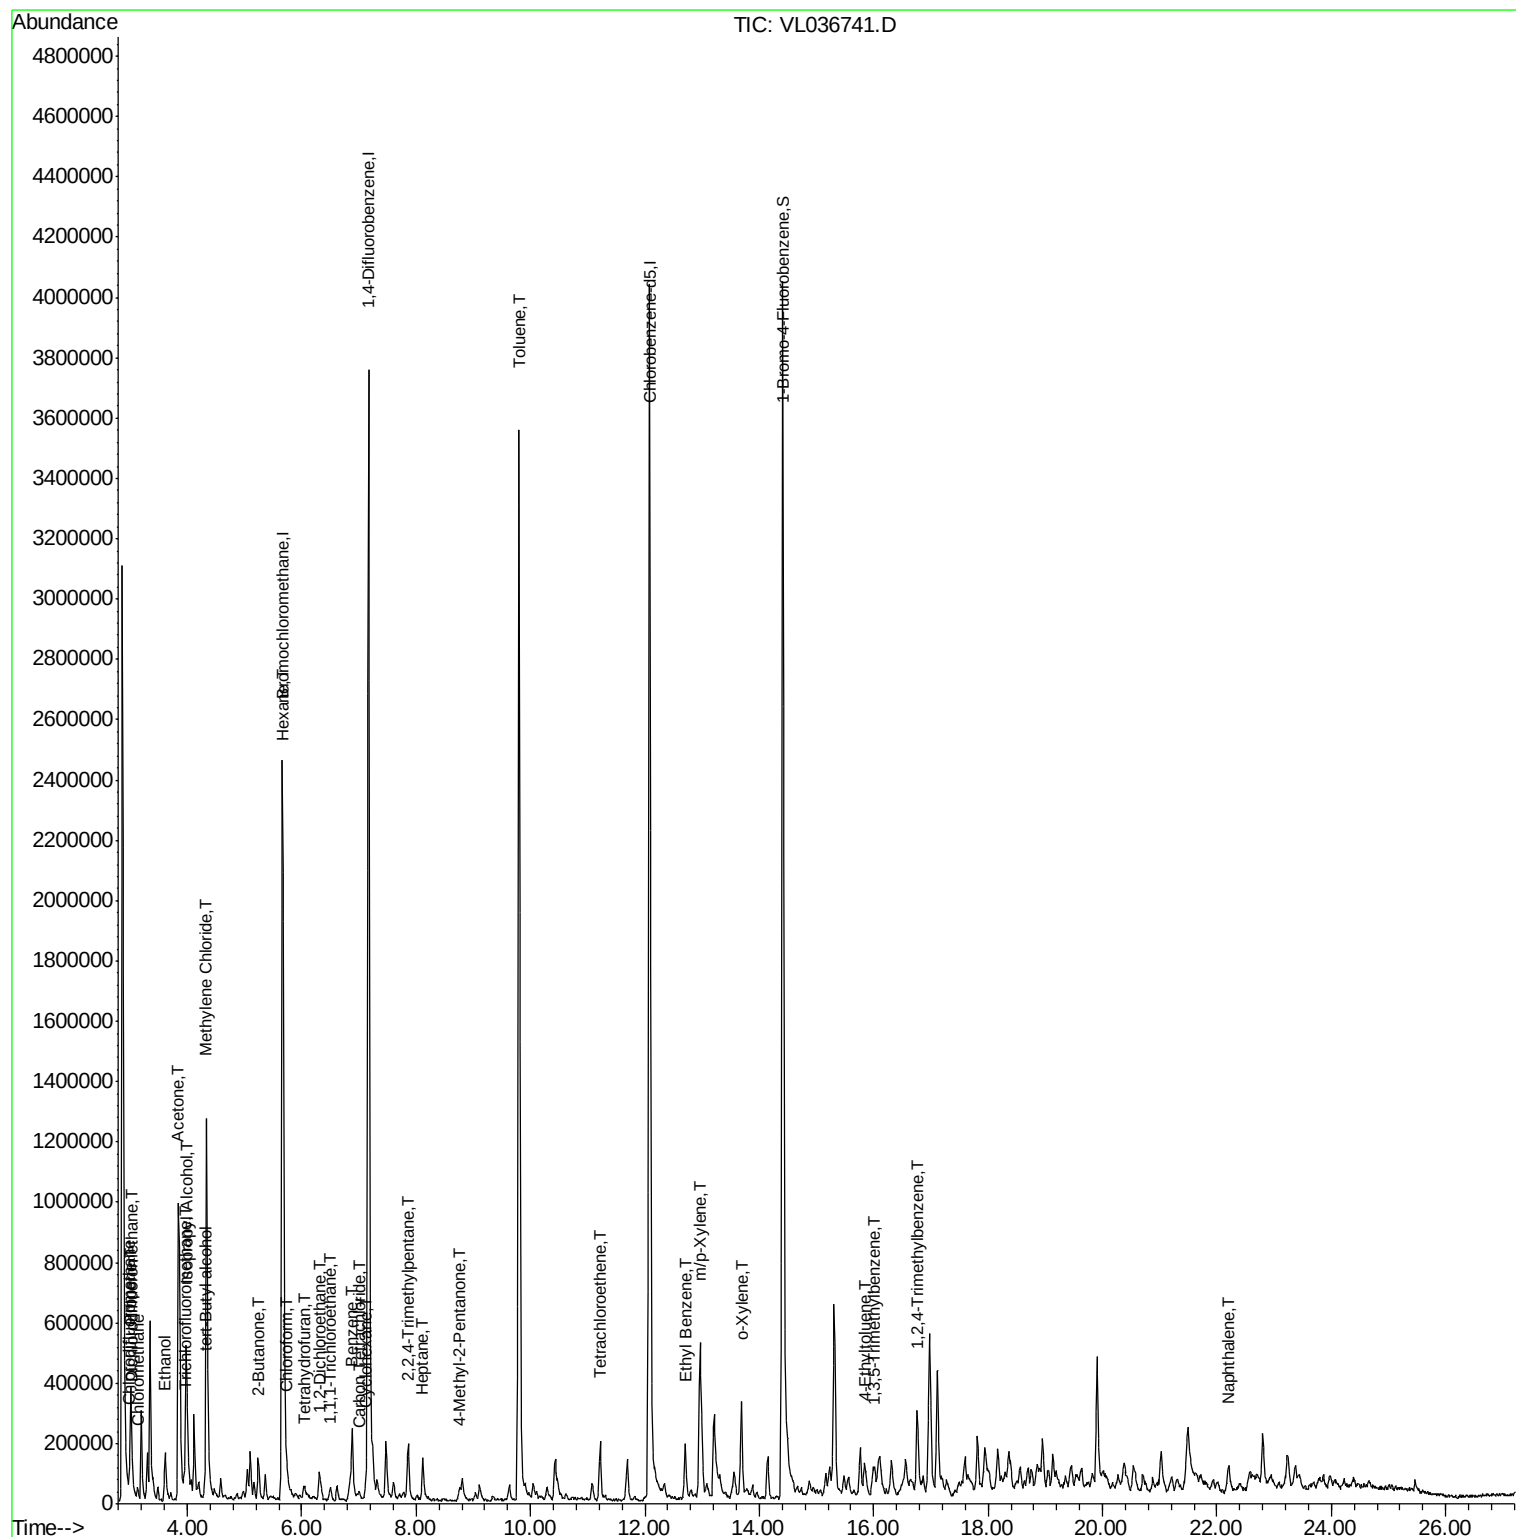

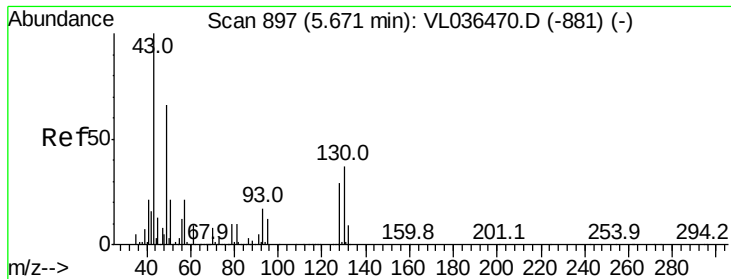

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.66 min Scan# 893

Delta R.T. -0.01 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Instrument :

MSVOA_L





ClientSampled :

FS-IA-03

Tot Ion:	49	Resp:	1277394
Ion	Ratio	Lower	Upper
49	100		
128	45.2	23.5	70.6
130	59.7	29.1	87.4

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:16:36 AM

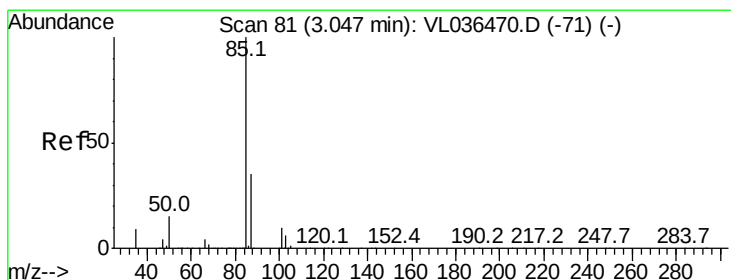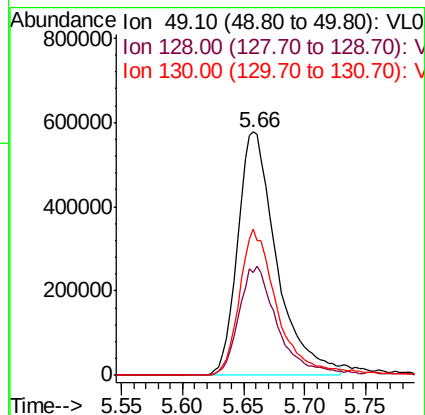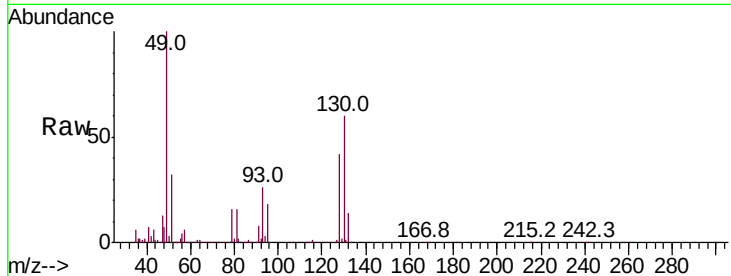

#2

Dichlorodifluoromethane

Concen: 0.242 ppbv m




RT: 3.04 min Scan# 78


Delta R.T. -0.01 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Tgt Ion:	85	Resp:	50332
Ion	Ratio	Lower	Upper
85	100		
87	21.9	27.8	41.8#

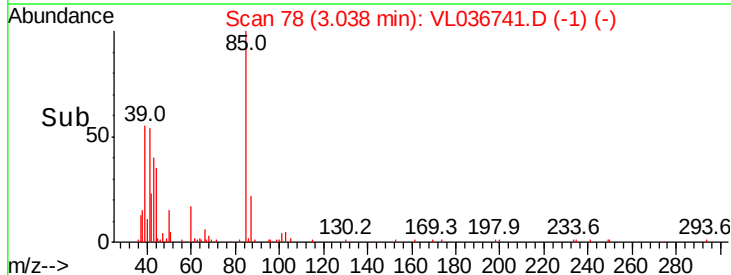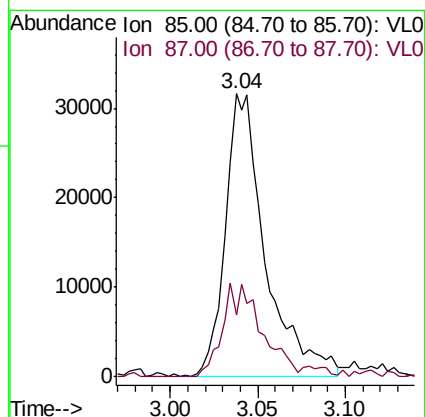

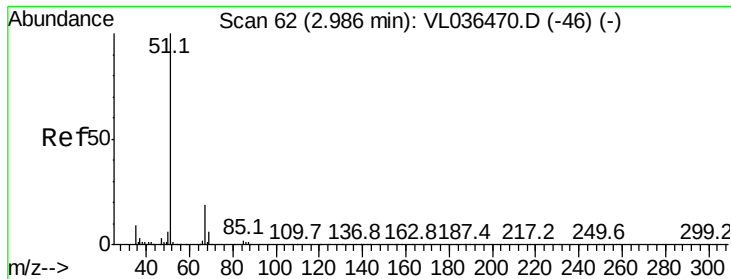

#3

Chlorodifluoromethane

Concen: 0.234 ppbv

RT: 2.98 min Scan# 60

Delta R.T. -0.01 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Instrument :

MSVOA_L

ClientSampleId :

FS-IA-03

Tot Ion: 51 Resp: 55897

Ion Ratio Lower Upper

51 100





67 18.4 14.7 22.1

Manual Integrations

APPROVED

MMDadoda

4/12/2021 11:16:36 AM

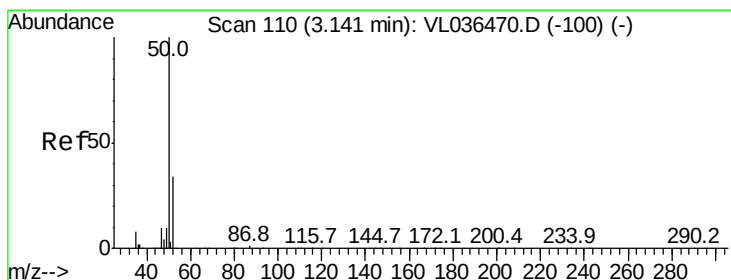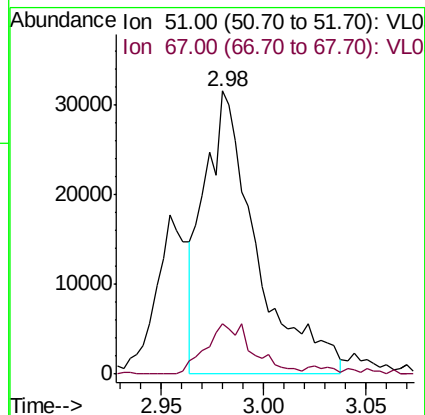

#4

Chloromethane

Concen: 0.424 ppbv

RT: 3.13 min Scan# 108

Delta R.T. -0.01 min

Lab File: VL036741.D




Acq: 8 Apr 2021 00:40


Tgt Ion: 50 Resp: 35715

Ion Ratio Lower Upper

50 100

52 34.0 27.0 40.6

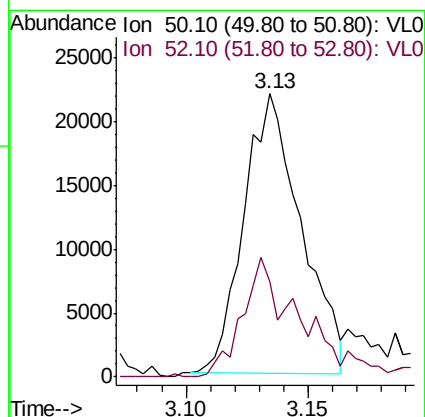

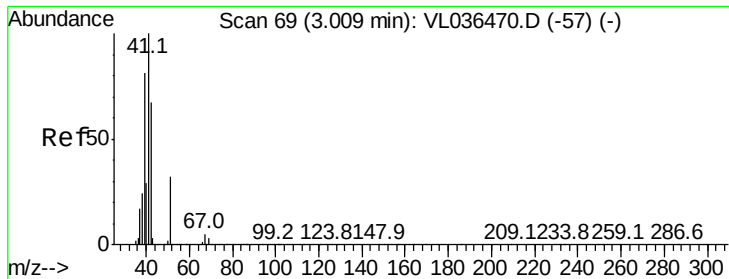

#9

Propene

Concen: 1.990 ppbv

RT: 3.01 min Scan# 68

Delta R.T. -0.00 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Instrument :

MSVOA_L

ClientSampleId :

FS-IA-03

Tot Ion: 41 Resp: 151418





Ion Ratio Lower Upper

41 100

42 60.1 57.0 85.4

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:16:36 AM

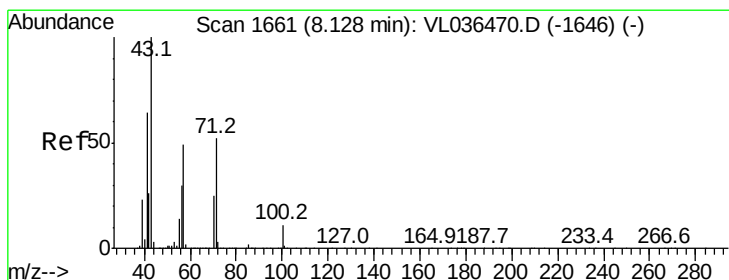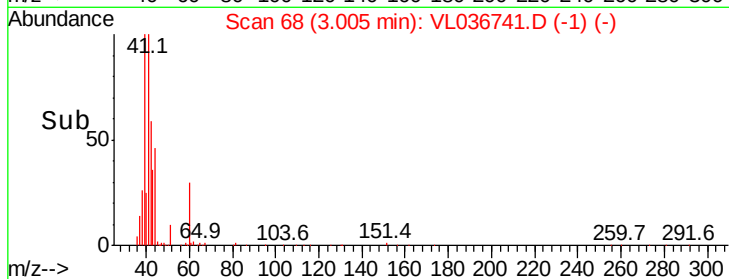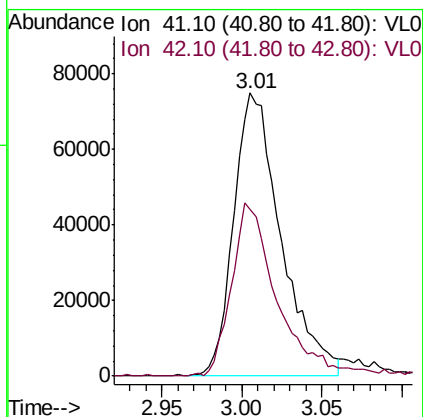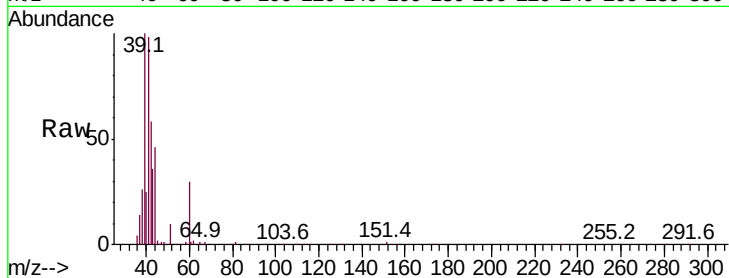

#10

Heptane

Concen: 0.266 ppbv m

RT: 8.11 min Scan# 1657

Delta R.T. -0.01 min

Lab File: VL036741.D




Acq: 8 Apr 2021 00:40


Tgt Ion: 43 Resp: 51616

Ion Ratio Lower Upper

43 100

57 52.4 39.0 58.6

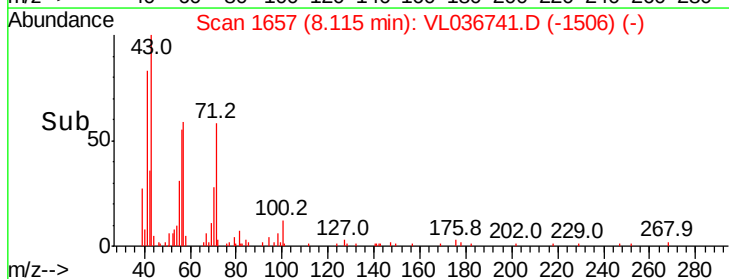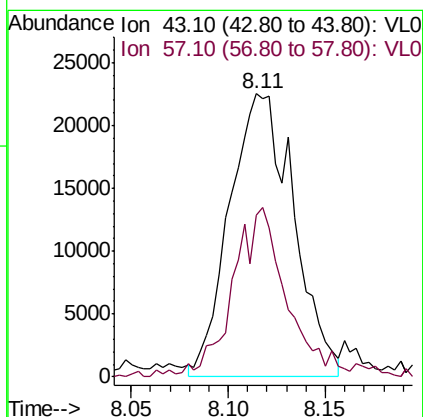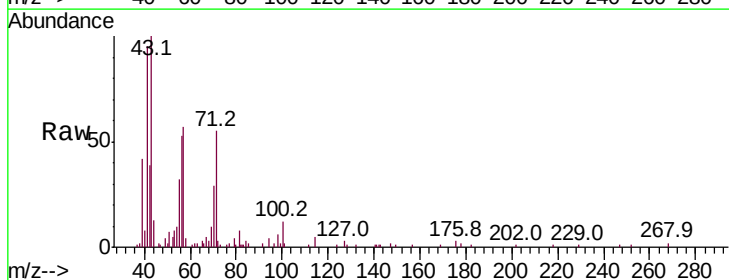

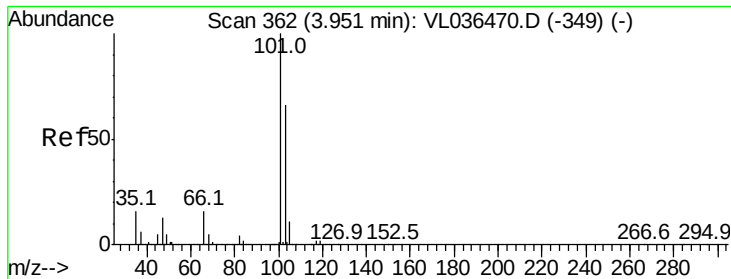





#11
Trichlorofluoromethane
Concen: 0.188 ppbv
RT: 3.95 min Scan# 361
Delta R.T. -0.00 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Instrument :
MSVOA_L
ClientSampleId :
FS-IA-03

Tot Ion:101 Resp: 39900
Ion Ratio Lower Upper
101 100
103 61.7 52.5 78.7




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:16:36 AM

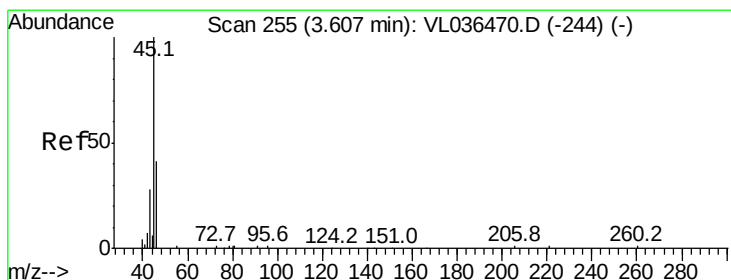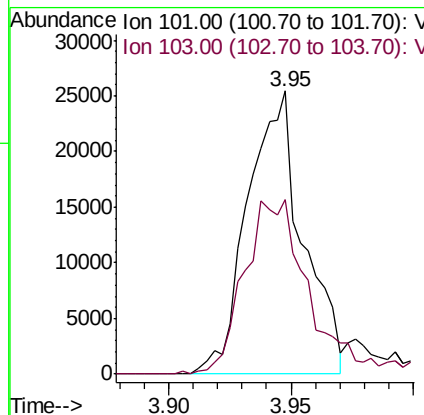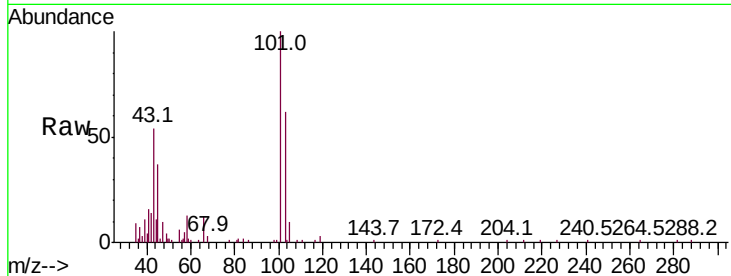

#13
Ethanol
Concen: 22.895 ppbv
RT: 3.61 min Scan# 257
Delta R.T. 0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Tgt Ion: 45 Resp: 207442
Ion Ratio Lower Upper
45 100
46 37.0 16.6 66.2

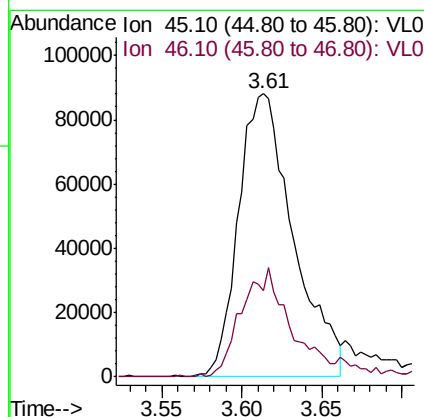

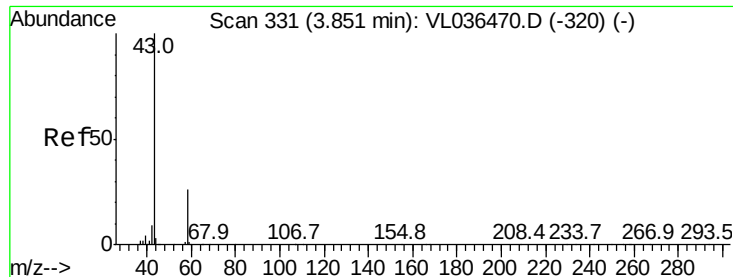

#15

Acetone

Concen: 11.477 ppbv

RT: 3.84 min Scan# 328

Delta R.T. -0.01 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Instrument :

MSVOA_L

ClientSampleId :

FS-IA-03

Tot Ion: 43 Resp: 1442896





Ion Ratio Lower Upper

43 100

58 22.8 21.2 31.8

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:16:36 AM

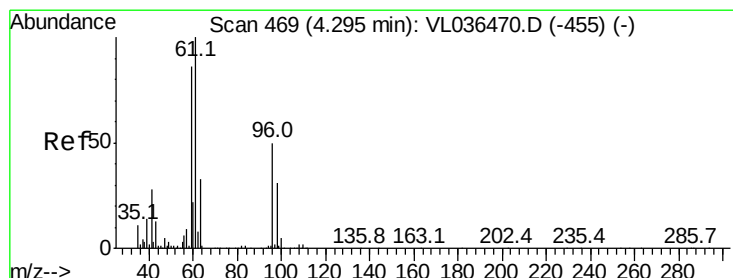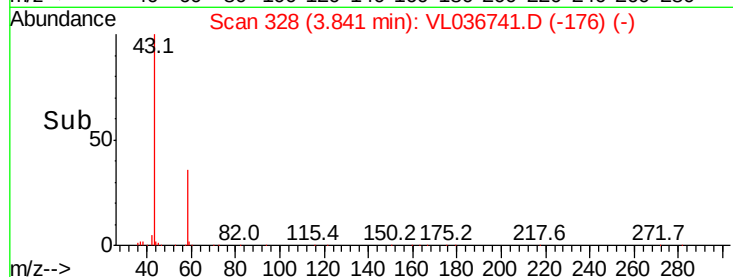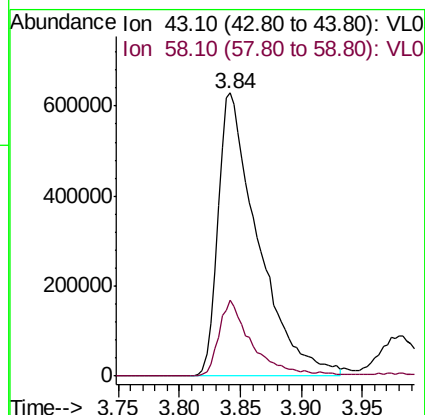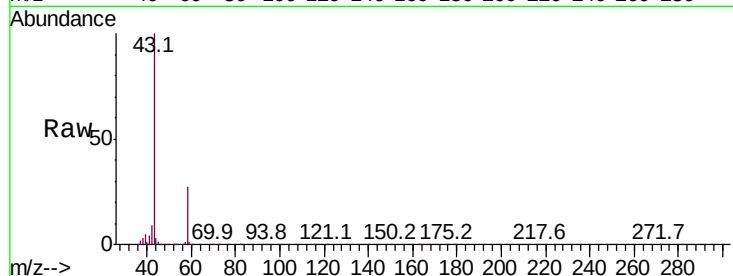

#17

tert-Butyl alcohol

Concen: 0.212 ppbv m

RT: 4.31 min Scan# 473

Delta R.T. 0.01 min

Lab File: VL036741.D




Acq: 8 Apr 2021 00:40


Tgt Ion: 59 Resp: 23203

Ion Ratio Lower Upper

59 100

57 0.0 8.6 12.8#

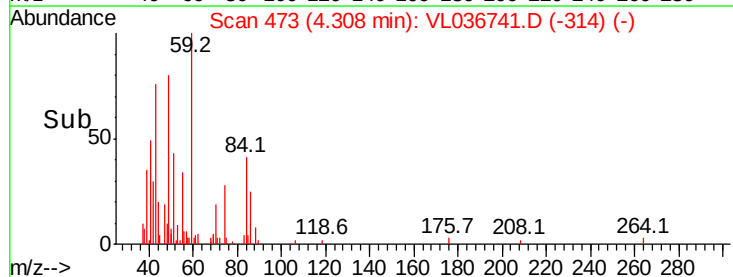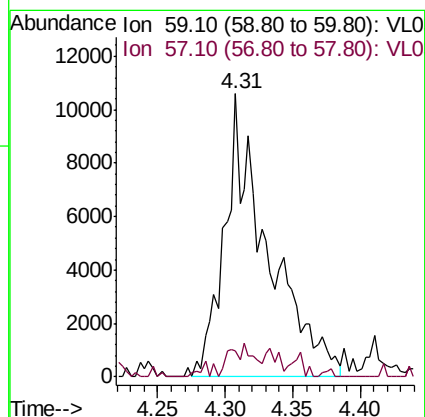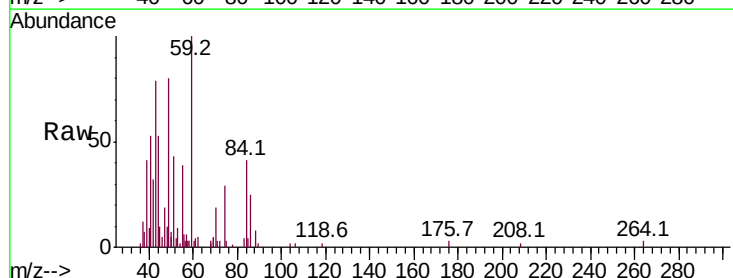



#19





Isopropyl Alcohol
 Concen: 10.846 ppbv
 RT: 3.98 min Scan# 371
 Delta R.T. 0.01 min
 Lab File: VL036741.D
 Acq: 8 Apr 2021 00:40

Instrument :
 MSVOA_L
 ClientSampleId :
 FS-IA-03

Tot Ion	Ratio	Lower	Upper
45	100		
58	2.5	2.9	4.3#

Manual Integrations
 APPROVED




MMDadoda
 4/12/2021 11:16:36 AM

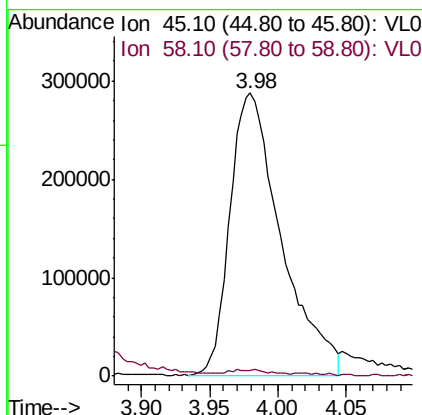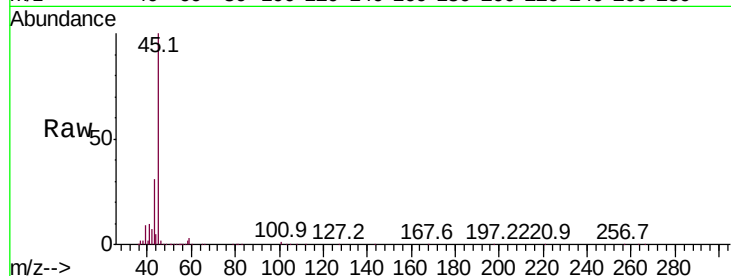


#20

Methylene Chloride
 Concen: 8.502 ppbv
 RT: 4.34 min Scan# 482
 Delta R.T. -0.01 min
 Lab File: VL036741.D
 Acq: 8 Apr 2021 00:40

Tgt Ion	Ratio	Lower	Upper
84	100		
49	164.9	122.9	184.3
51	49.6	36.9	55.3
86	59.4	48.2	72.4

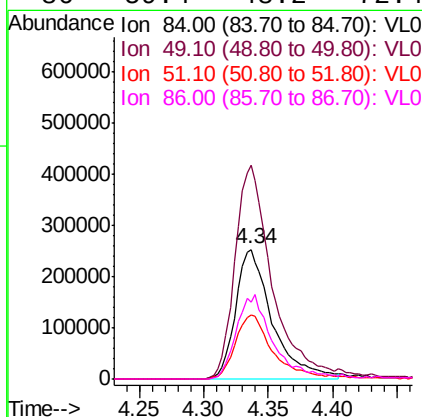

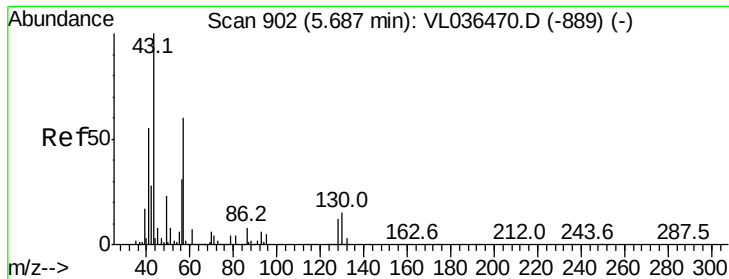





#26
Hexane
Concen: 2.818 ppbv
RT: 5.68 min Scan# 899
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Instrument :
MSVOA_L
ClientSampleId :
FS-IA-03

Tot Ion	Ratio	Lower	Upper
57	100		
41	99.0	77.2	115.8
43	76.3	173.8	260.6#
56	57.6	43.8	65.6




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:16:36 AM

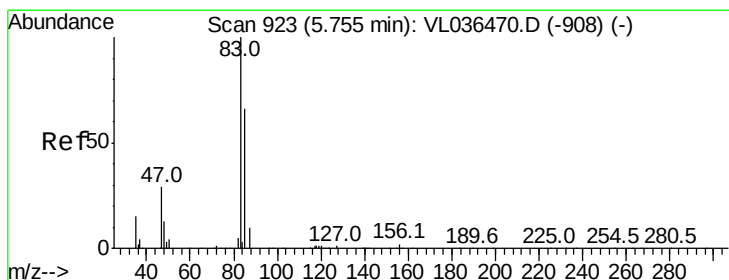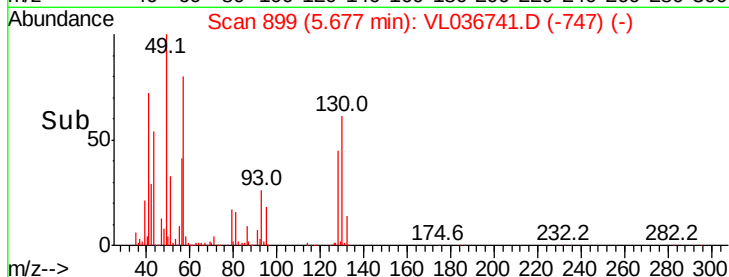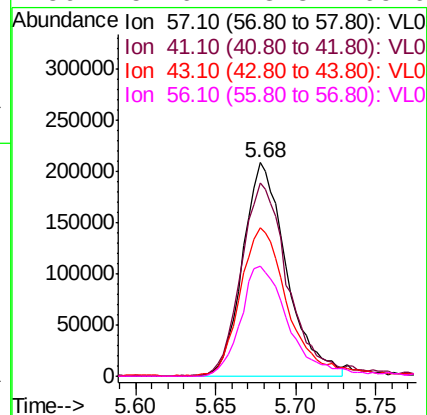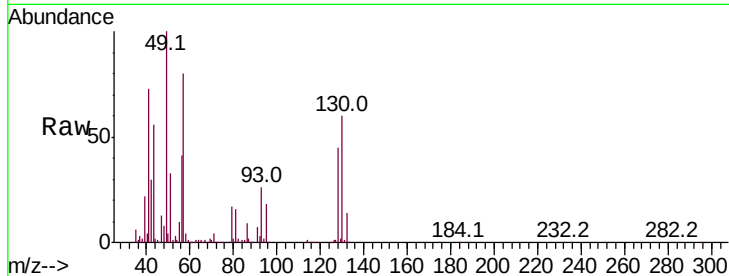

#29
Chloroform
Concen: 0.100 ppbv m
RT: 5.74 min Scan# 919
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Tgt Ion	Ratio	Lower	Upper
83	100		
85	64.7	52.6	78.8

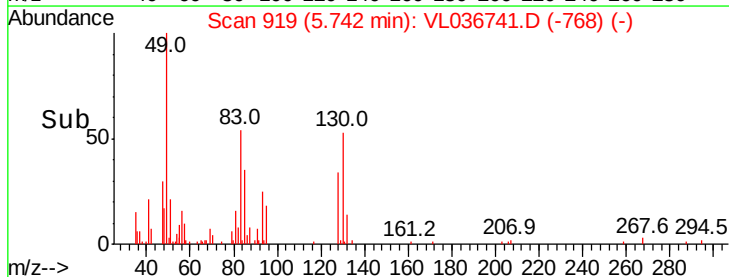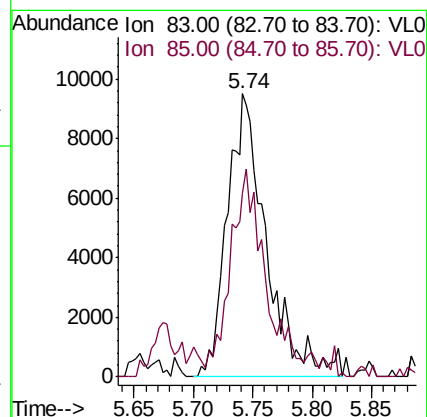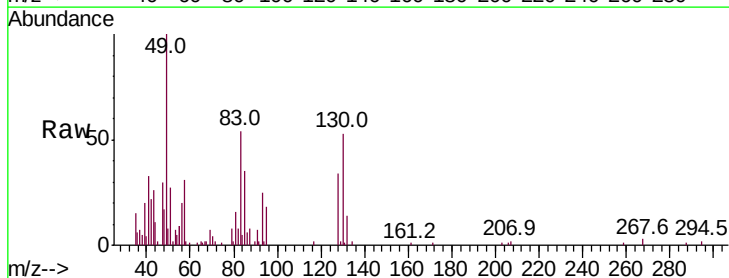

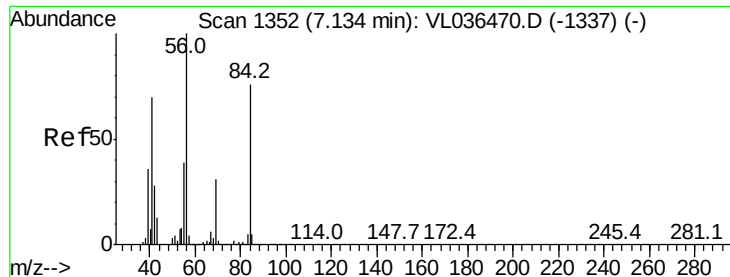





#30
Cyclohexane
Concen: 0.267 ppbv m
RT: 7.12 min Scan# 1348
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Instrument :
MSVOA_L
ClientSampled :
FS-IA-03

Tot Ion	Ratio	Lower	Upper
84	100		
56	0.0	114.6	171.8#
41	72.9	75.3	112.9#




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:16:36 AM

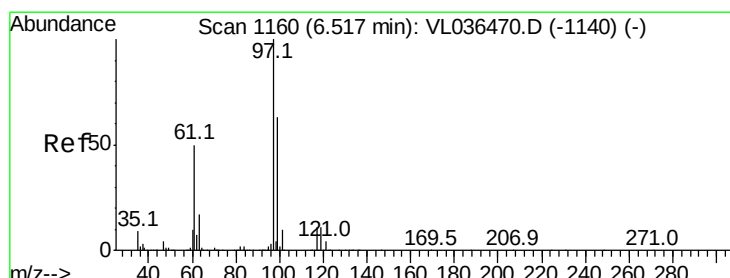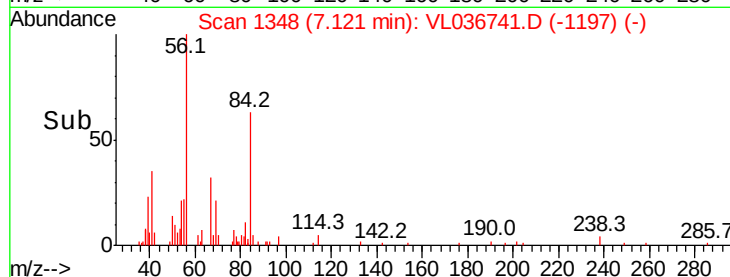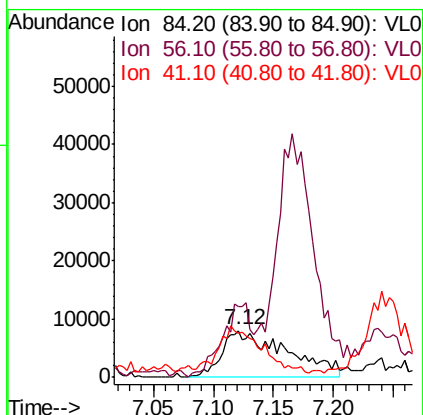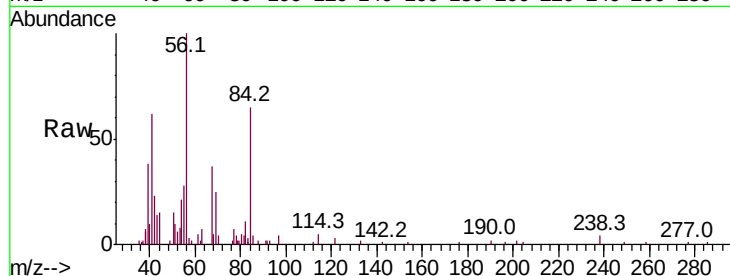

#32
1,1,1-Trichloroethane
Concen: 0.116 ppbv m
RT: 6.50 min Scan# 1156
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Tgt Ion	Ratio	Lower	Upper
97	100		
99	0.0	51.4	77.0#
61	54.6	40.6	60.8

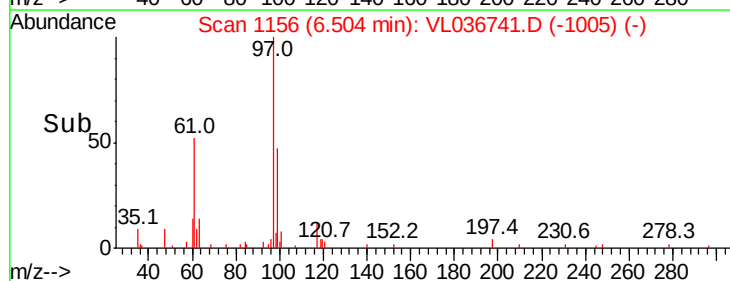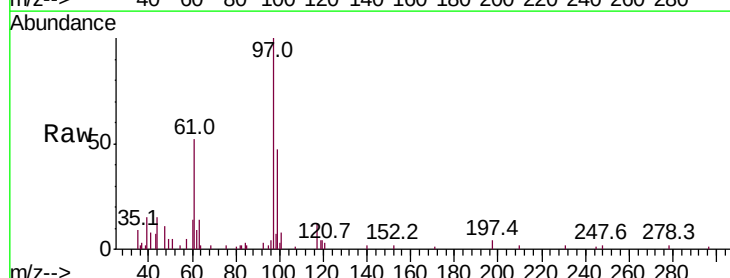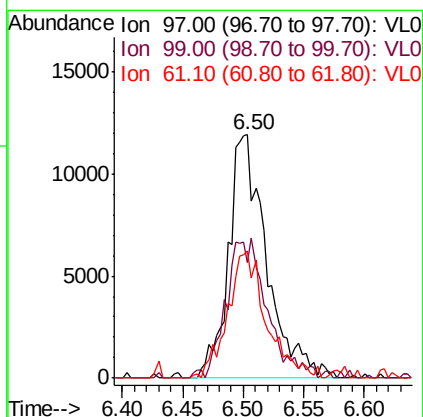







#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.17 min Scan# 1362
 Delta R.T. -0.01 min
 Lab File: VL036741.D
 Acq: 8 Apr 2021 00:40

Instrument :
 MSVOA_L
 ClientSampleId :
 FS-IA-03

Tot Ion	Ratio	Lower	Upper
114	100		
63	27.7	22.4	33.6
88	19.5	15.4	23.0




Manual Integrations
 APPROVED


MMDadoda
 4/12/2021 11:16:36 AM

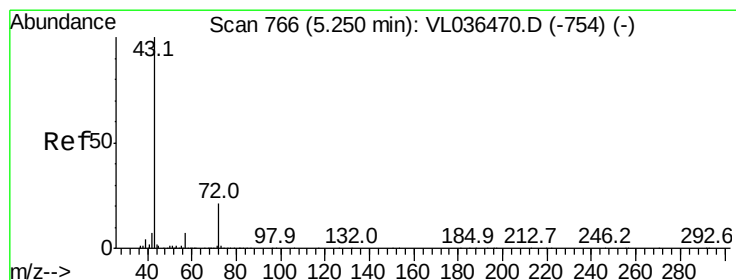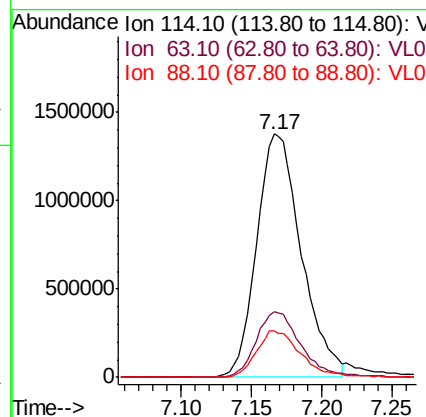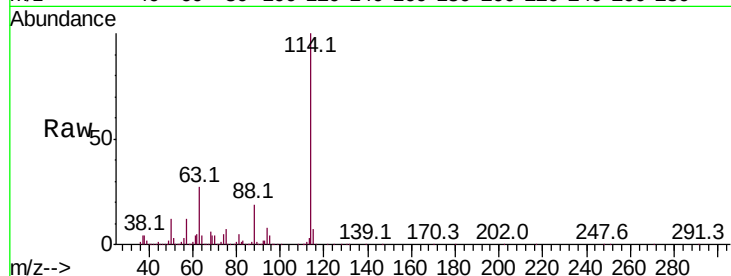

#34
 2-Butanone
 Concen: 1.217 ppbv
 RT: 5.24 min Scan# 763
 Delta R.T. -0.01 min
 Lab File: VL036741.D
 Acq: 8 Apr 2021 00:40

Tgt Ion	Ratio	Lower	Upper
43	100		
72	23.4	17.0	25.6

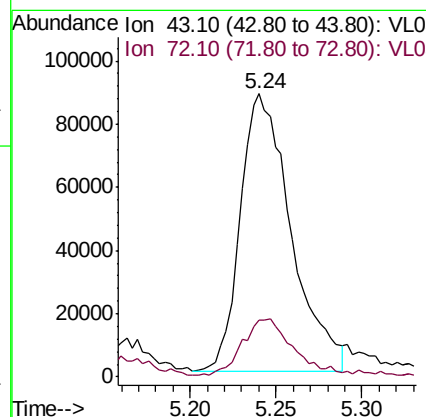

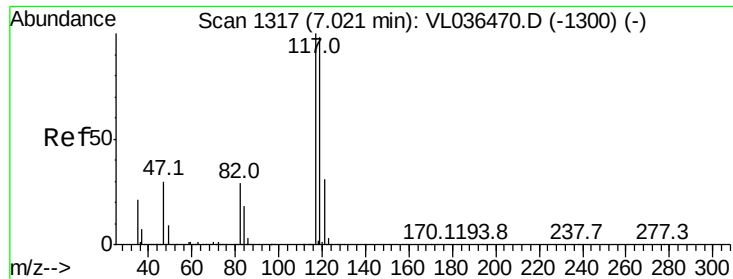





#35
Carbon Tetrachloride
Concen: 0.052 ppbv m
RT: 7.01 min Scan# 1314
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Instrument :
MSVOA_L
ClientSampled :
FS-IA-03

Tot Ion	Ratio	Lower	Upper
117	100		
119	76.0	78.2	117.2#
121	18.1	24.5	36.7#




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:16:36 AM

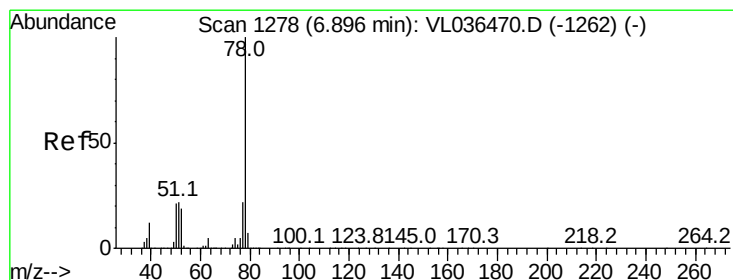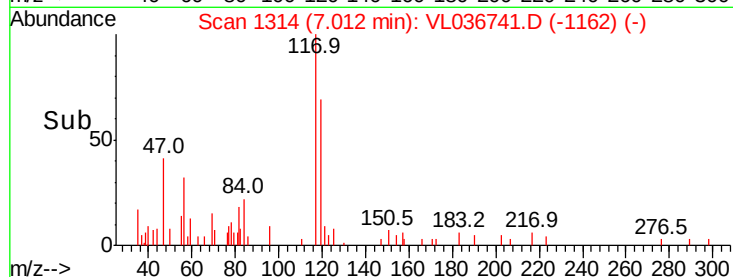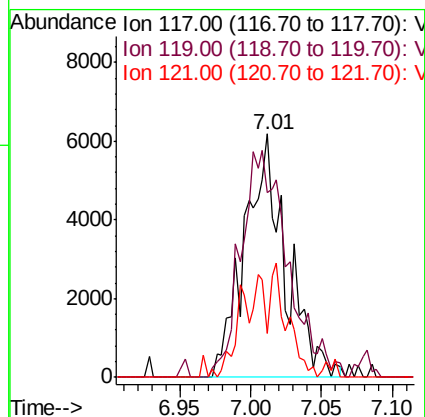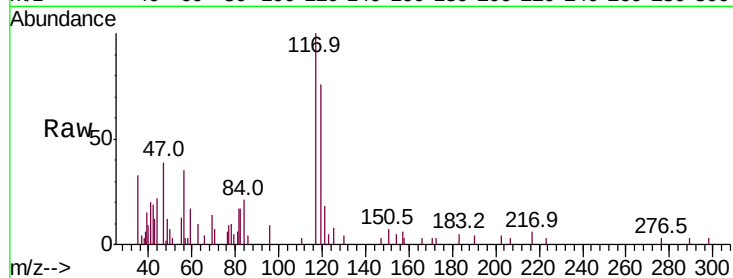

#36
Benzene
Concen: 0.695 ppbv m
RT: 6.88 min Scan# 1274
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Tgt Ion	Ratio	Lower	Upper
78	100		
77	19.8	18.0	27.0
50	15.5	16.5	24.7#

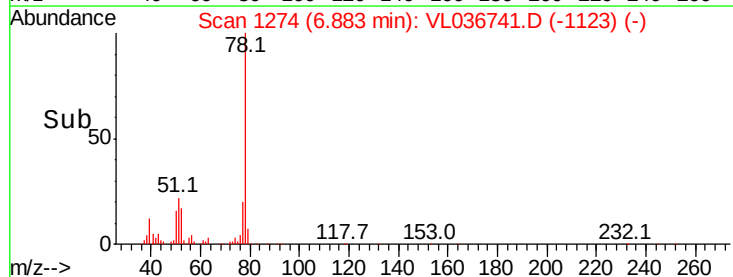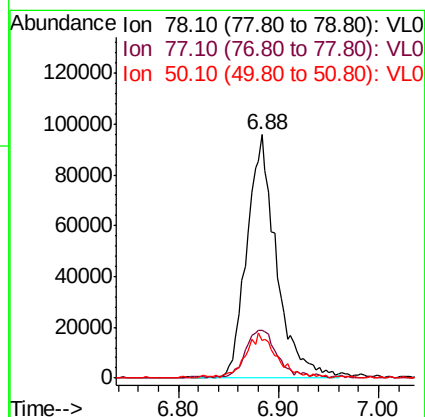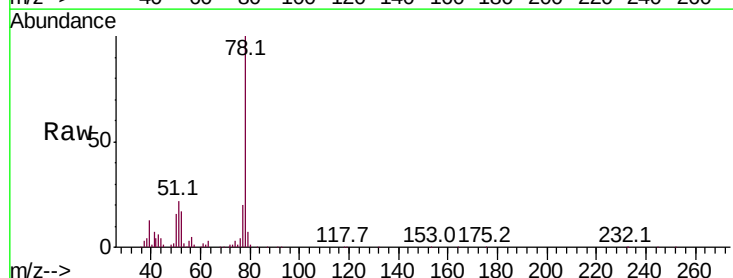

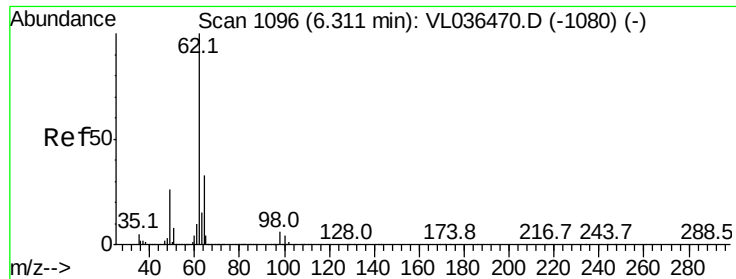





#37
 1,2-Dichloroethane
 Concen: 0.104 ppbv m
 RT: 6.29 min Scan# 1091
 Delta R.T. -0.02 min
 Lab File: VL036741.D
 Acq: 8 Apr 2021 00:40

Instrument :
 MSVOA_L
 ClientSampleId :
 FS-IA-03

Tot Ion	Ratio	Resp	Lower	Upper
62	100	17079		
98	8.7		4.9	7.3#




Manual Integrations
 APPROVED


MMDadoda
 4/12/2021 11:16:36 AM

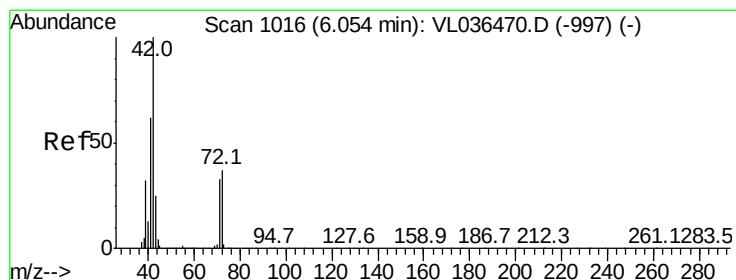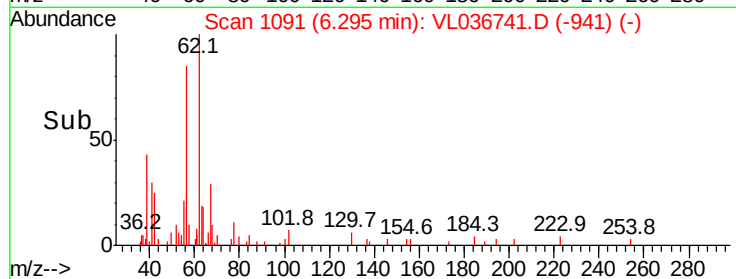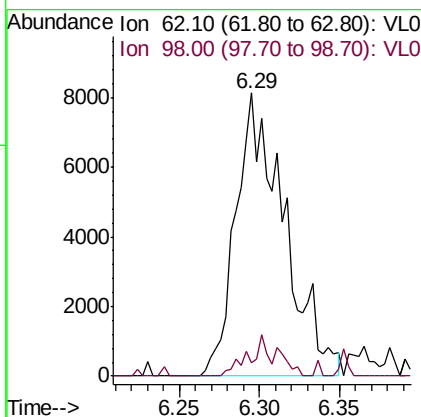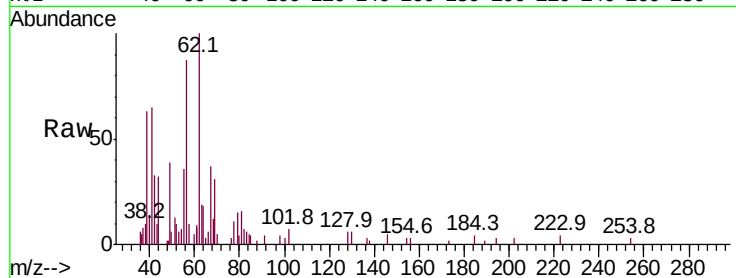

#41
 Tetrahydrofuran
 Concen: 0.386 ppbv m
 RT: 6.06 min Scan# 1017
 Delta R.T. 0.00 min
 Lab File: VL036741.D
 Acq: 8 Apr 2021 00:40

Tgt Ion	Ratio	Resp	Lower	Upper
42	100	26364		
72	0.0		27.6	41.4#
71	0.0		27.0	40.4#

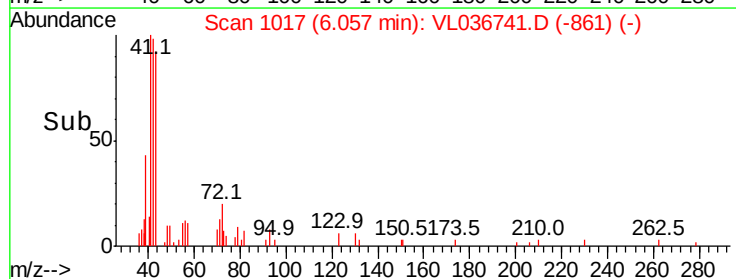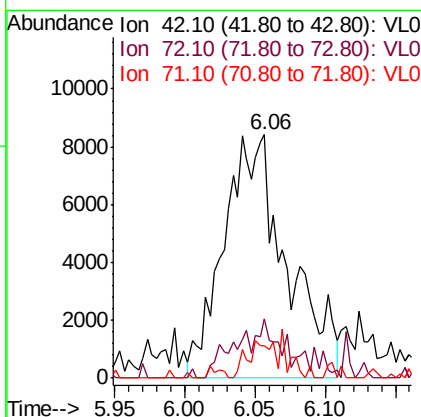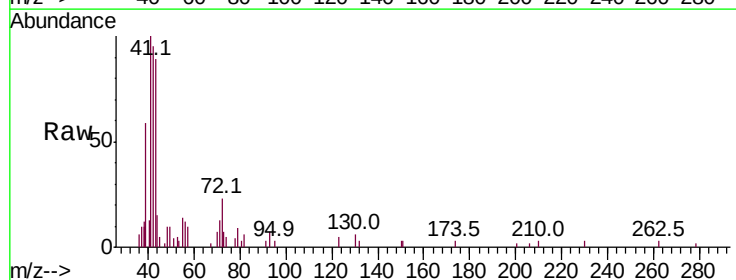

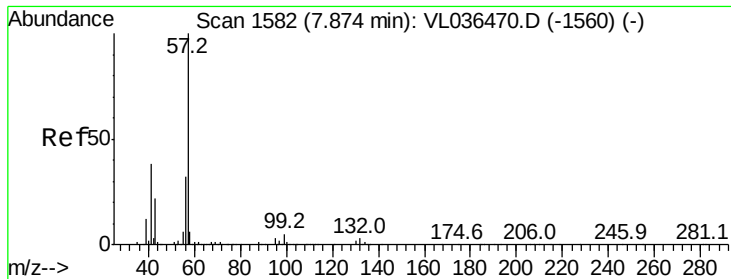

#44

2,2,4-Trimethylpentane

Concen: 0.320 ppbv m

RT: 7.86 min Scan# 1579

Delta R.T. -0.01 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Instrument :

MSVOA_L





ClientSampled :

FS-IA-03

Tot Ion:	57	Resp:	157753
Ion	Ratio	Lower	Upper
57	100		
41	43.4	28.8	43.2#
56	37.5	26.1	39.1

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:16:36 AM

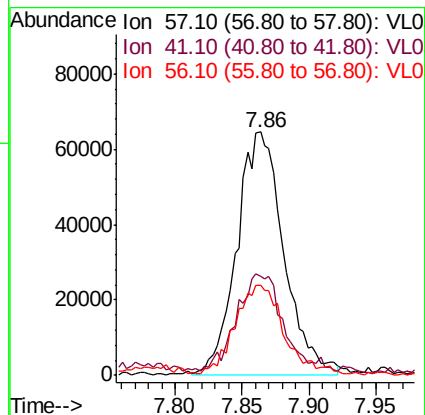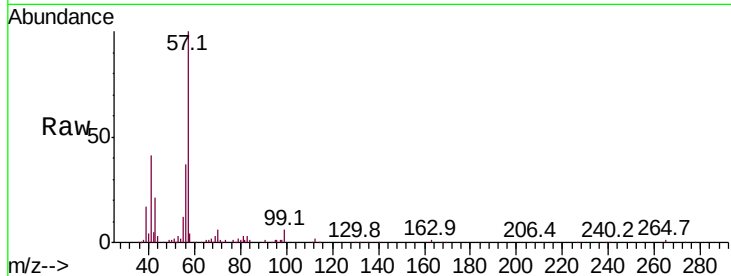

#50

4-Methyl-2-Pentanone

Concen: 0.179 ppbv m




RT: 8.75 min Scan# 1856


Delta R.T. 0.01 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Tgt Ion:	43	Resp:	38523
Ion	Ratio	Lower	Upper
43	100		
58	0.0	28.2	42.2#

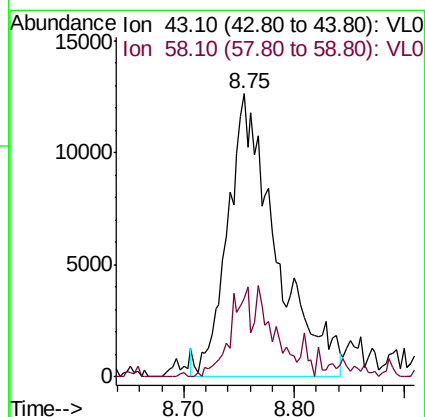

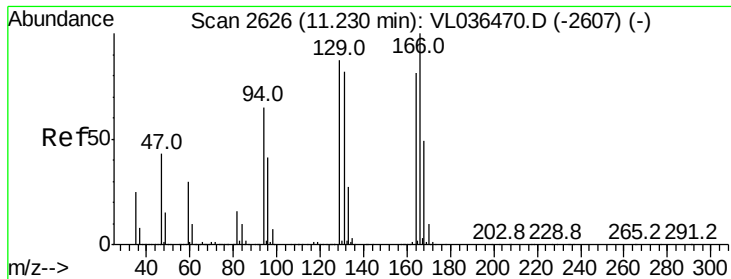





#52
Tetrachloroethene
Concen: 0.442 ppbv m
RT: 11.21 min Scan# 2621
Delta R.T. -0.02 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Instrument :
MSVOA_L
ClientSampleId :
FS-IA-03

Tot Ion	Ratio	Lower	Upper
164	100		
166	134.5	98.3	147.5
129	93.0	85.8	128.8
131	105.8	80.9	121.3




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:16:36 AM

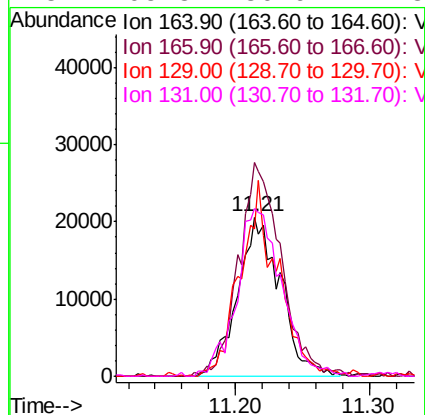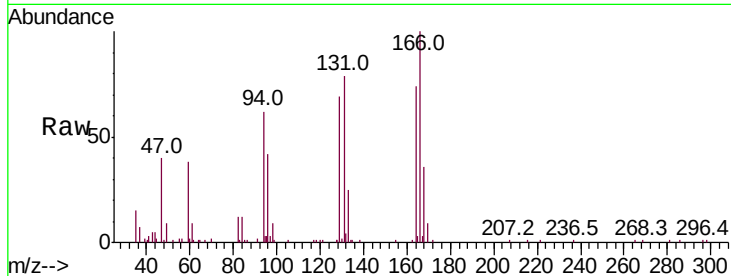

#53
Toluene
Concen: 10.052 ppbv
RT: 9.80 min Scan# 2181
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Tgt Ion	Ratio	Lower	Upper
91	100		
92	60.9	48.8	73.2

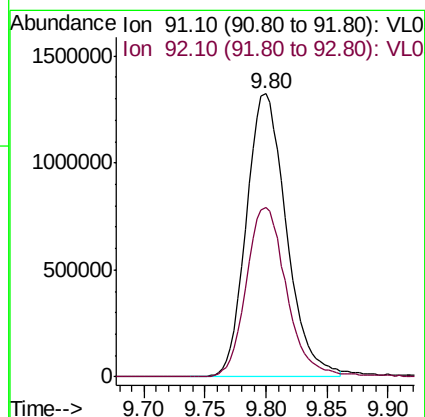

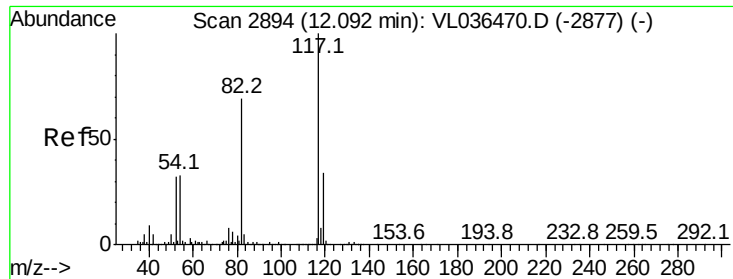





#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.08 min Scan# 2890
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Instrument :
MSVOA_L
ClientSampleId :
FS-IA-03

Tot Ion	Ratio	Lower	Upper
117	100		
82	68.6	57.4	86.0
119	33.1	47.4	71.0#




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:16:36 AM

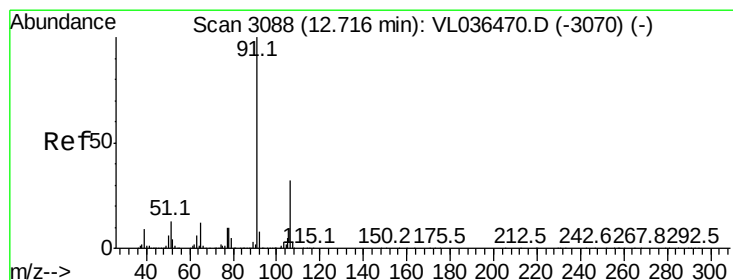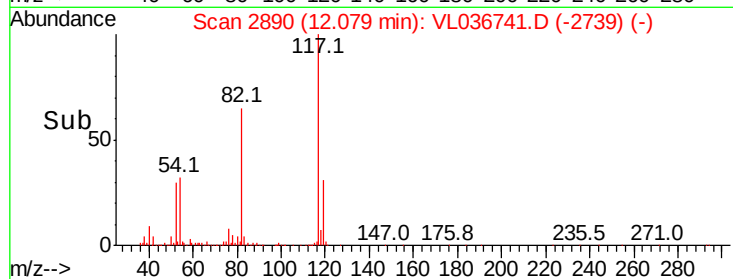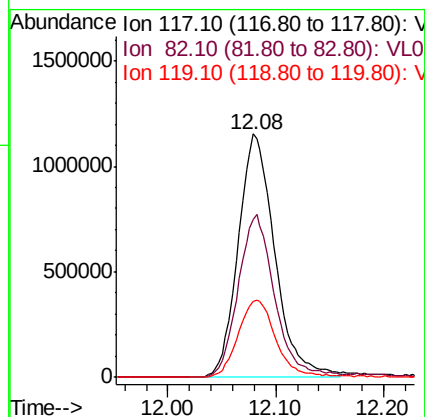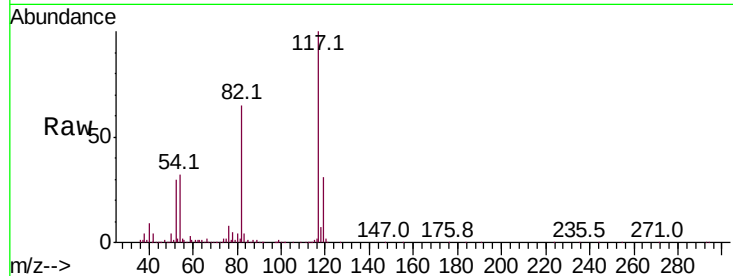

#58
Ethyl Benzene
Concen: 0.364 ppbv
RT: 12.71 min Scan# 3085
Delta R.T. -0.01 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Tgt Ion	Ratio	Lower	Upper
91	100		
106	28.5	25.3	37.9

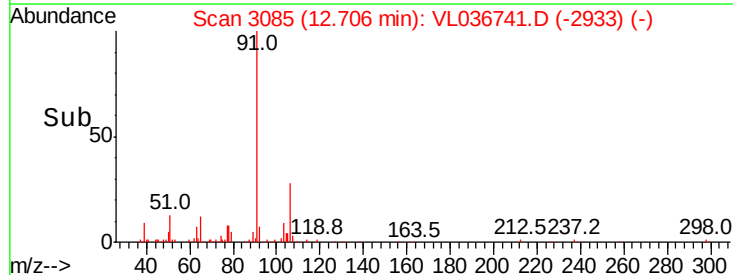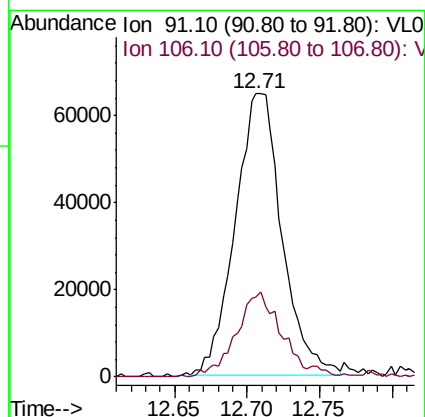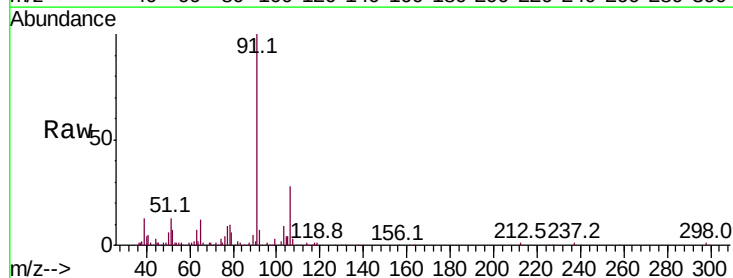

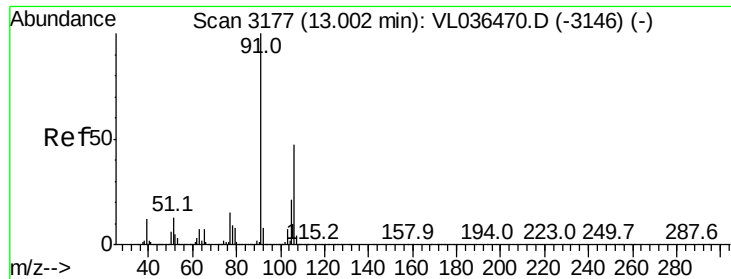





#59
m/p-Xylene
Concen: 1.589 ppbv
RT: 12.96 min Scan# 3163
Delta R.T. -0.05 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Instrument :
MSVOA_L
ClientSampleId :
FS-IA-03

Tot Ion: 91 Resp: 549795
Ion Ratio Lower Upper
91 100
106 47.8 35.3 52.9




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:16:36 AM

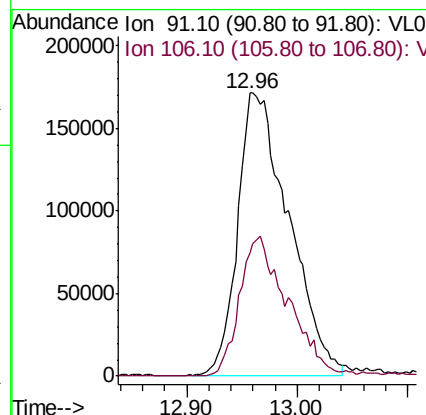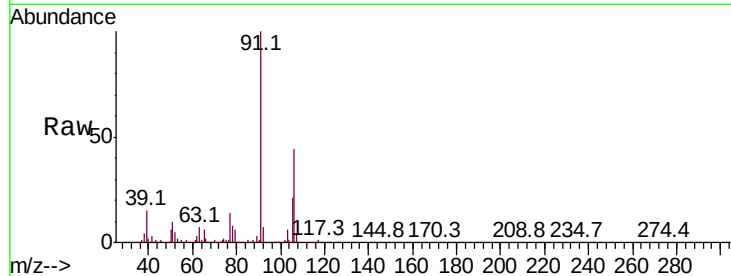

#60
o-Xylene
Concen: 0.757 ppbv m
RT: 13.68 min Scan# 3389
Delta R.T. -0.02 min
Lab File: VL036741.D
Acq: 8 Apr 2021 00:40

Tgt Ion: 91 Resp: 253175
Ion Ratio Lower Upper
91 100
106 0.0 22.3 66.9#

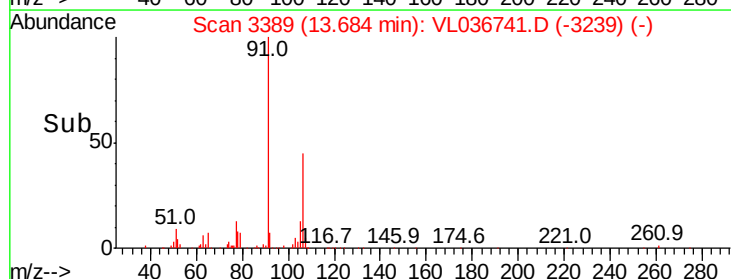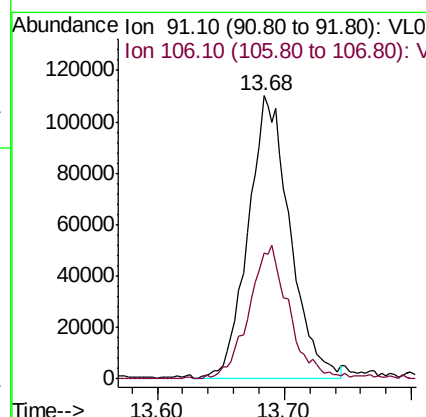







#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.717 ppbv
 RT: 14.41 min Scan# 3616
 Delta R.T. -0.01 min
 Lab File: VL036741.D
 Acq: 8 Apr 2021 00:40

Instrument :
 MSVOA_L
 ClientSampleId :
 FS-IA-03

Tot Ion: 95 Resp: 2112172
 Ion Ratio Lower Upper
 95 100
 174 67.2 51.0 76.6
 175 5.0 3.9 5.9




Manual Integrations
 APPROVED


MMDadoda
 4/12/2021 11:16:36 AM

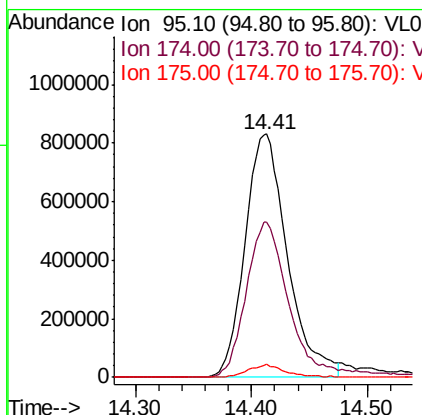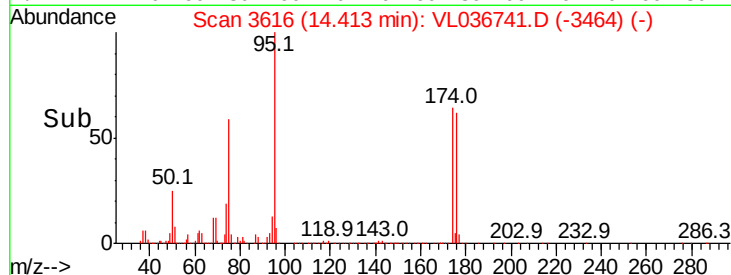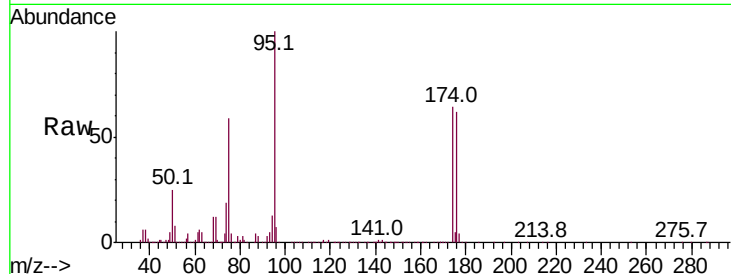

#72
 4-Ethyltoluene
 Concen: 0.156 ppbv m
 RT: 15.84 min Scan# 4060
 Delta R.T. -0.01 min
 Lab File: VL036741.D
 Acq: 8 Apr 2021 00:40

Tgt Ion: 105 Resp: 57264
 Ion Ratio Lower Upper
 105 100
 120 0.0 24.0 36.0#
 91 18.7 11.0 16.4#
 77 0.0 11.7 17.5#

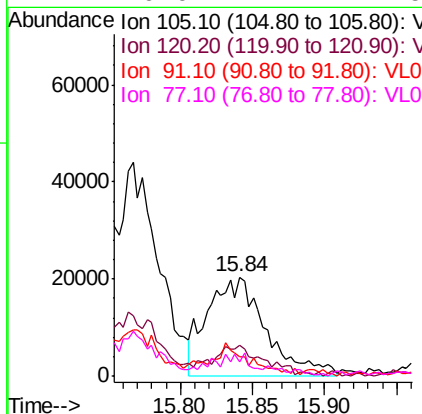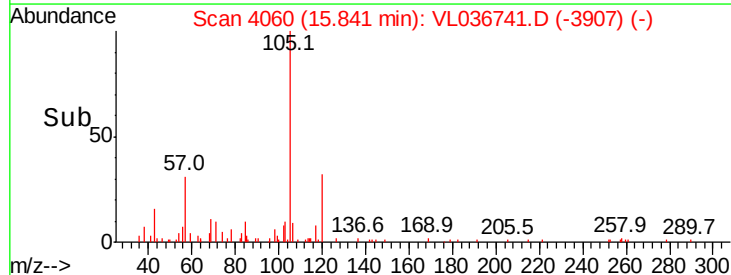

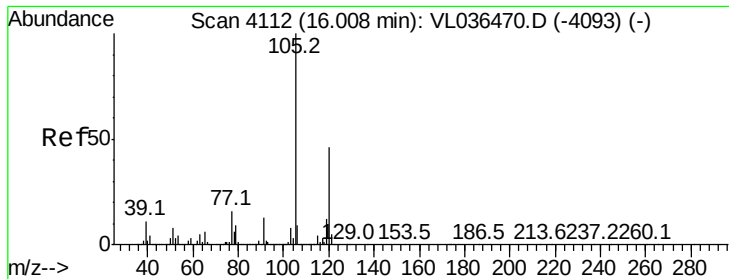

#73

1,3,5-Trimethylbenzene

Concen: 0.179 ppbv m

RT: 15.99 min Scan# 4107

Delta R.T. -0.02 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Instrument :

MSVOA_L

ClientSampled :

FS-IA-03

Tot Ion:105 Resp: 61332

Ion Ratio Lower Upper





105 100

120 42.1 36.6 54.8

Manual Integrations
APPROVED

MMDadoda

4/12/2021 11:16:36 AM

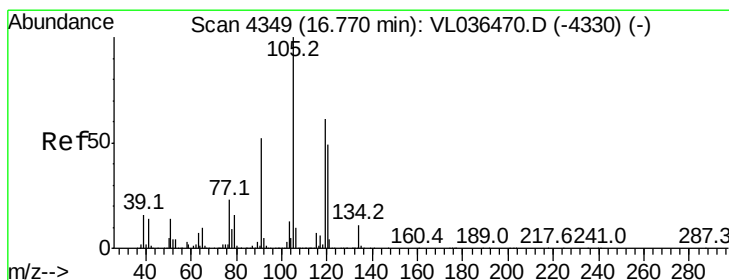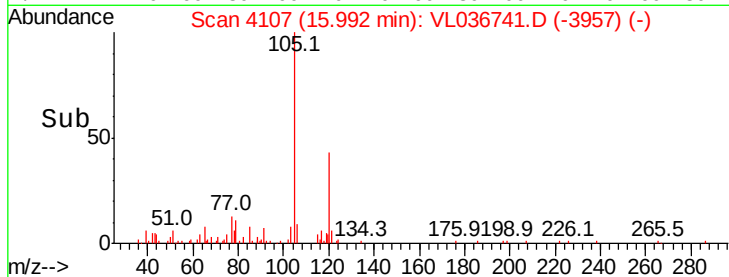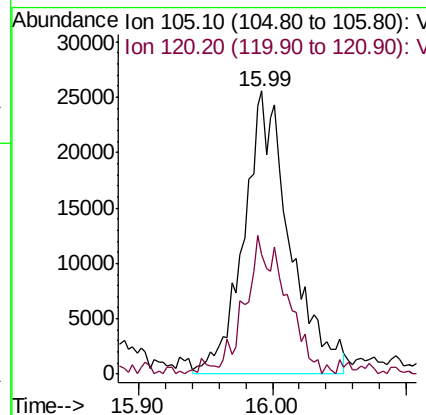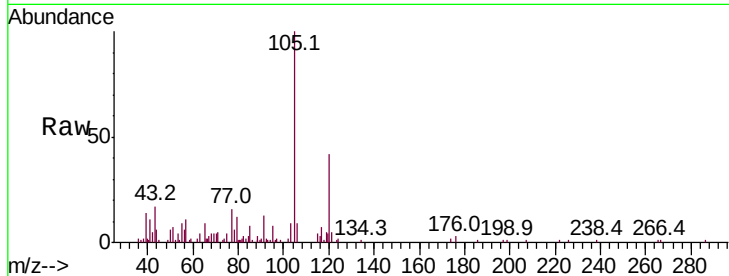

#74

1,2,4-Trimethylbenzene

Concen: 0.449 ppbv

RT: 16.77 min Scan# 4348

Delta R.T. -0.00 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Tgt Ion:105 Resp: 164434




Ion Ratio Lower Upper


105 100

120 37.8 39.2 58.8#

91 12.8 42.6 64.0#

77 11.6 18.6 28.0#

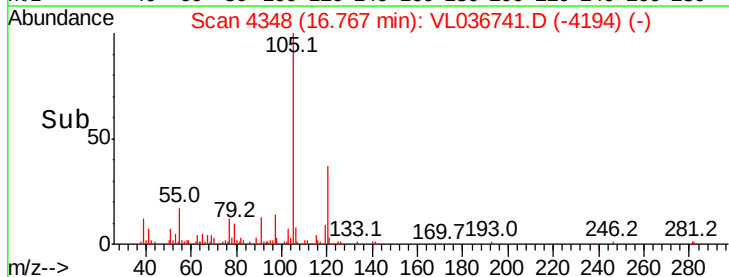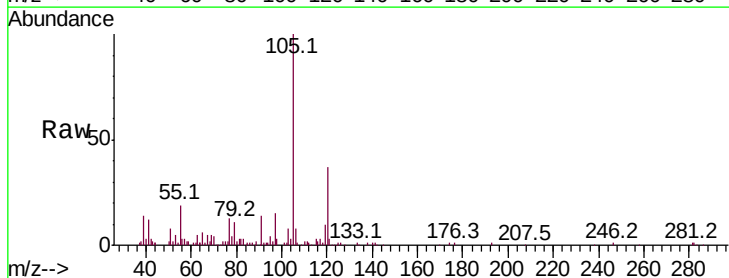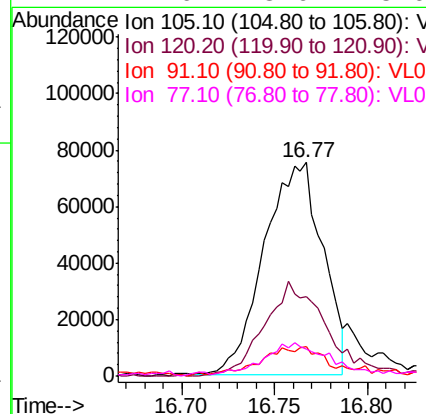

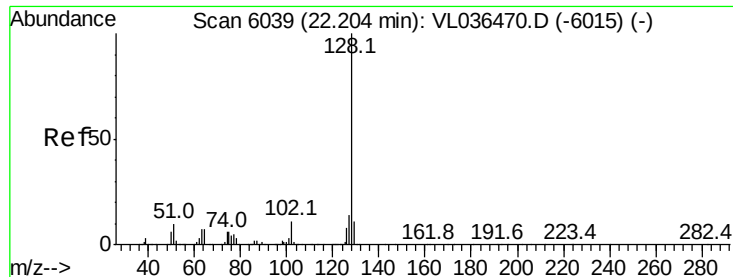

#79

Naphthalene

Concen: 0.214 ppbv m

RT: 22.21 min Scan# 6040

Delta R.T. 0.00 min

Lab File: VL036741.D

Acq: 8 Apr 2021 00:40

Instrument :

MSVOA_L

ClientSampleId :

FS-IA-03

Tot Ion:	128	Resp:	45645
Ion Ratio	Lower	Upper	
128	100		
127	8.4	10.9	16.3#
129	12.2	9.0	13.4

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:16:36 AM

