

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL040821\
 Data File : VL036762.D
 Acq On : 8 Apr 2021 23:10
 Operator : SY/AP
 Sample : M1981-04
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG-1

Manual Integrations
 APPROVED

MMDadoda
 4/12/2021 11:47:37 AM

Quant Time: Apr 09 11:37:14 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Mar 2
 QLast Update : Thu Mar 25 09:42:40 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	1289836	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.18	114	3205071	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.08	117	2622211	10.00	ppbv	-0.01

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
68) 1-Bromo-4-Fluorobenzene	14.41	95	1640501	7.85	ppbv	-0.01	
Spiked Amount	10.000	Range	65 - 135	Recovery	=	78.50%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
9) Propene	3.00	41	1348946	17.558	ppbv	96
10) Heptane	8.12	43	92539	0.473	ppbv	93
11) Trichlorofluoromethane	3.94	101	38251	0.178	ppbv	85
12) 1,1,2-Trichlorotrifluoroet	4.48	101	18946m	0.138	ppbv	
13) Ethanol	3.62	45	563224	61.563	ppbv	98
15) Acetone	3.85	43	18808092	148.154	ppbv #	80
19) Isopropyl Alcohol	3.98	45	324420	4.646	ppbv #	1
20) Methylene Chloride	4.35	84	4234230	71.237	ppbv	96
26) Hexane	5.68	57	3977076	28.395	ppbv #	47
27) Carbon Disulfide	4.54	76	348372	2.525	ppbv	98
30) Cyclohexane	7.13	84	60462m	0.532	ppbv	
31) cis-1,2-Dichloroethene	5.56	61	32255m	0.238	ppbv	
32) 1,1,1-Trichloroethane	6.51	97	12400m	0.055	ppbv	
34) 2-Butanone	5.24	43	2214945	14.158	ppbv	99
35) Carbon Tetrachloride	7.02	117	22350m	0.091	ppbv	
36) Benzene	6.89	78	952864	3.224	ppbv	100
38) Trichloroethene	7.83	130	22046m	0.192	ppbv	
44) 2,2,4-Trimethylpentane	7.87	57	240267m	0.462	ppbv	
50) 4-Methyl-2-Pentanone	8.74	43	557190	2.461	ppbv	98
51) 2-Hexanone	10.13	43	130364	1.141	ppbv #	92
52) Tetrachloroethene	11.22	164	7953m	0.073	ppbv	
53) Toluene	9.80	91	761616	2.419	ppbv	99
58) Ethyl Benzene	12.70	91	205450	0.539	ppbv	96
59) m/p-Xylene	12.96	91	378073m	1.136	ppbv	
60) o-Xylene	13.68	91	243348m	0.756	ppbv	
62) Isopropylbenzene	14.66	105	67098m	0.155	ppbv	
69) p-Isopropyltoluene	17.64	119	112240m	0.271	ppbv	
72) 4-Ethyltoluene	15.83	105	59625	0.169	ppbv #	82
73) 1,3,5-Trimethylbenzene	15.99	105	117574	0.357	ppbv	93
74) 1,2,4-Trimethylbenzene	16.75	105	187100	0.531	ppbv #	68
76) 1,4-Dichlorobenzene	17.13	146	28305m	0.144	ppbv	
79) Naphthalene	22.21	128	39604m	0.193	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL040821\
Data File : VL036762.D
Acq On : 8 Apr 2021 23:10
Operator : SY/AP
Sample : M1981-04
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SG-1

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:47:37 AM

Quant Time: Apr 09 11:37:14 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Mar
QLast Update : Thu Mar 25 09:42:40 2021
Response via : Initial Calibration

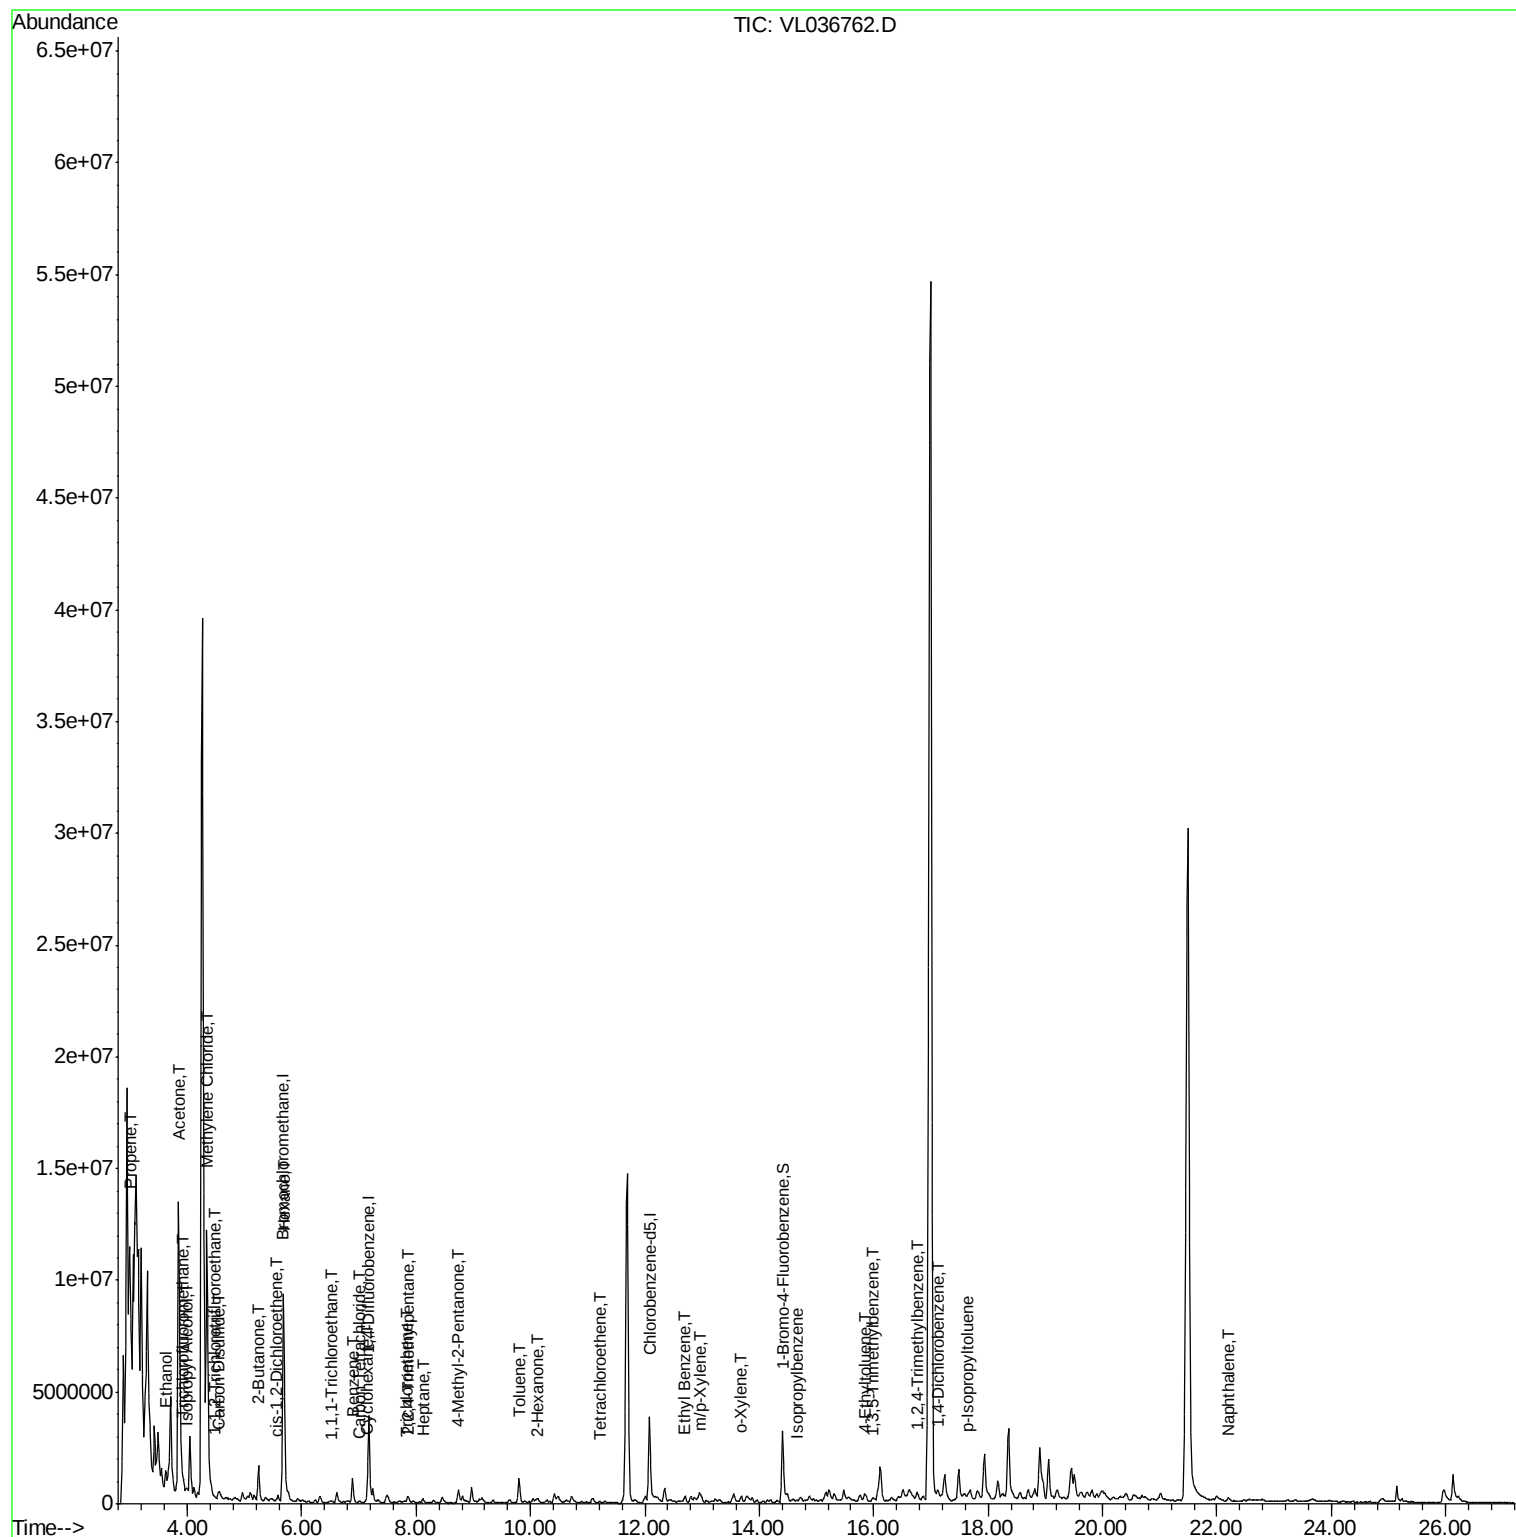



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.67 min Scan# 896

Delta R.T. -0.00 min

Lab File: VL036762.D

Acq: 8 Apr 2021 23:10

Instrument :

MSVOA_L

ClientSampled :

SG-1

Tot Ion: 49 Resp: 1289836

Ion Ratio Lower Upper

49 100





128 46.4 23.5 70.6

130 59.1 29.1 87.4

Manual Integrations
APPROVED

MMDadoda

4/12/2021 11:47:37 AM

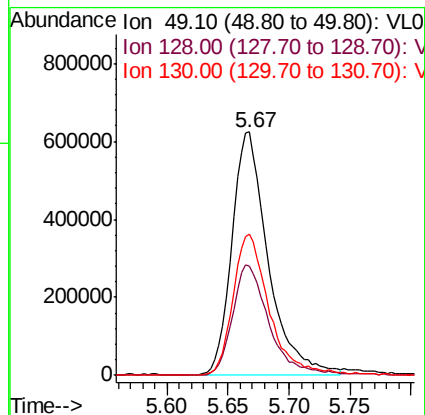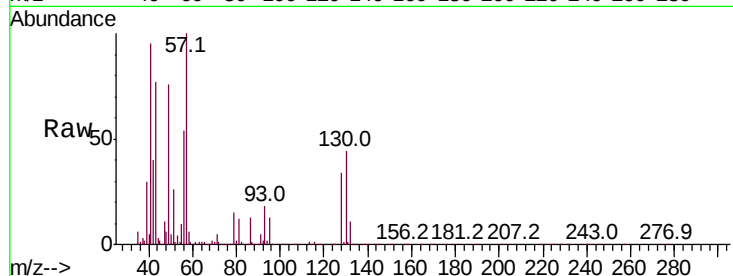

#9

Propene

Concen: 17.558 ppbv

RT: 3.00 min Scan# 67

Delta R.T. -0.01 min

Lab File: VL036762.D




Acq: 8 Apr 2021 23:10


Tgt Ion: 41 Resp: 1348946

Ion Ratio Lower Upper

41 100

42 67.7 57.0 85.4

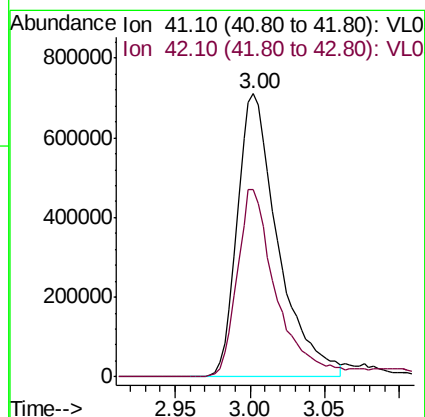

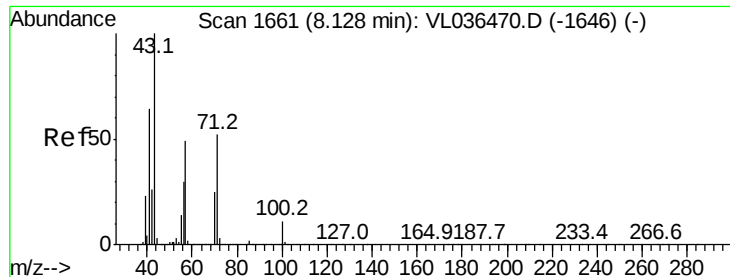





#10
Heptane
Concen: 0.473 ppbv
RT: 8.12 min Scan# 1658
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampled :
SG-1

Tot Ion	43	57	Ratio	100	53.5	Resp	92539	Lower	39.0	Upper	58.6
Ion	43	57	Ratio	100	53.5	Resp	92539	Lower	39.0	Upper	58.6




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

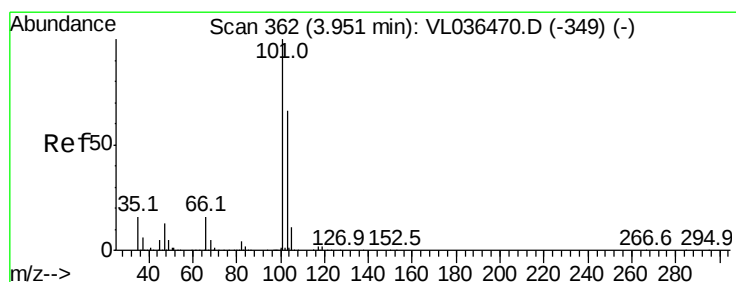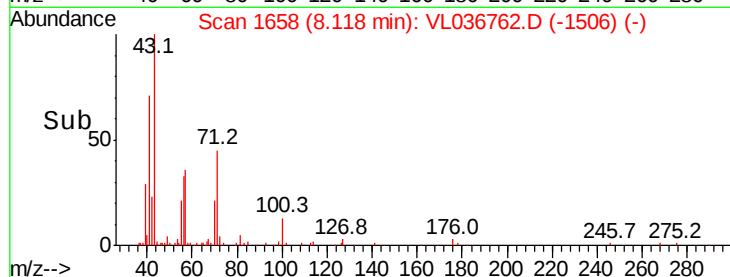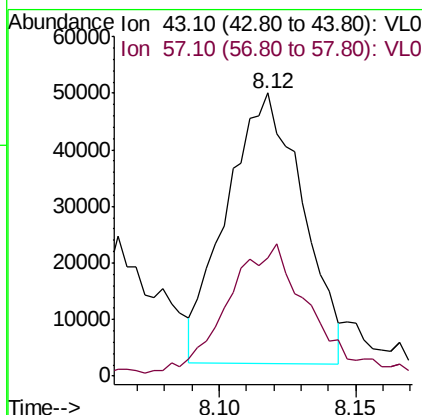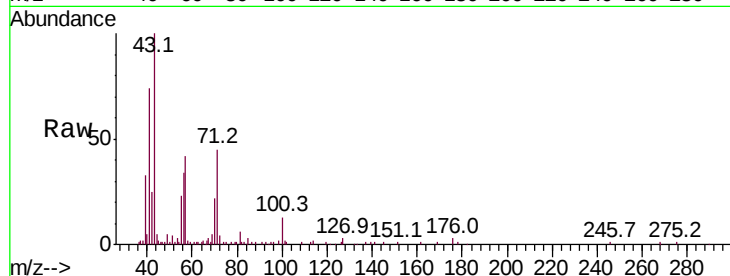

#11
Trichlorofluoromethane
Concen: 0.178 ppbv
RT: 3.94 min Scan# 359
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	101	103	Ratio	100	54.0	Resp	38251	Lower	52.5	Upper	78.7
Ion	101	103	Ratio	100	54.0	Resp	38251	Lower	52.5	Upper	78.7

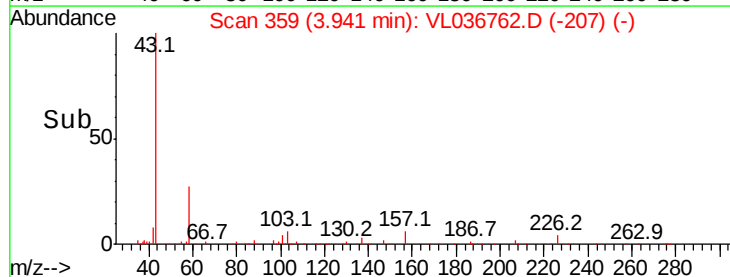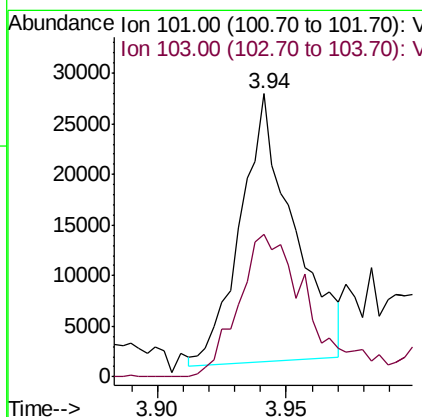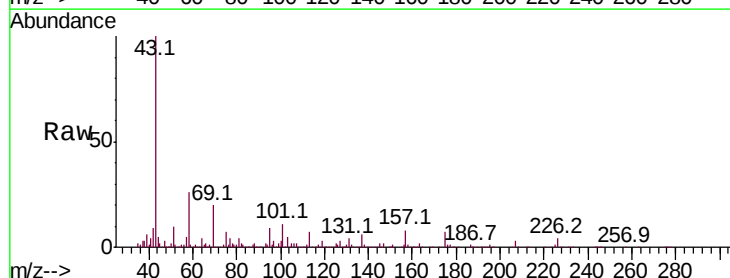

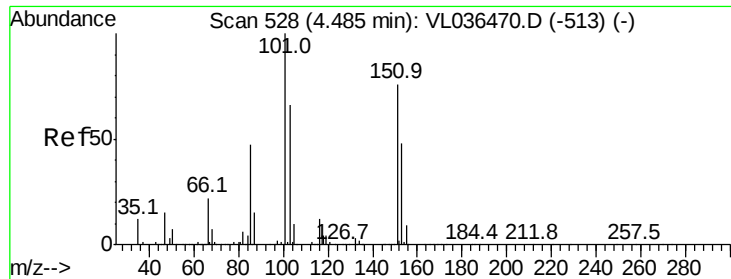

#12

1,1,2-Trichlorotrifluoroethane

Concen: 0.138 ppbv m

RT: 4.48 min Scan# 528

Delta R.T. -0.00 min

Lab File: VL036762.D

Acq: 8 Apr 2021 23:10

Instrument :

MSVOA_L

ClientSampled :

SG-1

Tot Ion:101 Resp: 18946

Ion Ratio Lower Upper

101 100





151 47.3 60.9 91.3#

Manual Integrations

APPROVED

MMDadoda

4/12/2021 11:47:37 AM

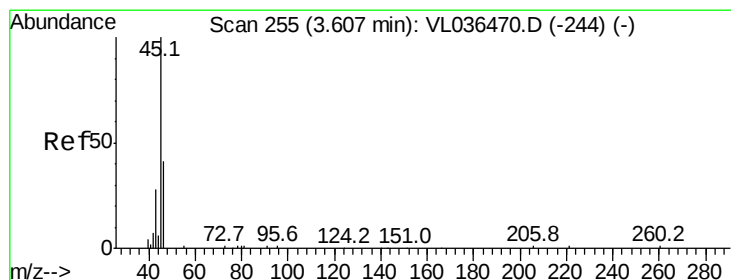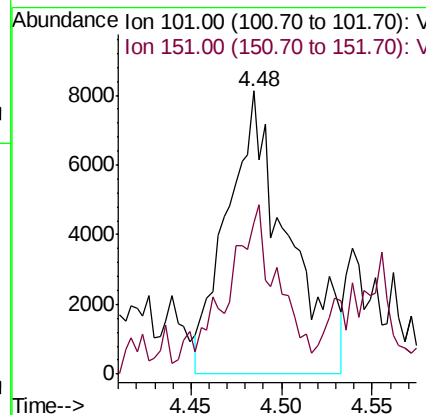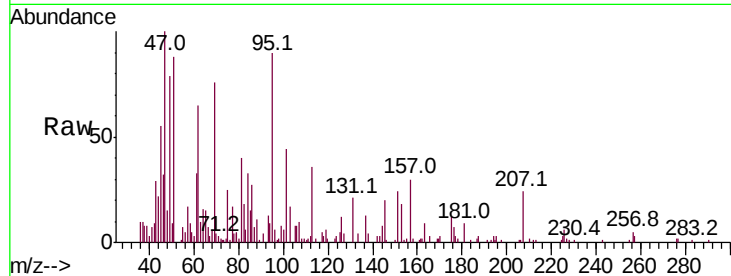

#13

Ethanol

Concen: 61.563 ppbv

RT: 3.62 min Scan# 259

Delta R.T. 0.01 min

Lab File: VL036762.D




Acq: 8 Apr 2021 23:10


Tgt Ion: 45 Resp: 563224

Ion Ratio Lower Upper

45 100

46 40.3 16.6 66.2

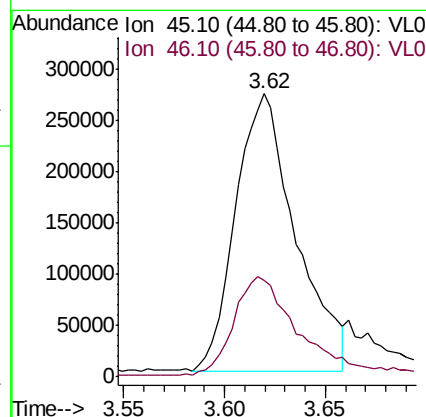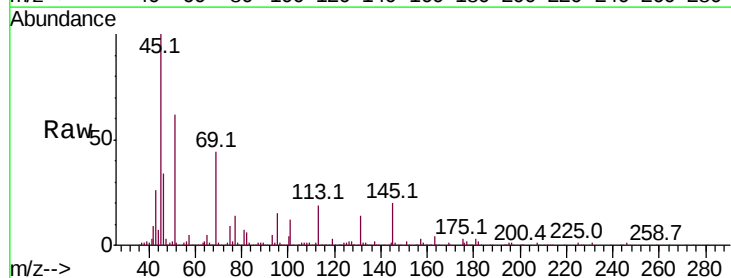

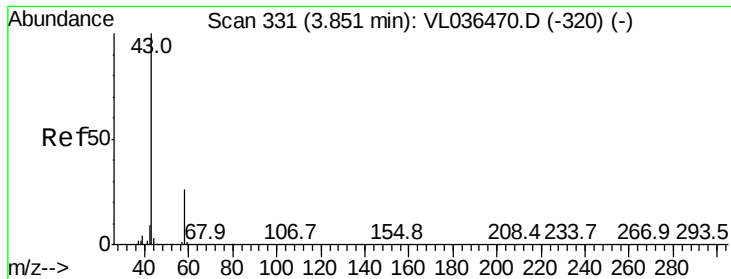

#15

Acetone

Concen: 148.154 ppbv

RT: 3.85 min Scan# 330

Delta R.T. -0.00 min

Lab File: VL036762.D

Acq: 8 Apr 2021 23:10

Instrument :

MSVOA_L

ClientSampleId :

SG-1

Tot Ion: 43 Resp:18808092

Ion Ratio Lower Upper





43 100

58 36.8 21.2 31.8#

Manual Integrations
APPROVED

MMDadoda

4/12/2021 11:47:37 AM

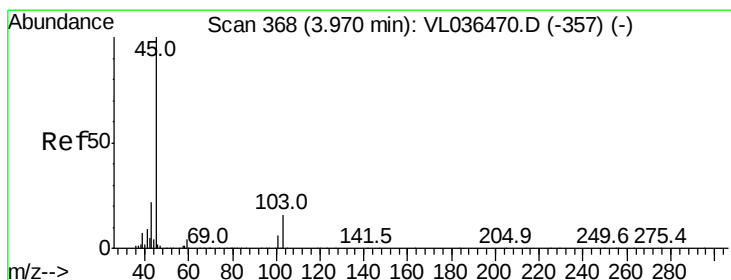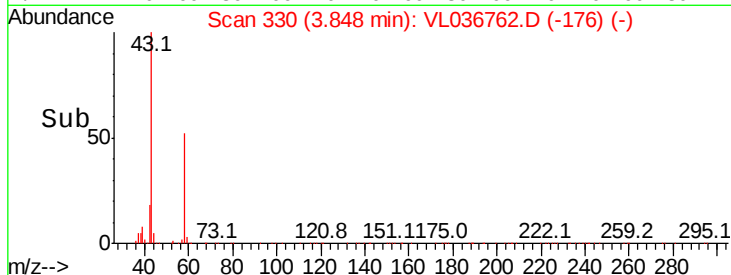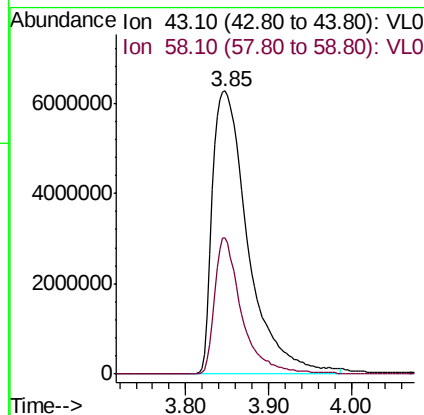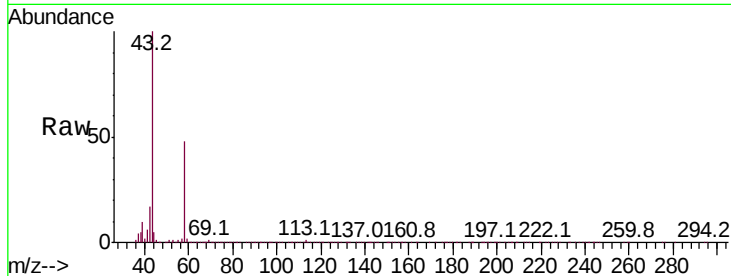

#19

Isopropyl Alcohol

Concen: 4.646 ppbv

RT: 3.98 min Scan# 372

Delta R.T. 0.01 min

Lab File: VL036762.D




Acq: 8 Apr 2021 23:10


Tgt Ion: 45 Resp: 324420

Ion Ratio Lower Upper

45 100

58 2143.0 2.9 4.3#

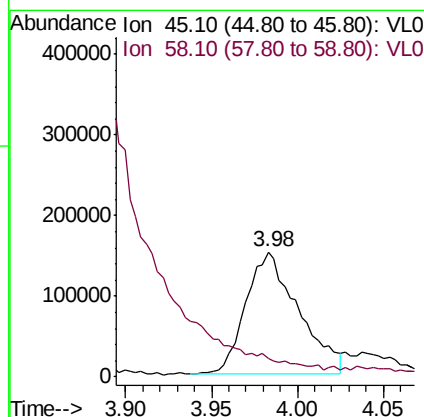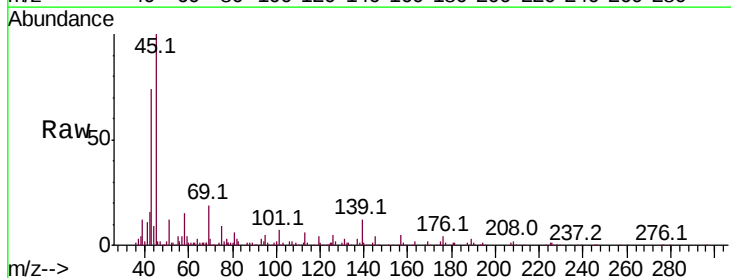







#20
Methvlene Chloride
Concen: 71.237 ppbv
RT: 4.35 min Scan# 485
Delta R.T. 0.00 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tot Ion	84	Resp	4234230
Ion	Ratio	Lower	Upper
84	100		
49	152.3	122.9	184.3
51	52.3	36.9	55.3
86	66.3	48.2	72.4




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

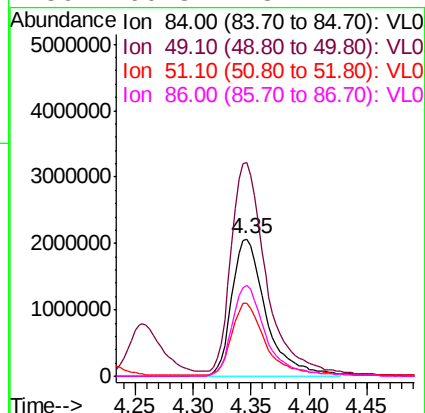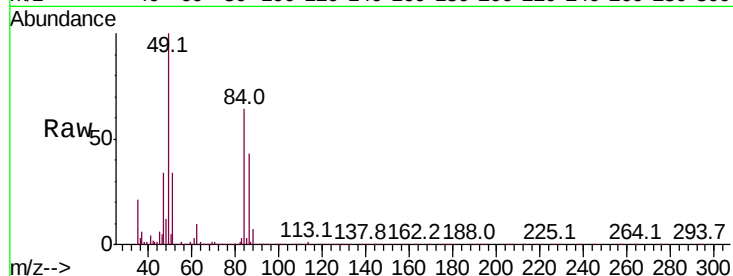

#26
Hexane
Concen: 28.395 ppbv
RT: 5.68 min Scan# 901
Delta R.T. -0.00 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	57	Resp	3977076
Ion	Ratio	Lower	Upper
57	100		
41	94.6	77.2	115.8
43	76.2	173.8	260.6#
56	54.2	43.8	65.6

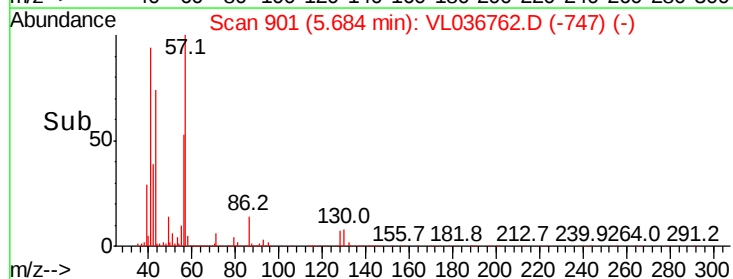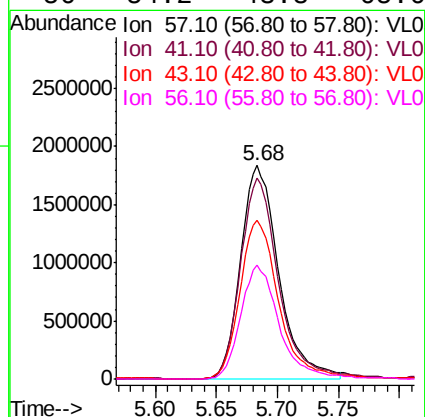

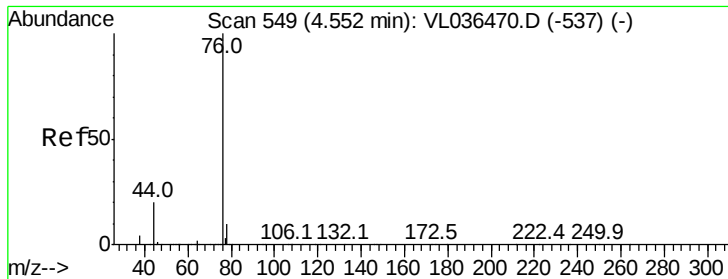





#27
Carbon Disulfide
Concen: 2.525 ppbv
RT: 4.54 min Scan# 546
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tot Ion	Ratio	Lower	Upper
76	100		
44	23.5	17.5	26.3
78	10.5	8.6	13.0




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

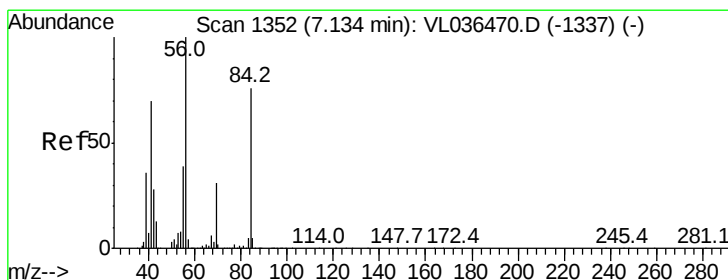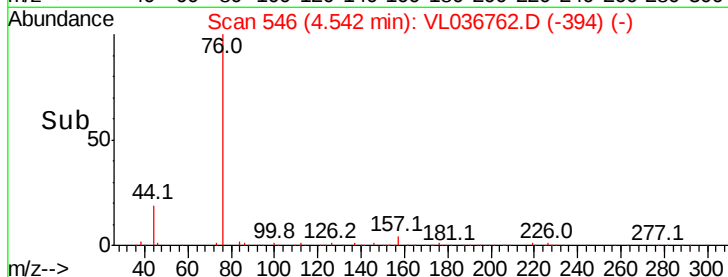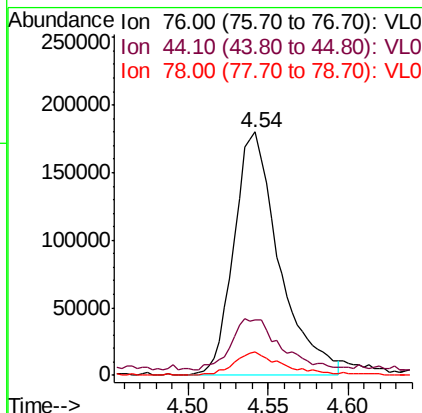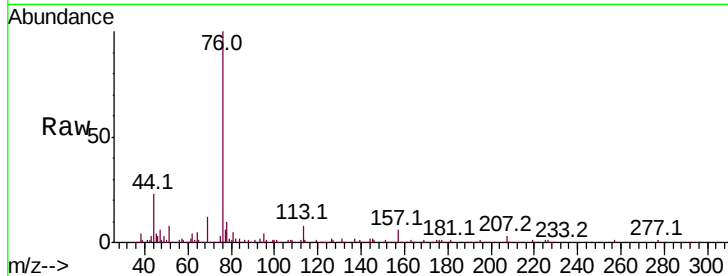

#30
Cyclohexane
Concen: 0.532 ppbv m
RT: 7.13 min Scan# 1351
Delta R.T. -0.00 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Lower	Upper
84	100		
56	0.0	114.6	171.8#
41	138.5	75.3	112.9#

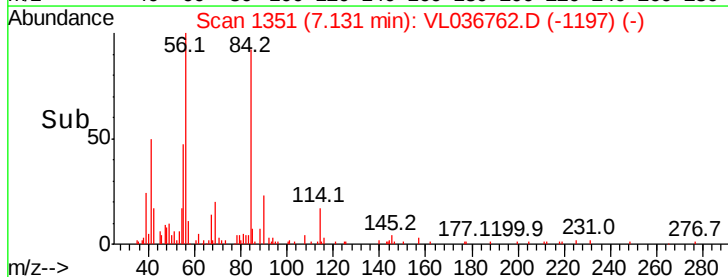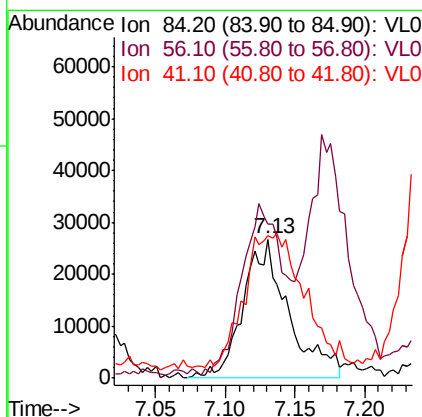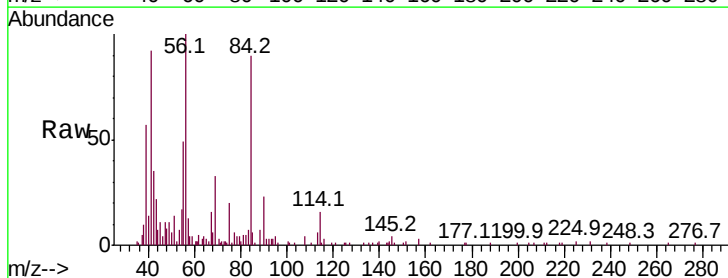



#31





cis-1,2-Dichloroethene
Concen: 0.238 ppbv m
RT: 5.56 min Scan# 861
Delta R.T. 0.00 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tot Ion	Ratio	Resp	Lower	Upper
61	100	32255		
96	57.9		48.7	73.1
98	40.2		31.4	47.0

Manual Integrations
APPROVED




MMDadoda
4/12/2021 11:47:37 AM

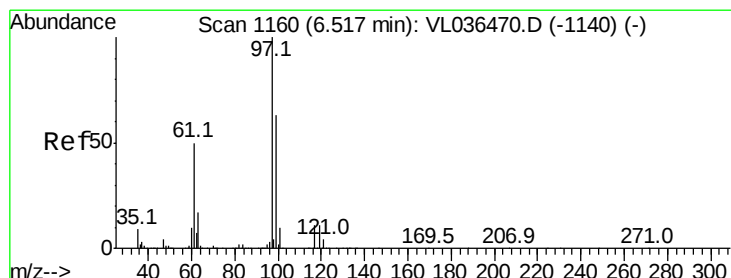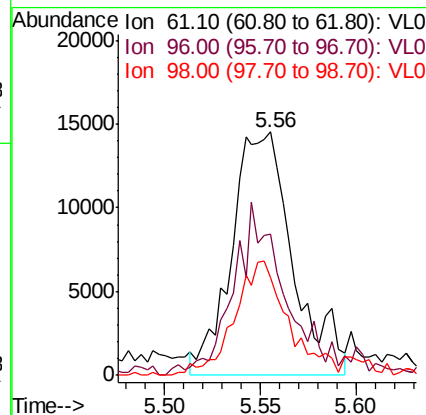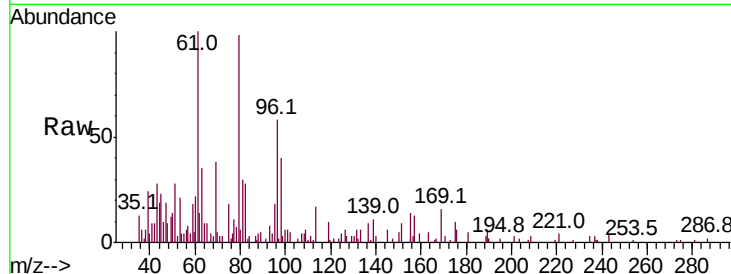


#32

1,1,1-Trichloroethane
Concen: 0.055 ppbv m
RT: 6.51 min Scan# 1158
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Resp	Lower	Upper
97	100	12400		
99	70.2		51.4	77.0
61	65.1		40.6	60.8#

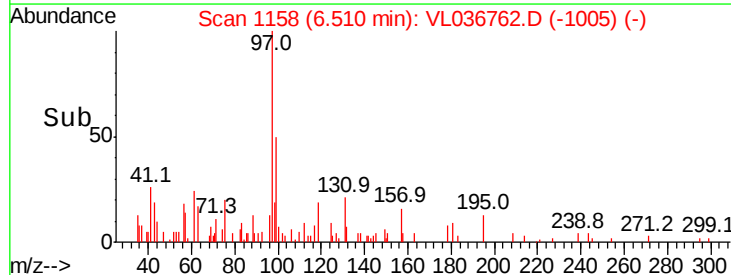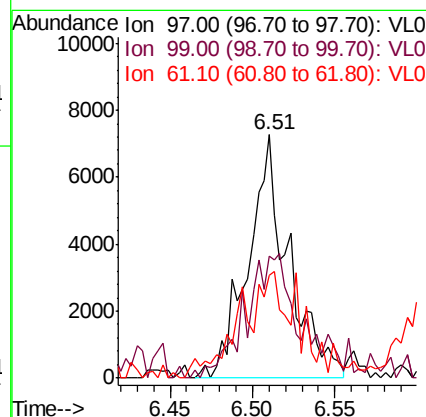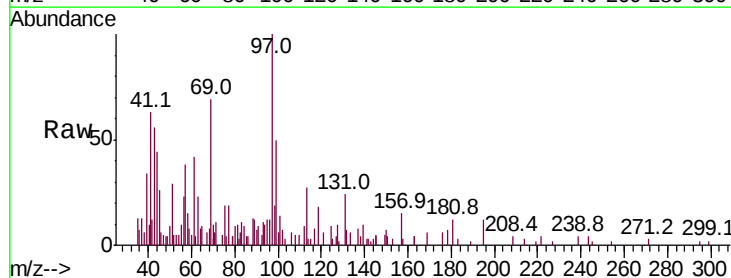

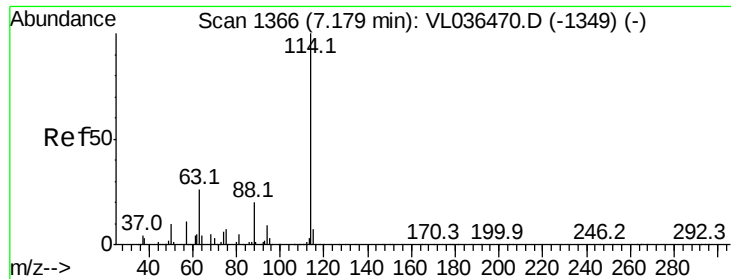

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.18 min Scan# 1365

Delta R.T. -0.00 min

Lab File: VL036762.D





Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tot Ion	Ratio	Lower	Upper
114	100		
63	26.8	22.4	33.6
88	19.1	15.4	23.0

Manual Integrations
APPROVED

MMDadoda
4/12/2021 11:47:37 AM

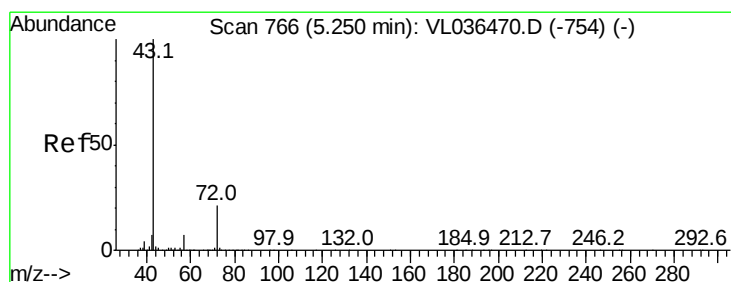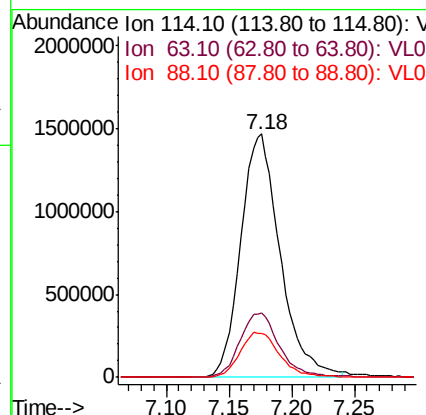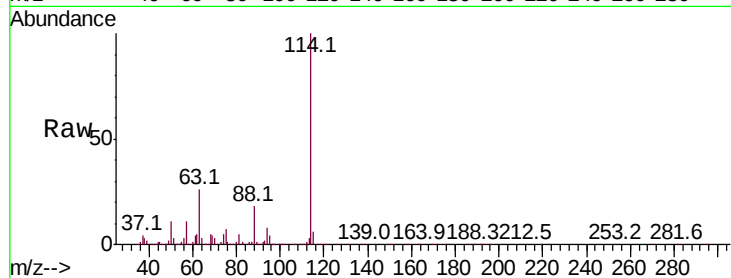

#34

2-Butanone

Concen: 14.158 ppbv




RT: 5.24 min Scan# 764


Delta R.T. -0.01 min

Lab File: VL036762.D

Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Lower	Upper
43	100		
72	21.0	17.0	25.6

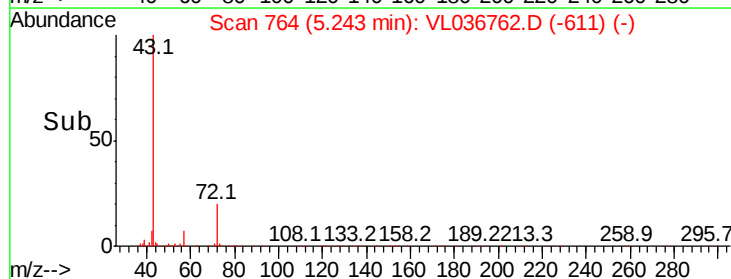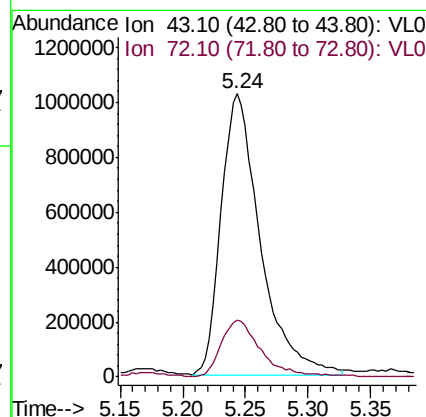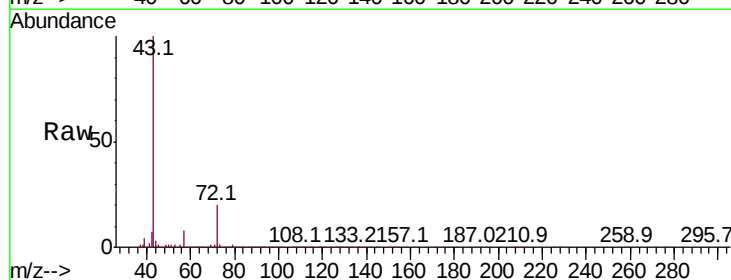

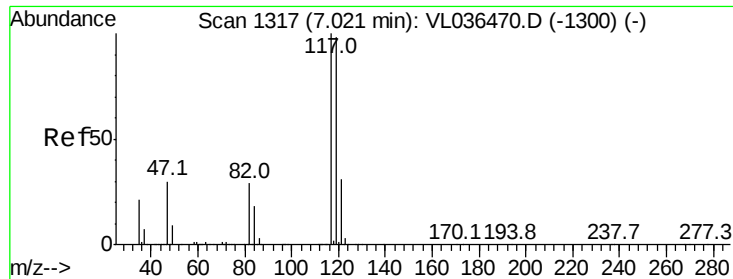





#35
Carbon Tetrachloride
Concen: 0.091 ppbv m
RT: 7.02 min Scan# 1316
Delta R.T. -0.00 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampled :
SG-1

Tot Ion	Ratio	Lower	Upper
117	100		
119	79.5	78.2	117.2
121	37.8	24.5	36.7#




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

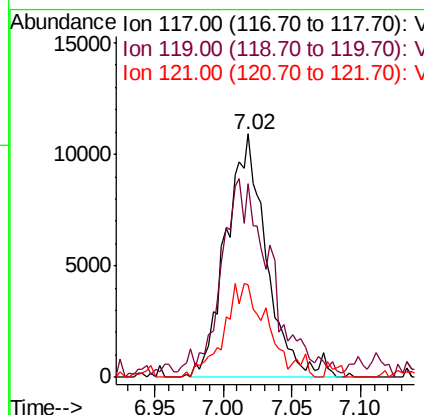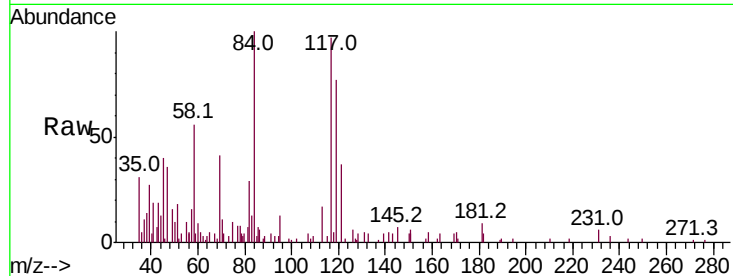

#36
Benzene
Concen: 3.224 ppbv
RT: 6.89 min Scan# 1276
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Lower	Upper
78	100		
77	22.8	18.0	27.0
50	20.7	16.5	24.7

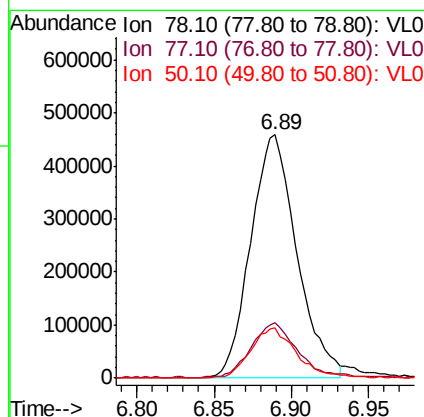

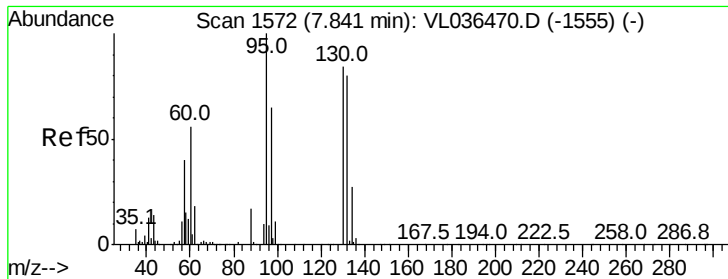





#38
 Trichloroethene
 Concen: 0.192 ppbv m
 RT: 7.83 min Scan# 1570
 Delta R.T. -0.01 min
 Lab File: VL036762.D
 Acq: 8 Apr 2021 23:10

Instrument :
 MSVOA_L
 ClientSampled :
 SG-1

Tot Ion	Ratio	Lower	Upper
130	100		
95	105.7	95.7	143.5
132	93.0	76.2	114.4
97	67.3	61.8	92.6




Manual Integrations
 APPROVED


MMDadoda
 4/12/2021 11:47:37 AM

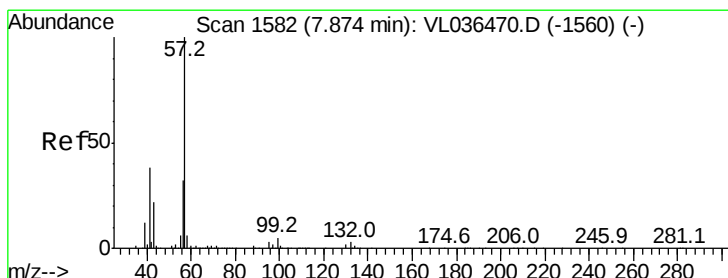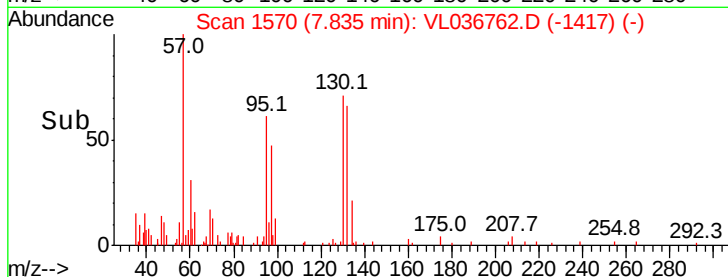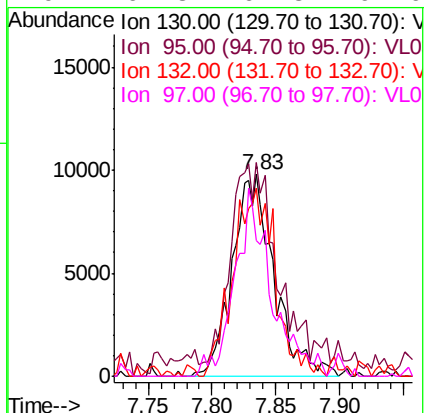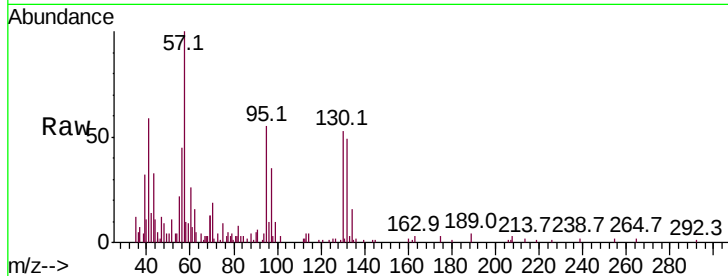

#44
 2,2,4-Trimethylpentane
 Concen: 0.462 ppbv m
 RT: 7.87 min Scan# 1580
 Delta R.T. -0.01 min
 Lab File: VL036762.D
 Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Lower	Upper
57	100		
41	45.4	28.8	43.2#
56	46.4	26.1	39.1#

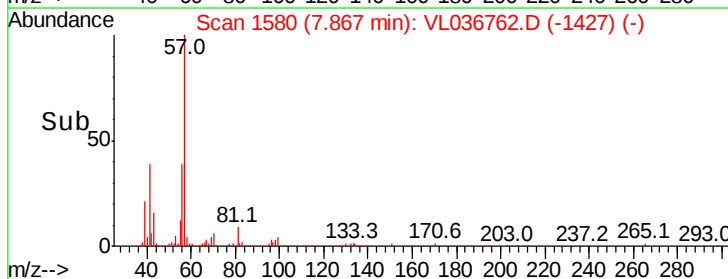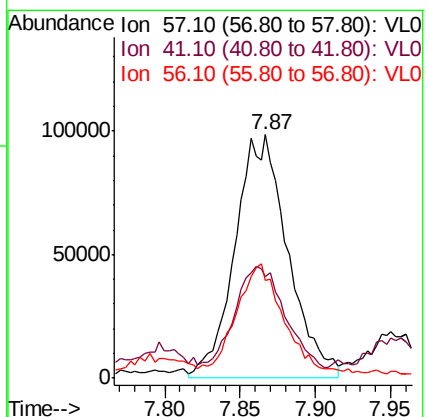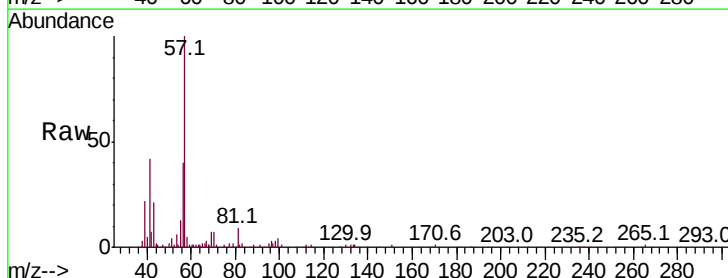

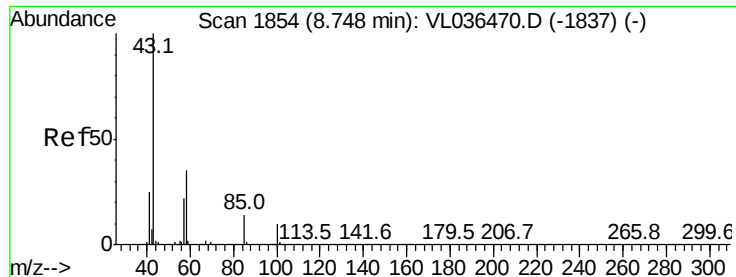





#50
4-Methyl-2-Pentanone
Concen: 2.461 ppbv
RT: 8.74 min Scan# 1851
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampled :
SG-1

Tot Ion	Ratio	Lower	Upper
43	100		
58	34.3	28.2	42.2




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

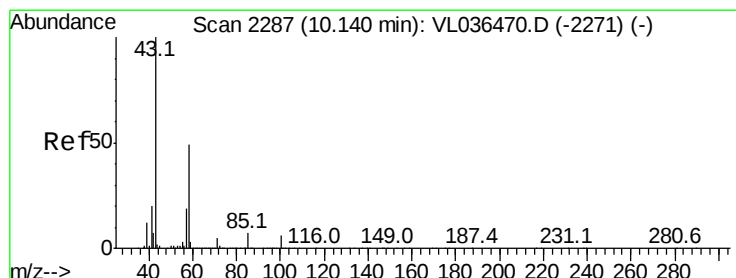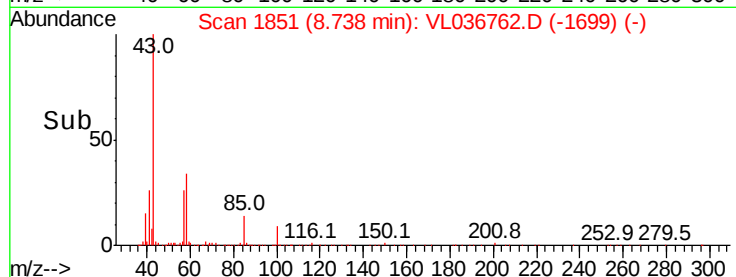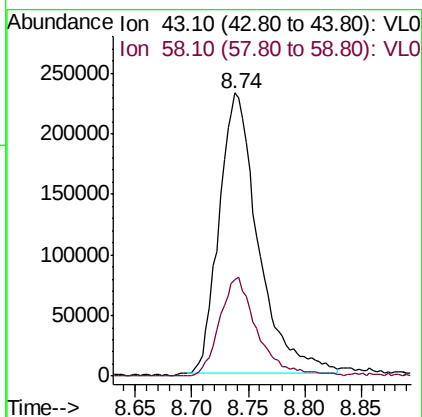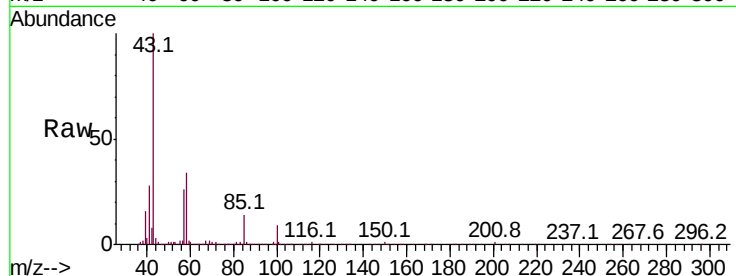

#51
2-Hexanone
Concen: 1.141 ppbv
RT: 10.13 min Scan# 2285
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Lower	Upper
43	100		
58	41.8	37.7	56.5
98	0.0	0.2	0.2#

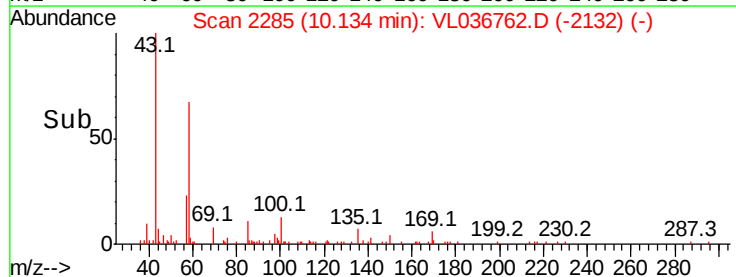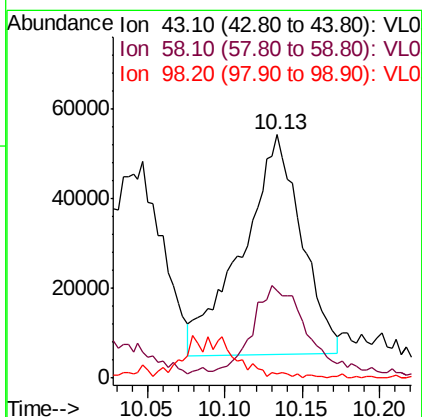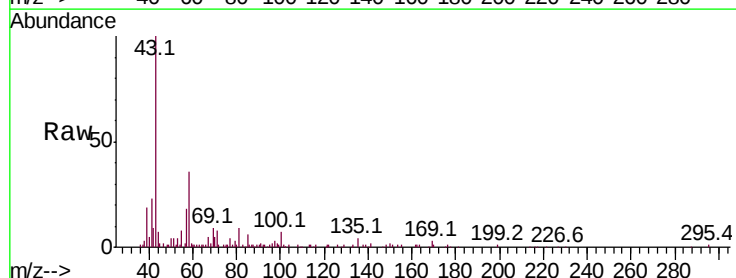







#52
Tetrachloroethene
Concen: 0.073 ppbv m
RT: 11.22 min Scan# 2624
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampled :
SG-1

Tot Ion	Ratio	Lower	Upper
164	100		
166	95.7	98.3	147.5#
129	92.8	85.8	128.8
131	66.0	80.9	121.3#




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

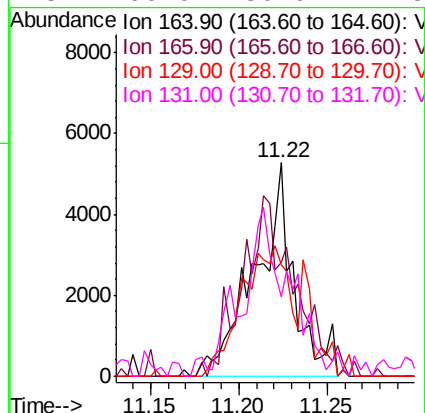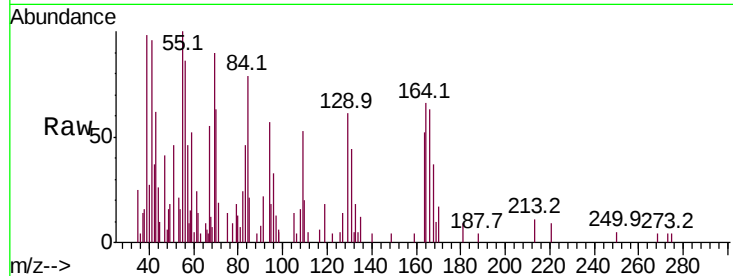

#53
Toluene
Concen: 2.419 ppbv
RT: 9.80 min Scan# 2180
Delta R.T. -0.02 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Lower	Upper
91	100		
92	60.6	48.8	73.2

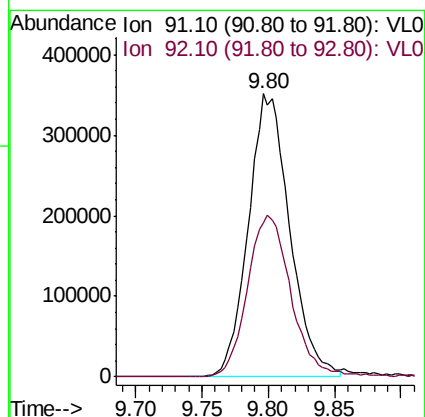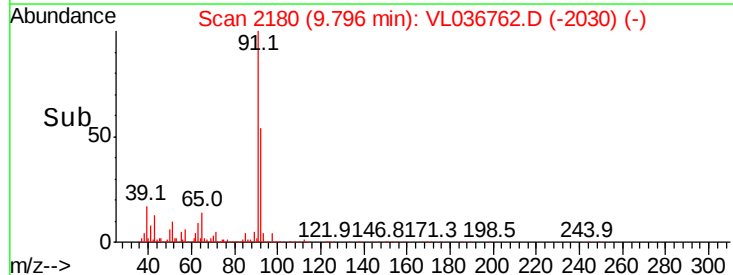







#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.08 min Scan# 2890
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampled :
SG-1

Tot Ion	Ratio	Lower	Upper
117	100		
82	65.6	57.4	86.0
119	33.6	47.4	71.0




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

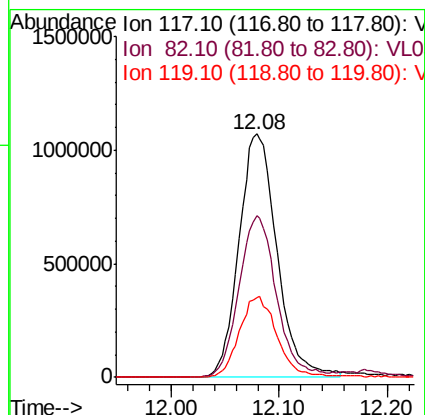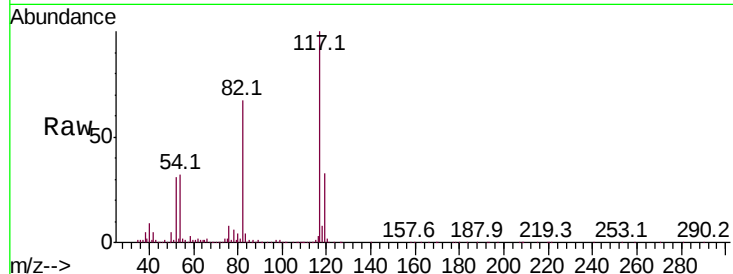

#58
Ethyl Benzene
Concen: 0.539 ppbv
RT: 12.70 min Scan# 3083
Delta R.T. -0.02 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Lower	Upper
91	100		
106	29.3	25.3	37.9

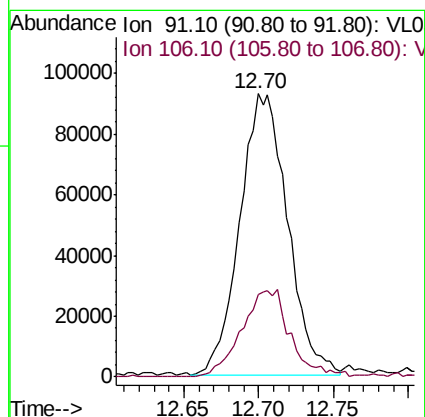

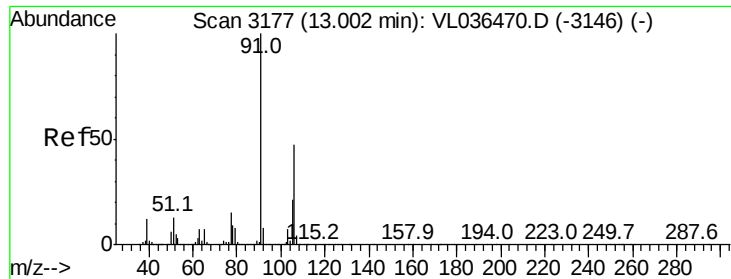





#59
m/p-Xylene
Concen: 1.136 ppbv m
RT: 12.96 min Scan# 3165
Delta R.T. -0.04 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampled :
SG-1

Tot Ion: 91 Resp: 378073
Ion Ratio Lower Upper
91 100
106 42.9 35.3 52.9




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

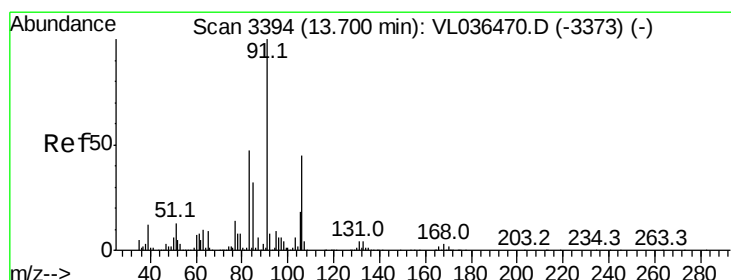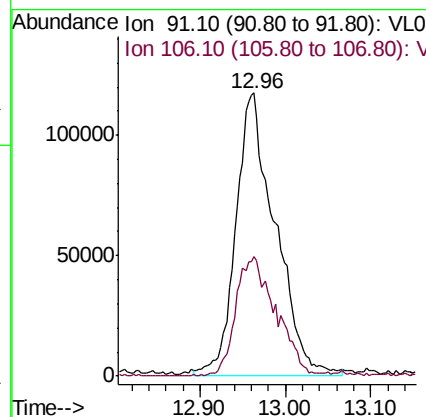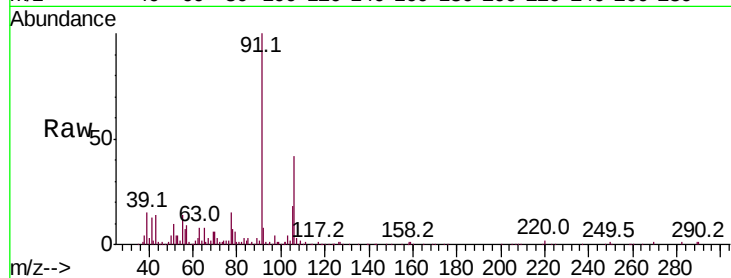

#60
o-Xylene
Concen: 0.756 ppbv m
RT: 13.68 min Scan# 3388
Delta R.T. -0.02 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion: 91 Resp: 243348
Ion Ratio Lower Upper
91 100
106 46.0 22.3 66.9

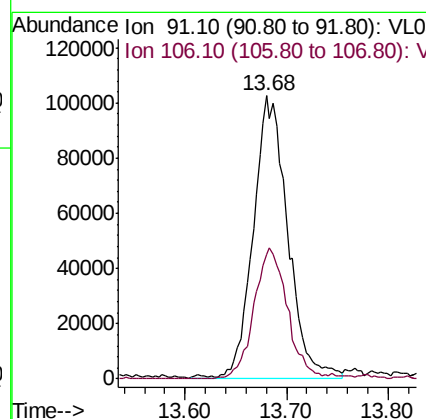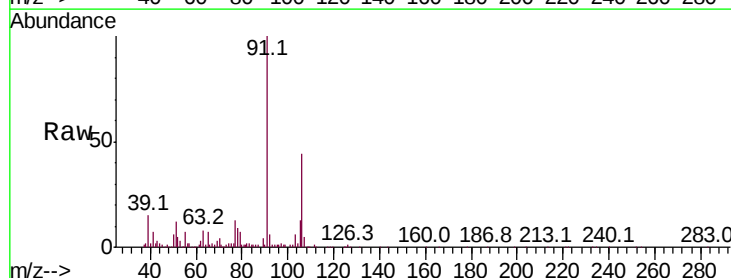

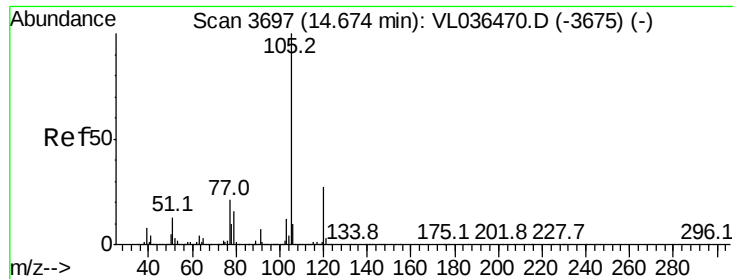





#62
Isopropylbenzene
Concen: 0.155 ppbv m
RT: 14.66 min Scan# 3694
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tot Ion: 105 Resp: 67098
Ion Ratio Lower Upper
105 100
120 26.5 20.6 31.0




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

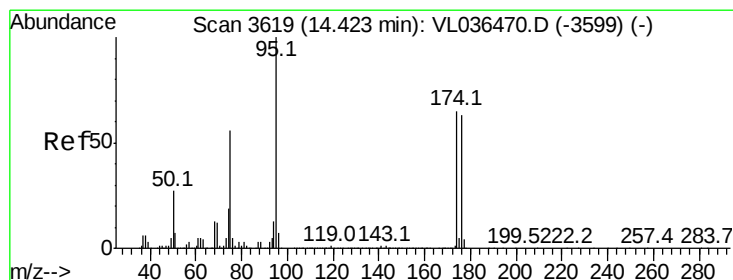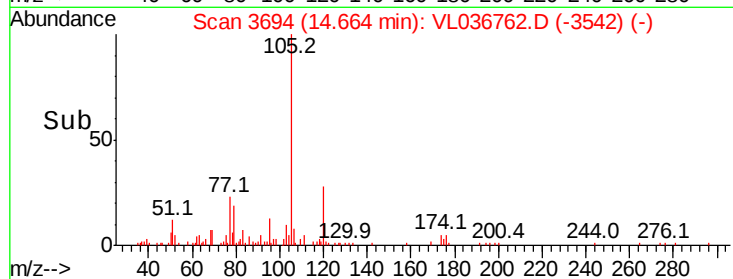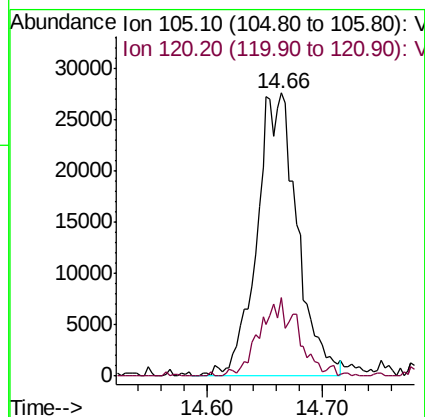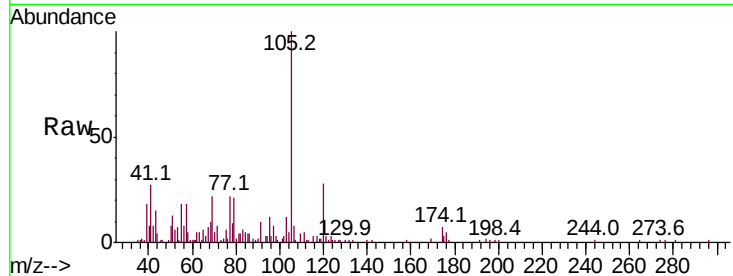

#68
1-Bromo-4-Fluorobenzene
Concen: 7.850 ppbv
RT: 14.41 min Scan# 3615
Delta R.T. -0.01 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion: 95 Resp: 1640501
Ion Ratio Lower Upper
95 100
174 68.7 51.0 76.6
175 5.3 3.9 5.9

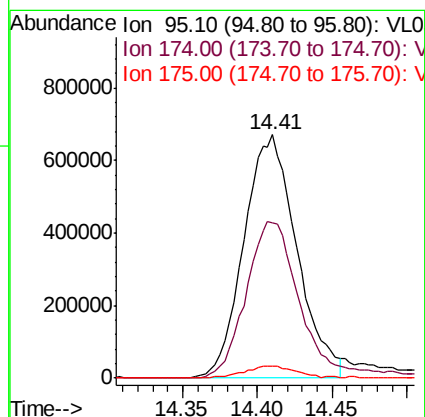

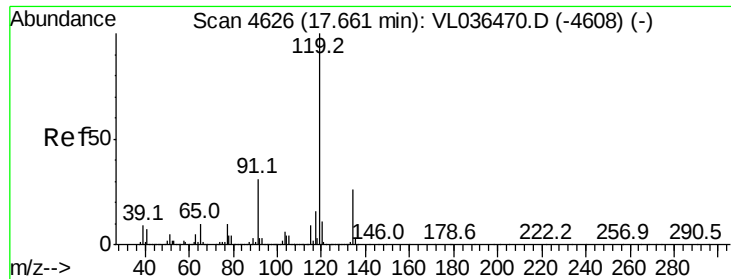





#69
p-Isopropyltoluene
Concen: 0.271 ppbv m
RT: 17.64 min Scan# 4621
Delta R.T. -0.02 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Instrument :
MSVOA_L
ClientSampleId :
SG-1

Tot Ion	Ratio	Resp	Lower	Upper
119	100			
134	24.0	20.6	30.8	
91	46.0	25.0	37.6	




Manual Integrations
APPROVED


MMDadoda
4/12/2021 11:47:37 AM

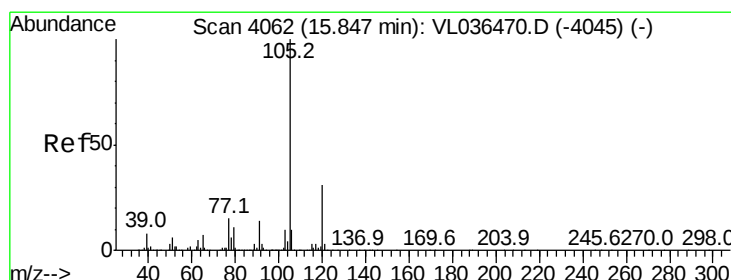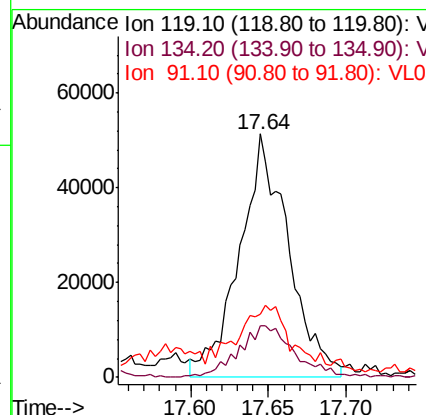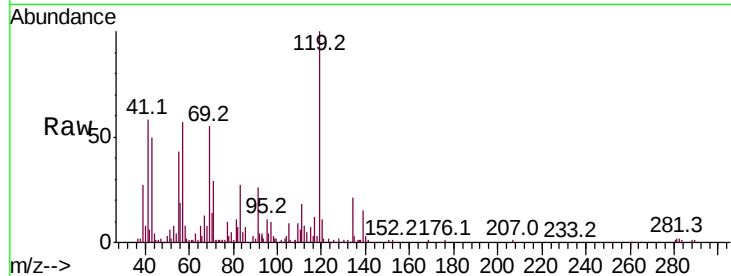

#72
4-Ethyltoluene
Concen: 0.169 ppbv
RT: 15.83 min Scan# 4057
Delta R.T. -0.02 min
Lab File: VL036762.D
Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Resp	Lower	Upper
105	100			
120	40.3	24.0	36.0	
91	20.0	11.0	16.4	
77	22.3	11.7	17.5	

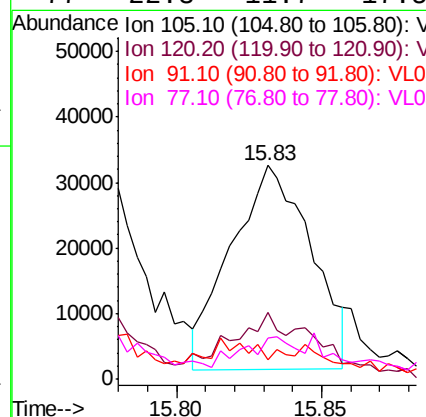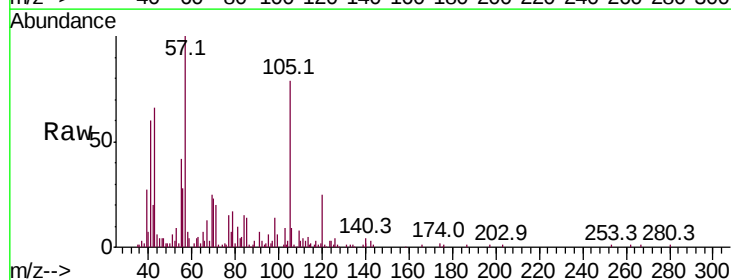

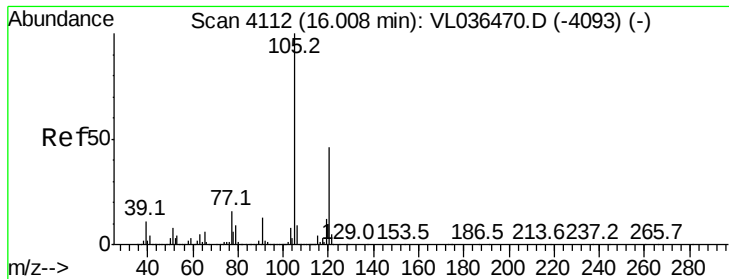

#73

1,3,5-Trimethylbenzene

Concen: 0.357 ppbv

RT: 15.99 min Scan# 4107

Delta R.T. -0.02 min

Lab File: VL036762.D

Acq: 8 Apr 2021 23:10

Instrument :

MSVOA_L

ClientSampled :

SG-1

Tot Ion:105 Resp: 117574

Ion Ratio Lower Upper


105 100

120 40.9 36.6 54.8

Manual Integrations
APPROVED

MMDadoda

4/12/2021 11:47:37 AM

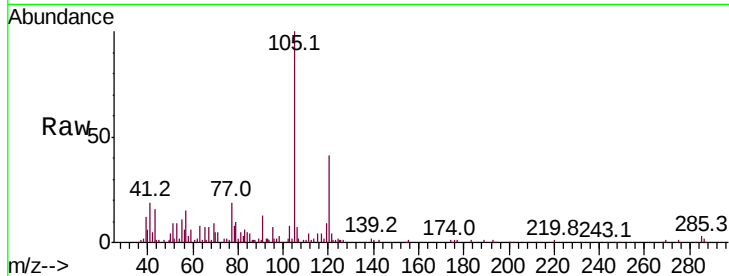

Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

60000

50000

40000

30000



20000

10000

0

15.90 15.95 16.00 16.05

Time-->

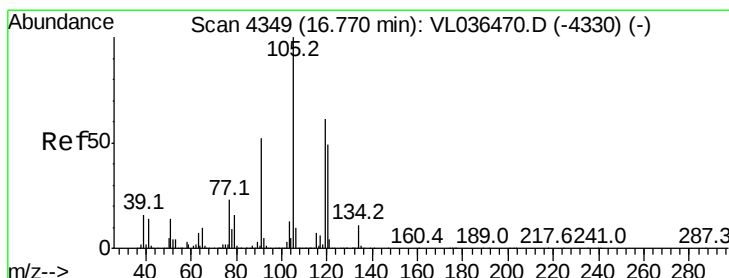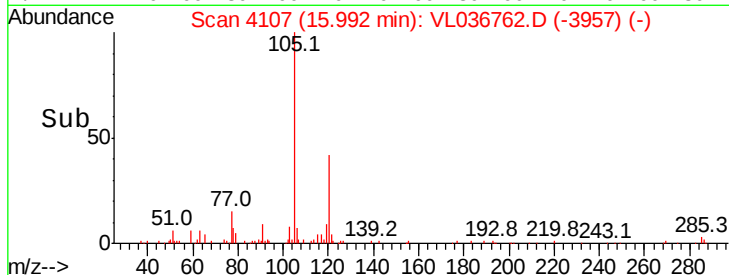

#74

1,2,4-Trimethylbenzene

Concen: 0.531 ppbv

RT: 16.75 min Scan# 4344

Delta R.T. -0.02 min

Lab File: VL036762.D

Acq: 8 Apr 2021 23:10

Tgt Ion:105 Resp: 187100

Ion Ratio Lower Upper

105 100

120 39.4 39.2 58.8

91 15.8 42.6 64.0#

77 13.5 18.6 28.0#

Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

120000

100000

80000

60000



40000


20000

0

16.70 16.75 16.80

Time-->

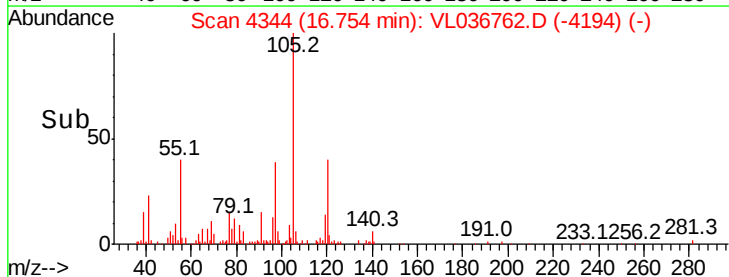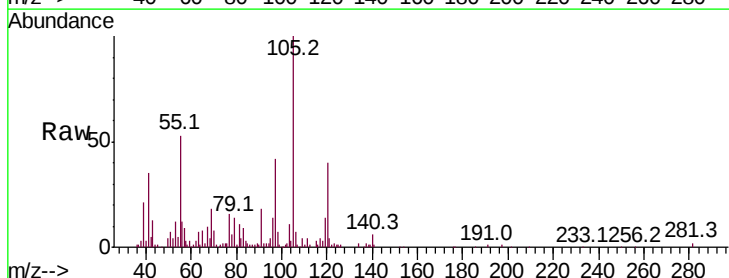

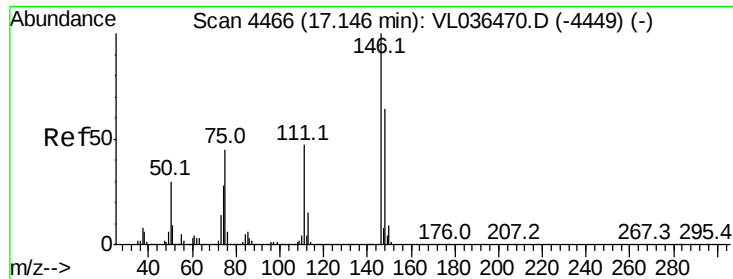





#76
 1,4-Dichlorobenzene
 Concen: 0.144 ppbv m
 RT: 17.13 min Scan# 4460
 Delta R.T. -0.02 min
 Lab File: VL036762.D
 Acq: 8 Apr 2021 23:10

Instrument :
 MSVOA_L
 ClientSampled :
 SG-1

Tot Ion	Ratio	Lower	Upper
146	100		
111	116.0	24.3	72.8#
148	63.7	33.0	98.9

Manual Integrations
 APPROVED

MMDadoda
 4/12/2021 11:47:37 AM

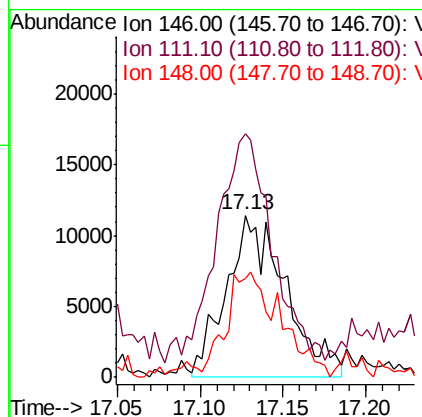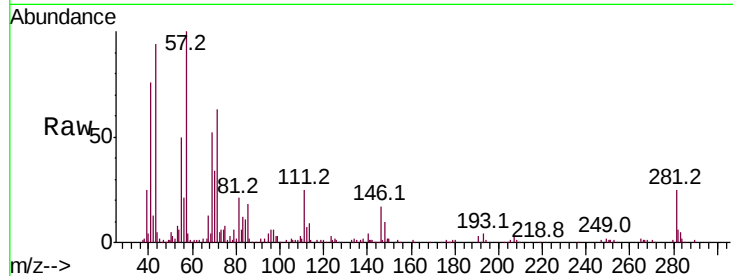

#79
 Naphthalene
 Concen: 0.193 ppbv m
 RT: 22.21 min Scan# 6041
 Delta R.T. 0.01 min
 Lab File: VL036762.D
 Acq: 8 Apr 2021 23:10

Tgt Ion	Ratio	Lower	Upper
128	100		
127	13.0	10.9	16.3
129	6.9	9.0	13.4#

