


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL040821\  
 Data File : VL036745.D  
 Acq On : 8 Apr 2021 9:55  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 400mL/MSVOA L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL032521AIR.M  
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Thu Mar 25 09:42:40 2021  
 Last Update : Thu Mar 25 09:42:40 2021

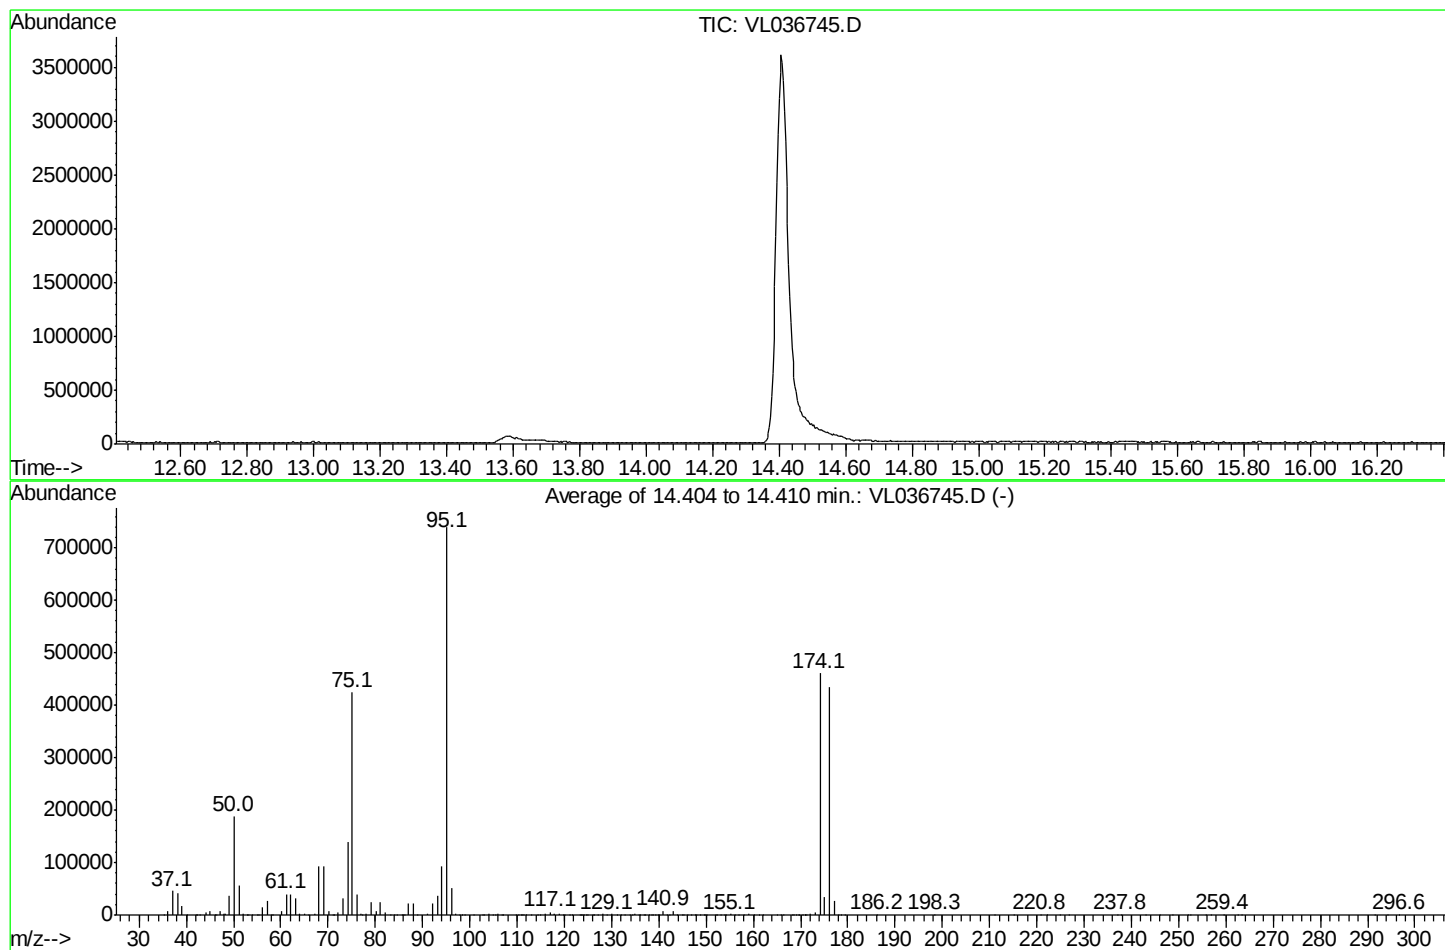

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3585

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 25.4      | 187484  | PASS             |
| 75          | 95           | 30           | 66           | 57.4      | 424298  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 738880  | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 51146   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 4251    | PASS             |
| 174         | 95           | 50           | 120          | 62.3      | 460224  | PASS             |
| 175         | 174          | 4            | 9            | 7.7       | 35216   | PASS             |
| 176         | 174          | 93           | 101          | 94.3      | 433834  | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 27242   | PASS             |