

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL041019\
Data File : VL033566.D
Acq On : 10 Apr 2019 16:17
Operator : SY/AP
Sample : QC040319 CAN 10284
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC040319 CAN 10284

Quant Time: Apr 11 04:00:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032519AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019
QLast Update : Tue Mar 26 16:00:50 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.76	49	931891	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.29	114	2324996	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.24	117	2262843	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.58	95	1773996	10.00	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.00%


Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL041019\
Data File : VL033566.D
Acq On : 10 Apr 2019 16:17
Operator : SY/AP
Sample : QC040319 CAN 10284
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC040319 CAN 10284

Quant Time: Apr 11 04:00:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019
QLast Update : Tue Mar 26 16:00:50 2019
Response via : Initial Calibration

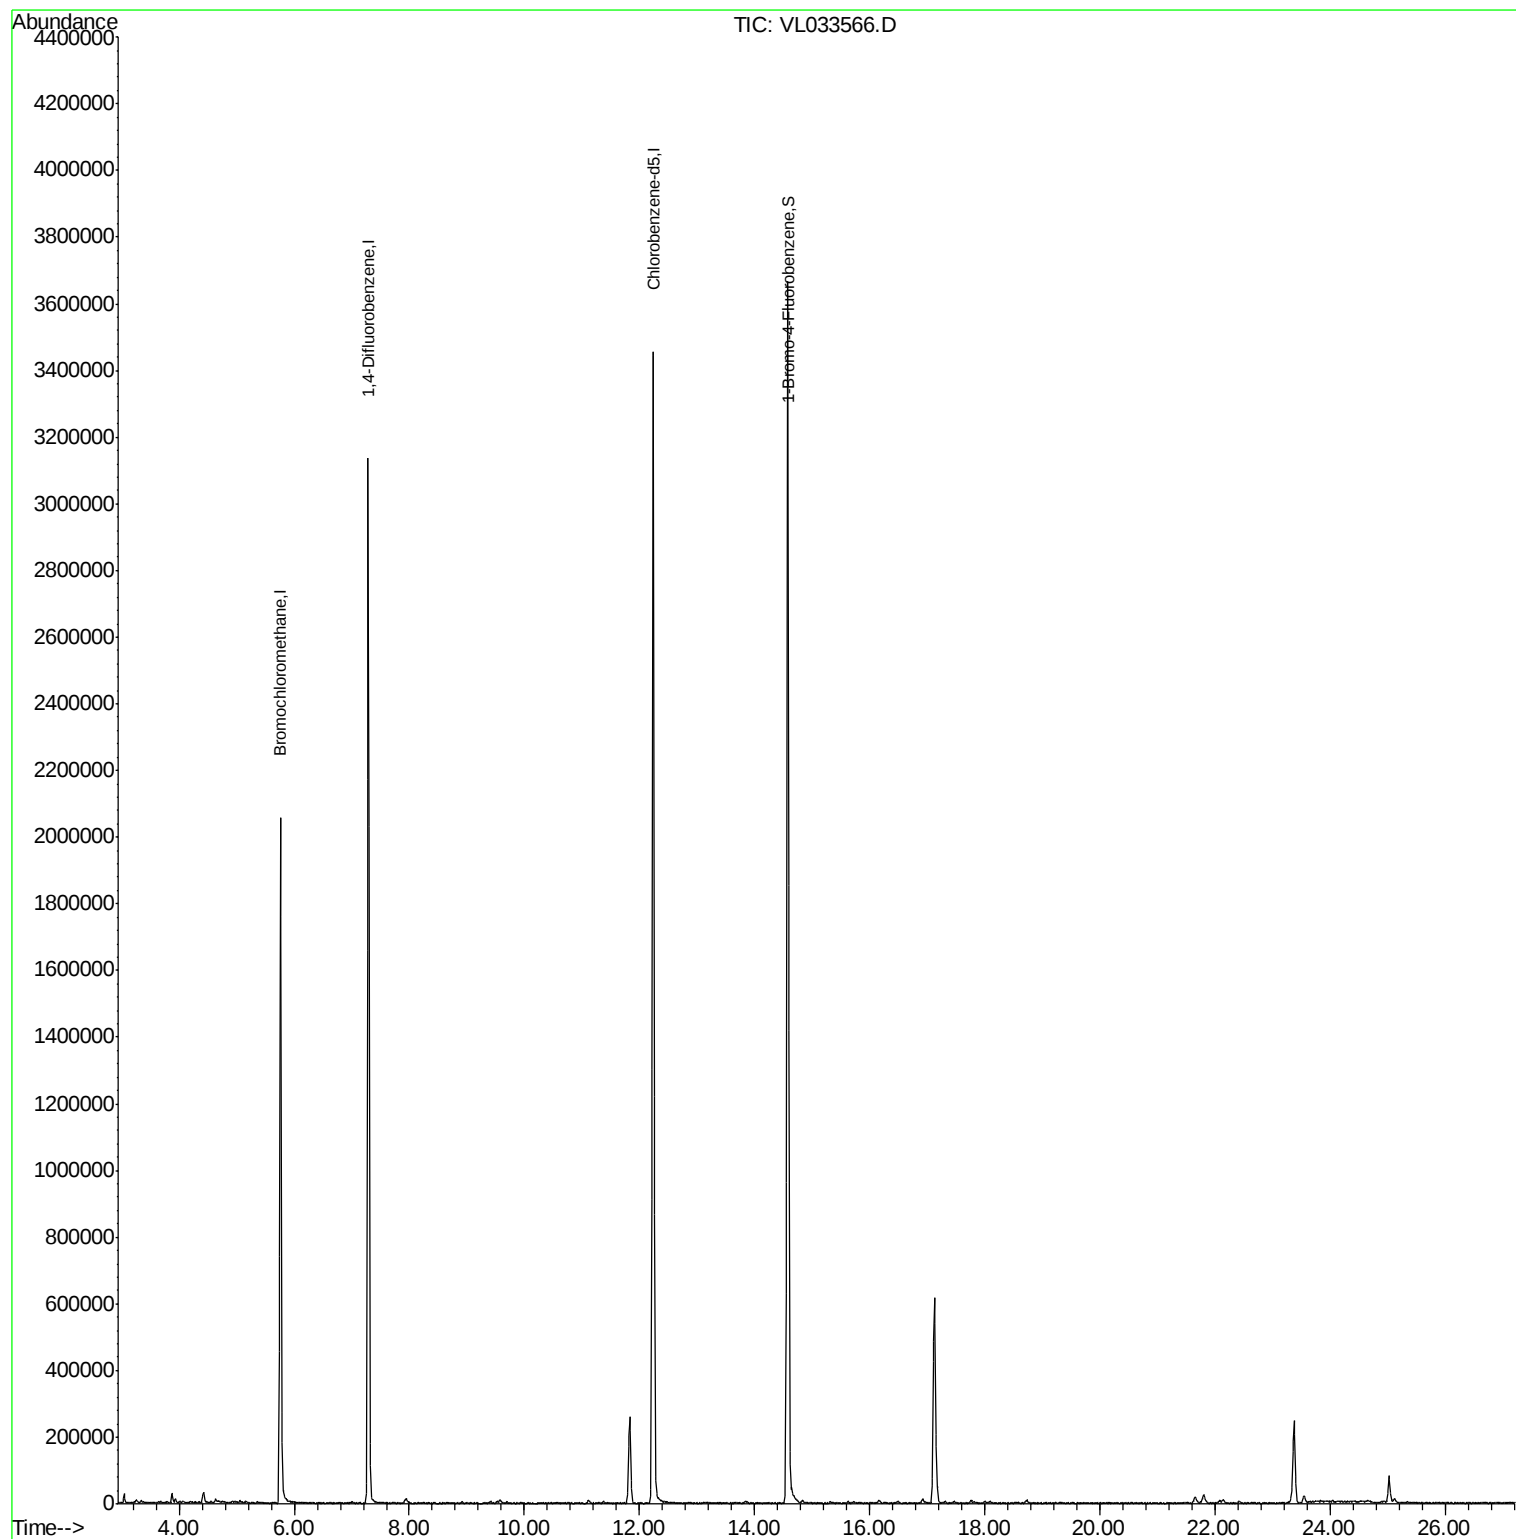



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.76 min Scan# 878

Delta R.T. -0.00 min

Lab File: VL033566.D

Acq: 10 Apr 2019 16:17

Instrument :

MSVOA_L

ClientSampleId :

QC040319 CAN 10284


Tot Ion: 49 Resp: 931891

Ion Ratio Lower Upper

49 100

128 51.3 24.0 72.0




130 66.1 31.2 93.6

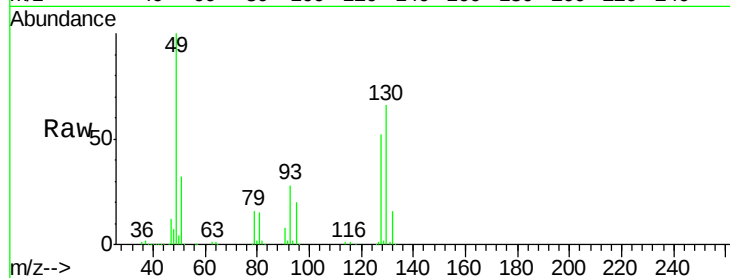

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

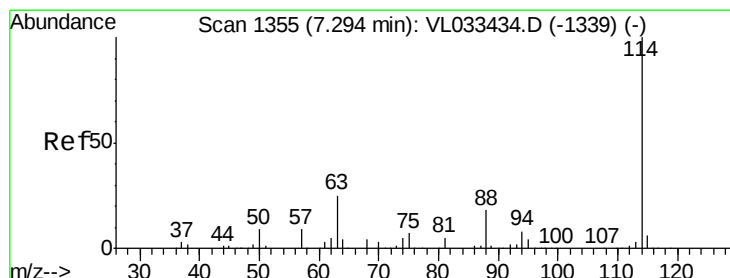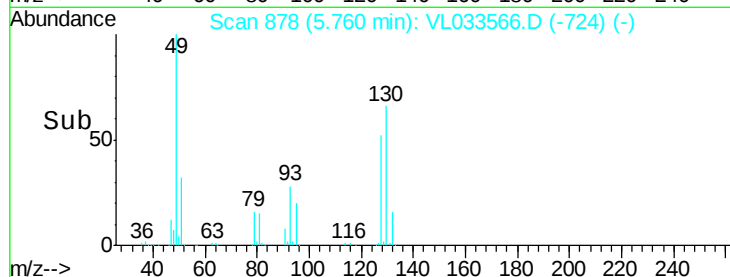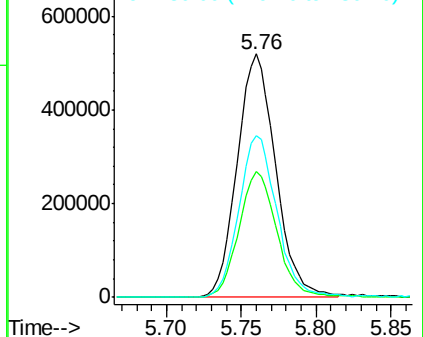

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.29 min Scan# 1353

Delta R.T. -0.01 min

Lab File: VL033566.D

Acq: 10 Apr 2019 16:17


Tgt Ion: 114 Resp: 2324996

Ion Ratio Lower Upper

114 100

63 24.7 21.5 32.3



88 17.6 14.5 21.7

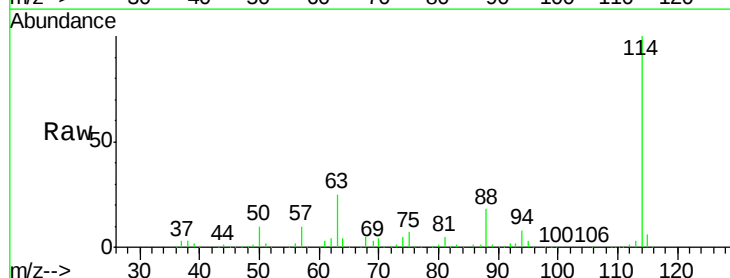


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



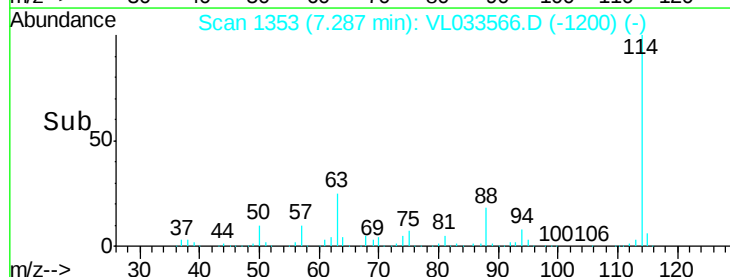
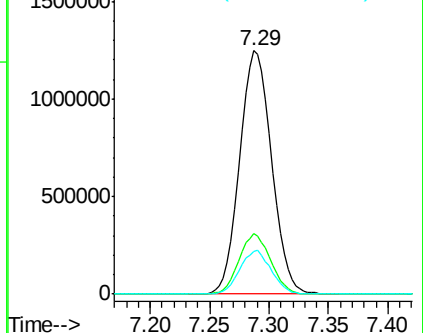


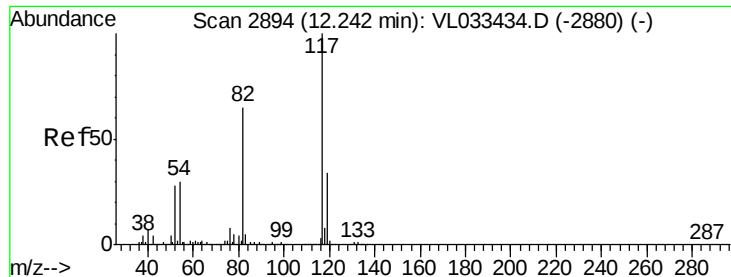

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.24 min Scan# 2892
Delta R.T. -0.01 min
Lab File: VL033566.D
Acq: 10 Apr 2019 16:17

Instrument :
MSVOA_L
ClientSampleId :
QC040319 CAN 10284

Tot Ion:117 Resp: 2262843
Ion Ratio Lower Upper
117 100
82 64.1 51.5 77.3
119 32.4 25.5 38.3

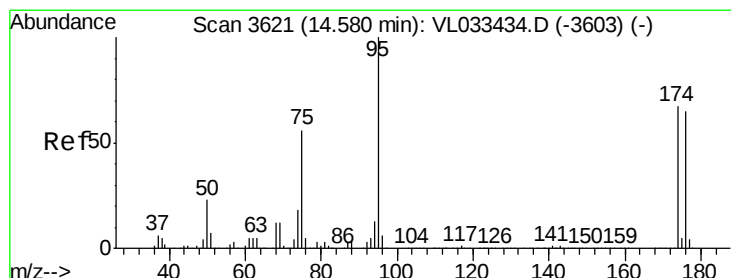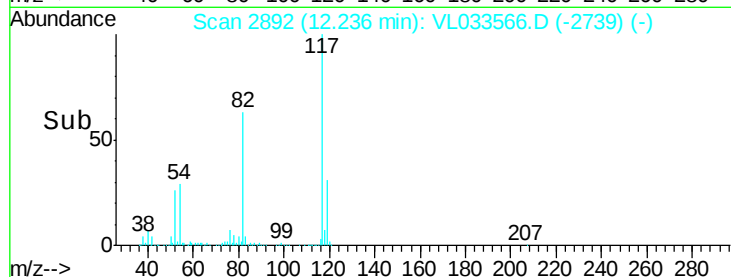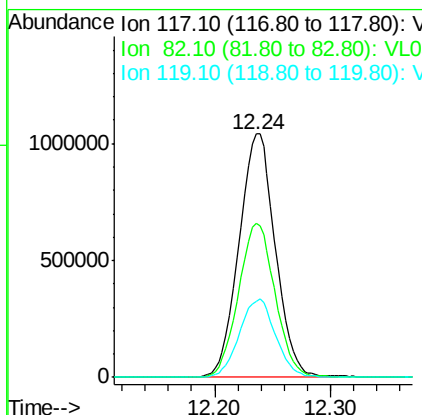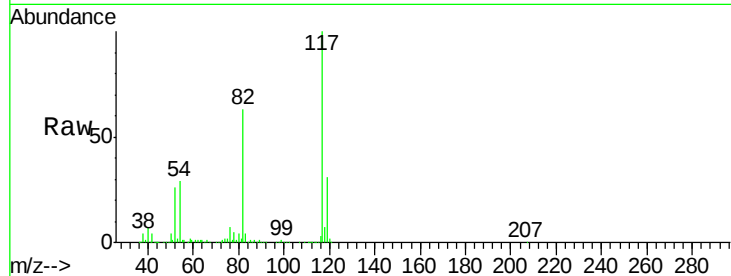

#68
1-Bromo-4-Fluorobenzene
Concen: 10.000 ppbv
RT: 14.58 min Scan# 3620
Delta R.T. -0.00 min
Lab File: VL033566.D
Acq: 10 Apr 2019 16:17

Tgt Ion: 95 Resp: 1773996
Ion Ratio Lower Upper
95 100
174 69.8 52.9 79.3
175 4.9 3.8 5.6

