

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041019\
 Data File : VL033577.D
 Acq On : 10 Apr 2019 23:37
 Operator : SY/AP
 Sample : K2312-02
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 A-7

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 3
 Start Thrs: 0.001
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 0

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032519AIR.M

Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.992	6	17	30	rBV	5728819	7796463	100.00%	19.920%
2	3.049	30	35	41	rVV2	122378	172440	2.21%	0.441%
3	3.239	82	94	104	rBV2	220572	286741	3.68%	0.733%
4	3.394	133	142	152	rVB2	133664	174069	2.23%	0.445%
5	3.654	208	223	246	rBV	882479	1717775	22.03%	4.389%
6	3.902	289	300	321	rBV	572005	909689	11.67%	2.324%
7	4.033	324	341	362	rVB2	224336	503881	6.46%	1.287%
8	4.191	381	390	399	rBV2	68981	98191	1.26%	0.251%
9	4.410	437	458	472	rBV	501372	828279	10.62%	2.116%
10	5.766	862	880	900	rBV3	2396572	5487523	70.38%	14.021%
11	7.287	1338	1353	1368	rBV	2731725	5059991	64.90%	12.928%
12	7.368	1368	1378	1389	rVB4	63688	132926	1.70%	0.340%
13	7.596	1436	1449	1451	rBV3	81055	107078	1.37%	0.274%
14	8.242	1640	1650	1664	rVB5	71656	140232	1.80%	0.358%
15	9.943	2160	2179	2198	rBV	659187	1326700	17.02%	3.390%
16	10.766	2421	2435	2450	rVB5	41789	96677	1.24%	0.247%
17	12.236	2872	2892	2915	rBV	3012687	6575241	84.34%	16.800%
18	14.573	3599	3619	3648	rBV2	3183745	7170430	91.97%	18.321%
19	17.123	4395	4412	4427	rBV4	48955	132100	1.69%	0.338%
20	18.110	4705	4719	4736	rBV8	111895	268430	3.44%	0.686%
21	21.647	5799	5819	5838	rBV2	49829	153850	1.97%	0.393%


Sum of corrected areas: 39138706

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041019\
Data File : VL033577.D
Acq On : 10 Apr 2019 23:37
Operator : SY/AP
Sample : K2312-02
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
A-7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

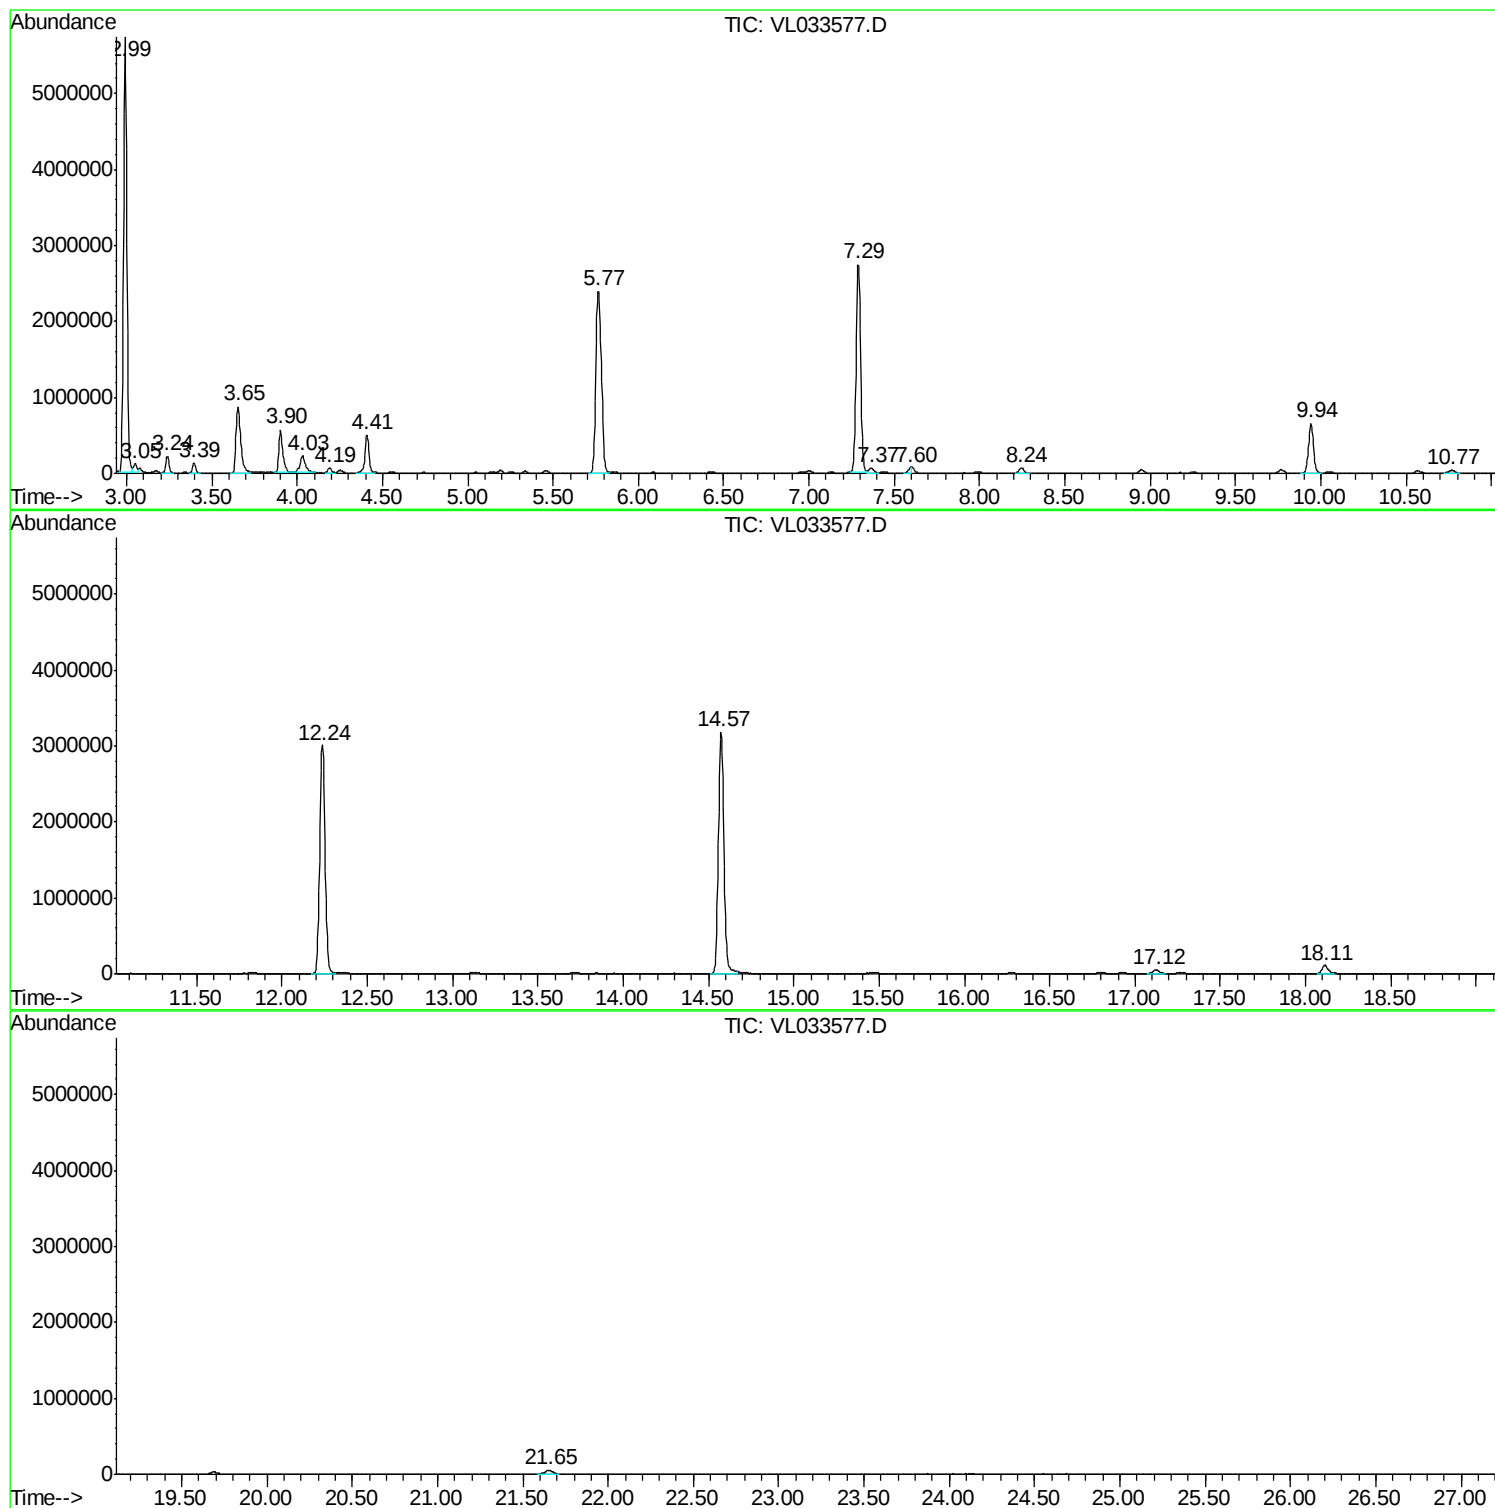

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041019\
Data File : VL033577.D
Acq On : 10 Apr 2019 23:37
Operator : SY/AP
Sample : K2312-02
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
A-7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041019\
Data File : VL033577.D
Acq On : 10 Apr 2019 23:37
Operator : SY/AP
Sample : K2312-02
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
A-7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc