
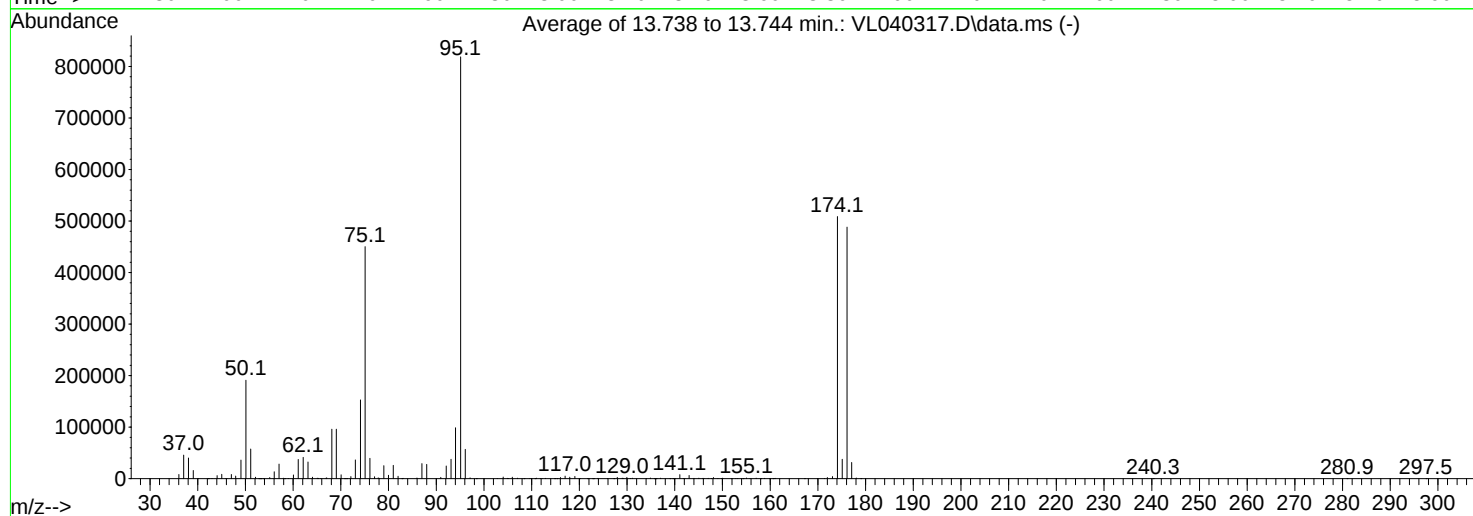


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041023\
 Data File : VL040317.D
 Acq On : 10 Apr 2023 9:37
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031523AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Apr 11 04:15:53 2023

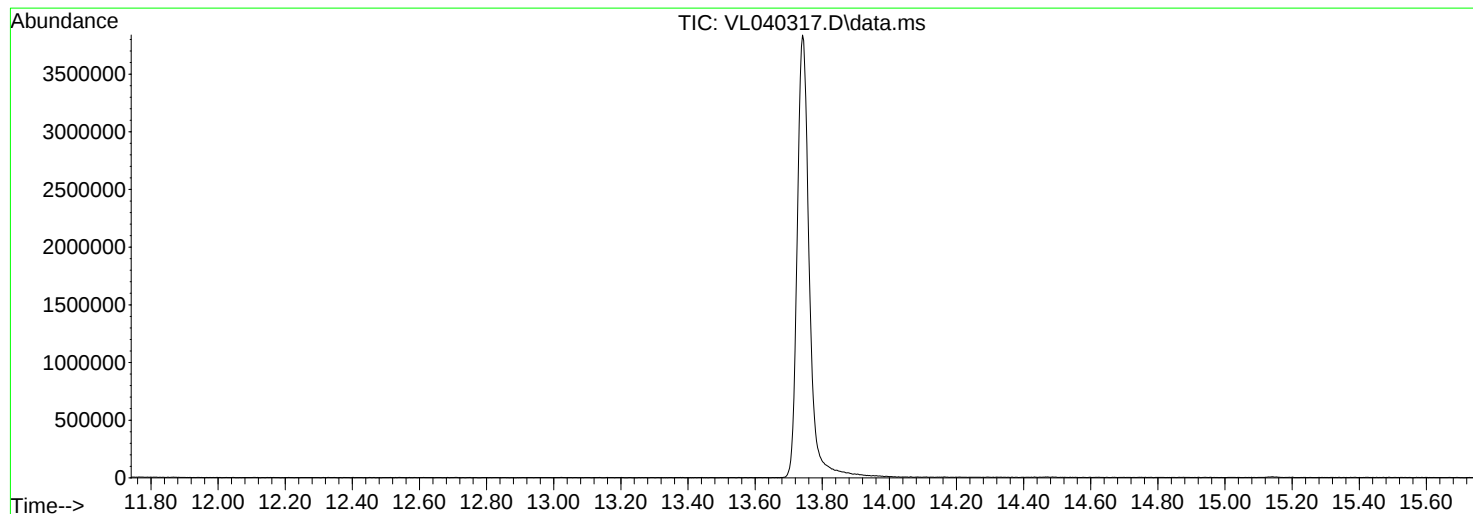

AutoFind: Scans 3463, 3464, 3465; Background Corrected with Scan 3441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.3	190848	PASS
75	95	30	66	55.0	450176	PASS
95	95	100	100	100.0	818667	PASS
96	95	5	9	7.0	57019	PASS
173	174	0.00	2	0.8	4202	PASS
174	95	50	120	62.2	508843	PASS
175	174	4	9	7.4	37707	PASS
176	174	93	101	96.0	488256	PASS
177	176	5	9	6.4	31293	PASS

Average of 13.738 to 13.744 min.: VL040317.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8083	47.05	8050	56.05	13289	65.30	691
37.05	45555	47.95	4977	57.05	28376	65.80	20
38.05	40035	49.05	36133	57.95	883	66.90	80
39.05	15999	50.10	190848	58.20	189	67.05	155
40.20	235	51.10	57451	59.00	385	68.10	95899
42.20	50	52.10	2659	60.05	7010	69.05	95931
43.00	392	52.80	57	61.05	37128	70.05	7563
44.05	5957	53.10	76	62.10	41429	70.80	66
45.05	8318	53.30	71	63.10	32405	71.20	54
45.90	434	53.80	57	64.05	2826	72.10	3955
46.10	231	55.10	2301	65.05	943	73.05	36213

Average of 13.738 to 13.744 min.: VL040317.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.10	152683	83.05	525	98.40	103	111.00	947
75.10	450176	85.95	1128	102.80	273	111.85	317
76.10	39325	87.00	29328	104.05	3204	112.20	314
77.05	3730	88.00	27667	104.90	586	112.90	513
77.85	1538	90.95	2480	105.10	328	114.80	178
78.10	701	92.10	24464	105.95	2746	115.00	449
79.00	25117	93.10	37709	107.05	902	115.30	94
80.00	6553	94.05	98837	108.40	54	116.05	2249
81.00	25723	95.10	818667	109.65	361	117.00	4937
82.00	4826	96.10	57019	110.00	346	118.00	2925
82.80	157	97.10	1451	110.70	181	119.05	4395

Average of 13.738 to 13.744 min.: VL040317.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
120.00	51	129.95	2427	139.90	253	147.70	240
121.70	120	130.70	327	140.10	355	148.10	2177
122.05	281	131.10	977	141.05	7916	149.05	241
122.80	54	134.05	360	141.80	259	149.80	268
123.00	176	134.90	1227	142.10	241	150.05	840
123.90	521	135.70	152	143.00	6348	151.85	111
125.90	363	135.90	98	144.00	581	152.80	299
127.20	100	136.10	65	145.05	1097	153.20	365
127.95	2605	137.05	1037	145.90	634	154.00	348
129.00	955	139.00	179	146.10	520	154.30	93
129.20	542	139.60	76	147.00	552	155.05	1189

Average of 13.738 to 13.744 min.: VL040317.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.80	307	172.00	2286				
157.05	1117	173.05	4202				
158.00	58	174.10	508843				
158.85	774	175.10	37707				
159.90	89	176.10	488256				
160.60	165	177.10	31293				
160.90	364	178.05	1251				
161.15	528	179.00	68				
167.20	87	240.30	63				
169.90	200	280.95	159				
171.40	224	297.50	126				