
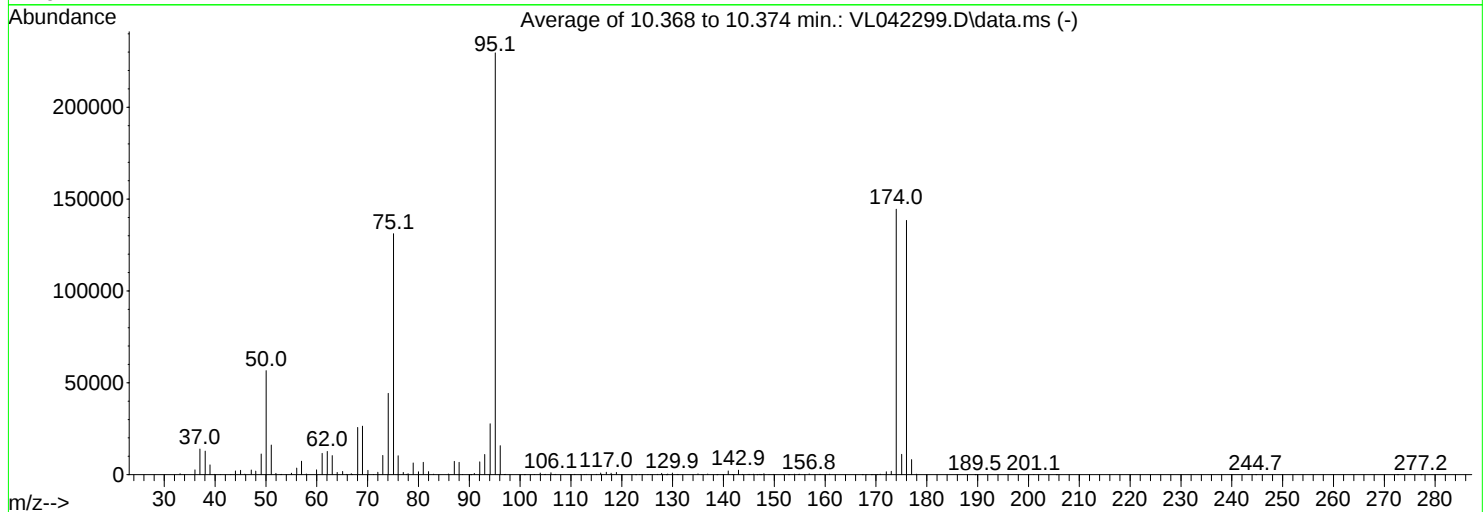


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
Data File : VL042299.D
Acq On : 10 Apr 2025 08:46
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

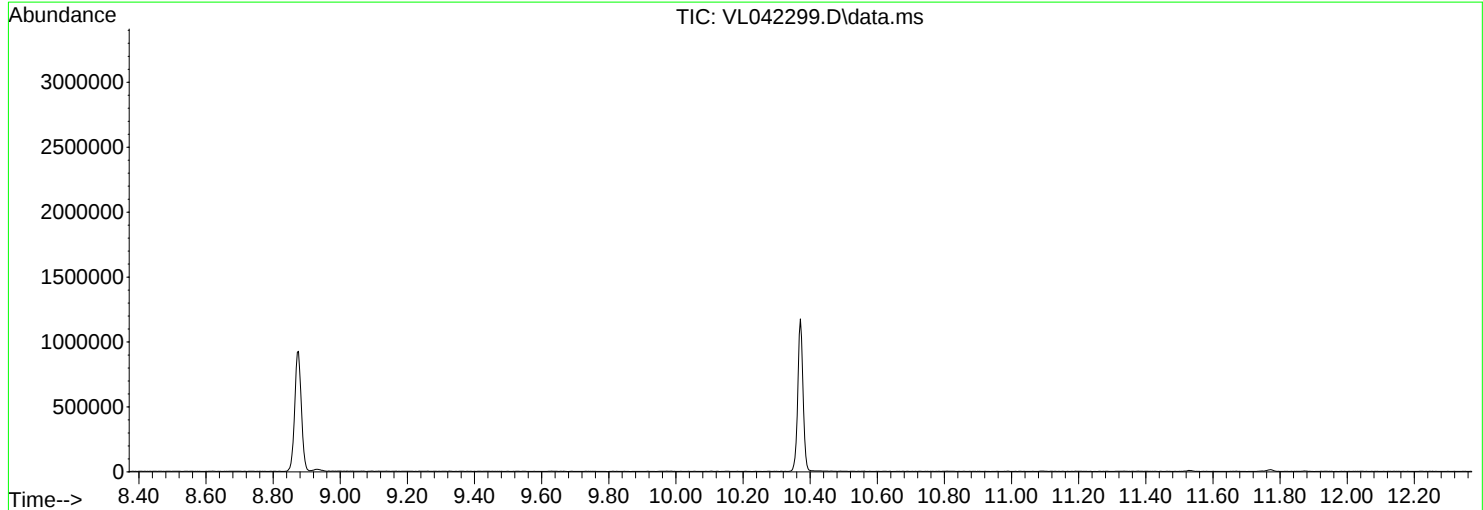

AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.7	56629	PASS
75	95	30	66	57.1	131205	PASS
95	95	100	100	100.0	229611	PASS
96	95	5	9	6.9	15747	PASS
173	174	0.00	2	1.3	1863	PASS
174	95	50	120	62.9	144533	PASS
175	174	4	9	7.7	11082	PASS
176	174	93	101	95.7	138363	PASS
177	176	5	9	5.9	8219	PASS

Average of 10.368 to 10.374 min.: VL042299.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	542	45.85	292	56.05	3600	67.05	81
33.95	84	47.10	2565	57.00	7283	68.05	2569
36.05	2659	48.00	1913	57.95	377	69.00	2641
37.00	13919	49.05	11234	59.95	2593	70.05	238
38.05	12833	50.05	56629	61.05	11581	71.20	86
39.00	5308	51.05	16154	62.05	12665	72.00	1342
39.90	197	51.95	677	63.05	10413	73.00	10462
41.10	84	52.80	92	64.00	1209	74.05	44235
43.10	125	53.05	195	65.10	1775	75.10	131205
44.00	2002	54.00	71	65.90	204	76.00	10260
45.00	2324	55.00	801	66.80	574	77.00	1187

Average of 10.368 to 10.374 min.: VL042299.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.70	195	90.30	41	103.95	891	115.00	207
77.95	531	91.00	716	104.80	99	115.85	856
78.95	6405	92.05	6988	104.95	197	116.95	1334
80.00	1559	93.05	10996	106.05	1018	117.90	753
80.95	6677	94.10	27683	106.70	72	118.95	1261
82.00	1644	95.10	229611	107.00	148	120.00	60
83.00	289	96.10	15747	109.90	102	122.70	33
85.90	397	96.90	97	110.75	195	122.90	75
87.05	7211	97.05	223	111.90	61	123.50	66
88.00	6689	100.85	45	112.60	112	124.05	100
88.70	67	102.80	92	113.00	136	125.15	73

Average of 10.368 to 10.374 min.: VL042299.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.70	82	138.70	27	146.60	28	156.00	78
127.00	141	138.90	68	147.10	155	156.85	423
127.85	672	139.90	28	147.30	47	158.00	133
128.80	10	140.95	2027	147.95	518	159.00	140
129.05	376	141.80	132	148.95	104	160.90	308
129.95	876	142.10	96	149.90	173	167.30	26
130.90	191	142.95	2483	151.85	69	168.20	50
131.10	85	143.75	216	152.80	21	169.10	44
135.00	400	144.85	199	154.00	256	169.60	91
135.75	64	145.10	199	154.80	155	170.30	48
136.90	316	145.90	248	154.95	300	170.85	224

Average of 10.368 to 10.374 min.: VL042299.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.05	1591	272.60	24				
173.00	1863	277.20	40				
174.00	144533						
175.05	11082						
176.00	138363						
177.00	8219						
177.95	289						
189.50	19						
201.05	49						
205.50	23						
244.70	29						