


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041122\
 Data File : VL038868.D
 Acq On : 11 Apr 2022 9:44
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL040522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Apr 06 06:12:53 2022
 Last Update : Wed Apr 06 06:12:53 2022

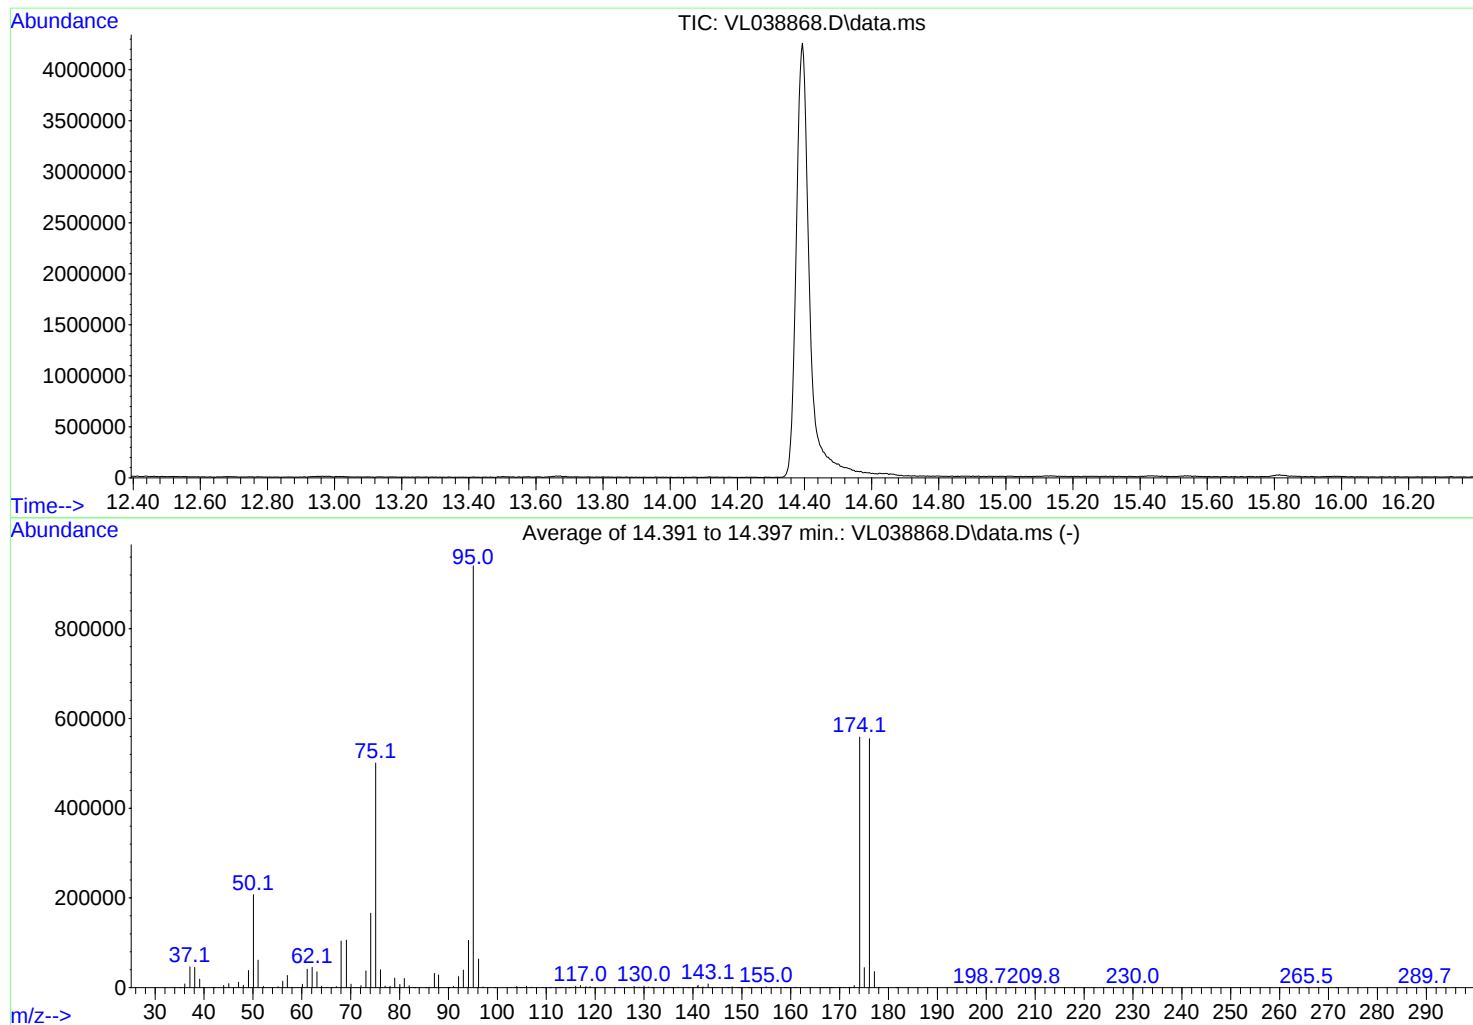

AutoFind: Scans 3609, 3610, 3611; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	207253	PASS
75	95	30	66	53.3	500779	PASS
95	95	100	100	100.0	940384	PASS
96	95	5	9	6.8	63880	PASS
173	174	0.00	2	0.8	4726	PASS
174	95	50	120	59.4	558464	PASS
175	174	4	9	8.0	44507	PASS
176	174	93	101	99.4	555243	PASS
177	176	5	9	6.4	35579	PASS

Average of 14.391 to 14.397 min.: VL038868.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	58	47.05	11973	61.10	41083	72.10	4811
36.05	8275	48.05	5416	62.10	45173	73.10	3740
37.10	46541	49.10	38035	63.10	35419	74.10	16584
38.10	45219	50.10	207253	64.05	3249	75.10	50077
39.10	19093	51.05	61408	65.00	383	76.10	39843
39.95	668	52.15	2383	66.10	71	77.05	3573
42.05	162	55.15	2234	67.05	2582	78.05	3063
43.00	459	56.10	14341	68.05	103789	79.00	21405
44.00	4987	57.05	27232	69.10	106085	80.05	7152
45.05	8880	58.10	864	70.05	7957	80.95	20392
46.15	352	60.10	7486	70.90	277	81.95	4175

Average of 14.391 to 14.397 min.: VL038868.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.90	546	94.10	105136	107.00	1118	114.60	112
83.10	66	95.05	940384	109.25	248	115.05	754
83.30	254	96.15	63880	109.80	120	116.00	3290
85.30	107	97.05	1846	110.00	461	117.00	4741
86.05	951	99.50	122	110.70	87	118.10	2581
87.10	31883	102.90	368	111.00	606	118.80	1080
87.95	28120	103.90	2068	111.90	448	119.00	2226
90.10	137	104.10	953	112.20	140	120.00	123
91.00	2863	104.85	674	112.70	144	122.15	285
92.05	24555	105.10	532	113.00	732	123.10	260
93.05	39195	105.95	3195	113.30	192	123.90	290

Average of 14.391 to 14.397 min.: VL038868.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.20	207	134.70	521	142.05	1338	149.50	84
124.95	261	135.10	1249	143.10	8364	150.05	1129
125.95	228	135.70	181	144.05	569	151.40	66
126.75	217	136.20	232	144.90	529	151.60	94
127.95	2986	137.00	1204	146.00	723	151.90	108
129.00	1241	138.80	352	146.20	429	152.90	440
130.00	3464	139.10	157	147.00	431	153.85	419
130.90	1516	140.05	568	147.20	90	155.00	1895
131.70	176	140.90	2590	148.00	1779	156.10	372
133.90	86	141.05	5358	149.00	360	156.70	289
134.10	151	141.90	506	149.20	194	157.15	662

Average of 14.391 to 14.397 min.: VL038868.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.90	271	168.80	450	176.10	555243	271.60	66
158.75	416	169.20	320	177.10	35579	289.70	51
158.90	487	169.70	234	178.00	239		
159.10	170	170.15	922	178.15	891		
159.80	50	170.80	665	181.60	53		
161.00	997	171.20	355	198.70	109		
166.10	93	171.90	852	204.60	59		
166.70	53	172.30	731	208.80	140		
167.25	167	173.00	4726	209.75	160		
167.80	65	174.10	558464	230.00	59		
168.30	155	175.05	44507	265.50	85		