


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL041218\
Data File : VL031850.D
Acq On : 11 Apr 2018 23:40
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL041218AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Apr 13 16:50:02 2018
Last Update : Fri Apr 13 16:50:02 2018

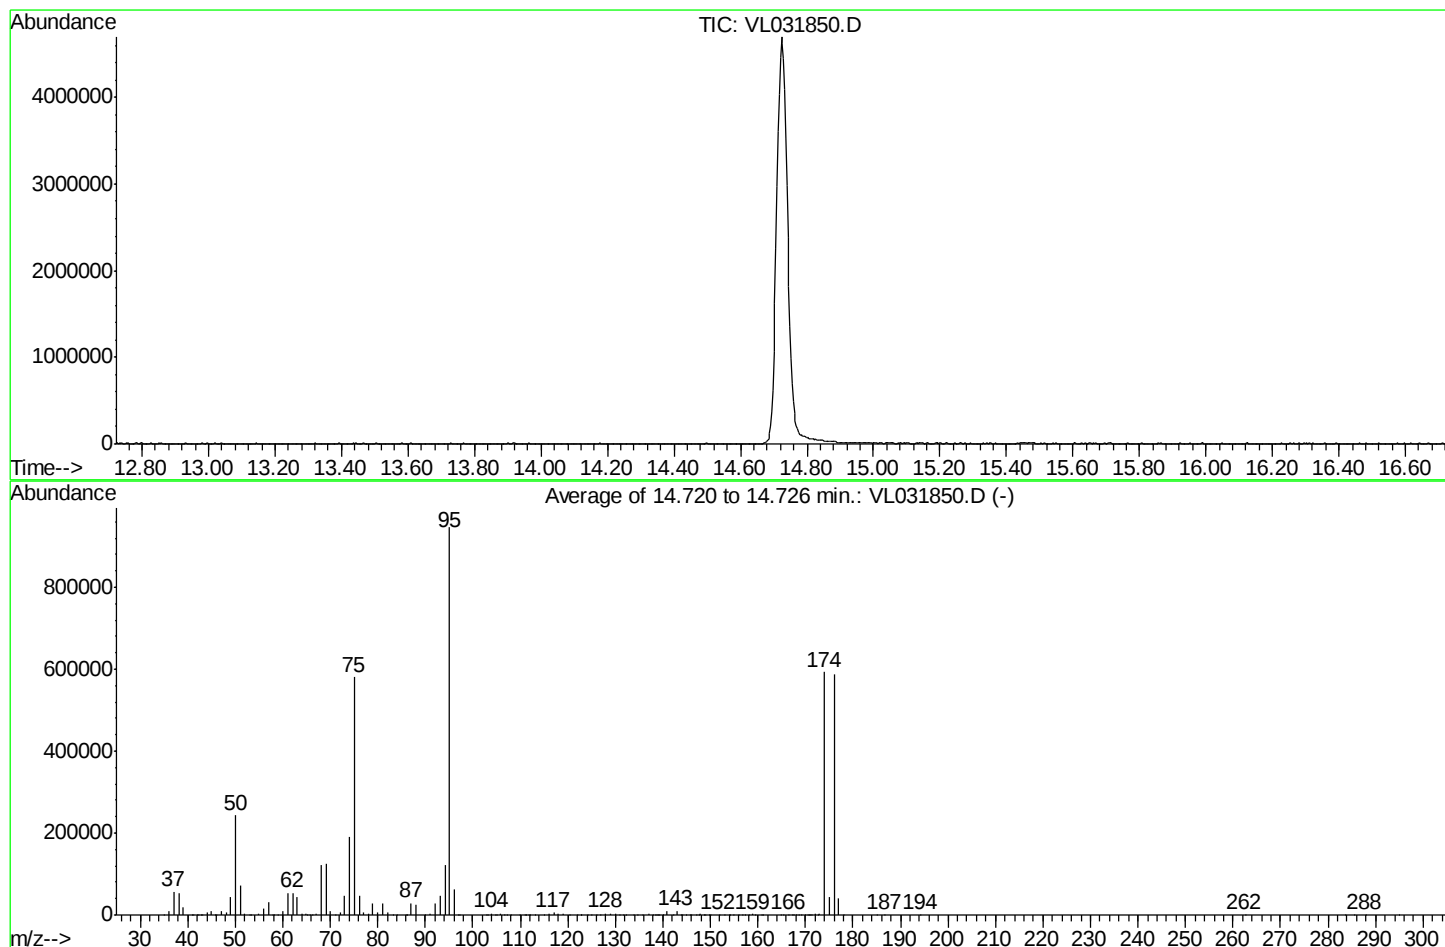

AutoFind: Scans 4240, 4241, 4242; Background Corrected with Scan 4215

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.7	243541	PASS
75	95	30	66	61.3	580373	PASS
95	95	100	100	100.0	946346	PASS
96	95	5	9	6.6	62002	PASS
173	174	0.00	2	0.6	3674	PASS
174	95	50	120	62.7	593514	PASS
175	174	4	9	7.3	43146	PASS
176	174	93	101	98.9	587072	PASS
177	176	5	9	6.7	39325	PASS