

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041223\
 Data File : VL040338.D
 Acq On : 12 Apr 2023 13:18
 Operator : SY/MD
 Sample : 02302-01 4X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SV-17_20230411

Quant Time: Apr 13 05:37:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031523AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Apr 11 04:15:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	5.189	49	1130956	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.655	114	2798536	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.478	117	2549948	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.790	95	2088152	9.779	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.800%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	2.719	85	15795	0.071	ppbv	93
3) Chlorodifluoromethane	2.665	51	5968	0.042	ppbv	97
4) Chloromethane	2.800	50	4335	0.049	ppbv	92
9) Propene	2.684	41	220430	4.046	ppbv	85
10) Heptane	7.581	43	13508	0.103	ppbv #	26
13) Ethanol	3.227	45	394901	98.828	ppbv	99
15) Acetone	3.456	43	2950833	21.432	ppbv	95
16) 1,3-Butadiene	2.957	39	173224	2.768	ppbv #	22
17) tert-Butyl alcohol	3.877	59	122198	0.934	ppbv	96
19) Isopropyl Alcohol	3.568	45	356435	5.404	ppbv #	90
20) Methylene Chloride	3.928	84	1179857	20.369	ppbv	95
23) Vinyl Acetate	4.619	43	14104	0.368	ppbv #	79
25) Ethyl Acetate	5.211	43	763722	2.963	ppbv #	76
26) Hexane	5.211	57	1095253	10.351	ppbv #	36
27) Carbon Disulfide	4.118	76	110205	0.746	ppbv #	85
29) Chloroform	5.275	83	19275	0.103	ppbv	96
30) Cyclohexane	6.603	84	2613	0.031	ppbv #	1
34) 2-Butanone	4.787	43	149747	1.084	ppbv	96
36) Benzene	6.369	78	29821	0.140	ppbv	93
39) 1,2-Dichloropropane	6.655	63	716684	8.565	ppbv #	24
41) Tetrahydrofuran	5.819	42	4195	0.053	ppbv #	38
44) 2,2,4-Trimethylpentane	7.333	57	17126	0.048	ppbv #	37
50) 4-Methyl-2-Pentanone	8.195	43	28634	0.134	ppbv #	31
51) 2-Hexanone	9.565	43	6545	0.040	ppbv #	1
53) Toluene	9.230	91	199972	0.895	ppbv	98
58) Ethyl Benzene	12.098	91	58915	0.203	ppbv #	84
59) m/p-Xylene	12.375	91	70984	0.267	ppbv #	33
60) o-Xylene	13.073	91	38326	0.151	ppbv #	27
69) p-Isopropyltoluene	17.005	119	13572	0.039	ppbv #	46
73) 1,3,5-Trimethylbenzene	15.355	105	7963	0.032	ppbv	99
74) 1,2,4-Trimethylbenzene	16.124	105	33908	0.118	ppbv #	74
75) 1,3-Dichlorobenzene	16.346	146	47372	0.305	ppbv #	5
79) Naphthalene	21.403	128	21548	0.127	ppbv #	97
80) Naphthalene,2-methyl-	24.394	142	3479	0.081	ppbv	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041223\
Data File : VL040338.D
Acq On : 12 Apr 2023 13:18
Operator : SY/MD
Sample : 02302-01 4X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411

Quant Time: Apr 13 05:37:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Apr 11 04:15:53 2023
Response via : Initial Calibration




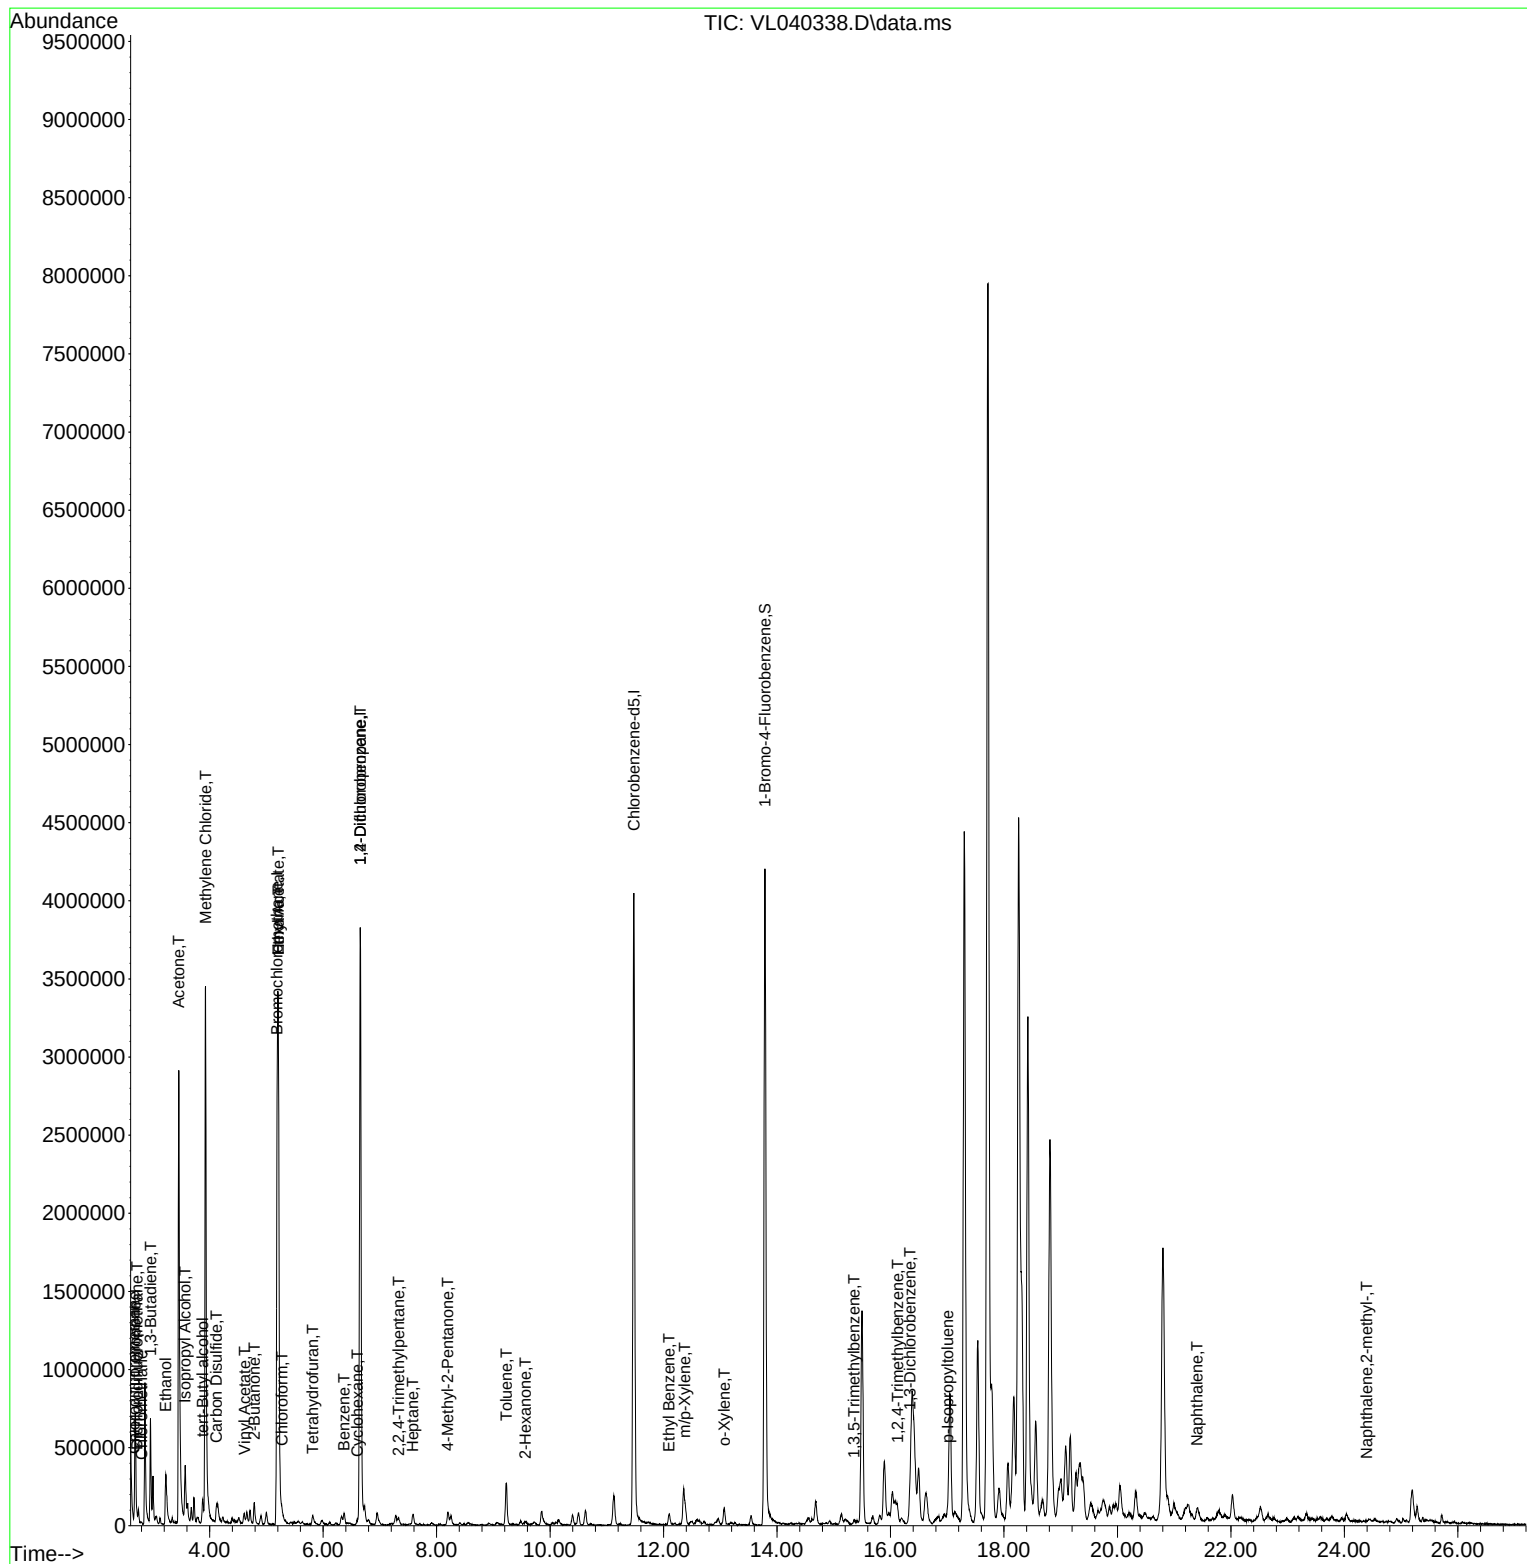




#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.189 min Scan# 804
 Delta R.T. -0.000 min
 Lab File: VL040338.D
 Acq: 12 Apr 2023 13:18




Instrument :
 MSVOA_L
 ClientSampleId :
 SV-17_20230411


Tgt Ion: 49 Resp: 1130956
 Ion Ratio Lower Upper
 49 100
 128 47.9 22.4 67.3
 130 61.2 28.7 86.1

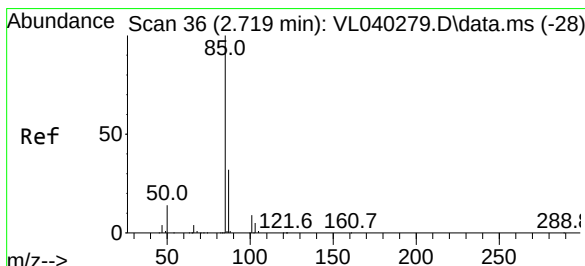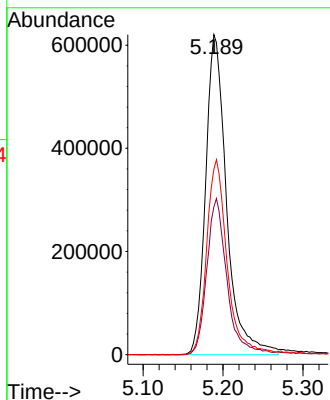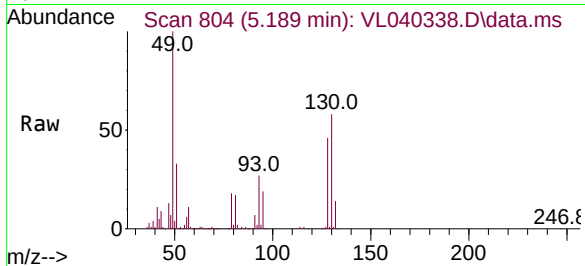

#2
 Dichlorodifluoromethane
 Concen: 0.071 ppbv
 RT: 2.719 min Scan# 36
 Delta R.T. 0.000 min
 Lab File: VL040338.D
 Acq: 12 Apr 2023 13:18

Tgt Ion: 85 Resp: 15795
 Ion Ratio Lower Upper
 85 100
 87 27.9 25.5 38.3


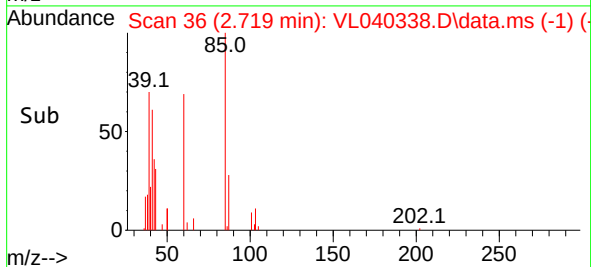
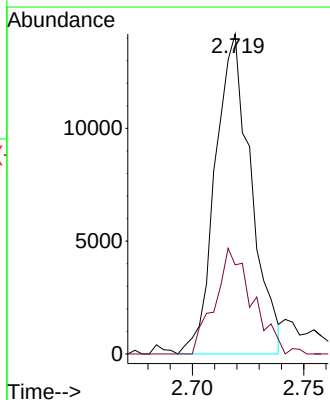
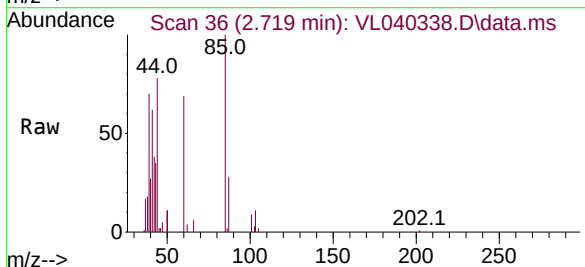


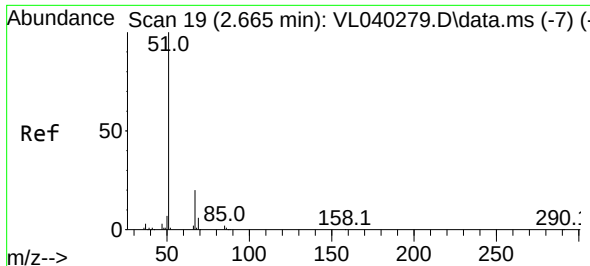

#3
Chlorodifluoromethane
Concen: 0.042 ppbv
RT: 2.665 min Scan# 19
Delta R.T. -0.000 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18




Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411


Tgt Ion: 51 Resp: 5968
Ion Ratio Lower Upper
51 100
67 18.6 16.0 24.0

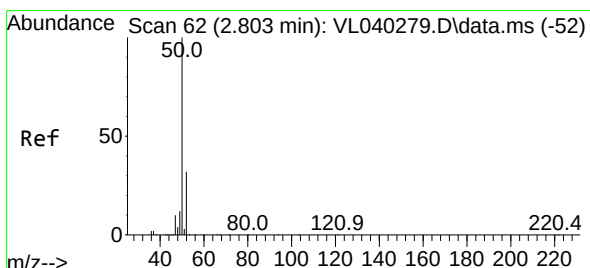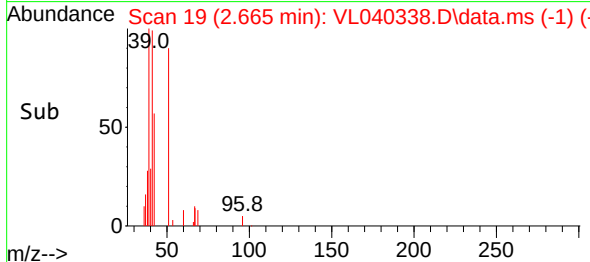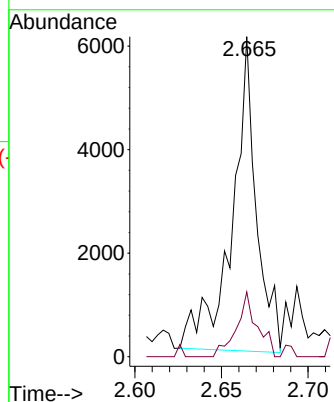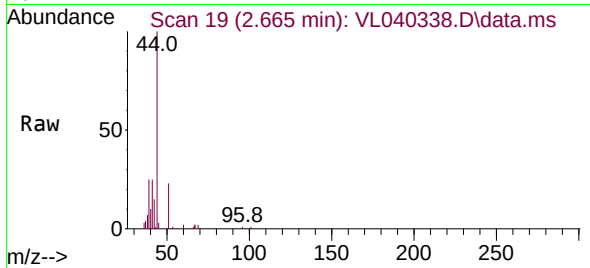

#4
Chloromethane
Concen: 0.049 ppbv
RT: 2.800 min Scan# 61
Delta R.T. -0.003 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion: 50 Resp: 4335
Ion Ratio Lower Upper
50 100
52 27.6 25.9 38.9


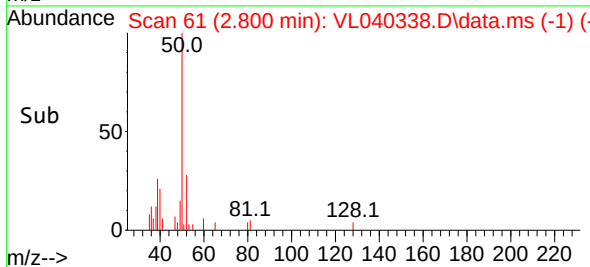
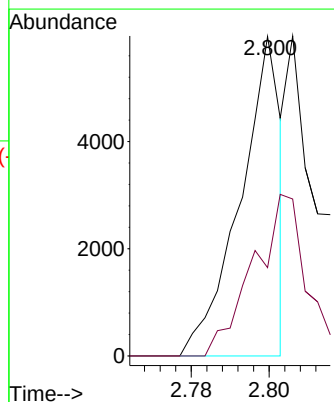
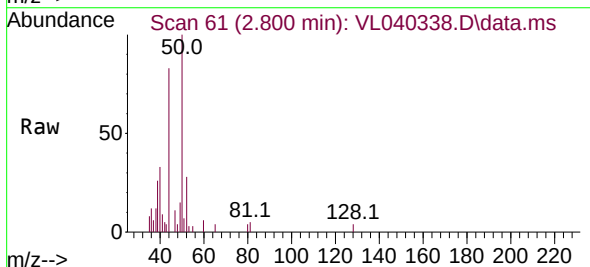


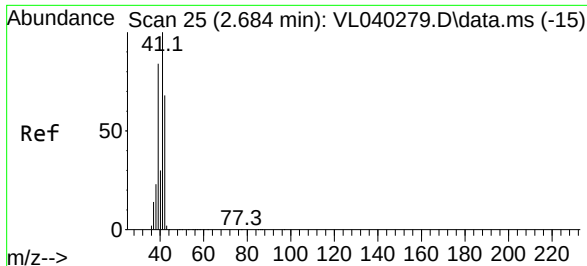

#9
 Propene
 Concen: 4.046 ppbv
 RT: 2.684 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VL040338.D
 Acq: 12 Apr 2023 13:18




Instrument :
 MSVOA_1
 ClientSampleId :
 SV-17_20230411


Tgt Ion: 41 Resp: 220430
 Ion Ratio Lower Upper
 41 100
 42 60.8 59.0 88.4

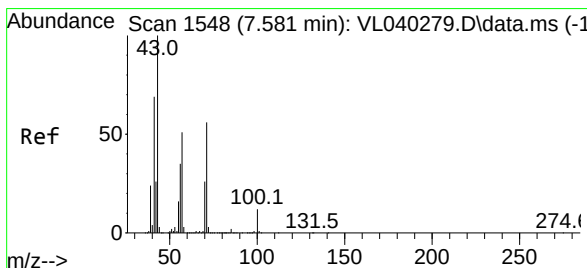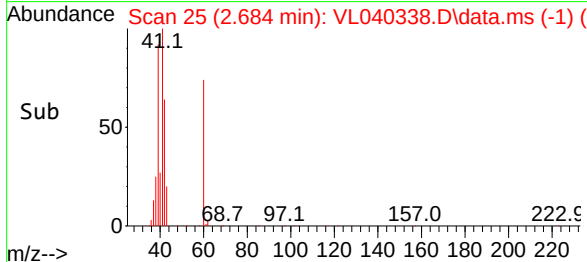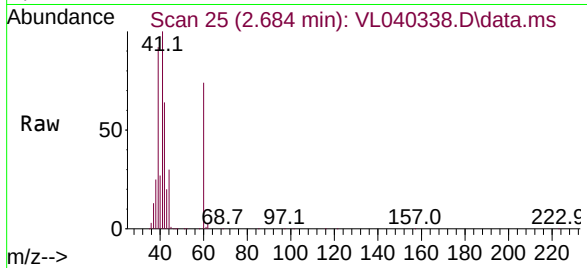

#10
 Heptane
 Concen: 0.103 ppbv
 RT: 7.581 min Scan# 1548
 Delta R.T. -0.000 min
 Lab File: VL040338.D
 Acq: 12 Apr 2023 13:18

Tgt Ion: 43 Resp: 13508
 Ion Ratio Lower Upper
 43 100
 57 0.0 41.7 62.5


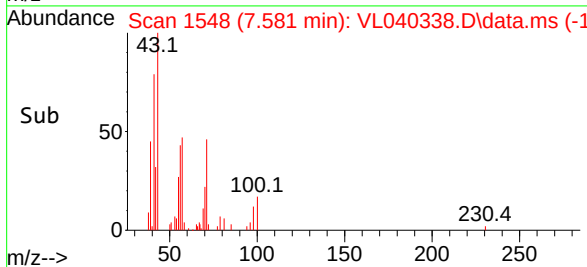

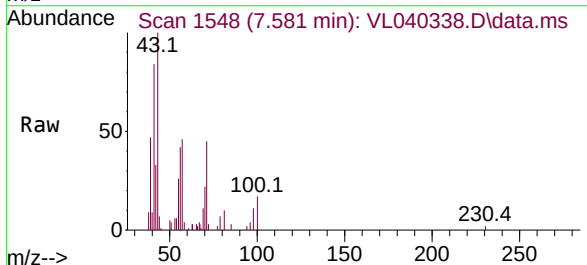




#13
Ethanol
Concen: 98.828 ppbv
RT: 3.227 min Scan# 197
Delta R.T. -0.010 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18




Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411


Tgt Ion: 45 Resp: 394901
Ion Ratio Lower Upper
45 100
46 37.1 15.0 60.2

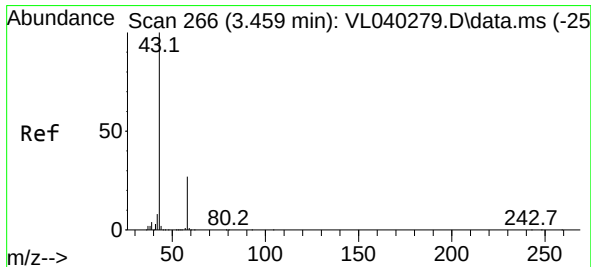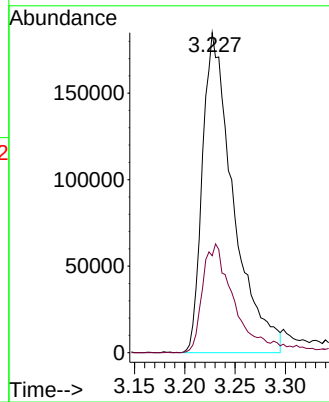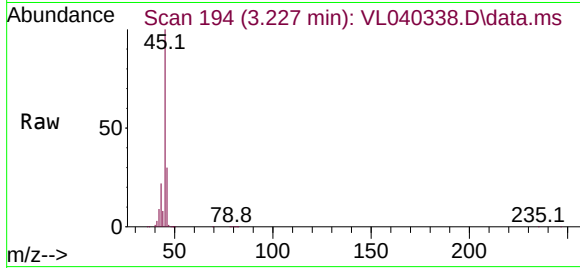

#15
Acetone
Concen: 21.432 ppbv
RT: 3.456 min Scan# 265
Delta R.T. -0.003 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion: 43 Resp: 2950833
Ion Ratio Lower Upper
43 100
58 30.1 21.8 32.8


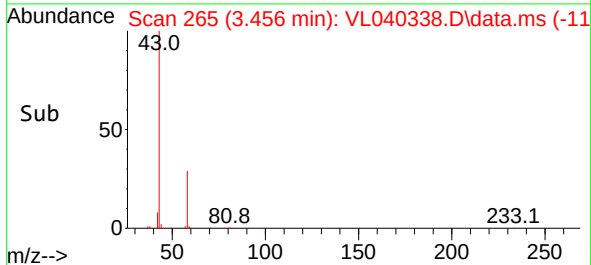
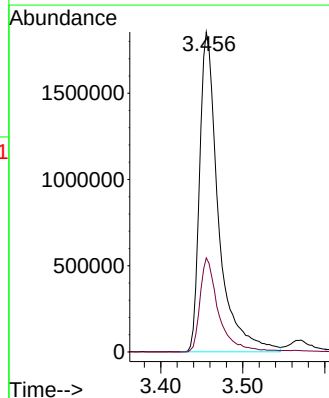
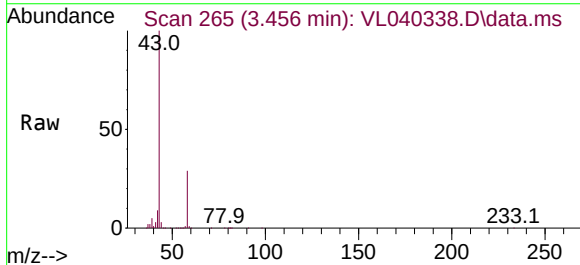




#16
1,3-Butadiene
Concen: 2.768 ppbv
RT: 2.957 min Scan# 116
Delta R.T. -0.019 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18




Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411


Tgt Ion: 39 Resp: 173224
Ion Ratio Lower Upper
39 100
54 14.3 68.4 102.6#

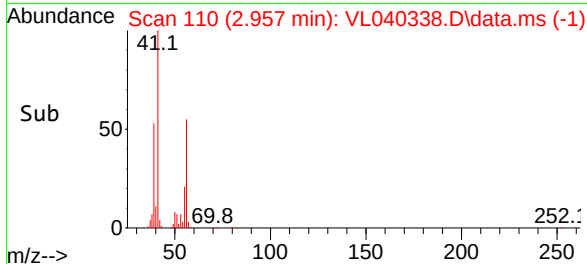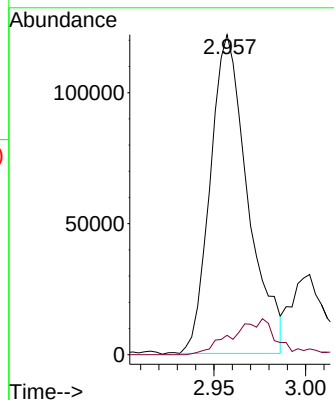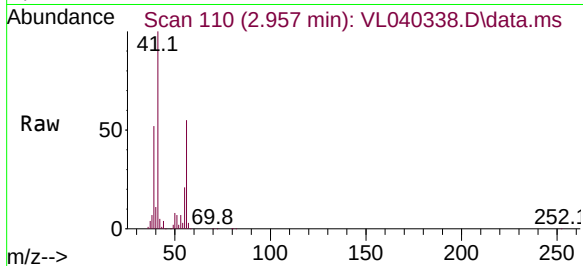

#17
tert-Butyl alcohol
Concen: 0.934 ppbv
RT: 3.877 min Scan# 396
Delta R.T. 0.007 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion: 59 Resp: 122198
Ion Ratio Lower Upper
59 100
57 12.2 8.5 12.7

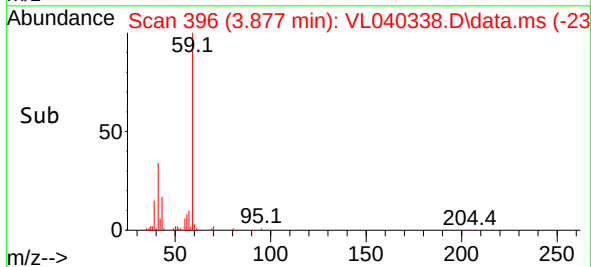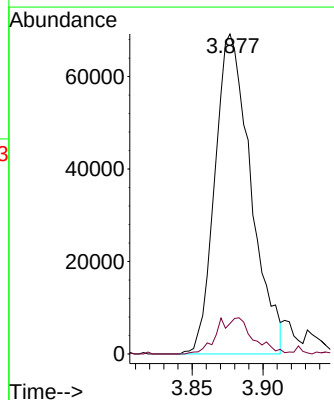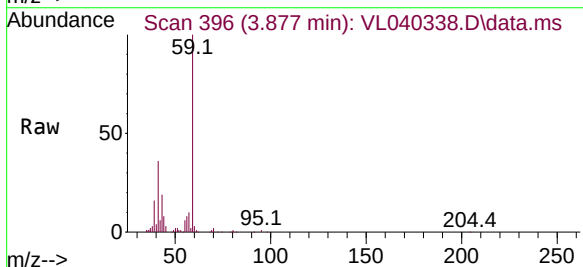



#19

Isopropyl Alcohol

Concen: 5.404 ppbv

RT: 3.568 min Scan# 300

Delta R.T. 0.003 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18

Instrument :

MSVOA_L

ClientSampleId :





SV-17_20230411

Tgt Ion: 45 Resp: 356435

Ion Ratio Lower Upper

45 100

58 0.0 2.7 4.1#

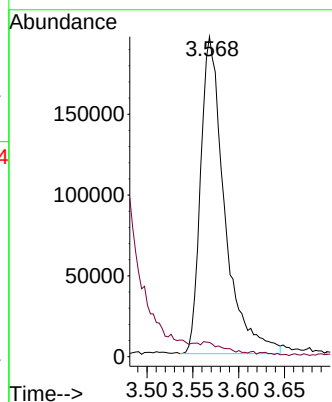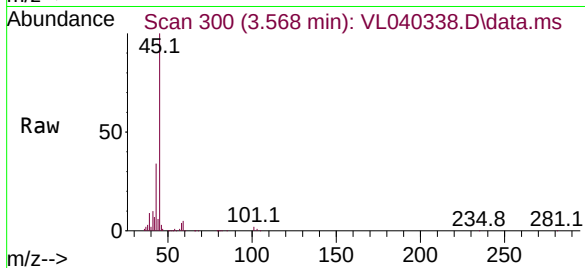

#20

Methylene Chloride

Concen: 20.369 ppbv

RT: 3.928 min Scan# 412

Delta R.T. 0.000 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18

Tgt Ion: 84 Resp: 1179857




Ion Ratio Lower Upper


84 100

49 153.8 117.5 176.3

51 46.8 36.9 55.3

86 62.8 53.3 79.9

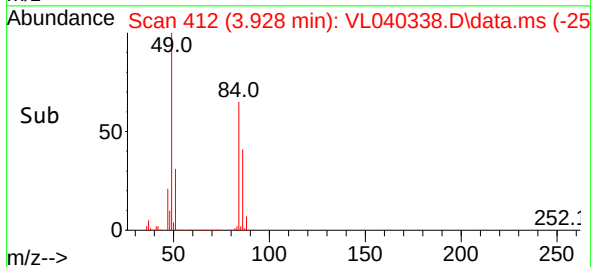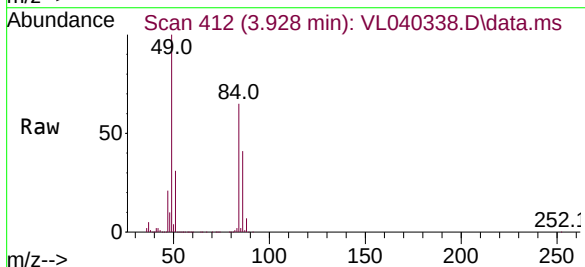







#23
 Vinyl Acetate
 Concen: 0.368 ppbv
 RT: 4.619 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: VL040338.D
 Acq: 12 Apr 2023 13:18

Instrument :
 MSVOA_L
 ClientSampleId :
 SV-17_20230411

Tgt Ion: 43 Resp: 14104




Ion	Ratio	Lower	Upper
43	100		
86	9.5	5.0	7.4#
42	0.0	9.1	13.7#
44	0.0	4.5	6.7#

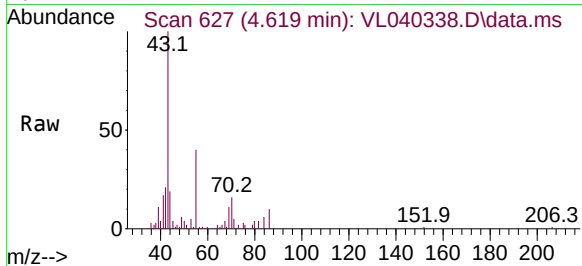


#25
 Ethyl Acetate
 Concen: 2.963 ppbv
 RT: 5.211 min Scan# 811
 Delta R.T. 0.010 min
 Lab File: VL040338.D
 Acq: 12 Apr 2023 13:18

Tgt Ion: 43 Resp: 763722

Ion	Ratio	Lower	Upper
43	100		
45	0.8	8.6	12.8#
61	0.4	8.4	12.6#
70	1.7	5.8	8.6#

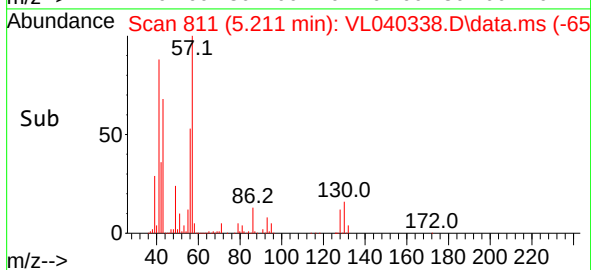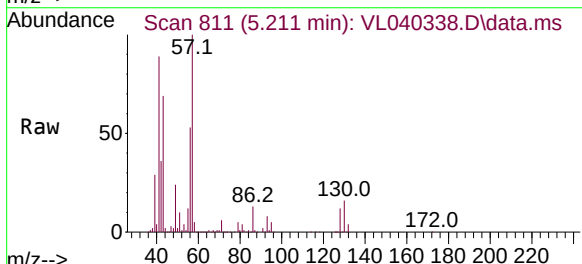







#26
Hexane
Concen: 10.351 ppbv
RT: 5.211 min Scan# 811
Delta R.T. 0.000 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411

Tgt Ion: 57 Resp: 1095253




Ion	Ratio	Lower	Upper
57	100		
41	89.3	73.5	110.3
43	70.1	196.3	294.5#
56	54.5	43.8	65.8

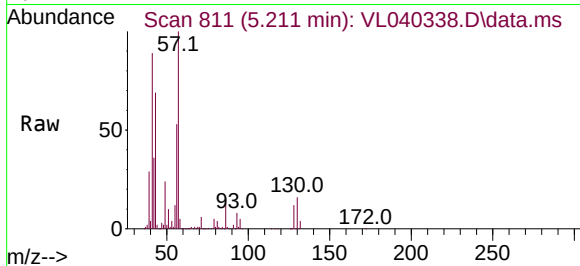


#27
Carbon Disulfide
Concen: 0.746 ppbv
RT: 4.118 min Scan# 471
Delta R.T. -0.000 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion: 76 Resp: 110205

Ion	Ratio	Lower	Upper
76	100		
44	27.3	15.2	22.8#
78	12.5	7.6	11.4#

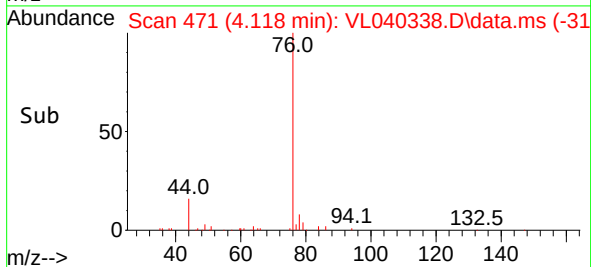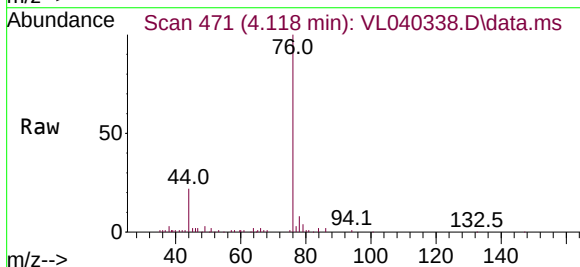



#29

Chloroform

Concen: 0.103 ppbv

RT: 5.275 min Scan# 81

Delta R.T. 0.003 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18

Instrument :

MSVOA_L

ClientSampleId :





SV-17_20230411

Tgt Ion: 83 Resp: 19275

Ion Ratio Lower Upper

83 100

85 62.8 52.8 79.2

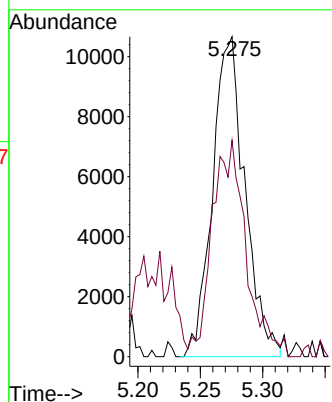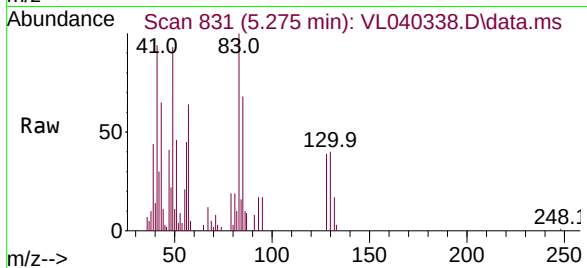

#30

Cyclohexane

Concen: 0.031 ppbv

RT: 6.603 min Scan# 1244

Delta R.T. 0.000 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18




Tgt Ion: 84 Resp: 2613


Ion Ratio Lower Upper

84 100

56 0.0 109.0 163.4#

41 373.3 67.9 101.9#

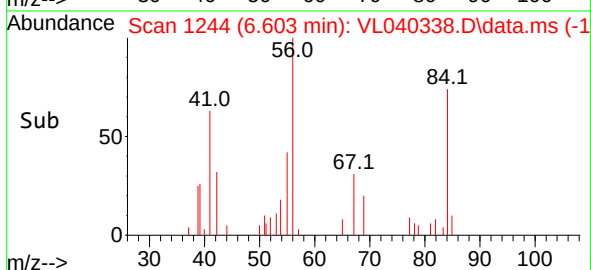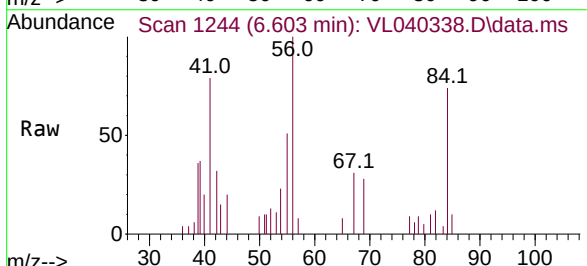



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.655 min Scan# 11

Delta R.T. -0.000 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18

Instrument :

MSVOA_L

ClientSampleId :

SV-17_20230411





Tgt Ion:114 Resp: 2798536

Ion Ratio Lower Upper

114 100

63 26.0 21.2 31.8

88 18.1 14.5 21.7



#34

2-Butanone

Concen: 1.084 ppbv

RT: 4.787 min Scan# 679

Delta R.T. 0.007 min

Lab File: VL040338.D




Acq: 12 Apr 2023 13:18


Tgt Ion: 43 Resp: 149747

Ion Ratio Lower Upper

43 100

72 24.9 18.3 27.5

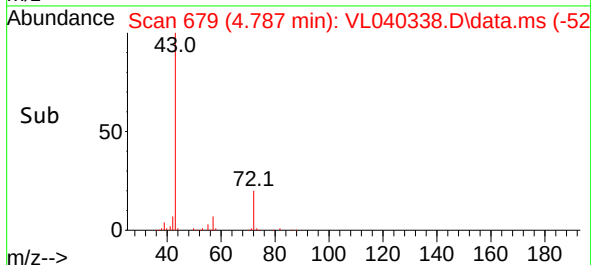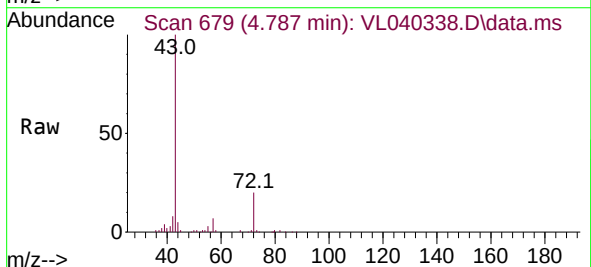



#36

Benzene

Concen: 0.140 ppbv

RT: 6.369 min Scan# 1171

Delta R.T. -0.003 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18

Instrument :

MSVOA_L

ClientSampleId :

SV-17_20230411





Tgt Ion: 78 Resp: 29821

Ion Ratio Lower Upper

78 100

77 18.2 17.8 26.8

50 22.1 15.4 23.2

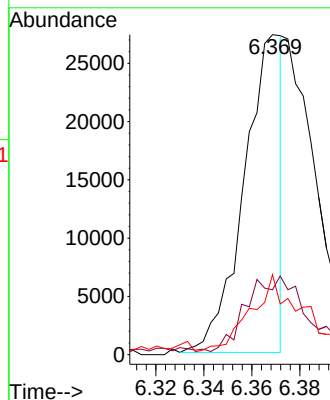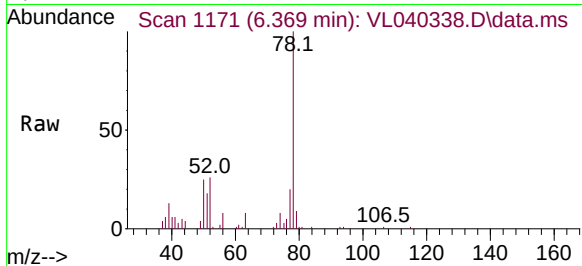

#39

1,2-Dichloropropane

Concen: 8.565 ppbv

RT: 6.655 min Scan# 1260

Delta R.T. -0.418 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18




Tgt Ion: 63 Resp: 716684


Ion Ratio Lower Upper

63 100

41 0.0 60.8 91.2#

62 17.8 54.1 81.1#



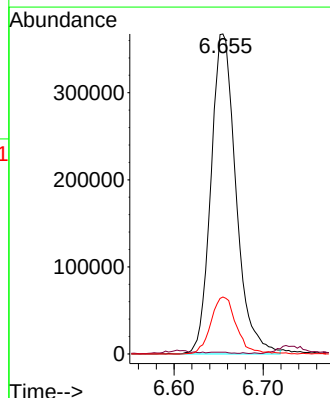
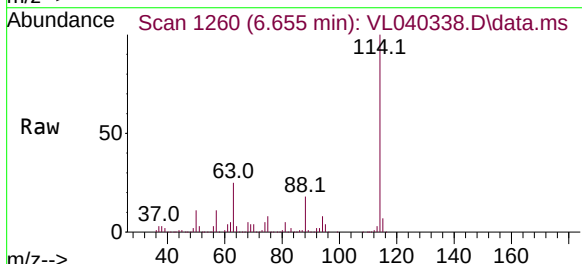




#41
Tetrahydrofuran
Concen: 0.053 ppbv
RT: 5.819 min Scan# 1000
Delta R.T. 0.264 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18




Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411


Tgt Ion: 42 Resp: 4195
Ion Ratio Lower Upper
42 100
72 3.7 32.6 49.0#
71 0.0 31.0 46.4#

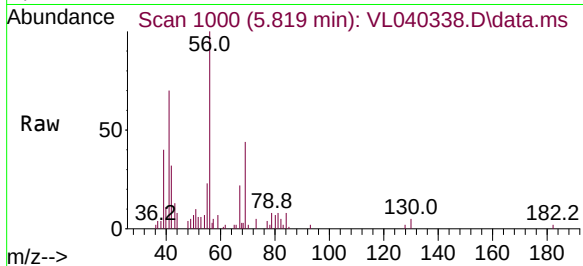

#44
2,2,4-Trimethylpentane
Concen: 0.048 ppbv
RT: 7.333 min Scan# 1471
Delta R.T. 0.003 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion: 57 Resp: 17126
Ion Ratio Lower Upper
57 100
41 63.6 26.8 40.2#
56 72.5 25.0 37.6#


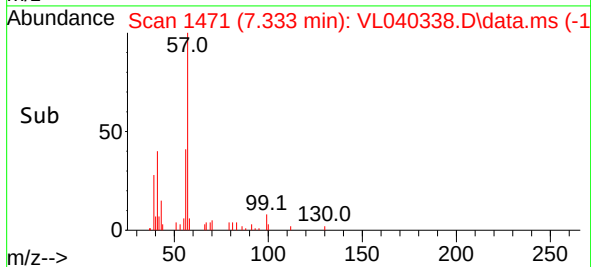

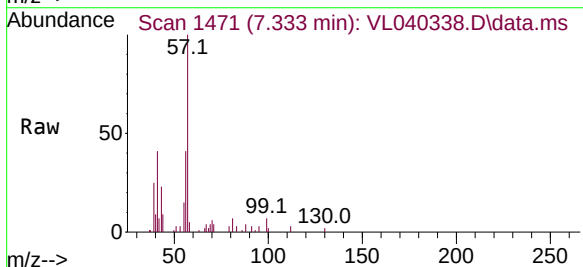




#50
4-Methyl-2-Pentanone
Concen: 0.134 ppbv
RT: 8.195 min Scan# 1739
Delta R.T. 0.010 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18




Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411


Tgt Ion: 43 Resp: 28634
Ion Ratio Lower Upper
43 100
58 77.1 29.2 43.8#

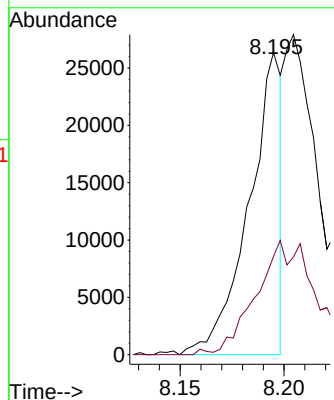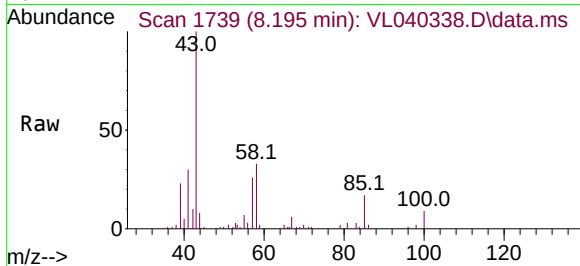

#51
2-Hexanone
Concen: 0.040 ppbv
RT: 9.565 min Scan# 2165
Delta R.T. 0.010 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion: 43 Resp: 6545
Ion Ratio Lower Upper
43 100
58 150.7 38.0 57.0#
98 0.0 0.5 0.7#


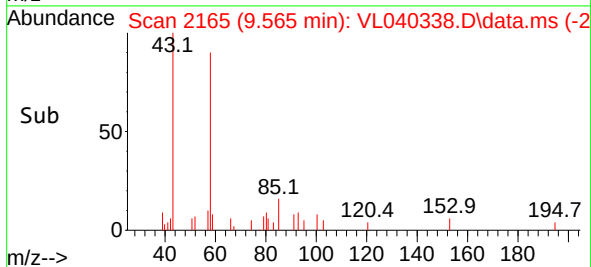
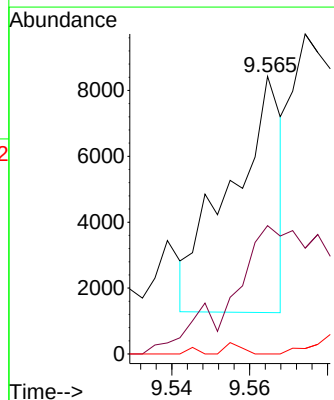
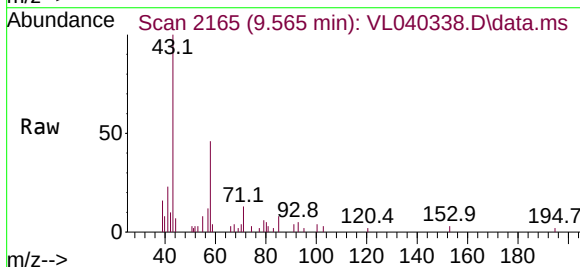




#53
Toluene
Concen: 0.895 ppbv
RT: 9.230 min Scan# 2061
Delta R.T. 0.003 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18




Instrument :
MSVOA_1
ClientSampleId :
SV-17_20230411


Tgt Ion: 91 Resp: 199972
Ion Ratio Lower Upper
91 100
92 61.2 48.0 72.0

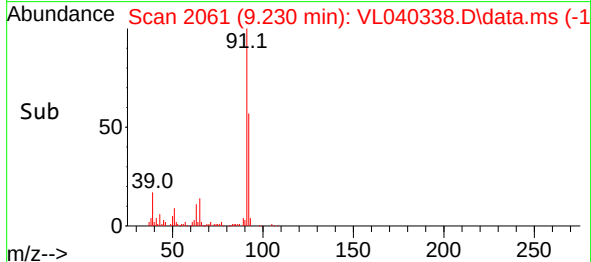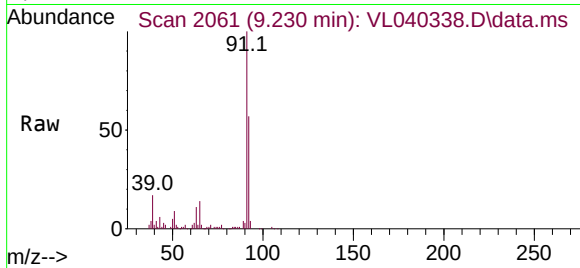

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.478 min Scan# 2760
Delta R.T. -0.000 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion: 117 Resp: 2549948
Ion Ratio Lower Upper
117 100
82 67.9 51.4 77.2
119 32.7 24.0 36.0


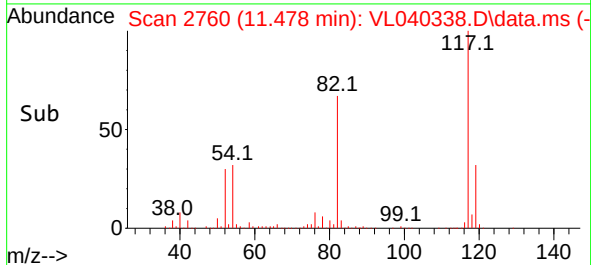

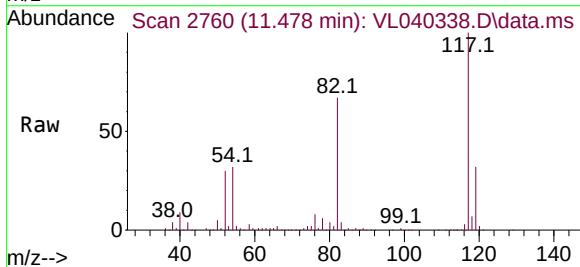




#58
Ethyl Benzene
Concen: 0.203 ppbv
RT: 12.098 min Scan# 2953
Delta R.T. 0.000 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18




Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411


Tgt Ion: 91 Resp: 58915
Ion Ratio Lower Upper
91 100
106 20.8 23.4 35.2#

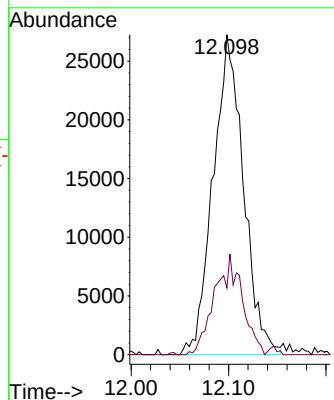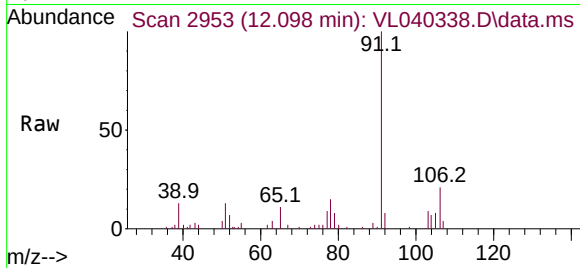

#59
m/p-Xylene
Concen: 0.267 ppbv
RT: 12.375 min Scan# 3039
Delta R.T. -0.006 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion: 91 Resp: 70984
Ion Ratio Lower Upper
91 100
106 0.0 34.0 51.0#

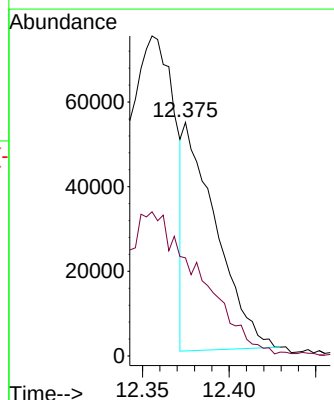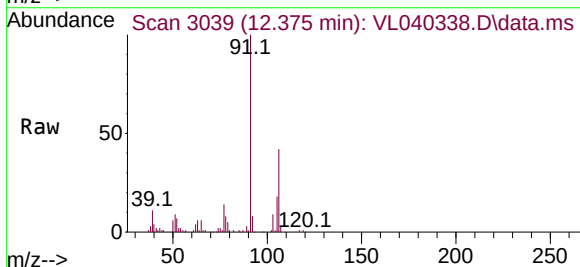



#60

o-Xylene

Concen: 0.151 ppbv

RT: 13.073 min Scan# 31

Delta R.T. 0.003 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18

Instrument :

MSVOA_L

ClientSampleId :





SV-17_20230411

Tgt Ion: 91 Resp: 38326

Ion Ratio Lower Upper

91 100

106 90.4 21.7 65.1#

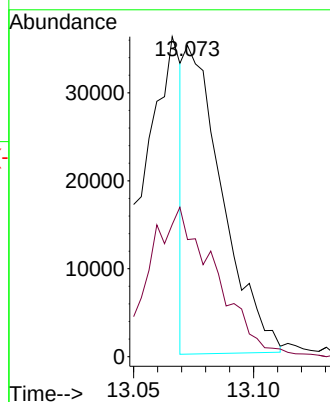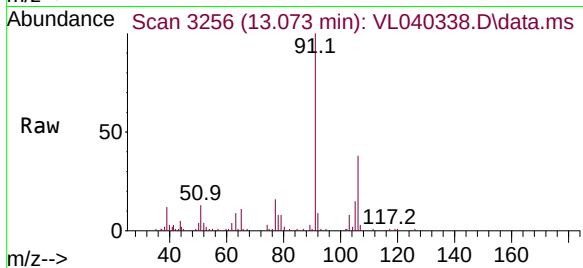

#68

1-Bromo-4-Fluorobenzene

Concen: 9.779 ppbv

RT: 13.790 min Scan# 3479

Delta R.T. 0.004 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18




Tgt Ion: 95 Resp: 2088152


Ion Ratio Lower Upper

95 100

174 60.0 47.0 70.6

175 4.3 3.4 5.2

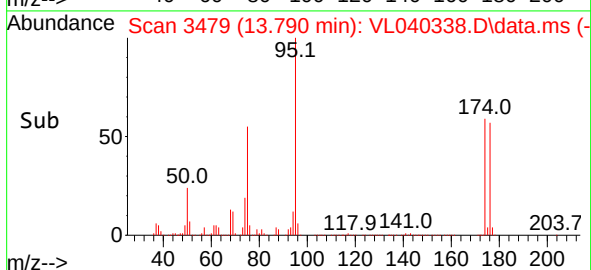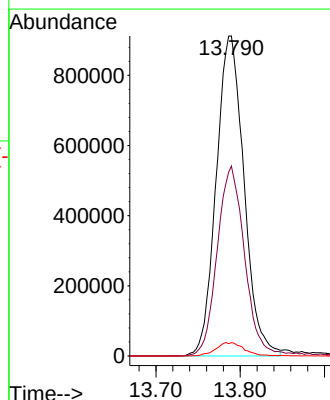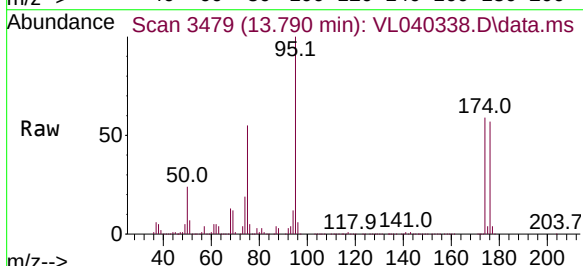



#69

p-Isopropyltoluene

Concen: 0.039 ppbv

RT: 17.005 min Scan# 4480

Delta R.T. -0.003 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18

Instrument :

MSVOA_L

ClientSampleId :

SV-17_20230411





Tgt Ion:119 Resp: 13572

Ion Ratio Lower Upper

119 100

134 0.0 20.2 30.2#

91 0.0 25.1 37.7#

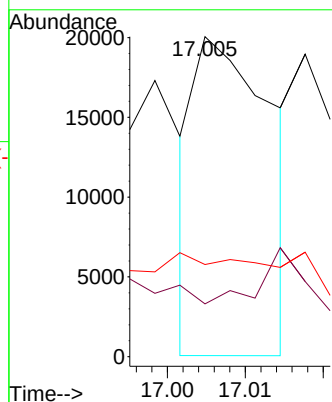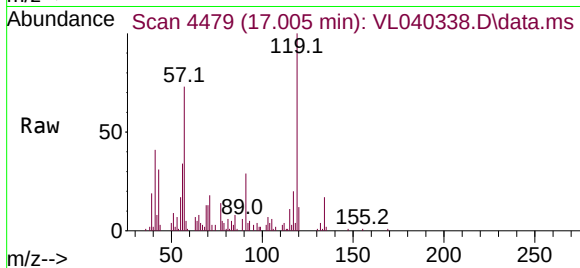

#73

1,3,5-Trimethylbenzene

Concen: 0.032 ppbv

RT: 15.355 min Scan# 3966

Delta R.T. -0.007 min

Lab File: VL040338.D




Acq: 12 Apr 2023 13:18


Tgt Ion:105 Resp: 7963

Ion Ratio Lower Upper

105 100

120 44.1 34.9 52.3

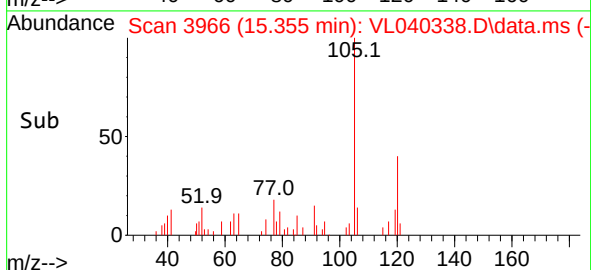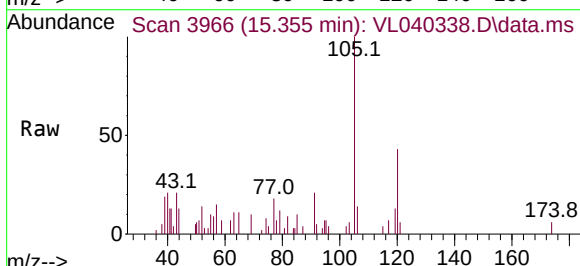

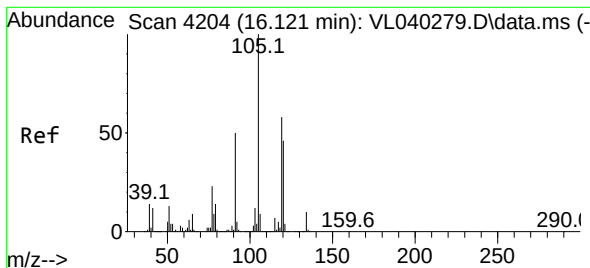

#74

1,2,4-Trimethylbenzene

Concen: 0.118 ppbv

RT: 16.124 min Scan# 41

Delta R.T. 0.003 min

Lab File: VL040338.D


Acq: 12 Apr 2023 13:18

Instrument :

MSVOA_1

ClientSampleId :

SV-17_20230411

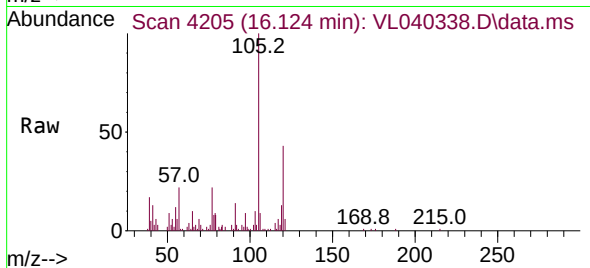

Tgt Ion:105 Resp: 33908




Ion Ratio Lower Upper

105 100

120 41.3 36.6 54.8

91 11.3 39.9 59.9#

77 23.8 18.6 27.8

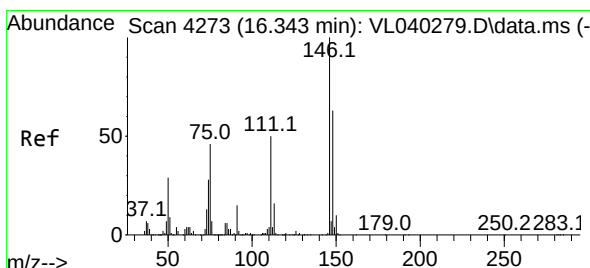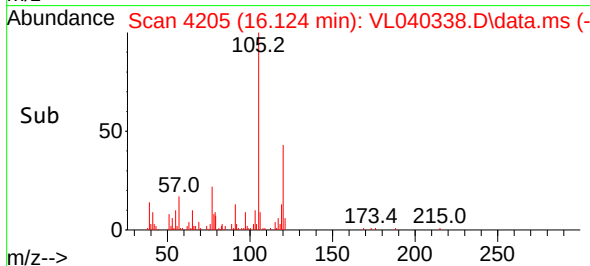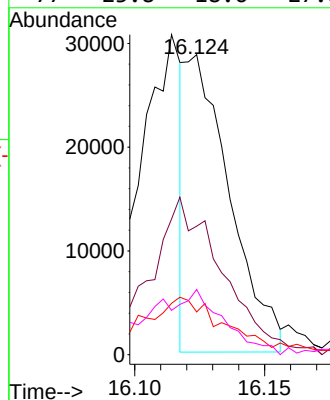

#75

1,3-Dichlorobenzene

Concen: 0.305 ppbv

RT: 16.346 min Scan# 4274

Delta R.T. 0.003 min

Lab File: VL040338.D

Acq: 12 Apr 2023 13:18




Tgt Ion:146 Resp: 47372


Ion Ratio Lower Upper

146 100

111 116.3 24.3 73.0#

148 135.4 31.9 95.5#


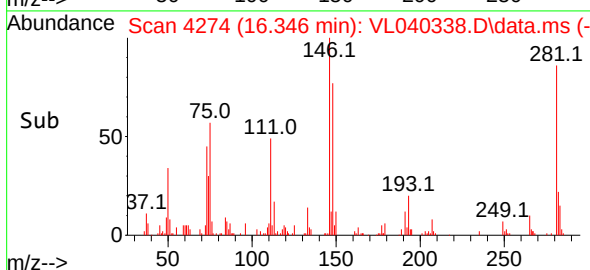
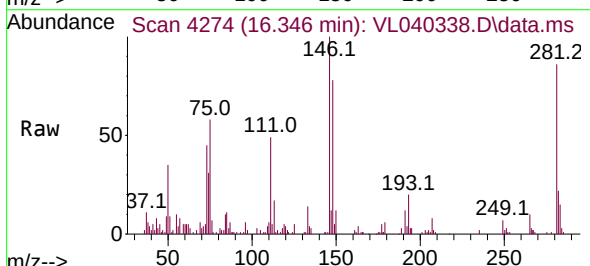
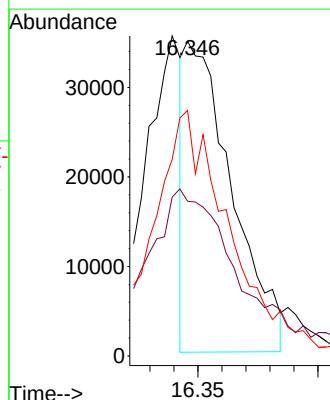




#79
Naphthalene
Concen: 0.127 ppbv
RT: 21.403 min Scan# 5847
Delta R.T. 0.006 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Instrument :
MSVOA_L
ClientSampleId :
SV-17_20230411

Tgt Ion:128 Resp: 21548
Ion Ratio Lower Upper
128 100
127 12.3 9.6 14.4
129 8.5 8.6 13.0#

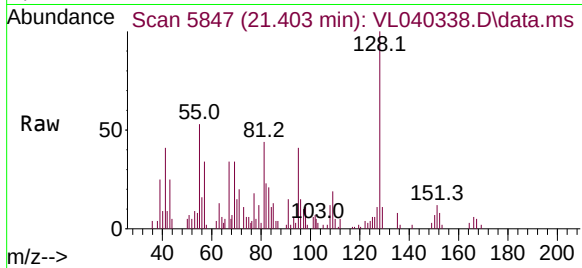

#80
Naphthalene,2-methyl-
Concen: 0.081 ppbv
RT: 24.394 min Scan# 6777
Delta R.T. 0.007 min
Lab File: VL040338.D
Acq: 12 Apr 2023 13:18

Tgt Ion:142 Resp: 3479
Ion Ratio Lower Upper
142 100
141 85.7 65.5 98.3
115 48.2 33.5 50.3

