
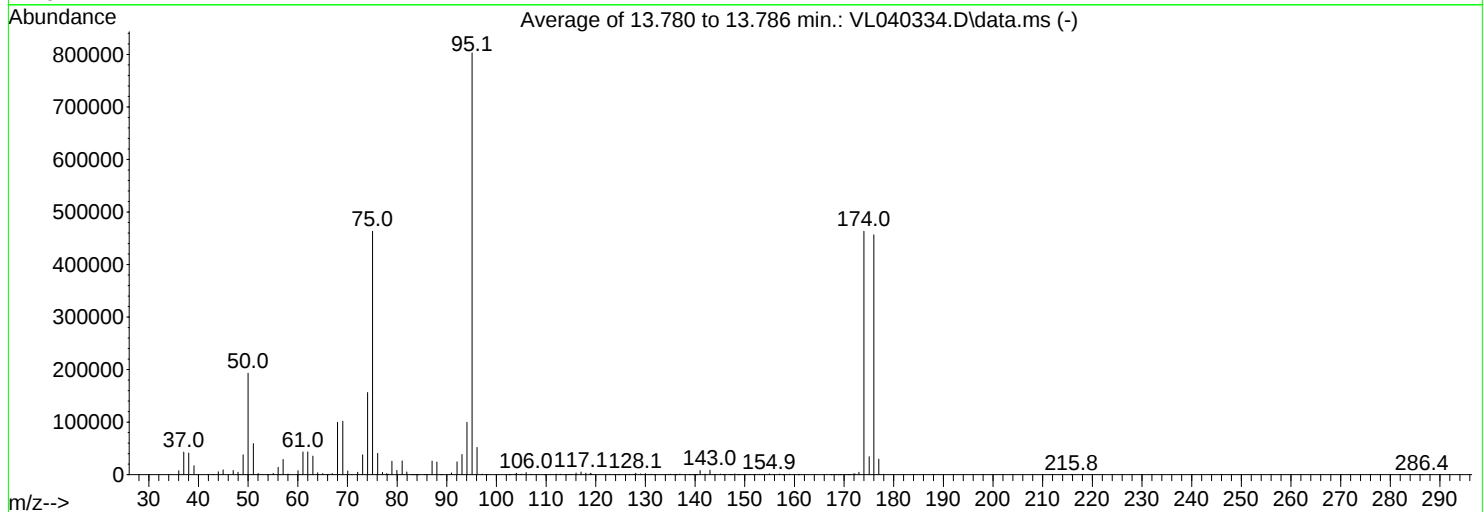


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041223\
Data File : VL040334.D
Acq On : 12 Apr 2023 8:24
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Apr 11 04:15:53 2023

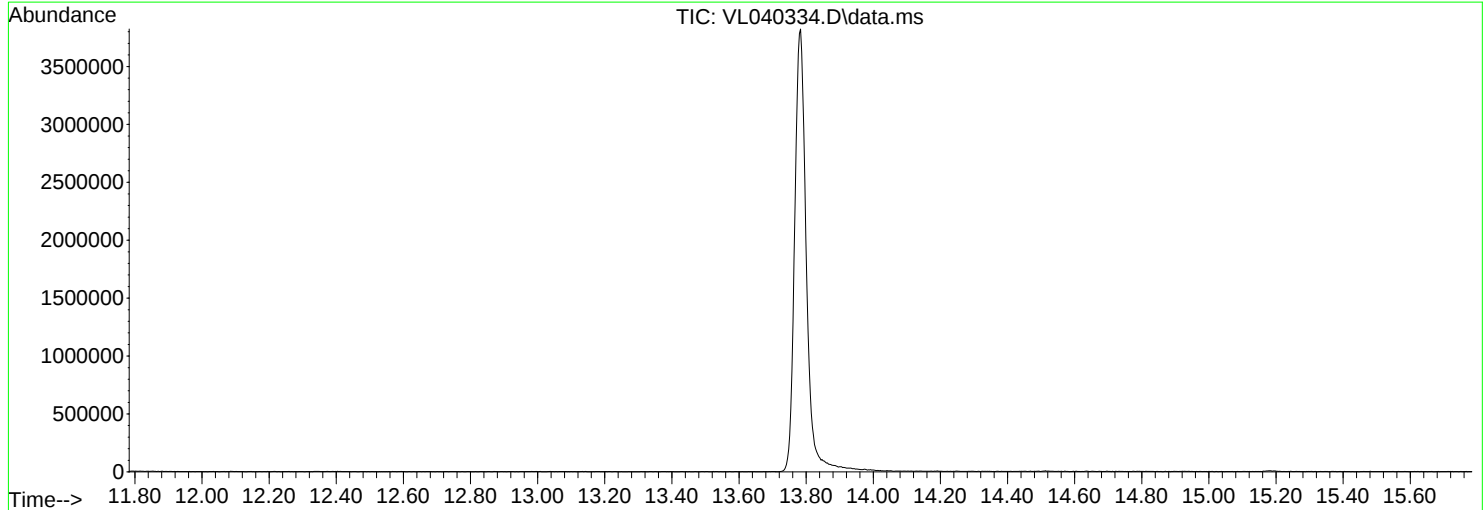

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	193237	PASS
75	95	30	66	57.7	463381	PASS
95	95	100	100	100.0	803008	PASS
96	95	5	9	6.4	51773	PASS
173	174	0.00	2	1.0	4475	PASS
174	95	50	120	57.7	463189	PASS
175	174	4	9	7.4	34072	PASS
176	174	93	101	98.6	456747	PASS
177	176	5	9	6.5	29493	PASS

Average of 13.780 to 13.786 min.: VL040334.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7716	47.00	7997	57.05	28808	68.00	9969
37.05	43043	47.95	4702	58.05	1242	69.05	10191
38.05	41155	49.00	37795	60.05	7679	70.05	714
39.10	17130	50.00	193237	61.05	43408	70.85	25
40.00	197	51.05	59163	62.00	43405	72.05	4620
41.90	280	51.90	929	63.05	35360	73.05	37805
42.80	204	52.10	1700	64.00	3700	74.05	156267
43.05	436	52.90	440	65.05	2291	75.05	463381
44.00	5418	53.85	177	65.90	71	76.10	40384
44.95	9158	55.05	2597	66.05	289	77.05	4135
46.05	793	56.05	13981	66.95	2132	77.85	1995

Average of 13.780 to 13.786 min.: VL040334.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.00	900	85.50	204	96.10	51773	106.85	487
78.20	892	85.70	325	96.90	415	107.10	358
78.95	25688	86.05	666	97.15	844	109.70	155
79.95	8156	87.05	25901	97.90	55	109.95	399
81.00	26280	88.00	24203	102.60	75	110.85	595
81.95	5274	88.80	147	102.90	376	112.05	985
82.85	422	90.95	3392	103.80	1209	112.85	973
83.10	374	92.05	24301	104.05	2443	114.00	108
83.30	109	93.05	38251	104.80	364	114.60	246
83.80	121	94.05	99728	105.05	927	114.80	371
84.15	156	95.10	803008	106.00	3887	115.05	607

Average of 13.780 to 13.786 min.: VL040334.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.05	2983	126.80	231	135.90	68	144.00	580
117.05	5244	127.80	491	136.20	116	145.10	1208
118.00	2763	128.05	2849	136.95	1186	145.70	325
118.90	2884	129.05	1636	138.90	158	146.00	696
119.10	1465	130.00	2281	139.70	70	146.80	298
122.10	393	130.70	233	140.00	458	147.10	144
122.90	242	131.15	826	140.20	128	147.50	214
123.80	159	131.80	56	141.00	7846	148.00	1511
123.95	410	134.10	226	142.00	1263	148.60	96
124.60	62	134.65	568	143.00	8552	149.00	326
126.00	309	135.10	994	143.80	215	149.90	223

Average of 13.780 to 13.786 min.: VL040334.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
150.10	459	159.00	945	172.00	1893		
151.05	214	160.80	157	172.20	1120		
151.80	54	160.95	643	173.00	4475		
152.05	197	167.40	57	174.00	463189		
153.00	600	168.20	83	175.05	34072		
153.65	234	168.80	126	176.00	456747		
153.95	419	169.20	124	177.00	29493		
154.95	1591	170.00	94	178.00	846		
157.05	1130	170.35	437	215.80	52		
157.70	139	170.70	141	286.40	116		
157.95	165	171.10	139				