

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041323\
 Data File : VL040369.D
 Acq On : 13 Apr 2023 22:24
 Operator : SY/MD
 Sample : VIBLK
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VIBLK

Quant Time: Apr 14 08:37:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041323AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Thu Apr 13 14:37:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.189	49	942786	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.655	114	2330302	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.478	117	2058210	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	13.786	95	1724538	10.132	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041323\
Data File : VL040369.D
Acq On : 13 Apr 2023 22:24
Operator : SY/MD
Sample : VIBLK
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Apr 14 08:37:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041323AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Thu Apr 13 14:37:02 2023
Response via : Initial Calibration




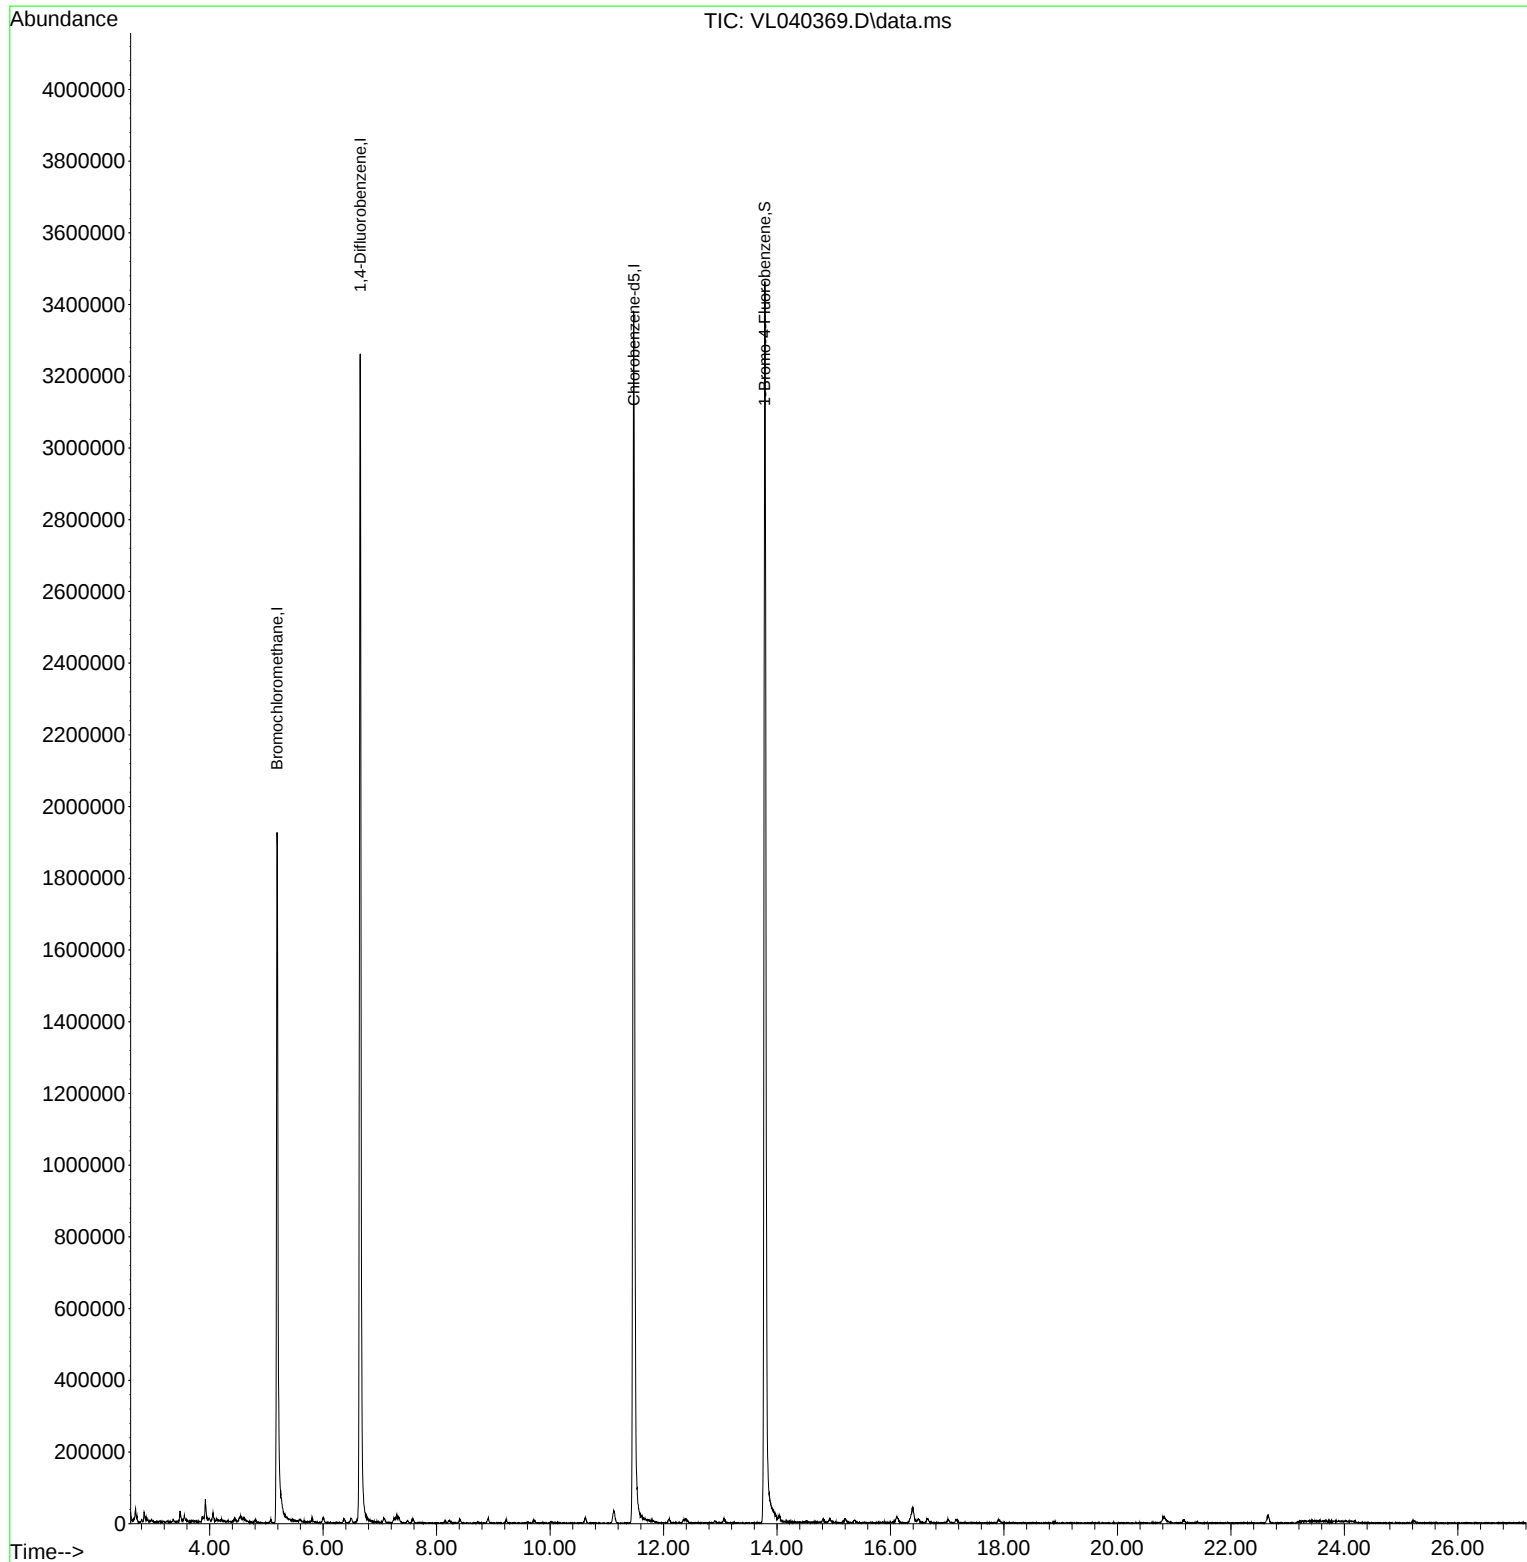


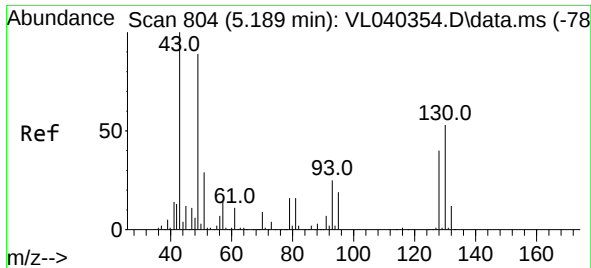

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.189 min Scan# 804
Delta R.T. -0.000 min
Lab File: VL040369.D
Acq: 13 Apr 2023 22:24




Instrument :
MSVOA_1
ClientSampleId :
VIBLK


Tgt Ion: 49 Resp: 942786
Ion Ratio Lower Upper
49 100
128 47.3 23.7 71.1
130 60.4 29.9 89.8

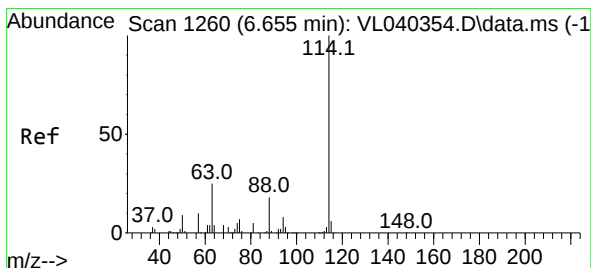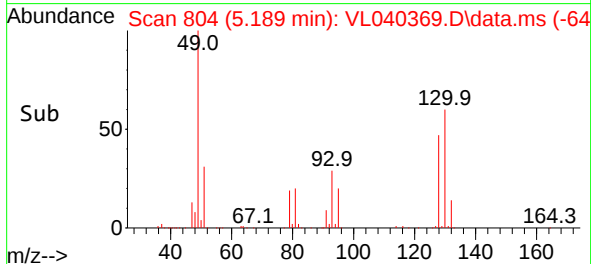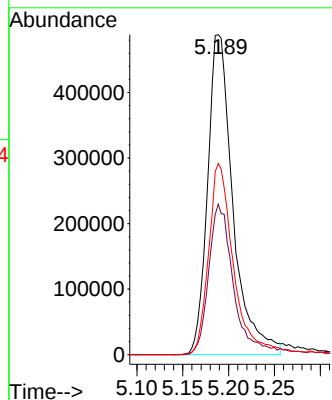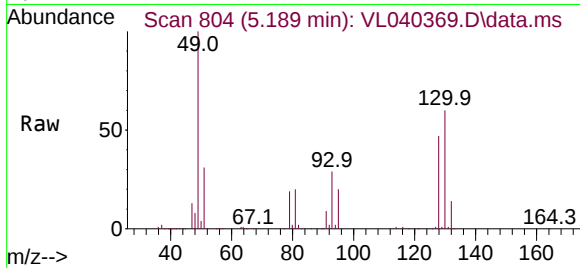

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.655 min Scan# 1260
Delta R.T. 0.000 min
Lab File: VL040369.D
Acq: 13 Apr 2023 22:24

Tgt Ion: 114 Resp: 2330302
Ion Ratio Lower Upper
114 100
63 26.9 21.4 32.0
88 18.5 14.6 22.0


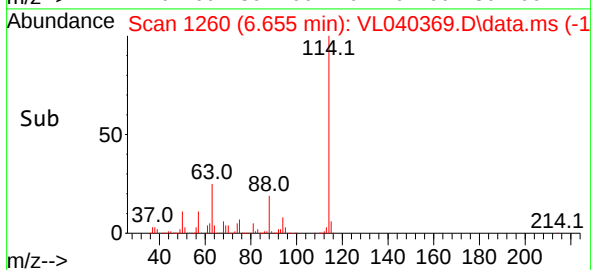
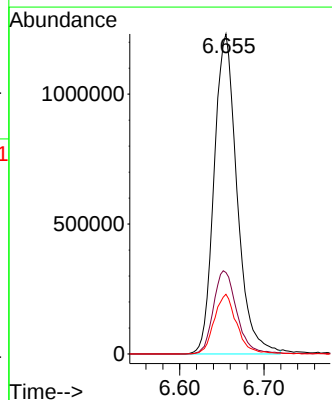
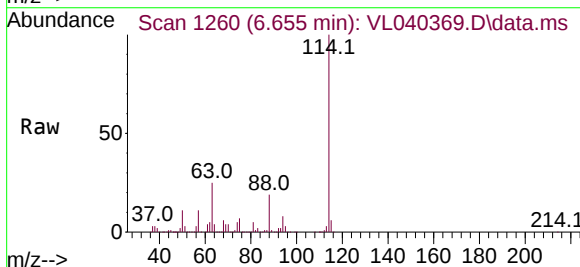


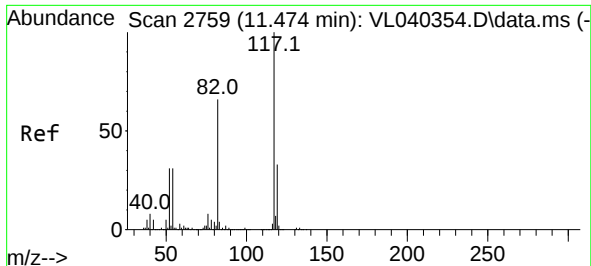

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.478 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL040369.D
Acq: 13 Apr 2023 22:24

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 2058210
Ion Ratio Lower Upper
117 100
82 68.9 52.5 78.7
119 32.7 24.3 36.5

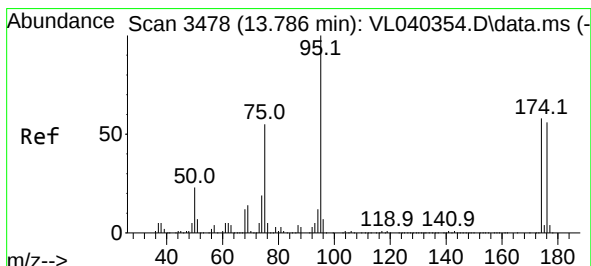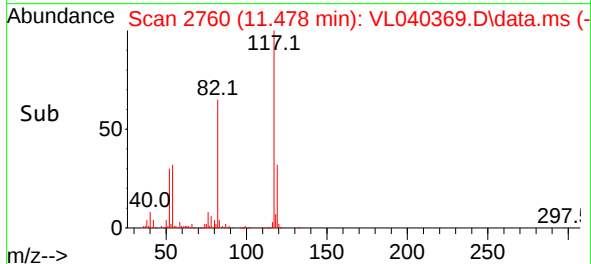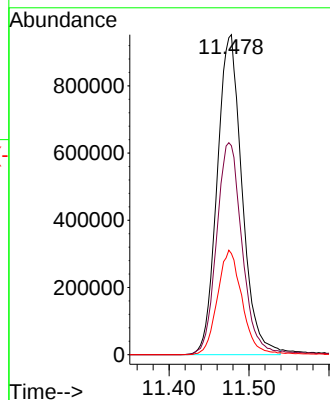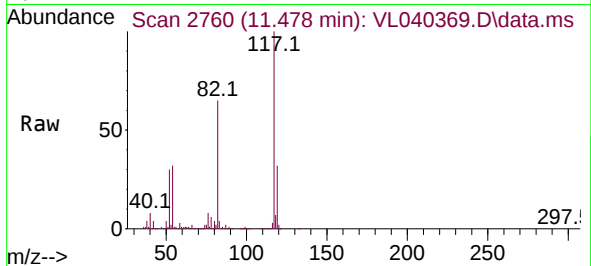

#68
1-Bromo-4-Fluorobenzene
Concen: 10.132 ppbv
RT: 13.786 min Scan# 3478
Delta R.T. 0.000 min
Lab File: VL040369.D
Acq: 13 Apr 2023 22:24

Tgt Ion: 95 Resp: 1724538
Ion Ratio Lower Upper
95 100
174 59.6 47.2 70.8
175 4.1 3.5 5.3

