
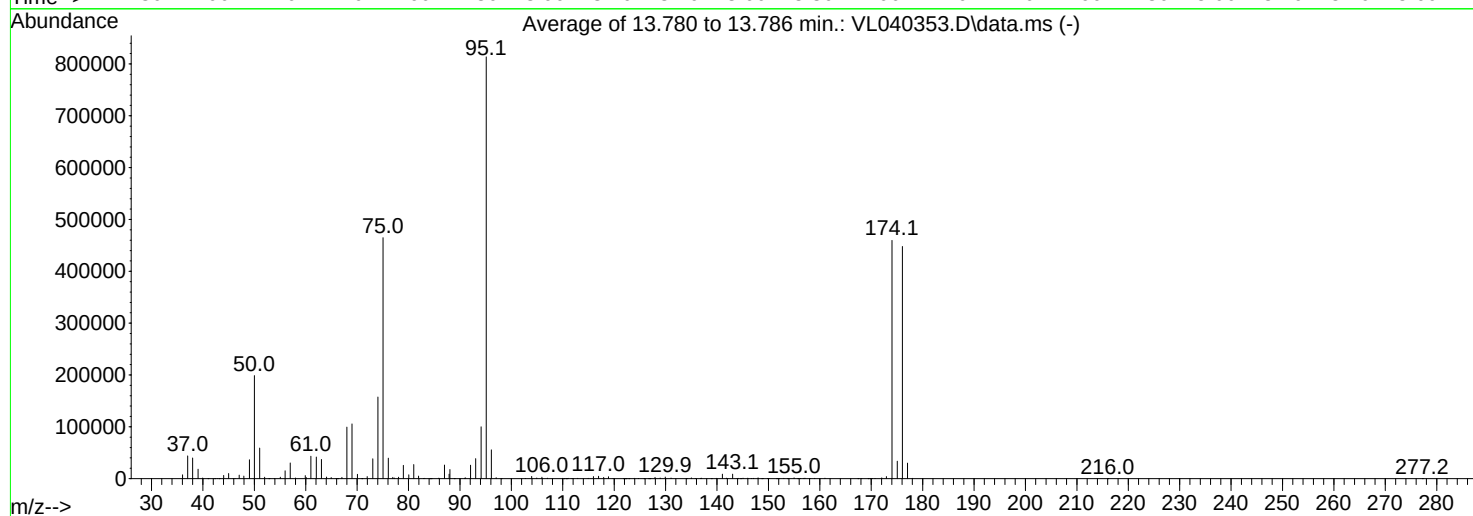


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041323\
 Data File : VL040353.D
 Acq On : 13 Apr 2023 9:26
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041323AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Thu Apr 13 14:37:02 2023

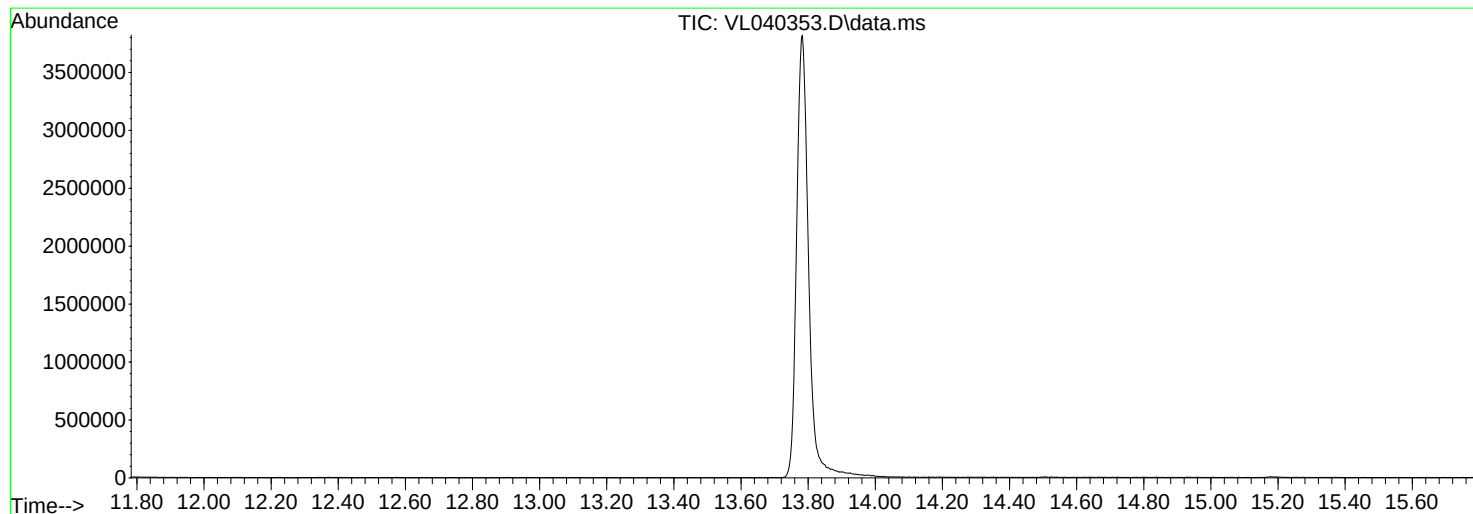

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	198656	PASS
75	95	30	66	57.1	465003	PASS
95	95	100	100	100.0	813739	PASS
96	95	5	9	6.8	55565	PASS
173	174	0.00	2	0.9	4183	PASS
174	95	50	120	56.5	459669	PASS
175	174	4	9	7.3	33541	PASS
176	174	93	101	97.4	447765	PASS
177	176	5	9	6.7	30019	PASS

Average of 13.780 to 13.786 min.: VL040353.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7566	45.90	329	55.05	2849	65.90	181
37.05	43880	46.25	407	56.00	15252	66.20	8
38.00	39960	47.05	6866	57.00	30285	67.05	241
39.05	18395	47.95	4902	58.00	1199	68.00	9954
39.95	1355	49.05	36536	59.90	5762	69.00	105736
41.00	112	50.00	198656	60.10	2073	70.05	8270
42.30	114	51.05	58915	61.00	43301	70.90	144
42.80	229	52.00	2936	62.05	41763	71.05	218
43.15	144	52.80	69	63.05	37125	71.95	4022
44.05	6347	53.00	193	64.05	3225	73.05	38147
45.00	9899	53.90	215	64.95	2212	74.05	157483

Average of 13.780 to 13.786 min.: VL040353.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.05	465003	84.20	153	94.10	99992	110.20	147
76.05	39568	84.40	85	95.10	813739	110.60	135
76.95	2467	85.90	1117	96.10	55565	110.80	147
77.20	1334	87.00	26117	97.05	1728	111.05	702
78.05	2658	87.90	8691	98.00	70	111.80	344
79.00	25581	88.05	17501	102.75	400	112.00	361
80.05	7297	88.90	68	103.95	4372	112.90	772
81.00	27080	90.90	1068	104.95	1272	114.95	697
81.95	4885	91.10	1601	105.95	2828	115.95	3978
82.90	239	92.05	26107	107.00	973	116.95	4788
83.15	638	93.05	38477	109.95	583	117.95	2594

Average of 13.780 to 13.786 min.: VL040353.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.90	3584	127.95	2522	141.05	8513	148.00	1626
119.80	343	128.95	1234	141.85	825	148.70	142
121.80	82	129.95	3050	142.10	325	149.00	337
122.10	139	131.05	1160	143.05	8730	149.85	387
122.30	122	134.00	56	143.90	251	150.10	352
122.85	191	135.00	1494	144.10	595	151.60	84
123.90	754	135.80	194	144.60	119	151.95	130
124.75	359	136.80	504	145.05	866	153.00	527
125.80	167	137.00	807	146.00	1032	153.70	73
126.70	131	138.90	150	146.70	221	154.00	201
126.95	150	139.85	690	147.10	507	155.00	1691

Average of 13.780 to 13.786 min.: VL040353.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.70	91	170.20	207				
156.20	222	170.75	307				
156.90	555	172.05	1688				
157.10	1071	172.95	4183				
158.10	283	174.05	459669				
159.00	607	175.05	33541				
161.00	1078	176.05	447765				
167.40	66	177.05	30019				
168.15	267	178.00	736				
169.40	118	216.00	50				
169.80	96	277.20	52				