

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL041422\
 Data File : VL038928.D
 Acq On : 14 Apr 2022 22:04
 Operator : SY/AP
 Sample : N2259-02
 Misc : 400mL/MSVOA L
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA L
 ClientSampleId :
 1165-19-SG-2

Quant Time: Apr 15 08:08:26 2022
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL040522AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Apr 06 06:12:53 2022
 QLast Update : Wed Apr 06 06:12:53 2022
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	1206982	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.18	114	2936460	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.09	117	2660218	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.41	95	2162217	10.72	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	107.20%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.05	85	110780	0.647	ppbv	97
3) Chlorodifluoromethane	2.97	51	3148484	21.374	ppbv #	61
4) Chloromethane	3.15	50	38757	0.508	ppbv	96
9) Propene	3.21	41	148366	1.904	ppbv	87
10) Heptane	8.12	43	2671392	13.608	ppbv	98
11) Trichlorofluoromethane	3.95	101	440754	3.204	ppbv	99
12) 1,1,2-Trichlorotrifluoroet	4.49	101	4468	0.042	ppbv #	8
13) Ethanol	3.61	45	640343	135.202	ppbv #	100
15) Acetone	3.85	43	24270483	201.975	ppbv #	74
16) 1,3-Butadiene	3.31	39	18232	0.265	ppbv	88
17) tert-Butyl alcohol	4.13	59	35076	0.326	ppbv #	1
19) Isopropyl Alcohol	3.97	45	372790	6.070	ppbv #	100
20) Methylene Chloride	4.36	84	187929	4.312	ppbv	90
21) Allyl Chloride	4.38	41	3329	0.037	ppbv #	21
23) Vinyl Acetate	5.07	43	59580	0.509	ppbv #	7
25) Ethyl Acetate	5.68	43	360748	1.183	ppbv	99
26) Hexane	5.69	57	183787	1.324	ppbv	89
30) Cyclohexane	7.13	84	89833	0.734	ppbv #	63
31) cis-1,2-Dichloroethene	5.67	61	25993	0.204	ppbv #	31
34) 2-Butanone	5.25	43	200203	1.725	ppbv	98
35) Carbon Tetrachloride	7.02	117	5976	0.034	ppbv #	66
36) Benzene	6.89	78	250481	0.938	ppbv	97
39) 1,2-Dichloropropane	7.18	63	746024	7.301	ppbv #	26
42) Bromodichloromethane	7.80	83	28369	0.147	ppbv #	27
44) 2,2,4-Trimethylpentane	7.87	57	212767	0.470	ppbv #	1
50) 4-Methyl-2-Pentanone	8.75	43	244225	0.936	ppbv	94
51) 2-Hexanone	10.11	43	16785	0.085	ppbv #	57
53) Toluene	9.81	91	14757662	47.856	ppbv	90
58) Ethyl Benzene	12.71	91	655578	1.649	ppbv	91
59) m/p-Xylene	12.97	91	1770707	5.302	ppbv	98
60) o-Xylene	13.69	91	693736	2.220	ppbv	94
61) Styrene	13.53	104	35069	0.184	ppbv	92
62) Isopropylbenzene	14.66	105	61733	0.132	ppbv #	77
64) n-propylbenzene	15.56	120	38523	0.316	ppbv #	1
65) tert-Butylbenzene	16.76	119	123607	0.297	ppbv #	56
66) Benzyl Chloride	17.21	91	25854	0.305	ppbv #	66
67) sec-Butylbenzene	17.29	105	83333	0.143	ppbv	99
69) p-Isopropyltoluene	17.64	119	45685	0.095	ppbv #	86
70) n-Butylbenzene	18.55	91	185670	0.384	ppbv #	57
71) 2-Chlorotoluene	15.83	91	23369	0.066	ppbv	71
72) 4-Ethyltoluene	15.83	105	385246	1.032	ppbv	98

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL041422\
Data File : VL038928.D
Acq On : 14 Apr 2022 22:04
Operator : SY/AP
Sample : N2259-02
Misc : 400mL/MSVOA L
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
1165-19-SG-2

Quant Time: Apr 15 08:08:26 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL040522AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Apr 06 06:12:53 2022
QLast Update : Wed Apr 06 06:12:53 2022
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
73) 1,3,5-Trimethylbenzene	16.00	105	339917	1.014	ppbv	92
74) 1,2,4-Trimethylbenzene	16.76	105	1197452	3.379	ppbv #	69
79) Naphthalene	22.17	128	17912	0.068	ppbv	98
80) Naphthalene,2-methyl-	24.97	142	23916	0.366	ppbv #	58

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL041422\
Data File : VL038928.D
Acq On : 14 Apr 2022 22:04
Operator : SY/AP
Sample : N2259-02
Misc : 400mL/MSVOA L
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
1165-19-SG-2


Quant Time: Apr 15 08:08:26 2022


Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL040522AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Apr 06 06:12:53 2022

QLast Update : Wed Apr 06 06:12:53 2022

Response via : Initial Calibration



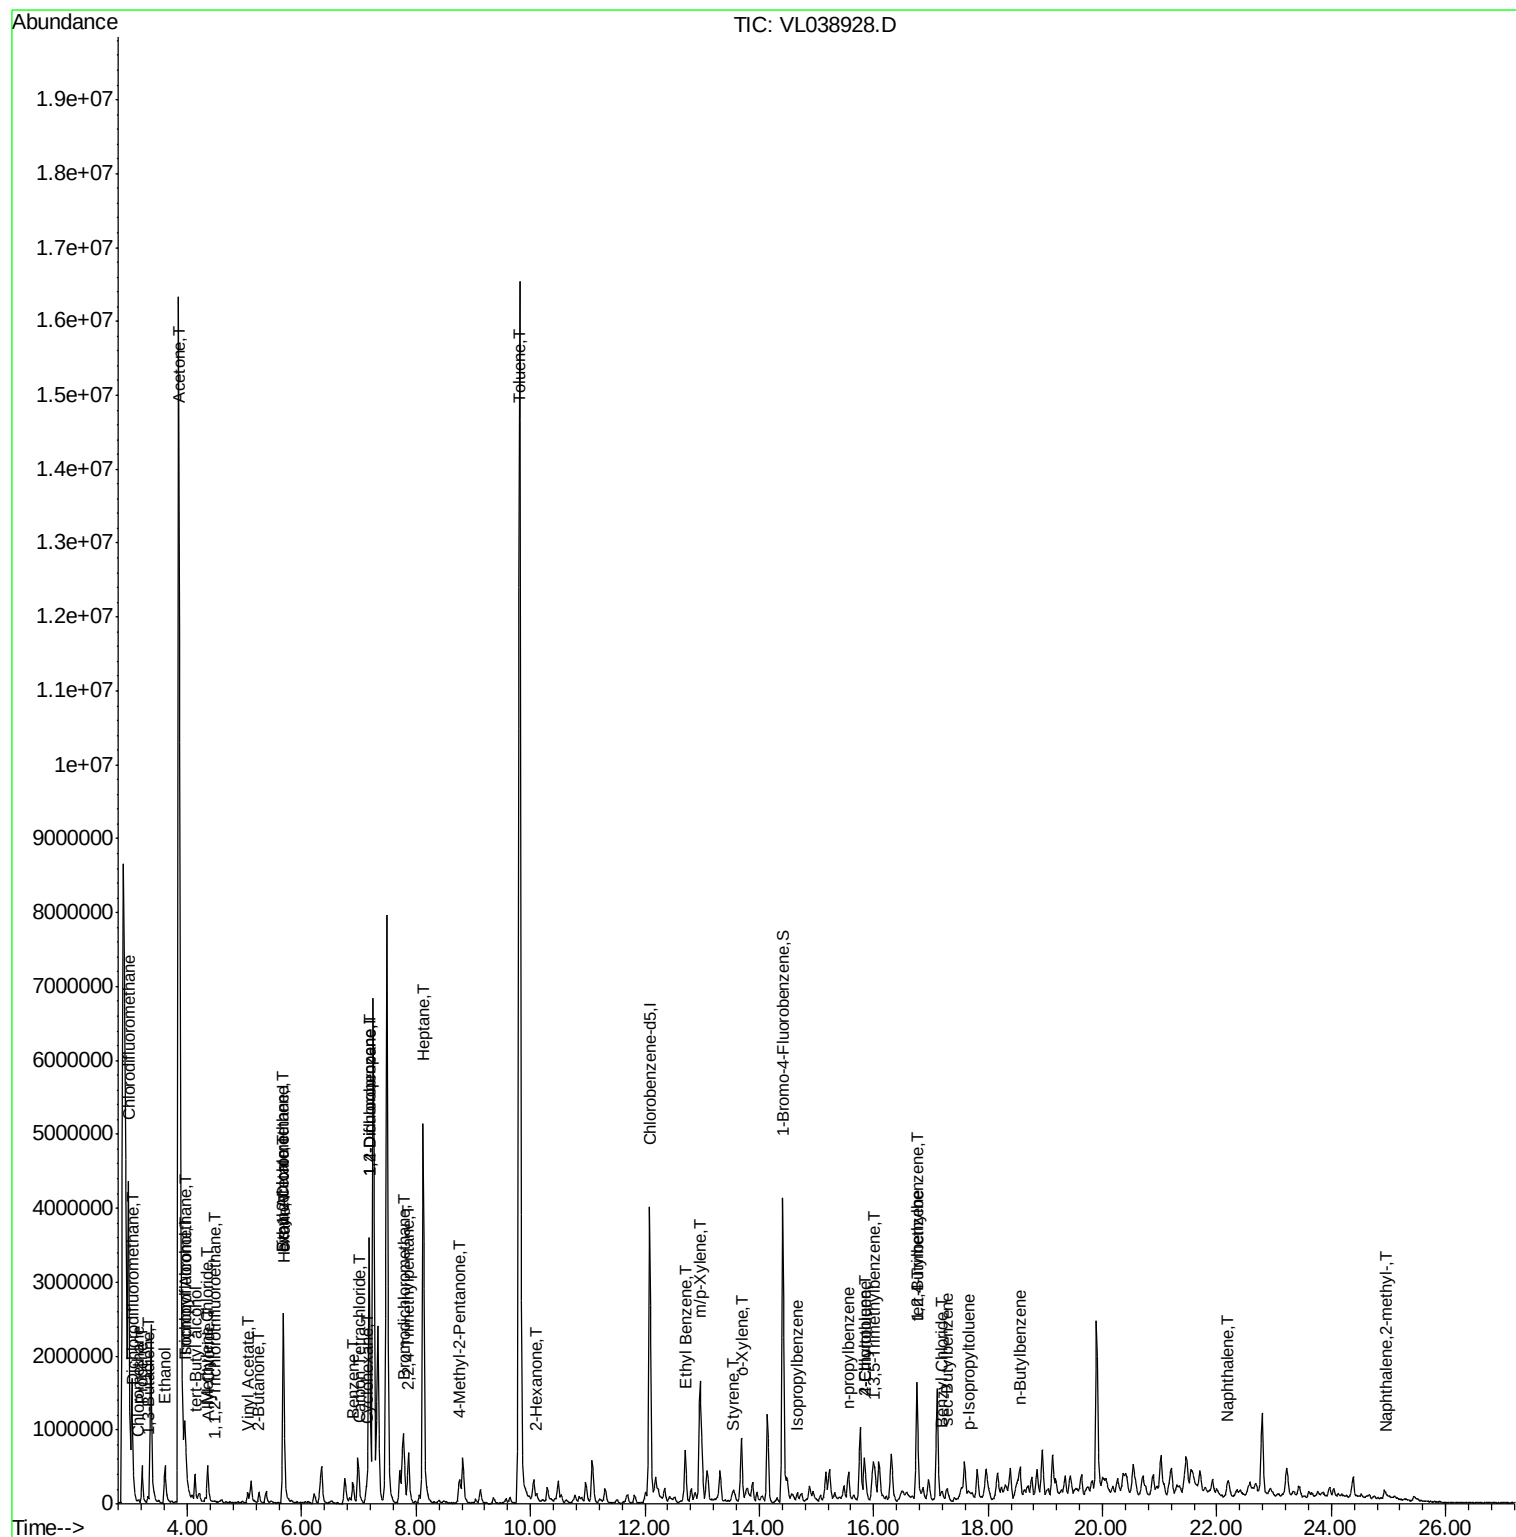




#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.67
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 1165-19-SG-2
 Acq: 14 Apr 2022 22:04

Tot Ion: 49 Resp: 1206982





Ion	Ratio	Lower	Upper
49	100		
128	46.3	24.1	72.3
130	58.7	30.9	92.8

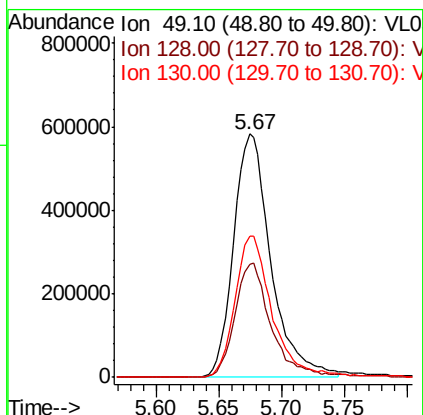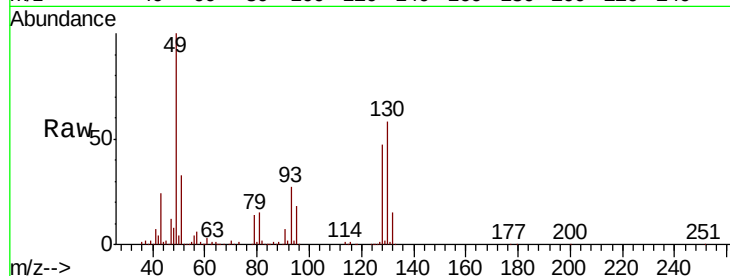


#2
 Dichlorodifluoromethane
 Concen: 0.647 ppbv
 RT: 3.05 min Scan# 83
 Delta R.T.: 0.00 min
 Lab File: VL038928.D
 Acq: 14 Apr 2022 22:04

Tgt Ion: 85 Resp: 110780





Ion	Ratio	Lower	Upper
85	100		
87	34.1	25.9	38.9

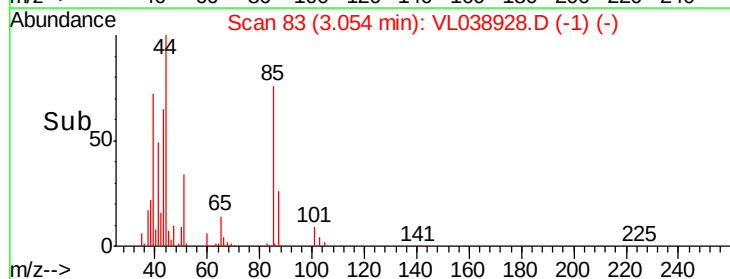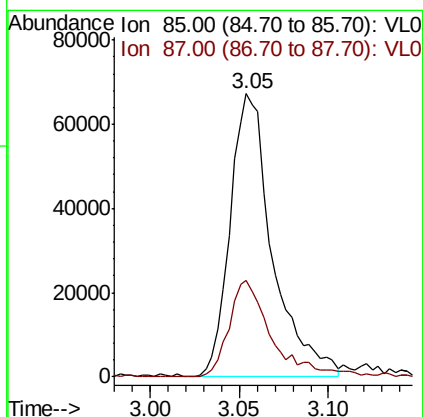






#3
 Chlorodifluoromethane
 Concen: 21.374 ppbv
 RT: 2.97
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 1165-19-SG-2
 Acq: 14 Apr 2022 22:04


Tot Ion: 51 Resp: 3148484
 Ion Ratio Lower Upper
 51 100
 67 0.0 13.4 20.0#

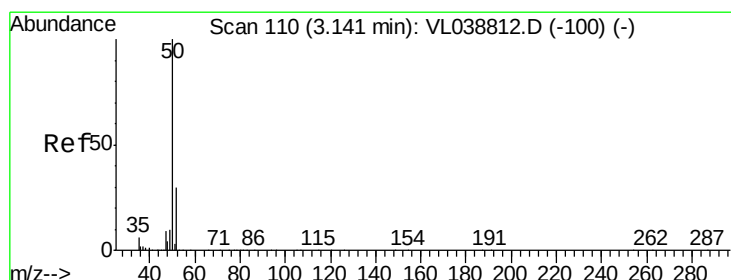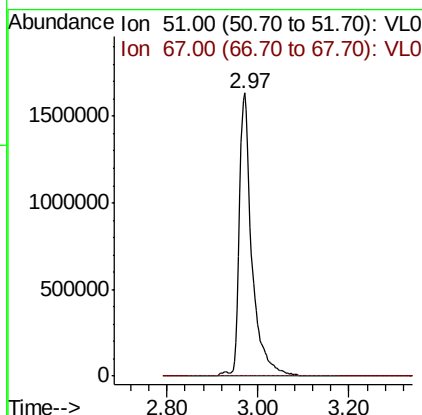

#4
 Chloromethane
 Concen: 0.508 ppbv
 RT: 3.15 min Scan# 112
 Delta R.T. 0.01 min
 Lab File: VL038928.D
 Acq: 14 Apr 2022 22:04

Tgt Ion: 50 Resp: 38757
 Ion Ratio Lower Upper
 50 100
 52 32.5 24.3 36.5

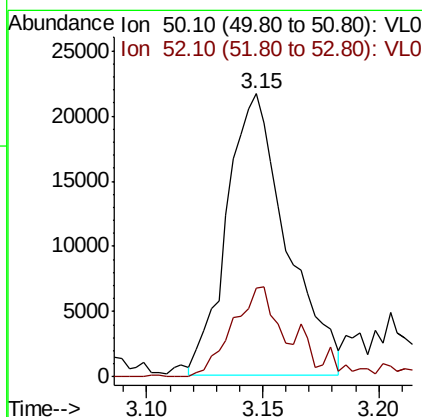



#9

Propene

Concen: 1.904 ppbv

RT: 3.21 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:





Acq: 14 Apr 2022 22:04

Tot Ion: 41 Resp: 148366

Ion Ratio Lower Upper

41 100

42 77.9 54.2 81.4

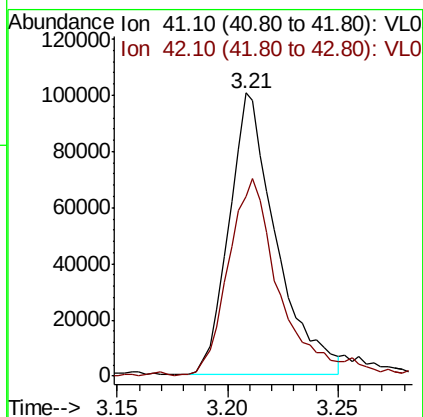

#10

Heptane

Concen: 13.608 ppbv

RT: 8.12 min Scan# 1660

Delta R.T. 0.01 min

Lab File: VL038928.D




Acq: 14 Apr 2022 22:04


Tgt Ion: 43 Resp: 2671392

Ion Ratio Lower Upper

43 100

57 50.2 39.3 58.9

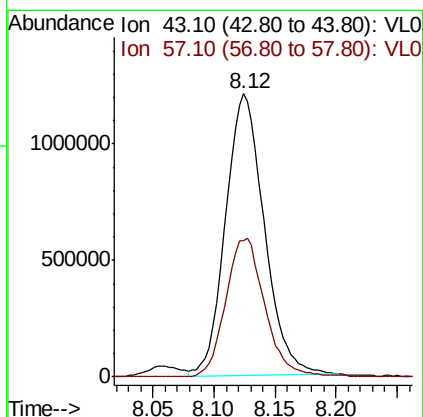



#11

Trichlorofluoromethane

Concen: 3.204 ppbv

RT: 3.95 Instrument: MSVOA_1

Delta R.T.

Lab File: ClientSampleId:


Acq: 14 Apr 2022 22:04

Tot Ion:101 Resp: 440754

Ion Ratio Lower Upper




101 100

103 63.3 51.4 77.0

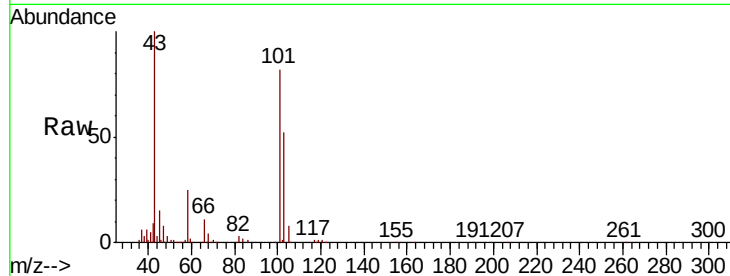

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 103.00 (102.70 to 103.70): V

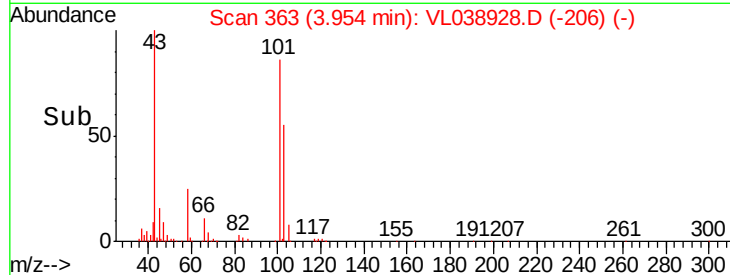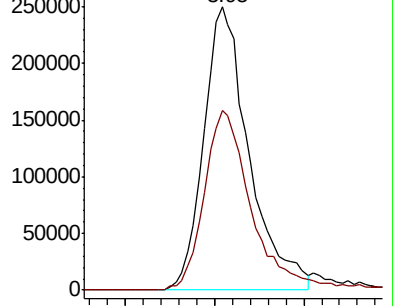

#12

1,1,2-Trichlorotrifluoroethane

Concen: 0.042 ppbv

RT: 4.49 min Scan# 529

Delta R.T. 0.00 min

Lab File: VL038928.D


Acq: 14 Apr 2022 22:04

Tgt Ion:101 Resp: 4468

Ion Ratio Lower Upper



101 100


151 153.3 59.9 89.9#

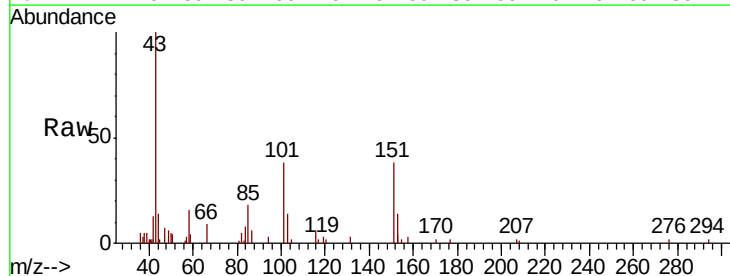

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 151.00 (150.70 to 151.70): V

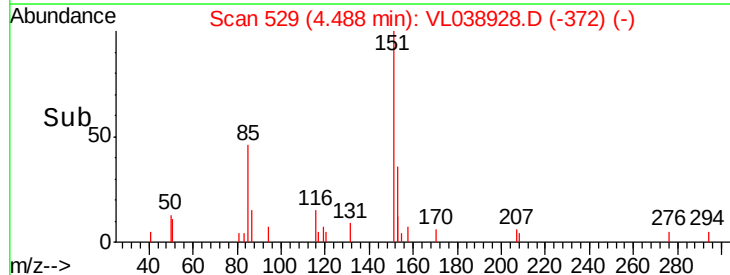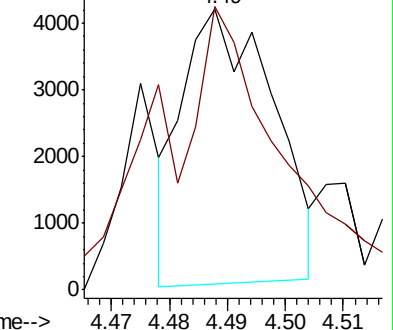



#13

Ethanol

Concen: 135.202 ppbv

RT: 3.61 Instrument: MSVOA_1

Delta R.T. 0.01

Lab File: ClientSampleId: 1165-19-SG-2





Acq: 14 Apr 2022 22:04

Tot Ion: 45 Resp: 640343

Ion Ratio Lower Upper

45 100

46 37.4 0.0 0.0#

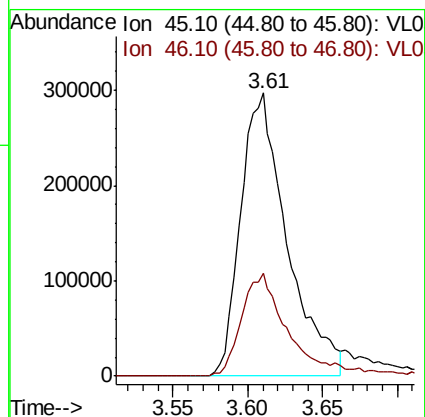

#15

Acetone

Concen: 201.975 ppbv

RT: 3.85 min Scan# 331

Delta R.T. 0.01 min

Lab File: VL038928.D




Acq: 14 Apr 2022 22:04


Tgt Ion: 43 Resp: 24270483

Ion Ratio Lower Upper

43 100





58 41.8 22.5 33.7#

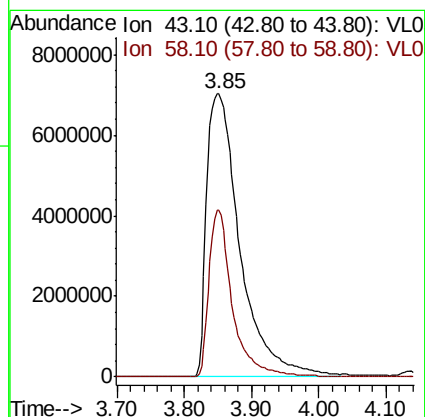

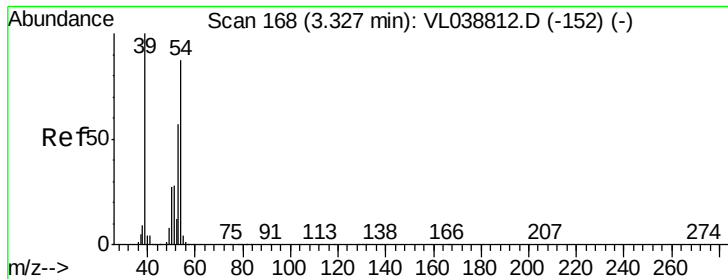




#16
 1,3-Butadiene
 Concen: 0.265 ppbv
 RT: 3.31
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 1165-19-SG-2
 Acq: 14 Apr 2022 22:04


Tot Ion: 39 Resp: 18232
 Ion Ratio Lower Upper
 39 100
 54 91.8 64.8 97.2

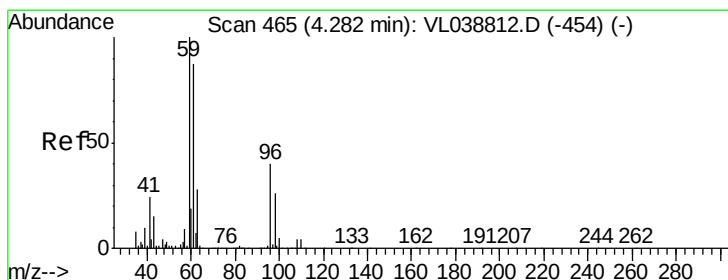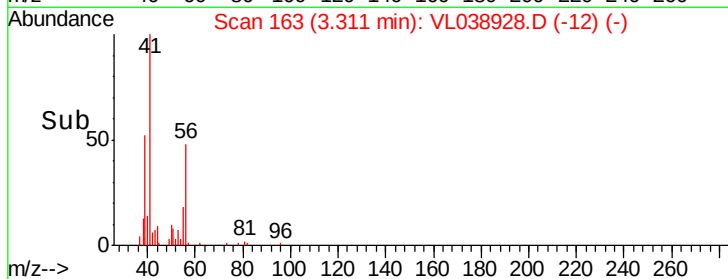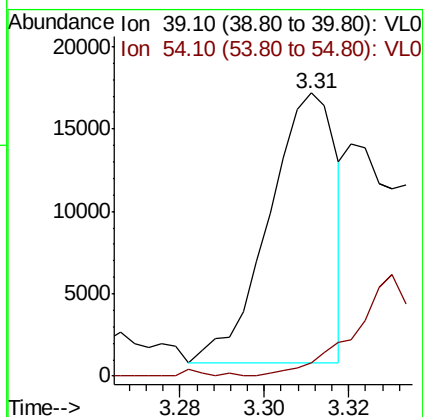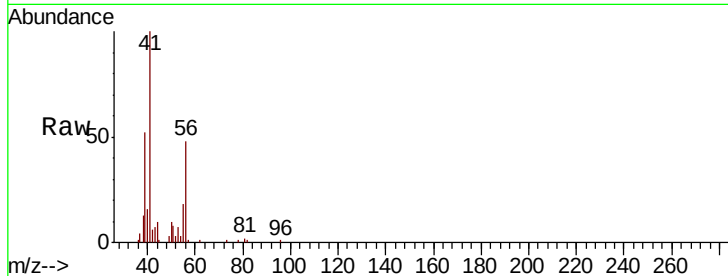

#17
 tert-Butyl alcohol
 Concen: 0.326 ppbv
 RT: 4.13 min Scan# 417
 Delta R.T. -0.15 min
 Lab File: VL038928.D
 Acq: 14 Apr 2022 22:04

Tgt Ion: 59 Resp: 35076
 Ion Ratio Lower Upper
 59 100
 57 74.7 8.5 12.7#

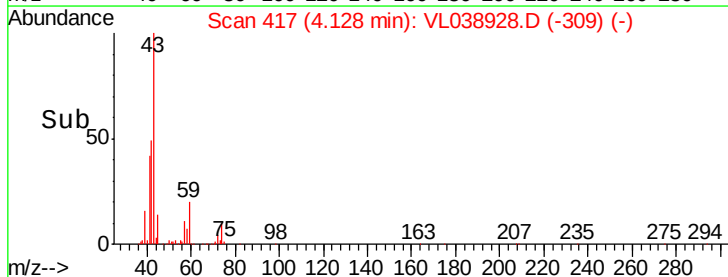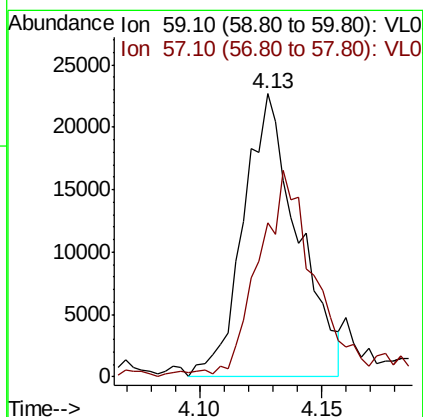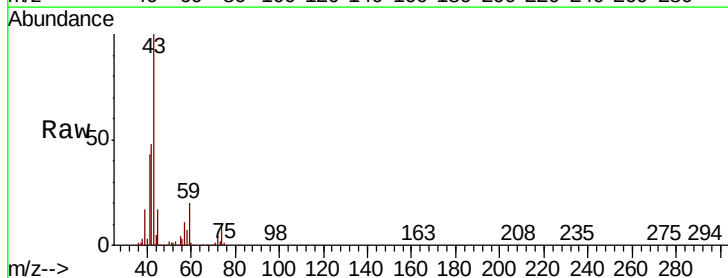



#19

Isopropyl Alcohol

Concen: 6.070 ppbv

RT: 3.97 Instrument:

Delta R.T. MSVOA_1

Lab File: ClientSampleId:


Acq: 14 Apr 2022 22:04

Tot Ion: 45 Resp: 372790

Ion Ratio Lower Upper




45 100

58 0.0 0.0 0.0



Abundance Ion 45.10 (44.80 to 45.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

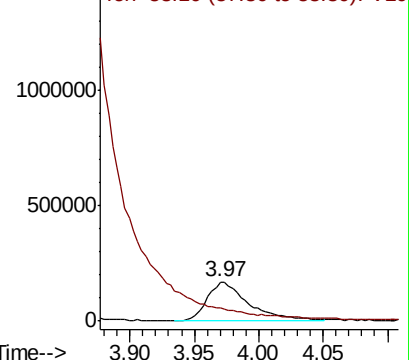

#20

Methylene Chloride

Concen: 4.312 ppbv

RT: 4.36 min Scan# 488

Delta R.T. 0.01 min

Lab File: VL038928.D

Acq: 14 Apr 2022 22:04

Tgt Ion: 84 Resp: 187929


Ion Ratio Lower Upper

84 100

49 148.1 129.4 194.0

51 42.6 37.4 56.2

86 56.1 51.4 77.2






Abundance Ion 84.00 (83.70 to 84.70): VL0

Ion 49.10 (48.80 to 49.80): VL0

Ion 51.10 (50.80 to 51.80): VL0





Ion 86.00 (85.70 to 86.70): VL0

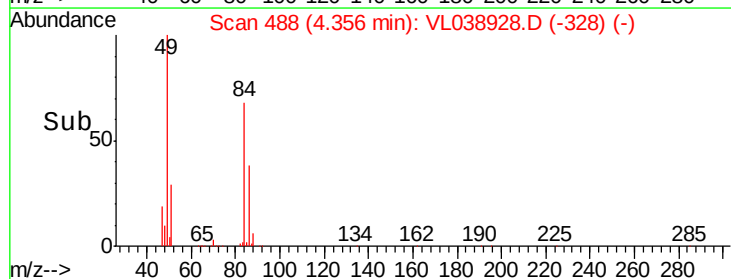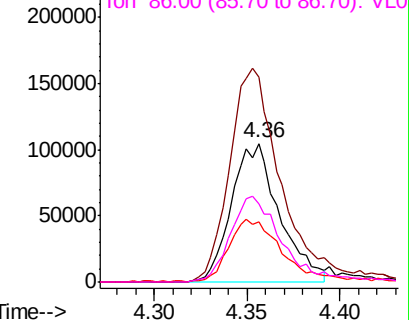






#21
Allvl Chloride
Concen: 0.037 ppbv
RT: 4.38
Delta R.T. MSVOA_L
Lab File: ClientSampleId:
Acq: 14 Apr 2022 22:04


Tot Ion: 41 Resp: 3329
Ion Ratio Lower Upper
41 100
76 2.1 23.7 35.5#
39 0.0 62.0 93.0#

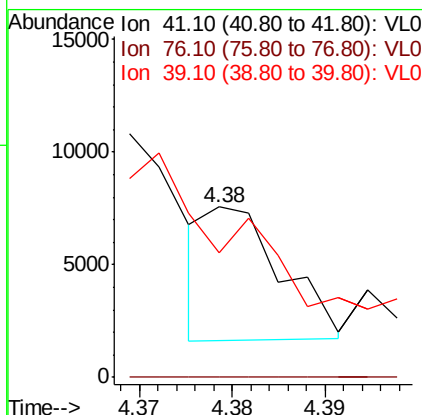

#23
Vinyl Acetate
Concen: 0.509 ppbv
RT: 5.07 min Scan# 709
Delta R.T. -0.00 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04





Tgt Ion: 43 Resp: 59580
Ion Ratio Lower Upper
43 100
86 9.9 5.8 8.6#
42 80.8 7.8 11.6#
44 0.0 3.6 5.4#

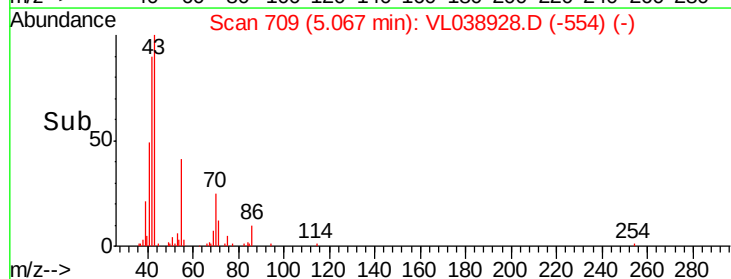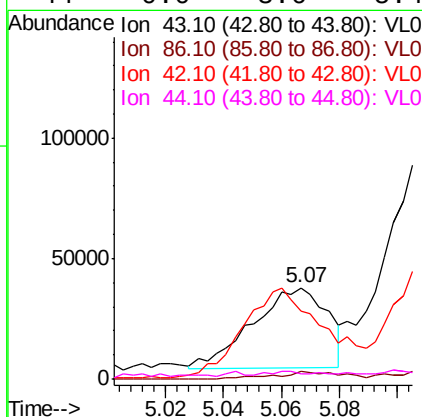

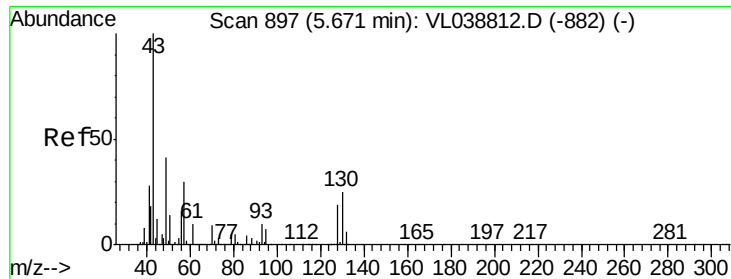




#25
Ethyl Acetate
Concen: 1.183 ppbv
RT: 5.68
Delta R.T. MSVOA_1
Lab File: ClientSampleId :
1165-19-SG-2
Acq: 14 Apr 2022 22:04


Tot Ion:	43	Resp:	360748
Ion	Ratio	Lower	Upper
43	100		
45	10.2	8.4	12.6
61	8.8	7.9	11.9
70	6.9	5.6	8.4

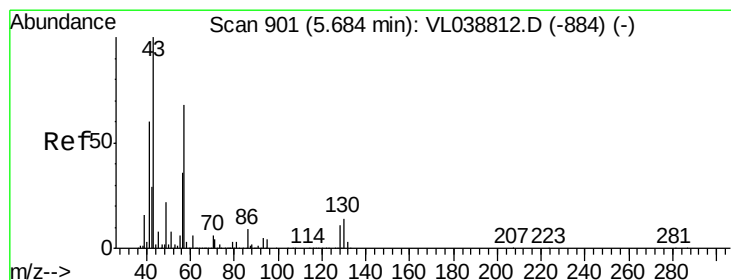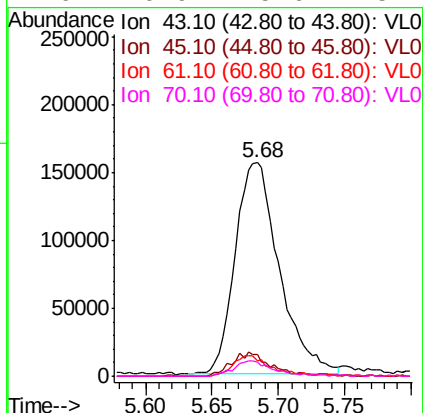

#26
Hexane
Concen: 1.324 ppbv
RT: 5.69 min Scan# 903
Delta R.T. 0.01 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04





Tgt Ion:	57	Resp:	183787
Ion	Ratio	Lower	Upper
57	100		
41	93.0	72.0	108.0
43	206.3	186.6	280.0
56	55.0	42.8	64.2

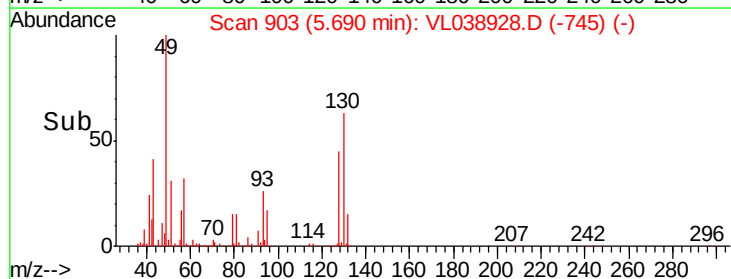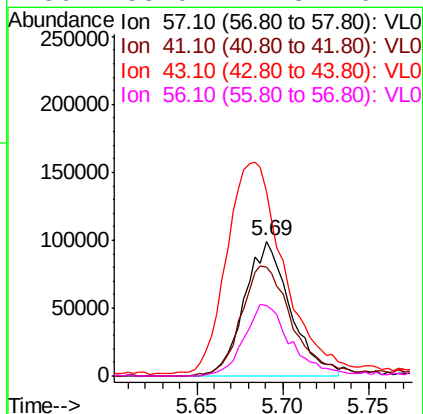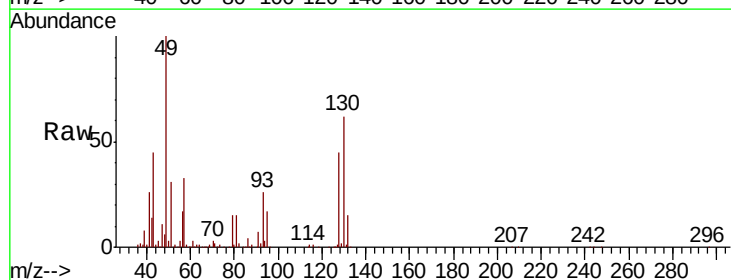

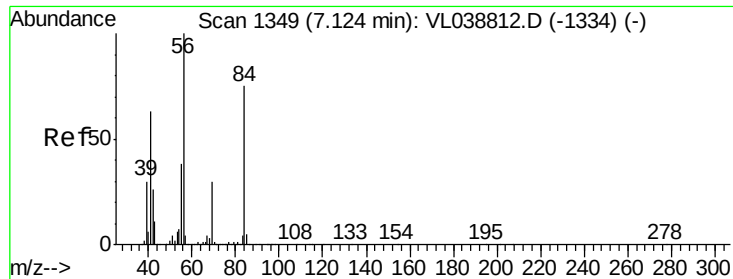




#30
Cvclohexane
Concen: 0.734 ppbv
RT: 7.13
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 14 Apr 2022 22:04


Tot Ion: 84 Resp: 89833
Ion Ratio Lower Upper
84 100
56 121.0 114.4 171.6
41 150.1 69.0 103.4#

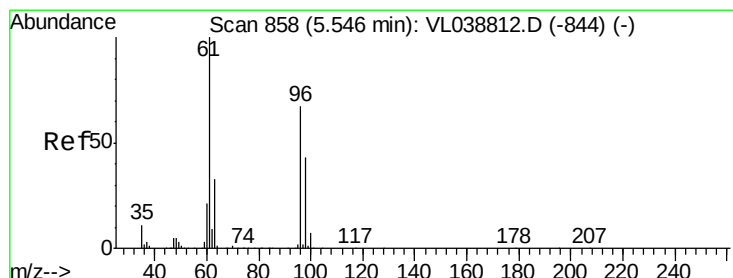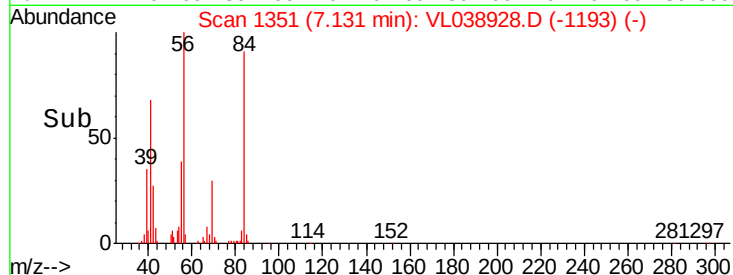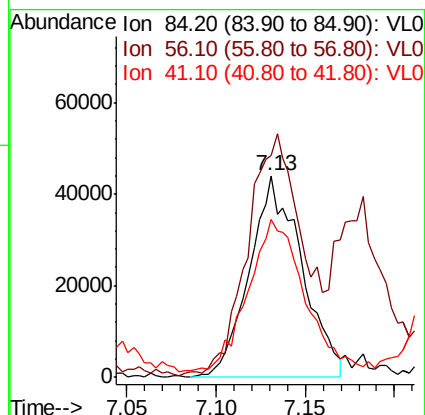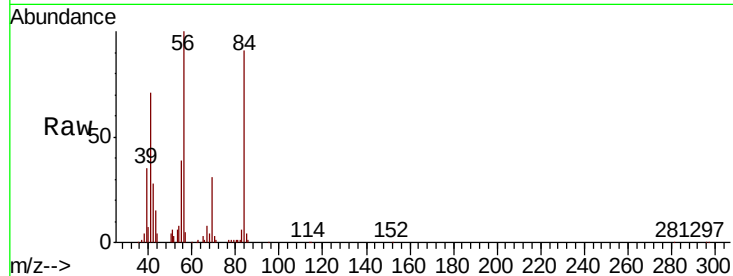

#31
cis-1,2-Dichloroethene
Concen: 0.204 ppbv
RT: 5.67 min Scan# 898
Delta R.T. 0.13 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04

Tgt Ion: 61 Resp: 25993
Ion Ratio Lower Upper
61 100
96 10.6 53.4 80.0#
98 0.0 34.2 51.4#

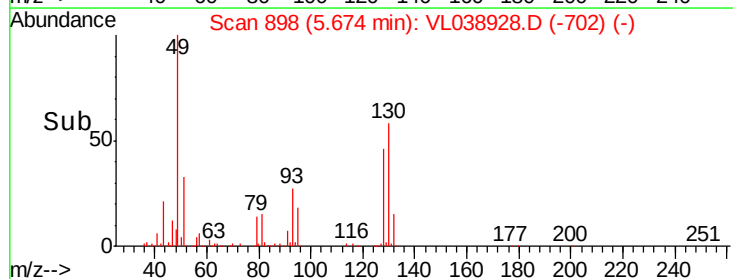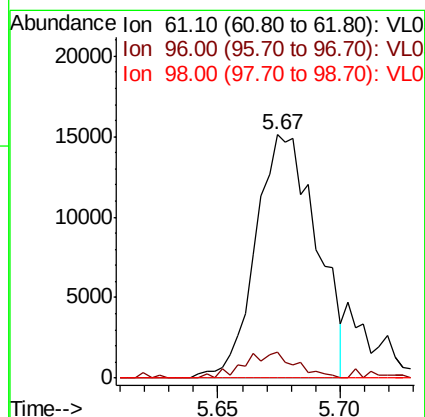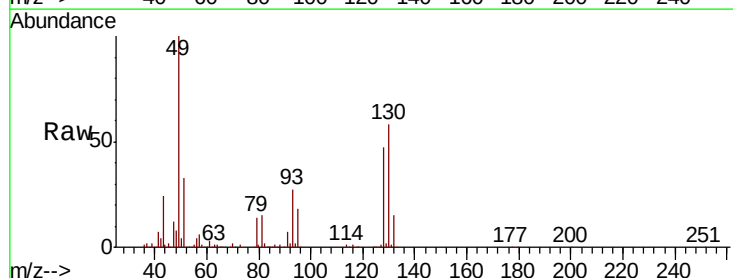

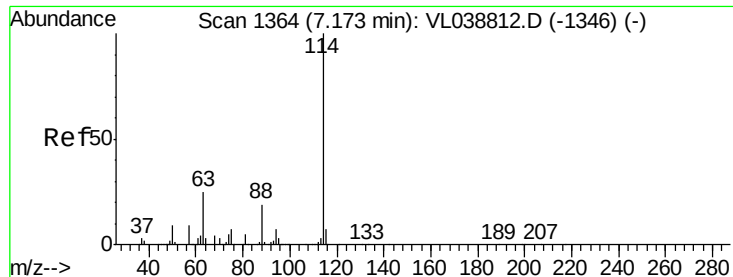

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.18 Instrument: MSVOA_1





Delta R.T. ClientSampleId:

Lab File: 1165-19-SG-2

Acq: 14 Apr 2022 22:04

Tot Ion:114 Resp: 2936460

Ion	Ratio	Lower	Upper
114	100		
63	26.5	19.8	29.8
88	18.8	14.2	21.4

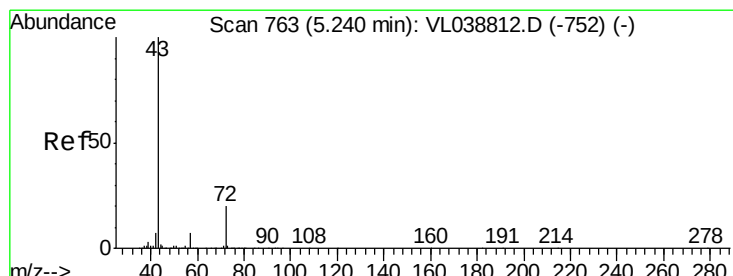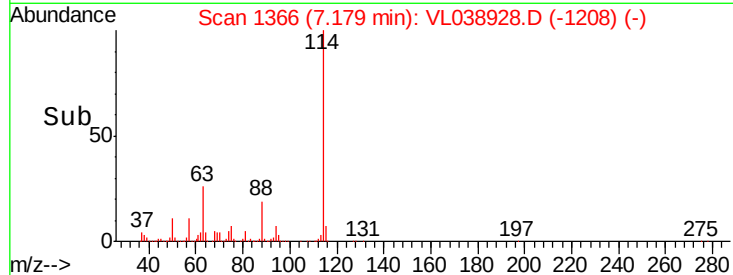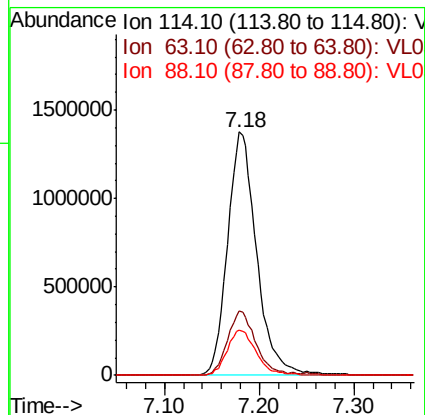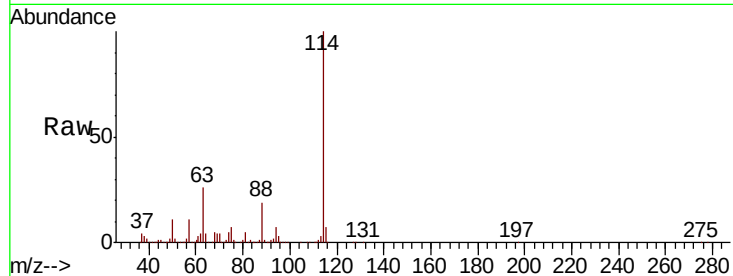

#34

2-Butanone

Concen: 1.725 ppbv

RT: 5.25 min Scan# 765




Delta R.T. 0.01 min


Lab File: VL038928.D

Acq: 14 Apr 2022 22:04

Tgt Ion: 43 Resp: 200203





Ion	Ratio	Lower	Upper
43	100		
72	21.8	16.9	25.3

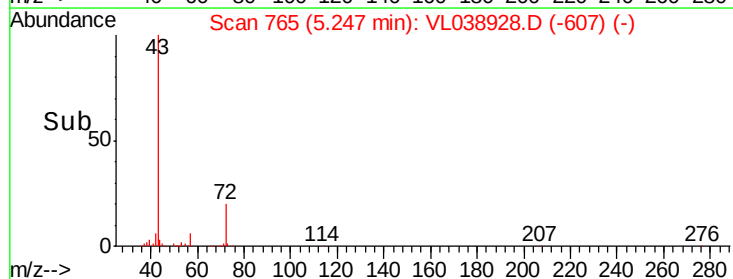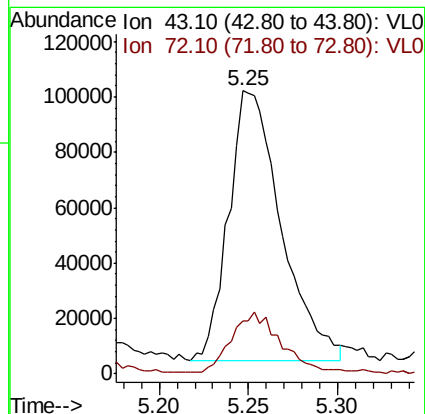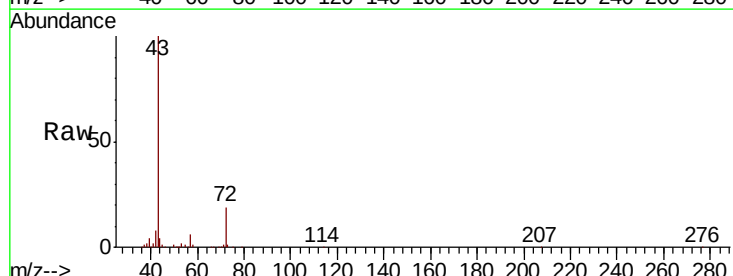

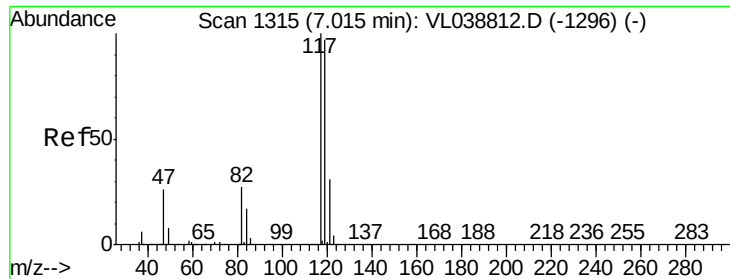




#35
Carbon Tetrachloride
Concen: 0.034 ppbv
RT: 7.02
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
Acq: 14 Apr 2022 22:04


Tot Ion: 117 Resp: 5976
Ion Ratio Lower Upper
117 100
119 131.6 77.7 116.5#
121 47.7 24.5 36.7#

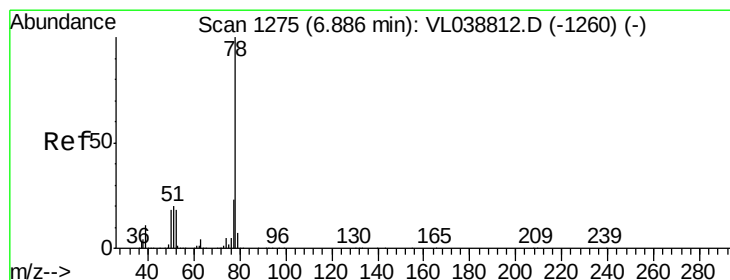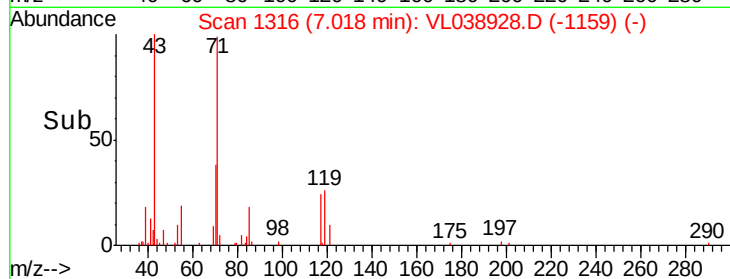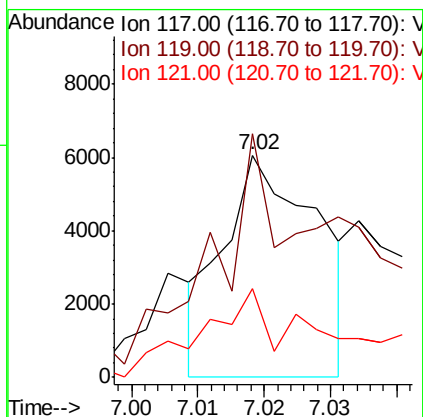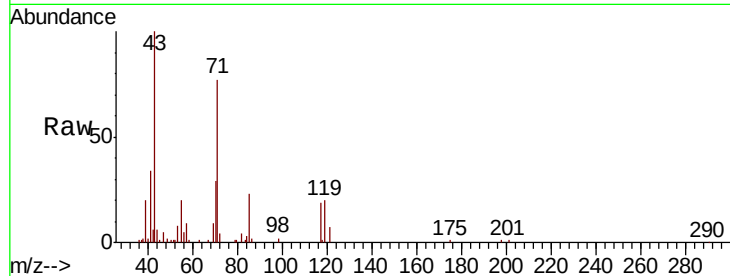

#36
Benzene
Concen: 0.938 ppbv
RT: 6.89 min Scan# 1277
Delta R.T. 0.01 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04

Tgt Ion: 78 Resp: 250481
Ion Ratio Lower Upper
78 100
77 20.2 18.2 27.2
50 17.6 14.0 21.0

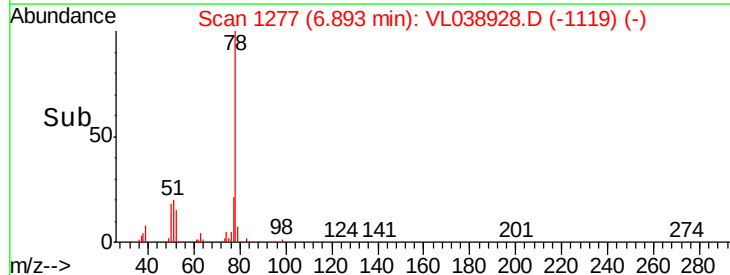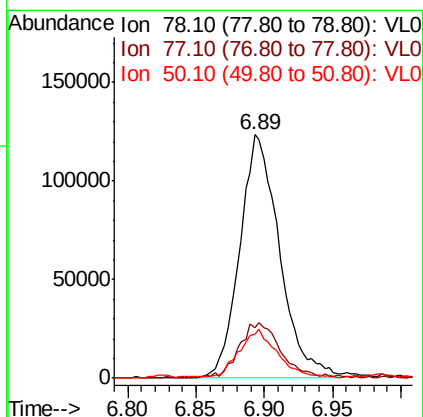

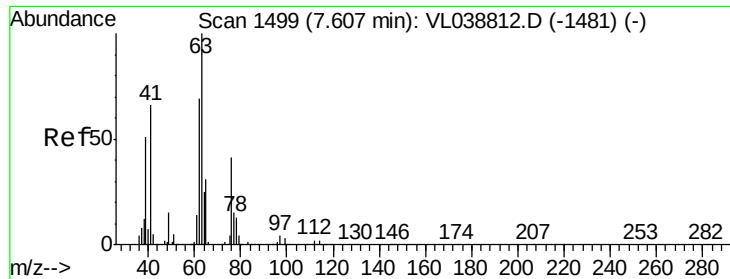

#39

1,2-Dichloropropane

Concen: 7.301 ppbv

RT: 7.18 Instrument:

Delta R.T. MSVOA_1

Lab File: ClientSampleId:

Acq: 14 Apr 2022 22:04


Tot Ion: 63 Resp: 746024

Ion Ratio Lower Upper

63 100

41 0.0 53.0 79.6#




62 15.7 55.0 82.4#



Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0

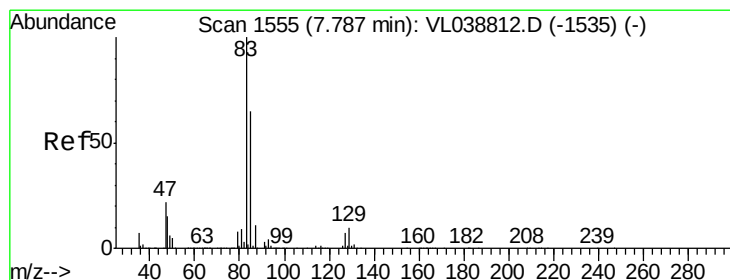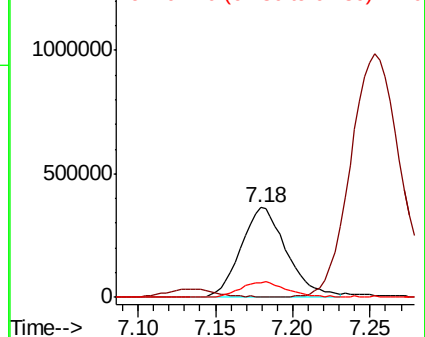

#42

Bromodichloromethane

Concen: 0.147 ppbv

RT: 7.80 min Scan# 1558

Delta R.T. 0.01 min

Lab File: VL038928.D

Acq: 14 Apr 2022 22:04


Tgt Ion: 83 Resp: 28369

Ion Ratio Lower Upper

83 100

85 2.8 51.7 77.5#



127 0.0 5.9 8.9#

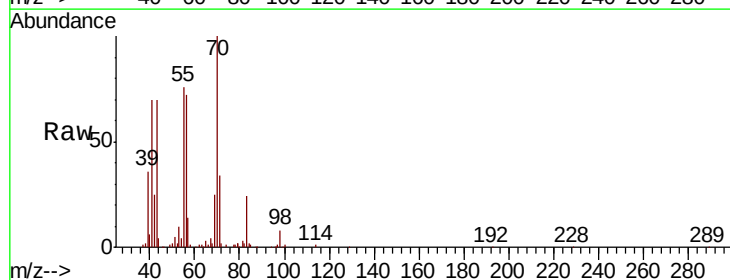


Abundance Ion 83.00 (82.70 to 83.70): VL0

Ion 85.00 (84.70 to 85.70): VL0

Ion 126.90 (126.60 to 127.60): V

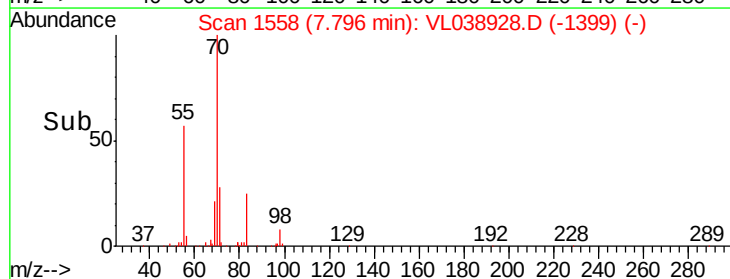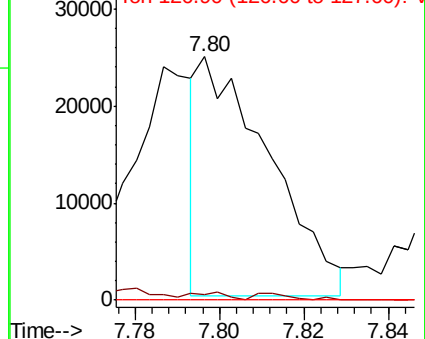

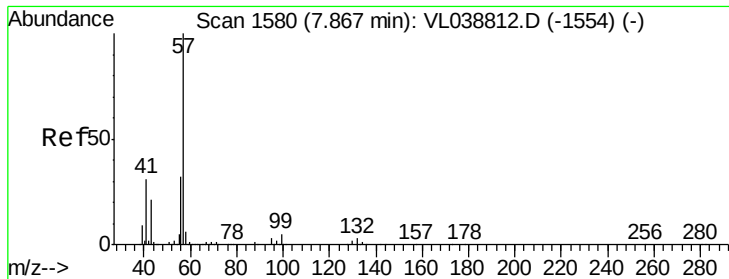

#44

2,2,4-Trimethylpentane

Concen: 0.470 ppbv

RT: 7.87 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 14 Apr 2022 22:04


Tot Ion: 57 Resp: 212767

Ion Ratio Lower Upper

57 100

41 109.5 25.0 37.4#

56 135.9 25.3 37.9#

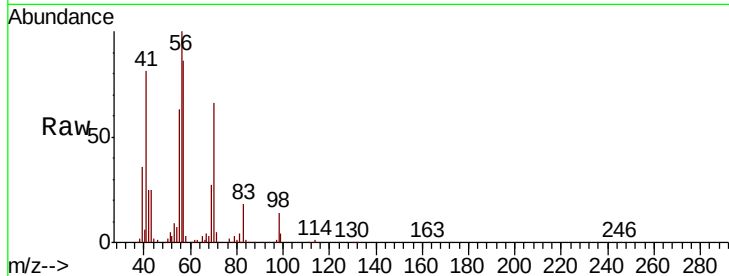

Abundance Ion 57.10 (56.80 to 57.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 56.10 (55.80 to 56.80): VL0

150000



100000

50000

0

7.80 7.85 7.90

Time-->

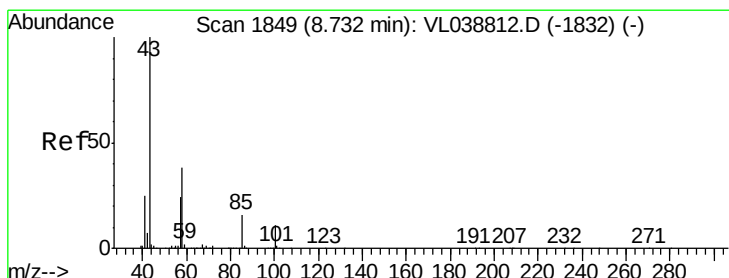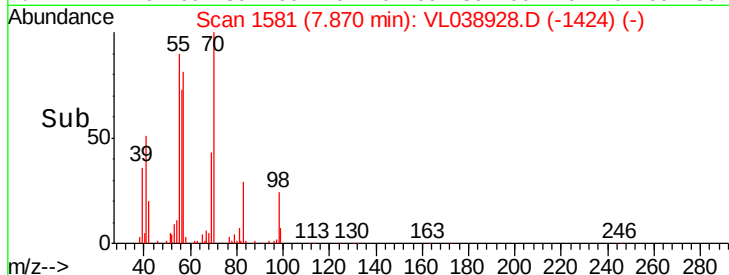

#50

4-Methyl-2-Pentanone

Concen: 0.936 ppbv

RT: 8.75 min Scan# 1855

Delta R.T. 0.02 min

Lab File: VL038928.D


Acq: 14 Apr 2022 22:04

Tgt Ion: 43 Resp: 244225

Ion Ratio Lower Upper

43 100

58 40.0 29.0 43.6

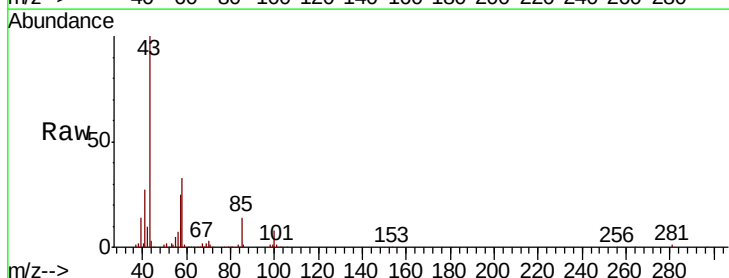

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

120000

100000

80000

60000


40000


20000

0

8.70 8.75 8.80


Time-->

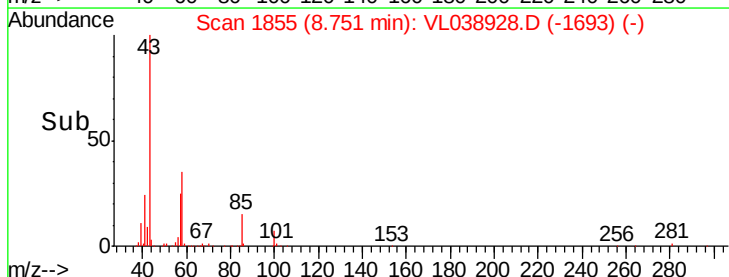



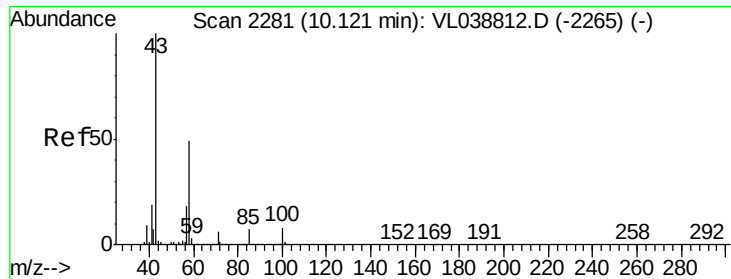


#51
2-Hexanone
Concen: 0.085 ppbv
RT: 10.11
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 14 Apr 2022 22:04

Tot Ion: 43 Resp: 16785
Ion Ratio Lower Upper
43 100
58 21.7 41.4 62.0#
98 0.0 0.1 0.1#




Abundance Ion 43.10 (42.80 to 43.80): VL0
Ion 58.10 (57.80 to 58.80): VL0
Ion 98.20 (97.90 to 98.90): VL0


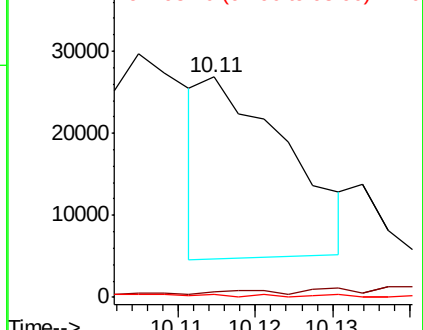



#53
Toluene
Concen: 47.856 ppbv
RT: 9.81 min Scan# 2185
Delta R.T. 0.01 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04

Tgt Ion: 91 Resp: 14757662
Ion Ratio Lower Upper
91 100
92 69.4 49.2 73.8







Abundance Ion 91.10 (90.80 to 91.80): VL0
Ion 92.10 (91.80 to 92.80): VL0

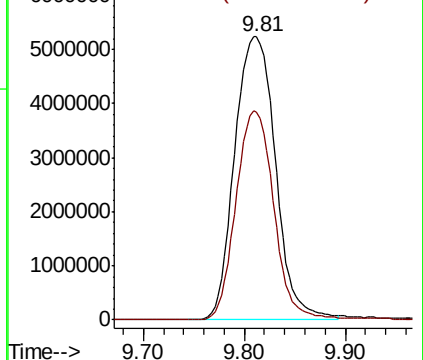






#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.09 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
Acq: 14 Apr 2022 22:04


Tot Ion: 117 Resp: 2660218
Ion Ratio Lower Upper
117 100
82 67.2 53.0 79.6
119 32.7 24.9 37.3

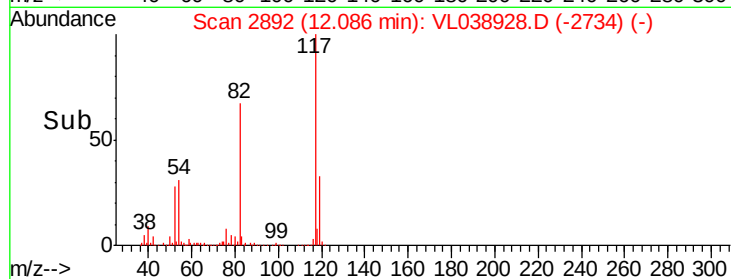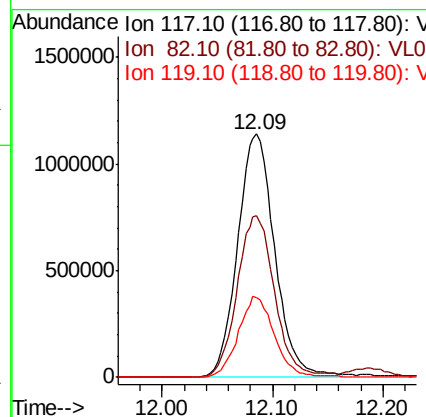

#58
Ethyl Benzene
Concen: 1.649 ppbv
RT: 12.71 min Scan# 3086
Delta R.T.: 0.01 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04





Tgt Ion: 91 Resp: 655578
Ion Ratio Lower Upper
91 100
106 28.3 26.7 40.1

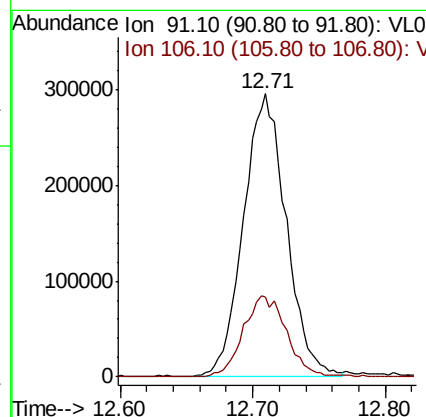

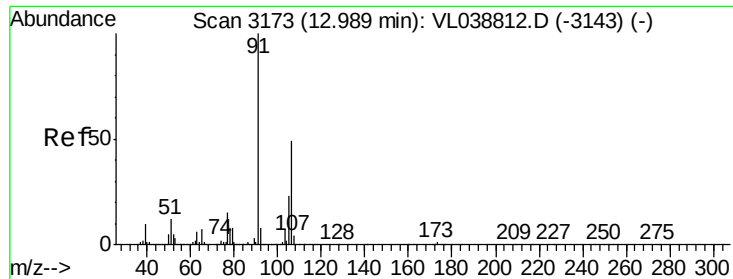




#59
m/p-Xylene
Concen: 5.302 ppbv
RT: 12.97 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
Acq: 14 Apr 2022 22:04


Tot Ion: 91 Resp: 1770707
Ion Ratio Lower Upper
91 100
106 45.0 37.1 55.7

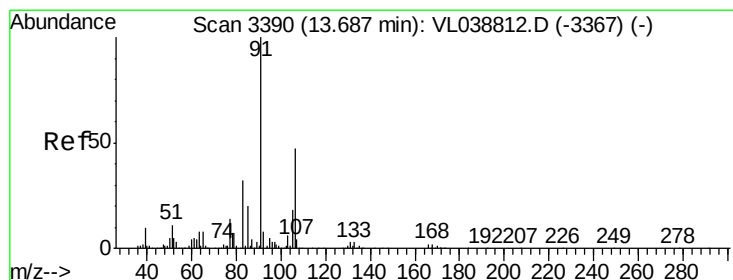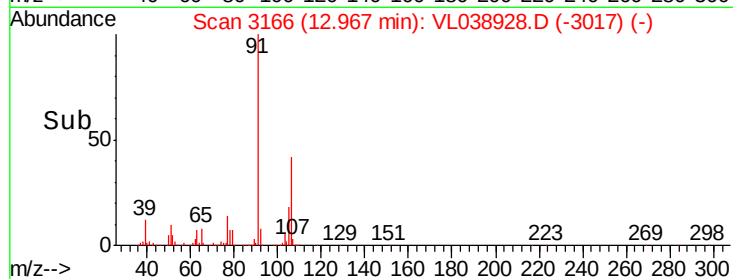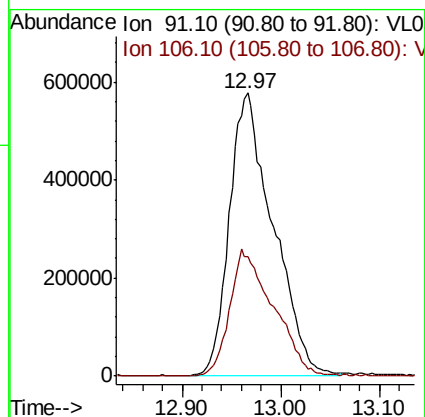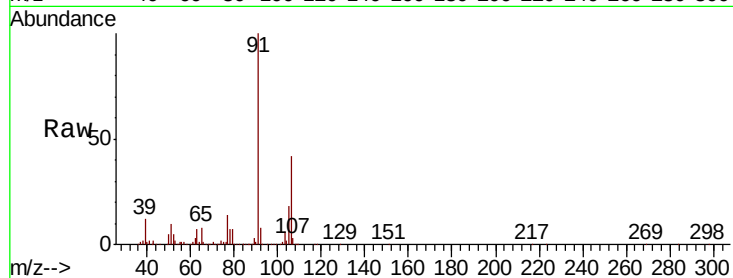

#60
o-Xylene
Concen: 2.220 ppbv
RT: 13.69 min Scan# 3391
Delta R.T.: 0.00 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04





Tgt Ion: 91 Resp: 693736
Ion Ratio Lower Upper
91 100
106 43.6 23.8 71.4

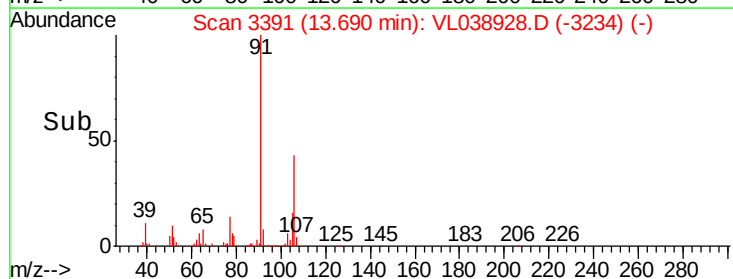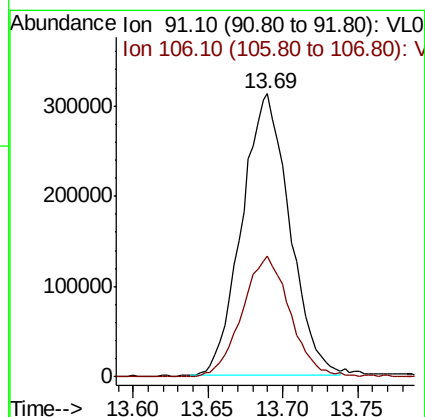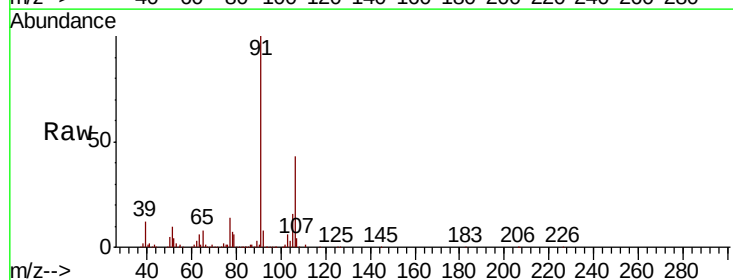

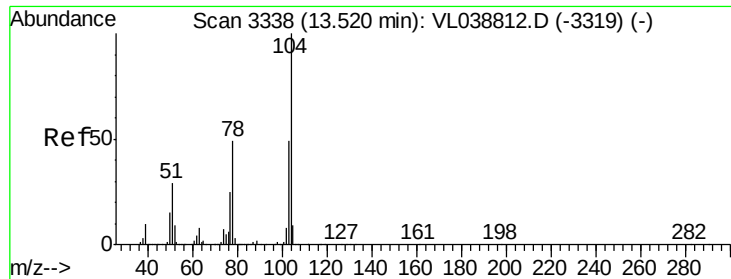




#61
Stvrene
Concen: 0.184 ppbv
RT: 13.53
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId : 1165-19-SG-2
Acq: 14 Apr 2022 22:04


Tot Ion	Ratio	Lower	Upper
104	100		
78	55.8	40.5	60.7
103	54.1	39.0	58.4

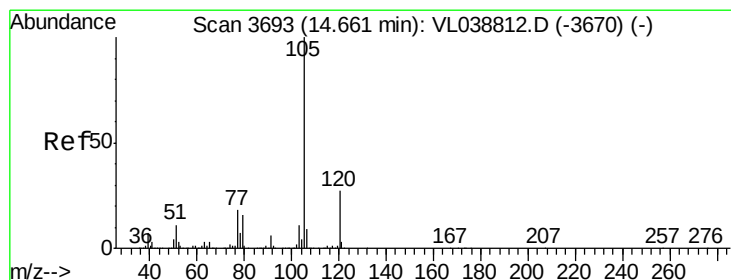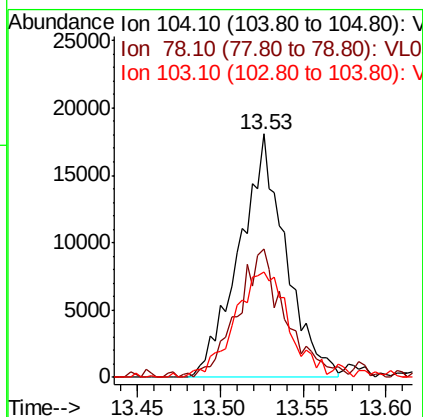

#62
Isopropylbenzene
Concen: 0.132 ppbv
RT: 14.66 min Scan# 3694
Delta R.T.: 0.00 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04

Tgt Ion	Ratio	Lower	Upper
105	100		
120	39.2	21.8	32.8#

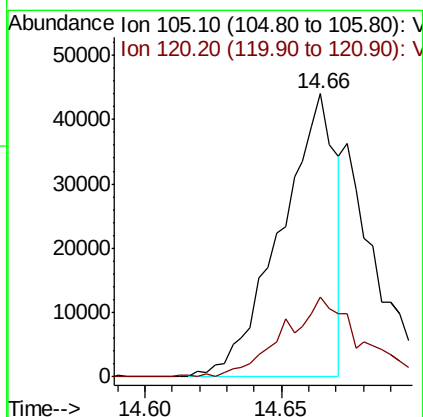



#64

n-propylbenzene

Concen: 0.316 ppbv

RT: 15.56

Delta R.T. MSVOA_L

Lab File: ClientSampleId:


Acq: 14 Apr 2022 22:04

Tot Ion:120 Resp: 38523

Ion Ratio Lower Upper




120 100

91 969.5 360.6 540.8#



Abundance Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

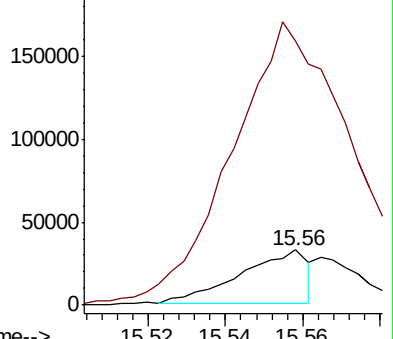

#65

tert-Butylbenzene

Concen: 0.297 ppbv

RT: 16.76 min Scan# 4346

Delta R.T. 0.03 min

Lab File: VL038928.D

Acq: 14 Apr 2022 22:04


Tgt Ion:119 Resp: 123607

Ion Ratio Lower Upper

119 100

91 116.8 62.8 94.2#



134 0.1 16.2 24.4#




Abundance Ion 119.20 (118.90 to 119.90): V

Ion 91.10 (90.80 to 91.80): VL0





Ion 134.20 (133.90 to 134.90): V

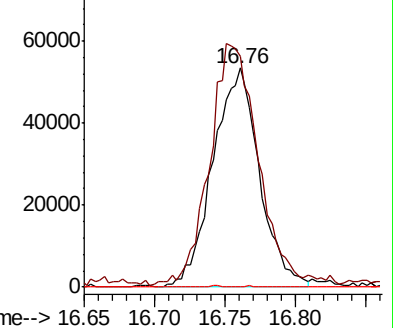






#66
Benzyl Chloride
Concen: 0.305 ppbv
RT: 17.21 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
Acq: 14 Apr 2022 22:04


Tot Ion: 91 Resp: 25854
Ion Ratio Lower Upper
91 100
126 1.6 15.4 23.0#
128 0.4 4.7 7.1#

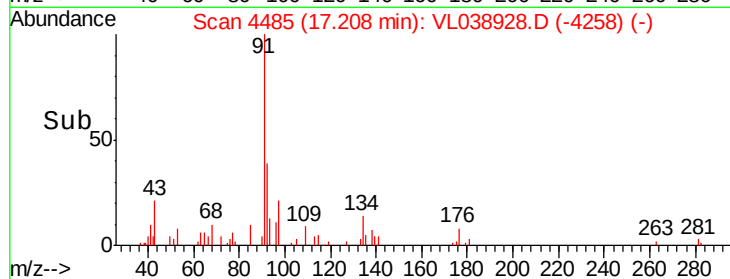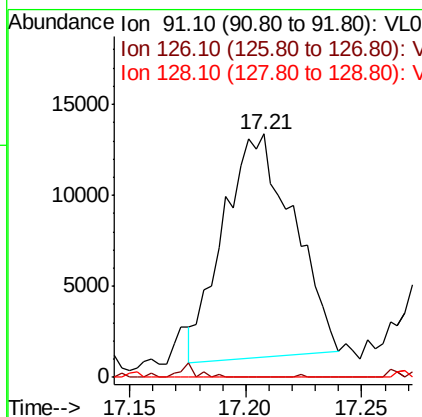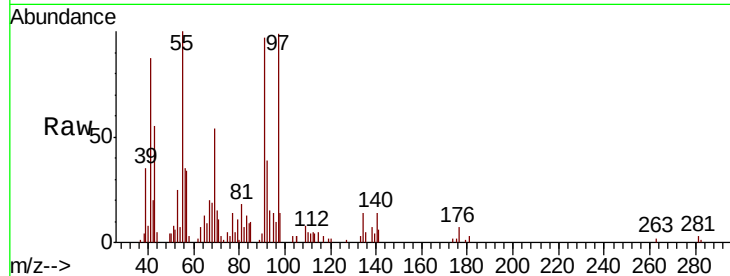

#67
sec-Butylbenzene
Concen: 0.143 ppbv
RT: 17.29 min Scan# 4510
Delta R.T.: 0.00 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04

Tgt Ion: 105 Resp: 83333
Ion Ratio Lower Upper
105 100
134 18.2 15.1 22.7

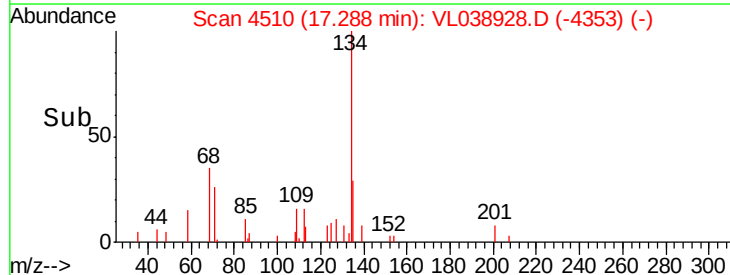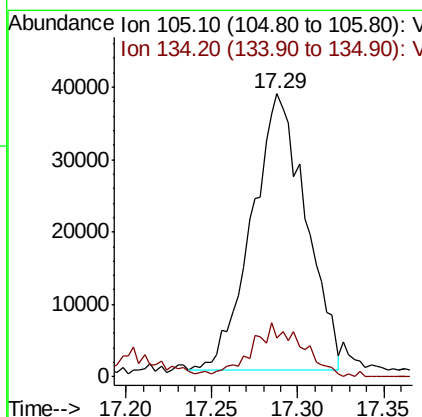



#68

1-Bromo-4-Fluorobenzene

Concen: 10.715 ppbv

RT: 14.41

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 14 Apr 2022 22:04


Tot Ion: 95 Resp: 2162217

Ion Ratio Lower Upper

95 100

174 62.3 52.0 78.0




175 4.6 4.0 6.0



Abundance Ion 95.10 (94.80 to 95.80): VL0

Ion 174.00 (173.70 to 174.70): V

Ion 175.00 (174.70 to 175.70): V

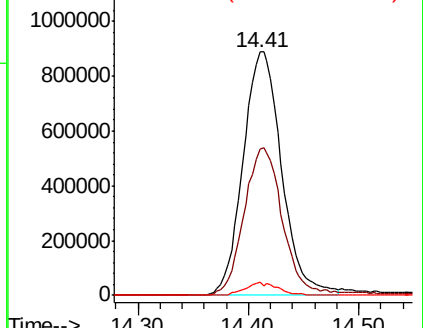

#69

p-Isopropyltoluene

Concen: 0.095 ppbv

RT: 17.64 min Scan# 4621

Delta R.T. 0.00 min

Lab File: VL038928.D

Acq: 14 Apr 2022 22:04


Tgt Ion: 119 Resp: 45685

Ion Ratio Lower Upper

119 100

134 30.5 20.8 31.2



91 38.2 22.6 34.0#




Abundance Ion 119.10 (118.80 to 119.80): V

Ion 134.20 (133.90 to 134.90): V





Ion 91.10 (90.80 to 91.80): VL0

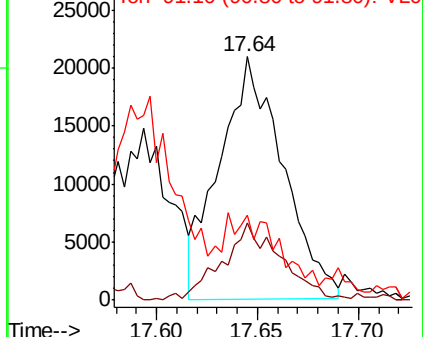






#70
n-Butylbenzene
Concen: 0.384 ppbv
RT: 18.55 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampled:
1165-19-SG-2
Acq: 14 Apr 2022 22:04


Tot Ion: 91 Resp: 185670
Ion Ratio Lower Upper
91 100
92 40.4 44.6 66.8#
134 70.3 19.2 28.8#

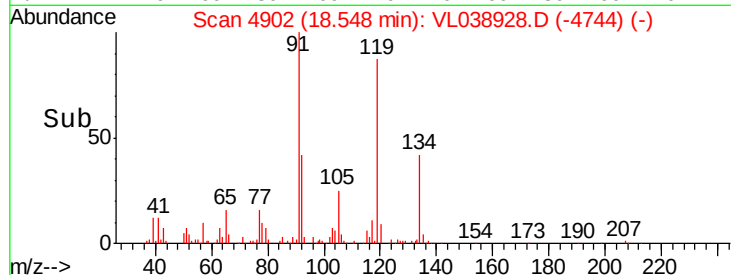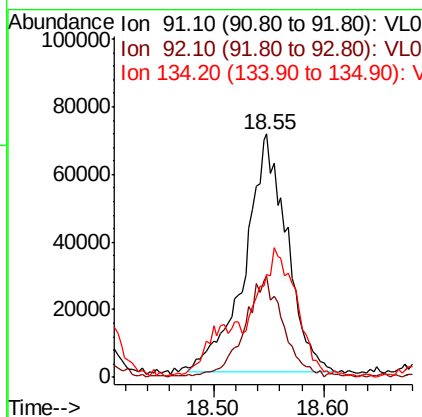

#71
2-Chlorotoluene
Concen: 0.066 ppbv
RT: 15.83 min Scan# 4057
Delta R.T.: 0.39 min
Lab File: VL038928.D
Acq: 14 Apr 2022 22:04

Tgt Ion: 91 Resp: 23369
Ion Ratio Lower Upper
91 100
126 15.9 13.0 51.8

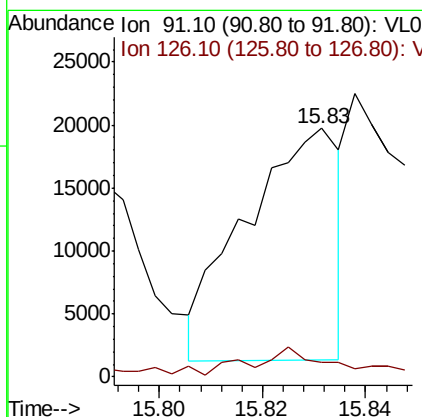



#72

4-Ethyltoluene

Concen: 1.032 ppbv


RT: 15.83

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 14 Apr 2022 22:04

Tot Ion:	105	Resp:	385246
Ion	Ratio	Lower	Upper
105	100		
120	29.9	24.3	36.5
91	13.2	9.4	14.2
77	13.9	10.6	15.8






Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

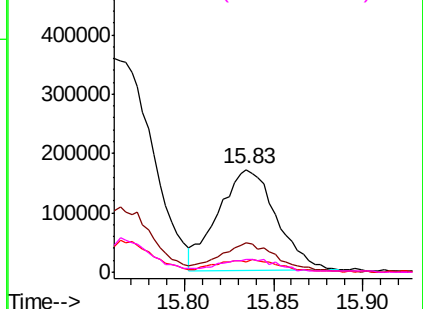

#73

1,3,5-Trimethylbenzene

Concen: 1.014 ppbv


RT: 16.00 min Scan# 4108

Delta R.T. 0.01 min

Lab File: VL038928.D



Acq: 14 Apr 2022 22:04


Tgt Ion:	105	Resp:	339917
Ion	Ratio	Lower	Upper
105	100		
120	43.2	38.7	58.1



Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

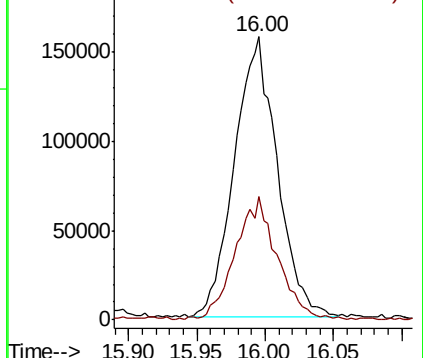

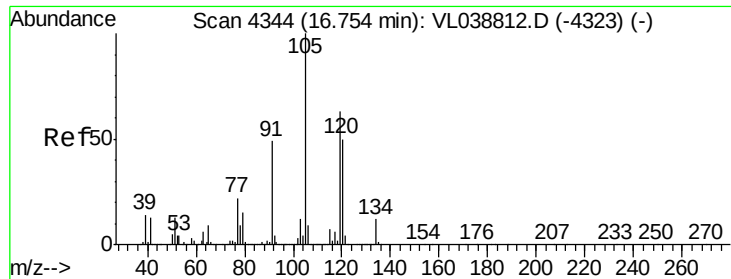

#74

1,2,4-Trimethylbenzene

Concen: 3.379 ppbv

RT: 16.76


Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 14 Apr 2022 22:04

Tot Ion:105 Resp: 1197452

Ion	Ratio	Lower	Upper
105	100		
120	39.6	39.8	59.8#
91	11.4	39.4	59.0#
77	14.5	17.3	25.9#




Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V


Ion 91.10 (90.80 to 91.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

Time-->



Time-->

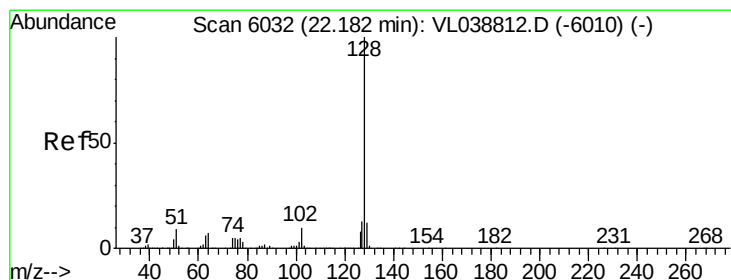

#79

Naphthalene

Concen: 0.068 ppbv

RT: 22.17 min Scan# 6029


Delta R.T. -0.01 min

Lab File: VL038928.D

Acq: 14 Apr 2022 22:04

Tgt Ion:128 Resp: 17912

Ion	Ratio	Lower	Upper
128	100		
127	12.3	10.6	15.8
129	11.0	9.4	14.0




Abundance Ion 128.10 (127.80 to 128.80): V


Ion 127.10 (126.80 to 127.80): V

Ion 129.10 (128.80 to 129.80): V

Time-->




Time-->

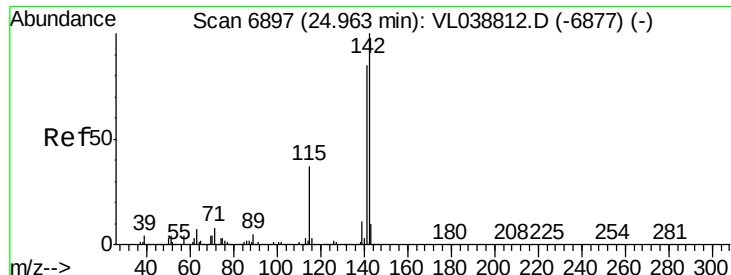

#80
 Naphthalene, 2-methyl-
 Concen: 0.366 ppbv
 RT: 24.97
 Delta R.T: MSVOA_L
 Lab File: ClientSampleId :
 1165-19-SG-2
 Acq: 14 Apr 2022 22:04

Tot Ion	Ratio	Lower	Upper
142	100		
141	78.4	68.8	103.2
115	110.2	31.6	47.4



Abundance

Ion 142.00 (141.70 to 142.70): V

Ion 141.00 (140.70 to 141.70): V

Ion 115.00 (114.70 to 115.70): V

