


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL041422\
 Data File : VL038915.D
 Acq On : 14 Apr 2022 12:34
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL040522AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Apr 06 06:12:53 2022
 Last Update : Wed Apr 06 06:12:53 2022

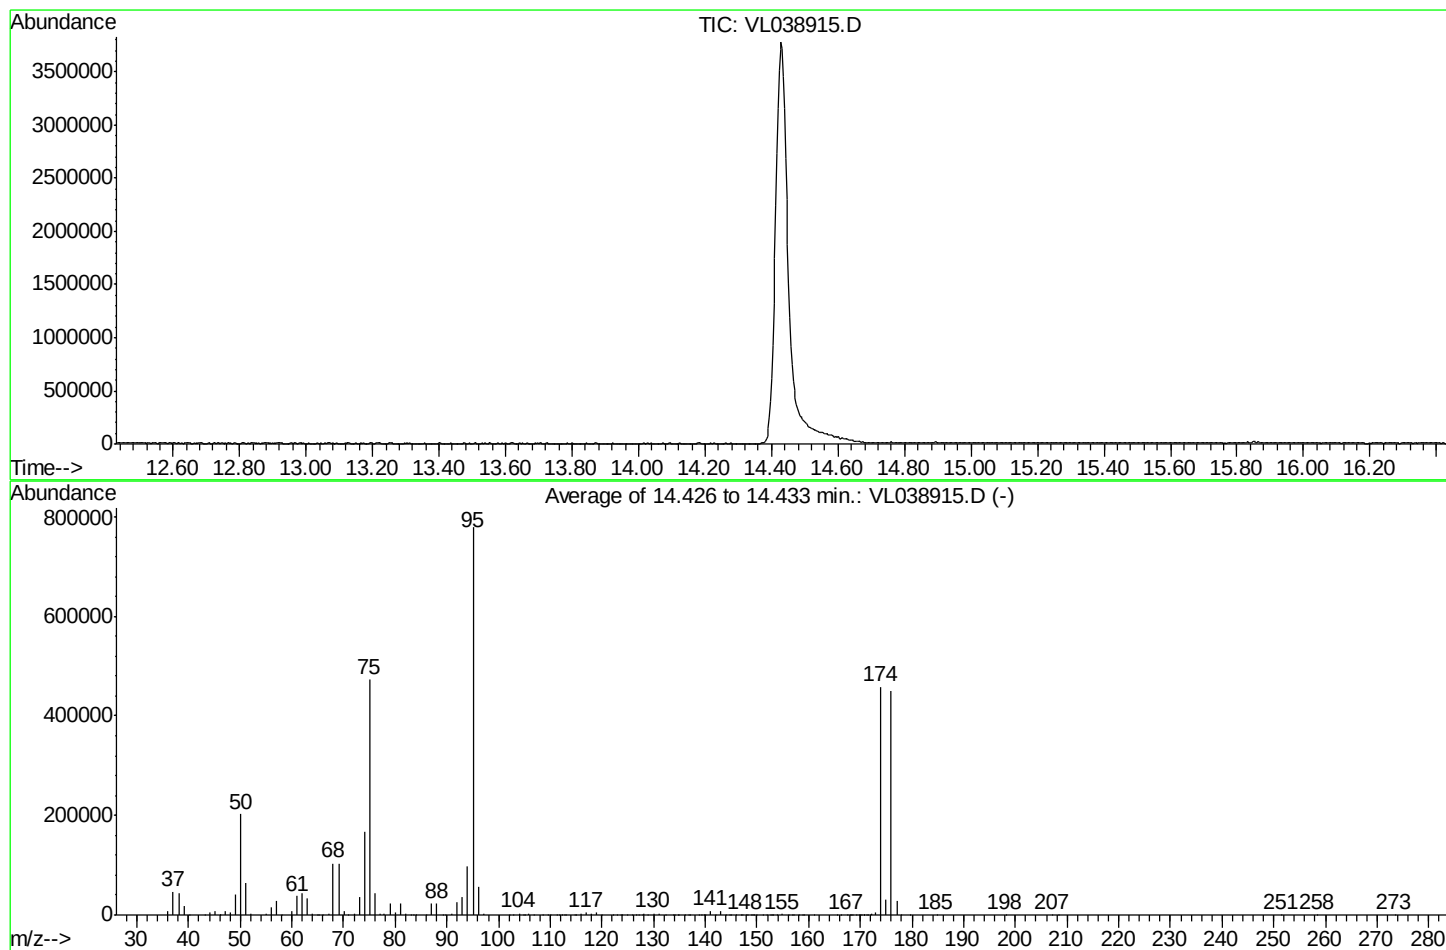

AutoFind: Scans 3620, 3621, 3622; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.0	202666	PASS
75	95	30	66	60.7	472720	PASS
95	95	100	100	100.0	778880	PASS
96	95	5	9	7.2	56053	PASS
173	174	0.00	2	1.1	5072	PASS
174	95	50	120	58.8	457962	PASS
175	174	4	9	7.0	32237	PASS
176	174	93	101	98.3	449984	PASS
177	176	5	9	6.5	29432	PASS