

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL041619\
 Data File : VL033588.D
 Acq On : 16 Apr 2019 11:31
 Operator : SY/AP
 Sample : VL0416ABL01
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0416ABL01

Quant Time: Apr 17 06:38:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032519AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019
 QLast Update : Tue Mar 26 16:00:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.76	49	829817	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.29	114	1997792	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.24	117	2076476	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.57	95	1677084	10.30	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	103.00%


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) Acetone	3.91	43	35267	0.353	ppbv #	84
20) Methylene Chloride	4.41	84	12256	0.289	ppbv #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL041619\
Data File : VL033588.D
Acq On : 16 Apr 2019 11:31
Operator : SY/AP
Sample : VL0416ABL01
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0416ABL01

Quant Time: Apr 17 06:38:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL032519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Mar 26 16:00:50 2019
QLast Update : Tue Mar 26 16:00:50 2019
Response via : Initial Calibration

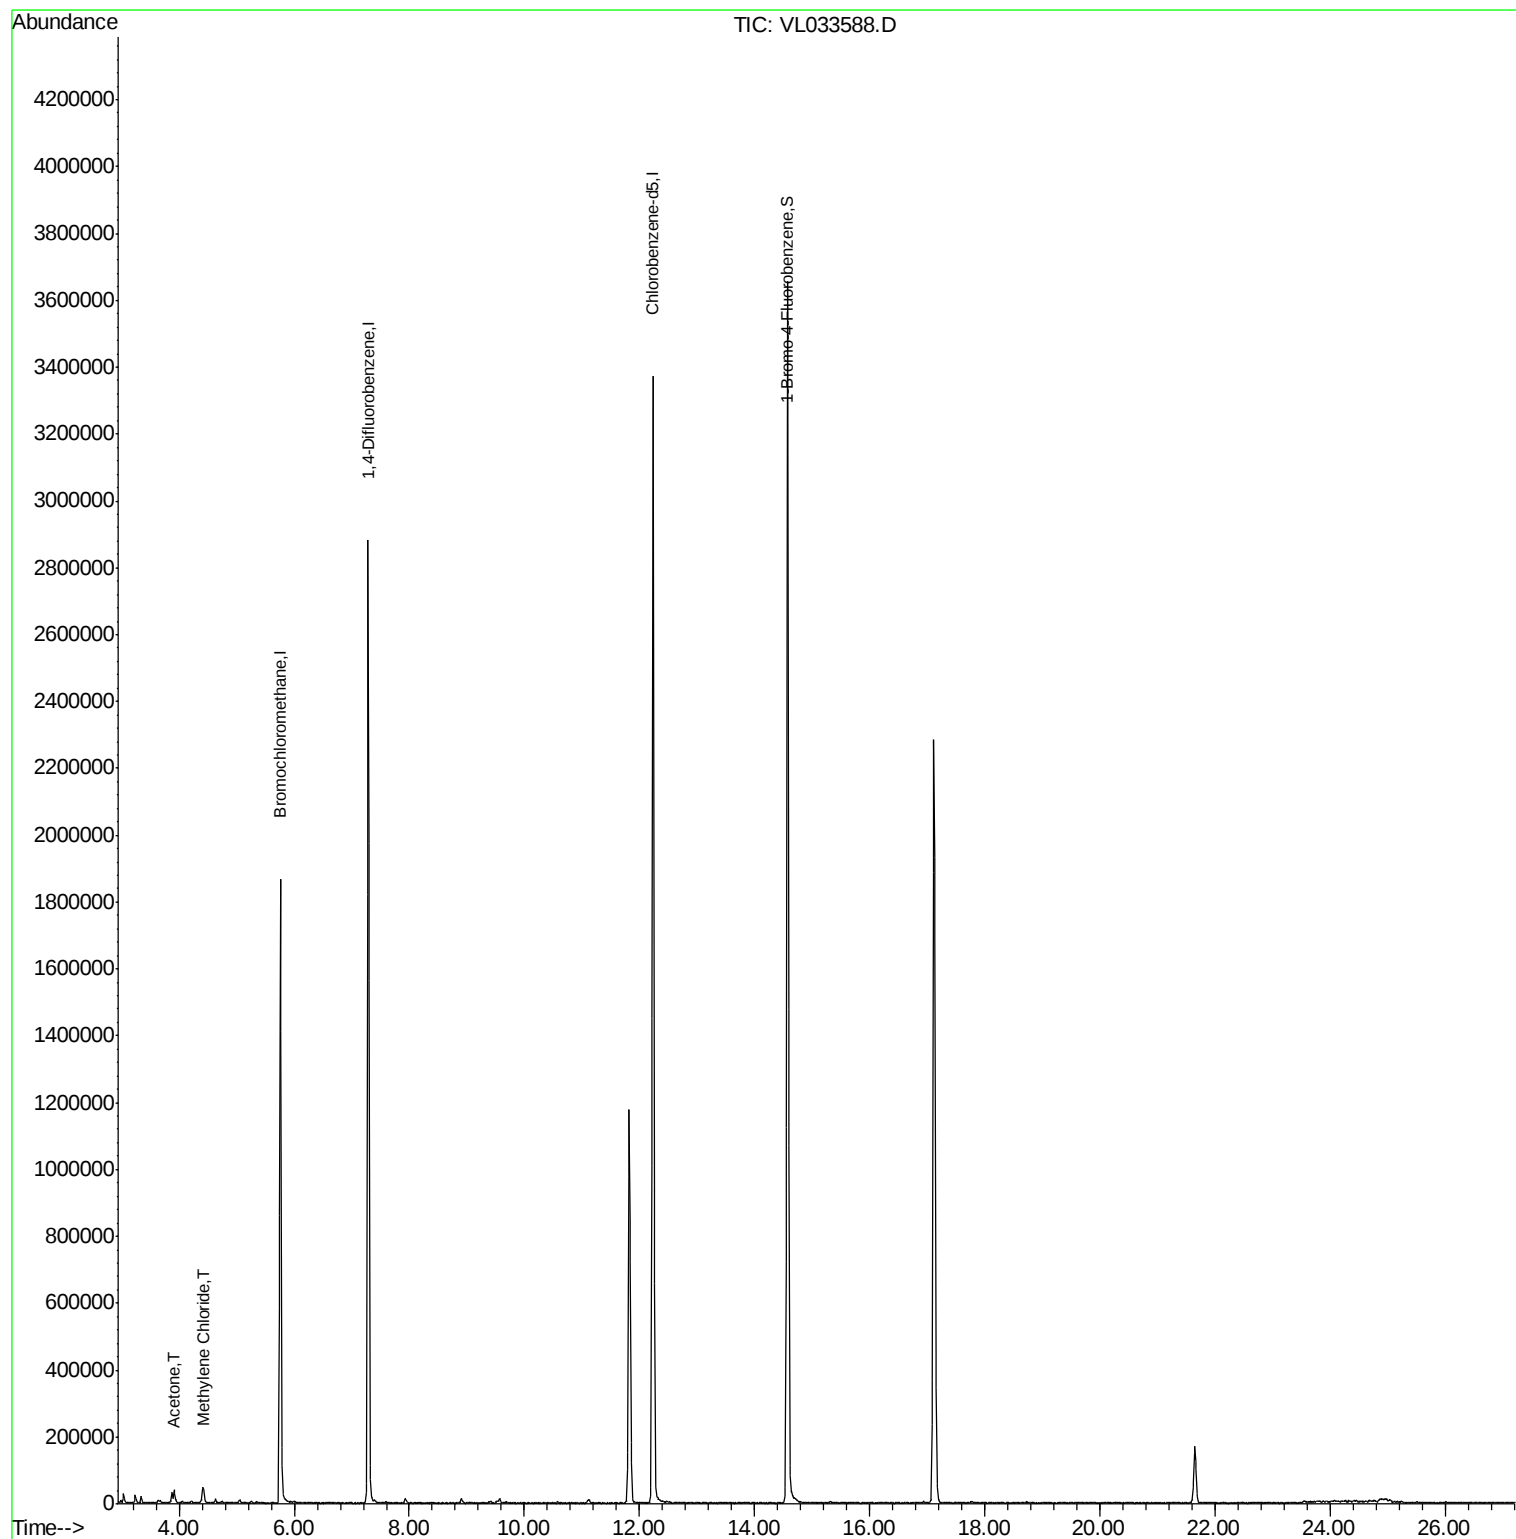

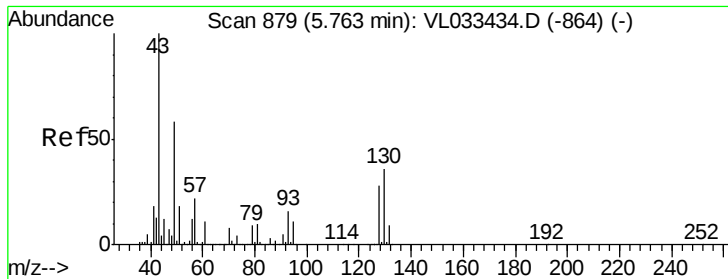

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.76 min Scan# 877

Delta R.T. -0.01 min

Lab File: VL033588.D

Acq: 16 Apr 2019 11:31

Instrument :

MSVOA_L

ClientSampleId :

VL0416ABL01


Tot Ion: 49 Resp: 829817

Ion Ratio Lower Upper

49 100

128 50.1 24.0 72.0




130 64.1 31.2 93.6

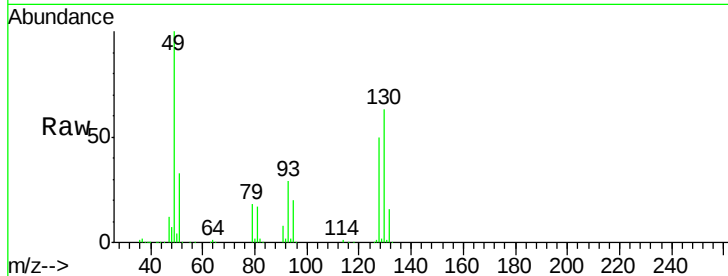

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

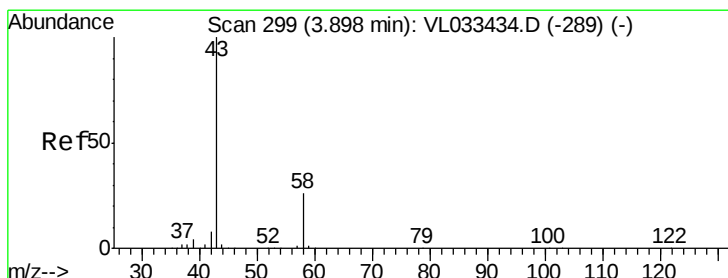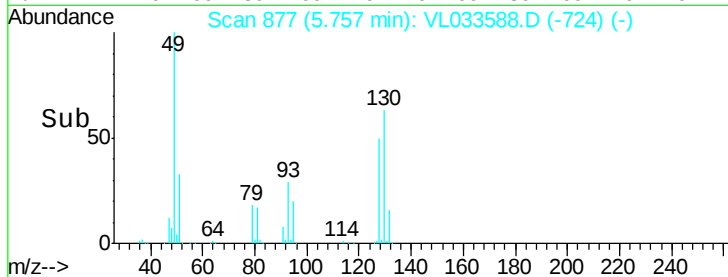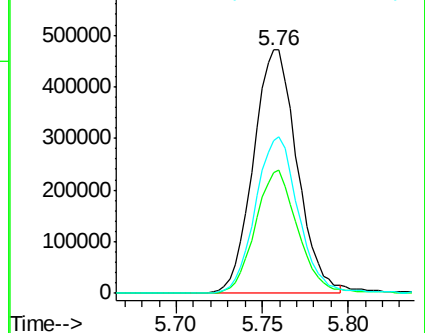

#15

Acetone

Concen: 0.353 ppbv

RT: 3.91 min Scan# 303

Delta R.T. 0.01 min

Lab File: VL033588.D


Acq: 16 Apr 2019 11:31

Tgt Ion: 43 Resp: 35267

Ion Ratio Lower Upper



43 100


58 33.5 20.5 30.7#

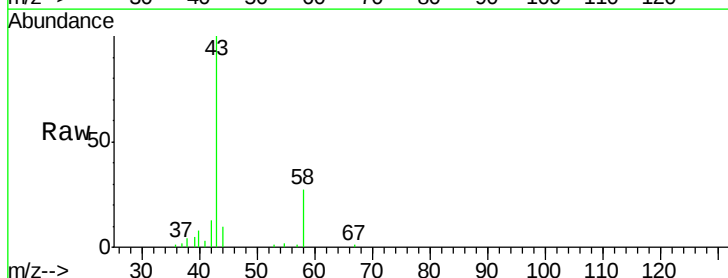

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0



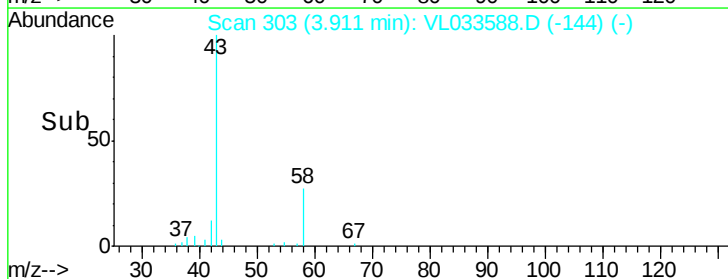
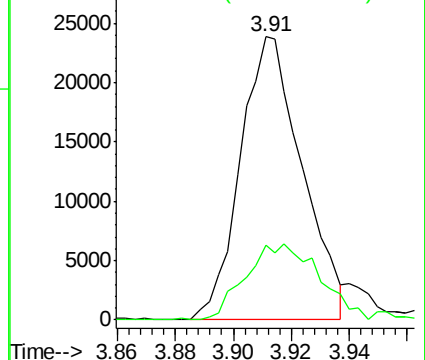


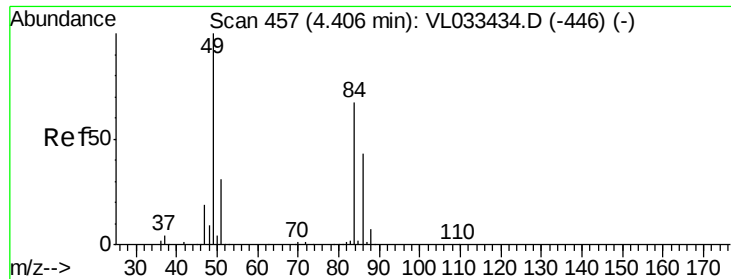

#20
Methylene Chloride
Concen: 0.289 ppbv
RT: 4.41 min Scan# 458
Delta R.T. 0.00 min
Lab File: VL033588.D
Acq: 16 Apr 2019 11:31




Instrument :
MSVOA_L
ClientSampleId :
VL0416ABL01


Tot Ion: 84 Resp: 12256
Ion Ratio Lower Upper
84 100
49 133.7 120.0 180.0
51 57.6 36.7 55.1#
86 59.4 51.9 77.9

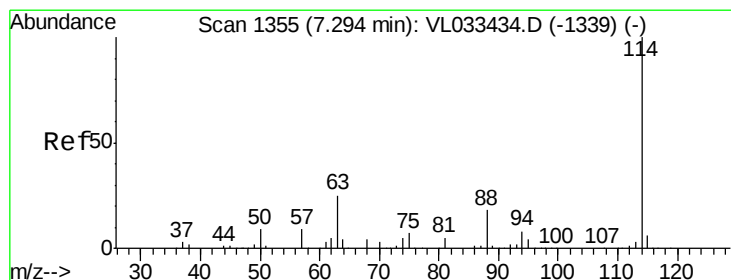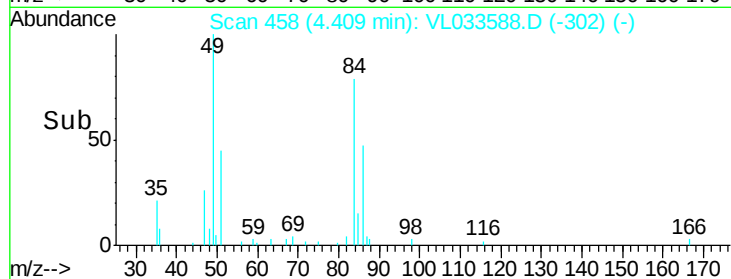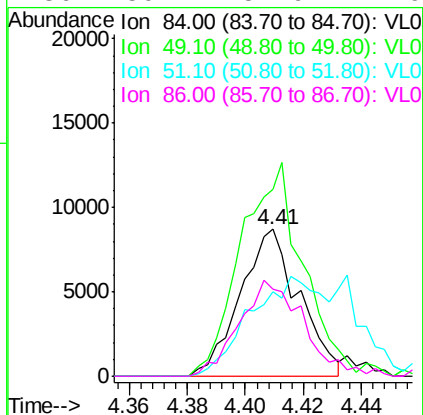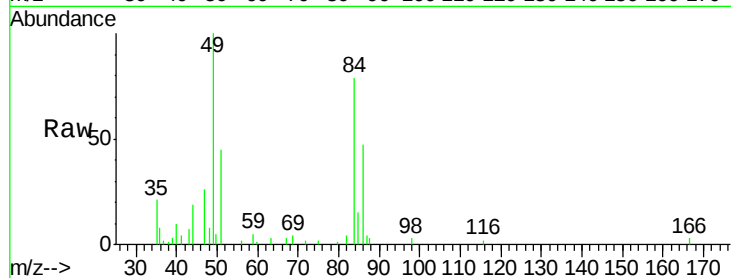

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.29 min Scan# 1353
Delta R.T. -0.01 min
Lab File: VL033588.D
Acq: 16 Apr 2019 11:31

Tgt Ion: 114 Resp: 1997792
Ion Ratio Lower Upper
114 100
63 26.6 21.5 32.3
88 18.2 14.5 21.7


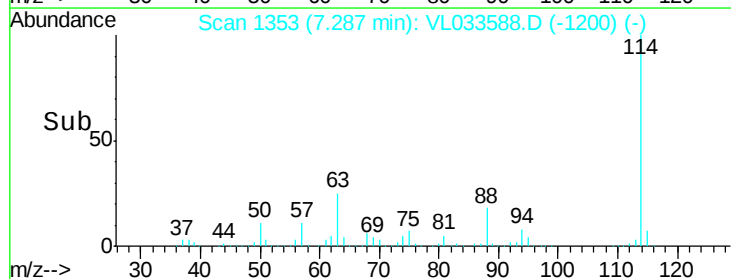
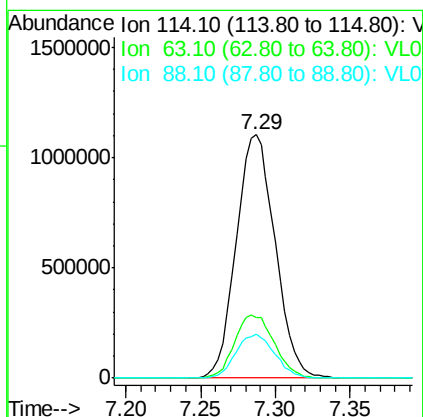
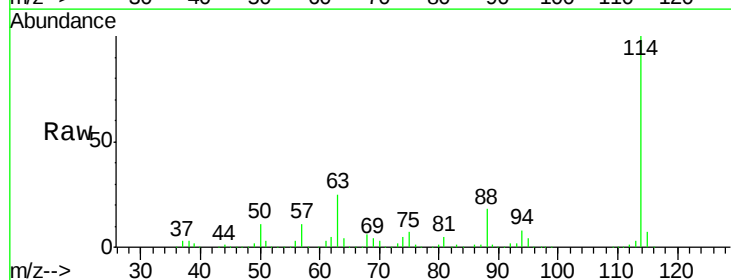


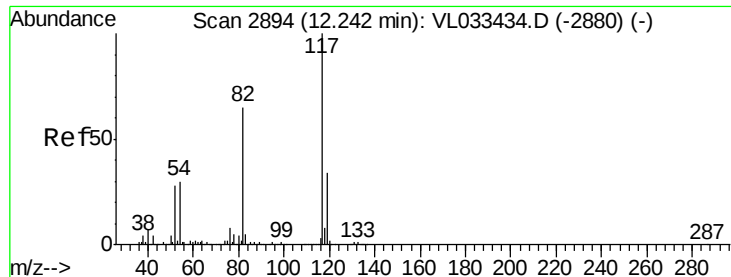

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.24 min Scan# 2892
Delta R.T. -0.01 min
Lab File: VL033588.D
Acq: 16 Apr 2019 11:31

Instrument :
MSVOA_L
ClientSampleId :
VL0416ABL01

Tot Ion:117 Resp: 2076476
Ion Ratio Lower Upper
117 100
82 67.2 51.5 77.3
119 32.6 25.5 38.3

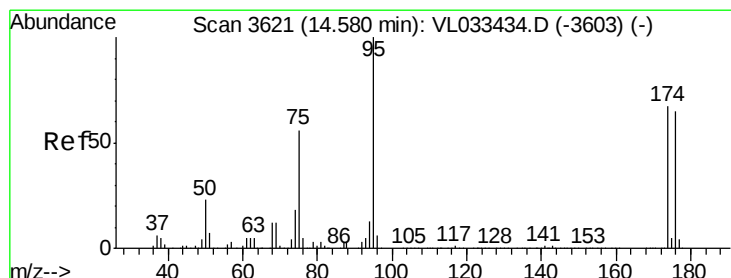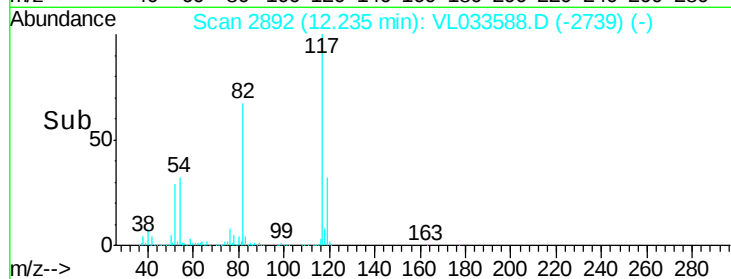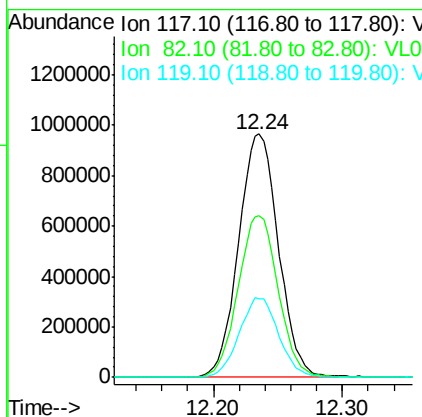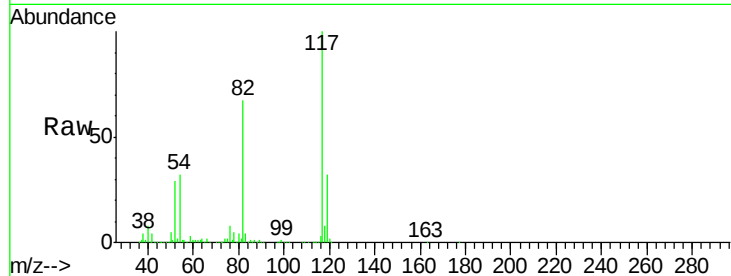

#68
1-Bromo-4-Fluorobenzene
Concen: 10.302 ppbv
RT: 14.57 min Scan# 3619
Delta R.T. -0.01 min
Lab File: VL033588.D
Acq: 16 Apr 2019 11:31

Tgt Ion: 95 Resp: 1677084
Ion Ratio Lower Upper
95 100
174 66.9 52.9 79.3
175 4.8 3.8 5.6

