

Data Path : W:\HPCHEM1\MSVOA L\DATA\VL041918\
Data File : VL031892.D
Acq On : 20 Apr 2018 00:14
Operator : SY/AP
Sample : QC040618 CAN 10595
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC040618 CAN 10595

Quant Time: Apr 20 08:23:54 2018
Quant Method : W:\HPCHEM1\MSVOA L\METHODS\VL041218AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Apr 13 16:50:02 2018
QLast Update : Fri Apr 13 16:50:02 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.88	49	1051884	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.42	114	2446687	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.39	117	2510775	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.72	95	2013465	9.97	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.70%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA L\DATA\VL041918\
Data File : VL031892.D
Acq On : 20 Apr 2018 00:14
Operator : SY/AP
Sample : OC040618 CAN 10595
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC040618 CAN 10595

Quant Time: Apr 20 08:23:54 2018
Quant Method : W:\HPCHEM1\MSVOA L\METHODS\VL041218AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Apr 13 16:50:02 2018
QLast Update : Fri Apr 13 16:50:02 2018
Response via : Initial Calibration

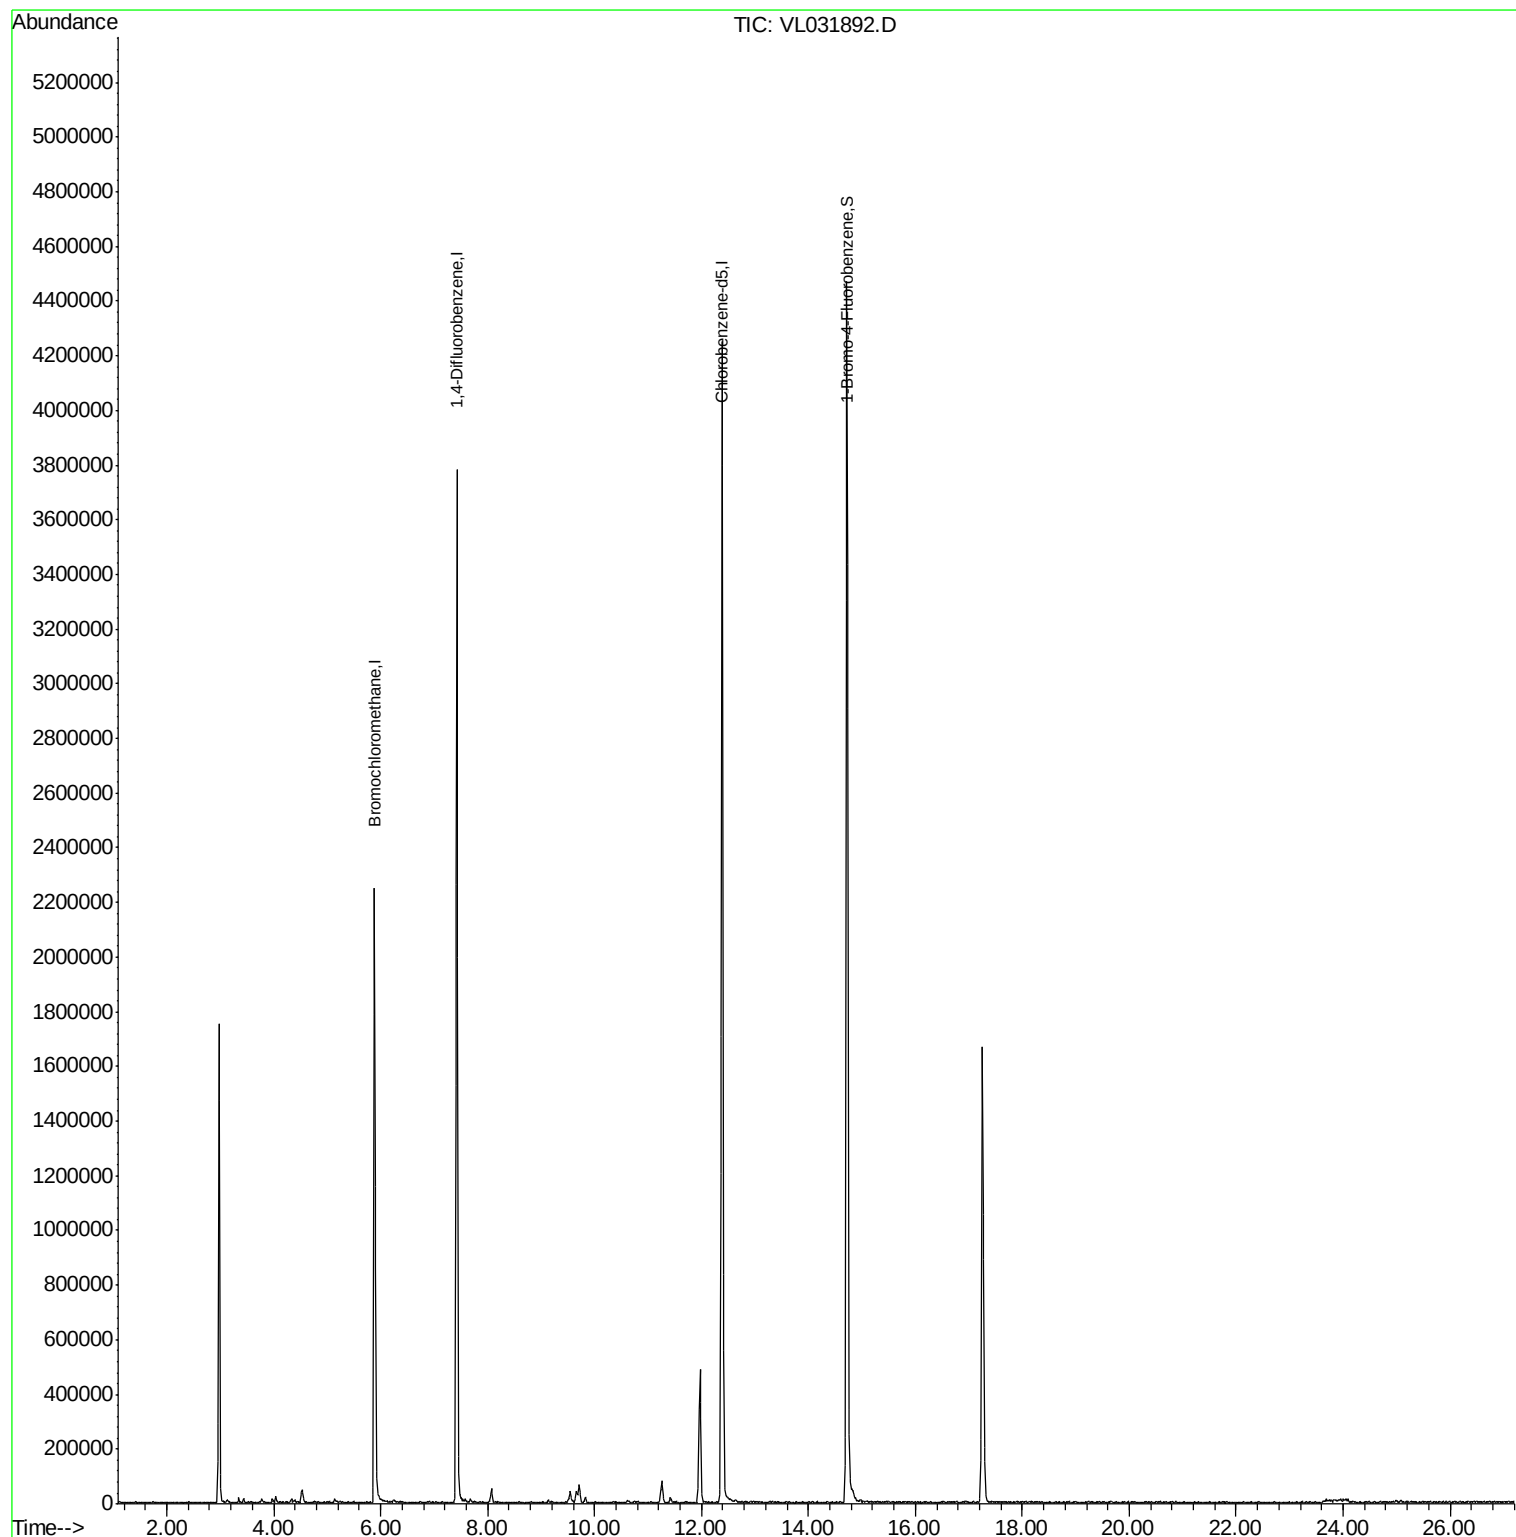

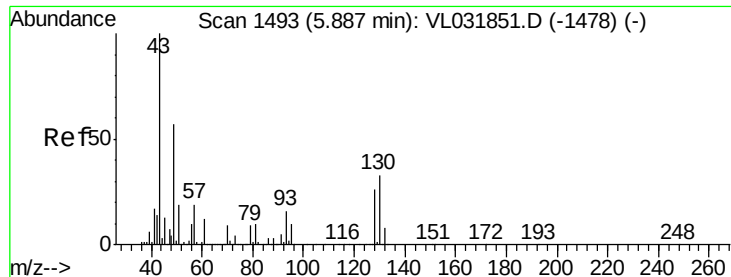

#1

Bromochloromethane

Concen: 10.00 ppbv

RT: 5.88 min Scan# 1492

Delta R.T. -0.01 min

Lab File: VL031892.D

Acq: 20 Apr 2018 00:14

Instrument :

MSVOA_L

ClientSampleId :

QC040618 CAN 10595


Tot Ion: 49 Resp: 1051884

Ion Ratio Lower Upper

49 100

128 49.3 23.9 71.7




130 63.1 30.9 92.7

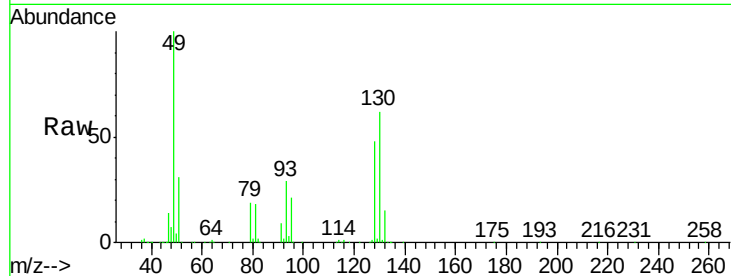

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

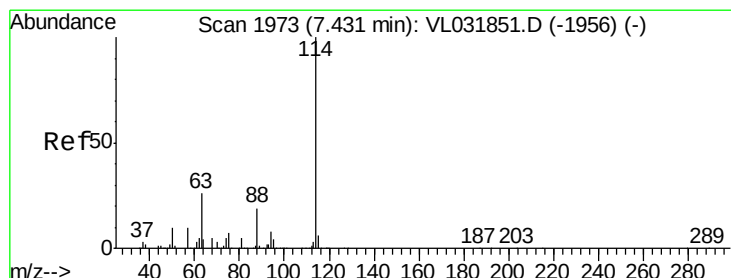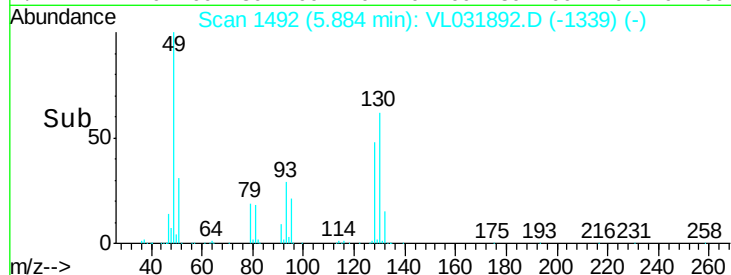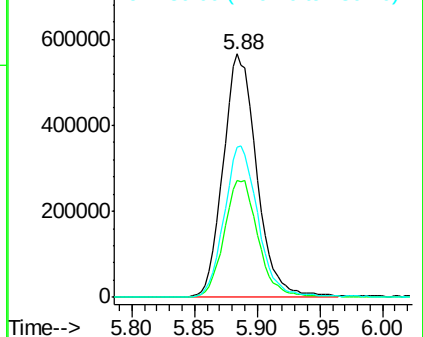

#33

1,4-Difluorobenzene

Concen: 10.00 ppbv

RT: 7.42 min Scan# 1971

Delta R.T. -0.01 min

Lab File: VL031892.D

Acq: 20 Apr 2018 00:14


Tgt Ion: 114 Resp: 2446687

Ion Ratio Lower Upper

114 100

63 27.5 21.8 32.6



88 18.8 14.6 22.0

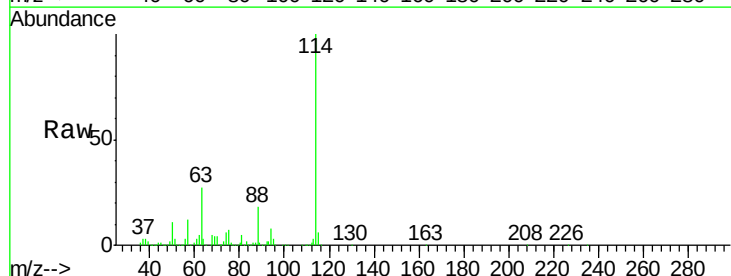


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



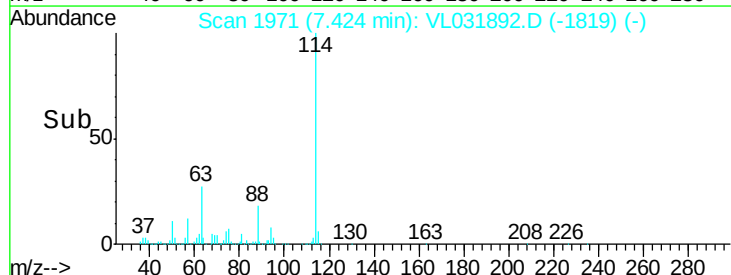
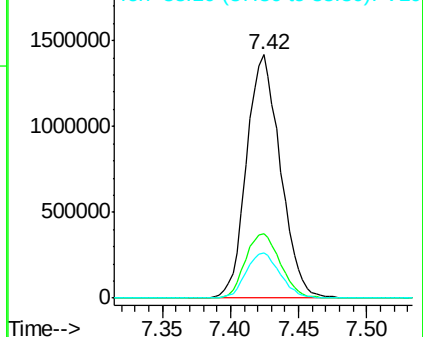


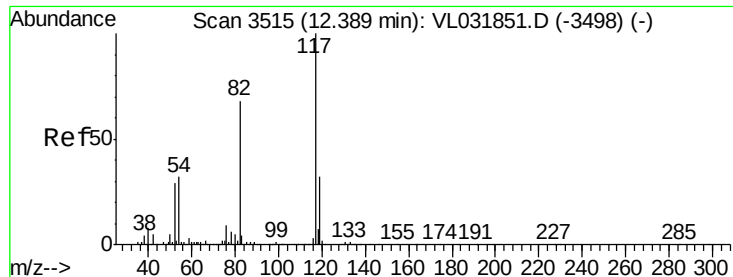

#55
Chlorobenzene-d5
Concen: 10.00 ppbv
RT: 12.39 min Scan# 3514
Delta R.T. -0.01 min
Lab File: VL031892.D
Acq: 20 Apr 2018 00:14

Instrument :
MSVOA_L
ClientSampleId :
QC040618 CAN 10595

Tot Ion:117 Resp: 2510775
Ion Ratio Lower Upper
117 100
82 69.1 54.6 81.8
119 32.0 26.0 39.0

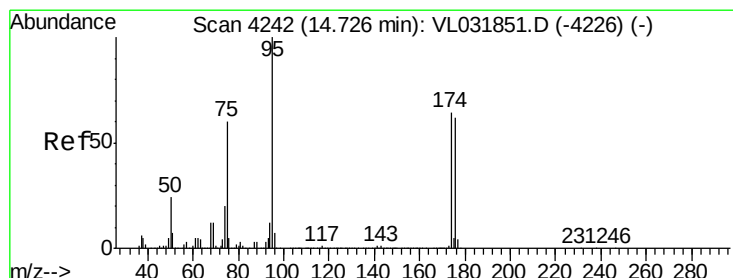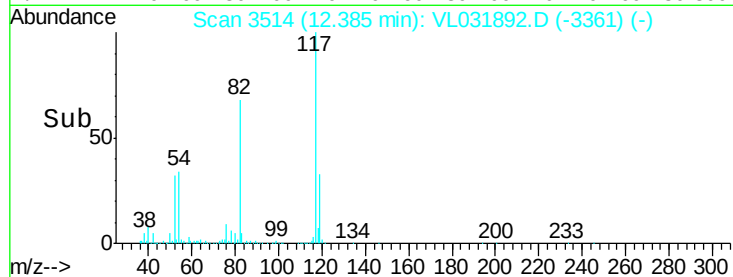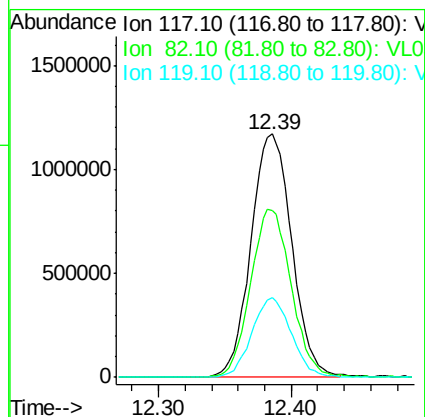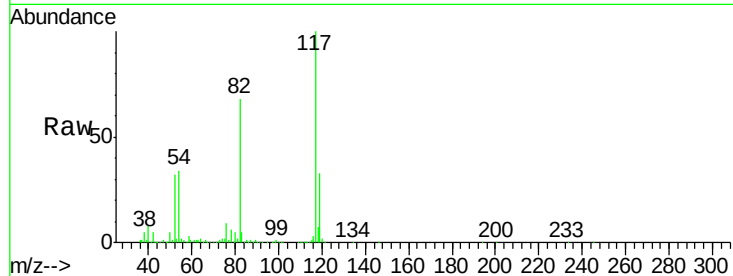

#68
1-Bromo-4-Fluorobenzene
Concen: 9.97 ppbv
RT: 14.72 min Scan# 4240
Delta R.T. -0.01 min
Lab File: VL031892.D
Acq: 20 Apr 2018 00:14

Tgt Ion: 95 Resp: 2013465
Ion Ratio Lower Upper
95 100
174 65.3 52.3 78.5
175 4.6 3.9 5.9

