


Data Path : W:\HPCHEM1\MSVOA L\Data\VL041918\
 Data File : VL031879.D
 Acq On : 19 Apr 2018 15:04
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL041218AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Apr 13 16:50:02 2018
 Last Update : Fri Apr 13 16:50:02 2018

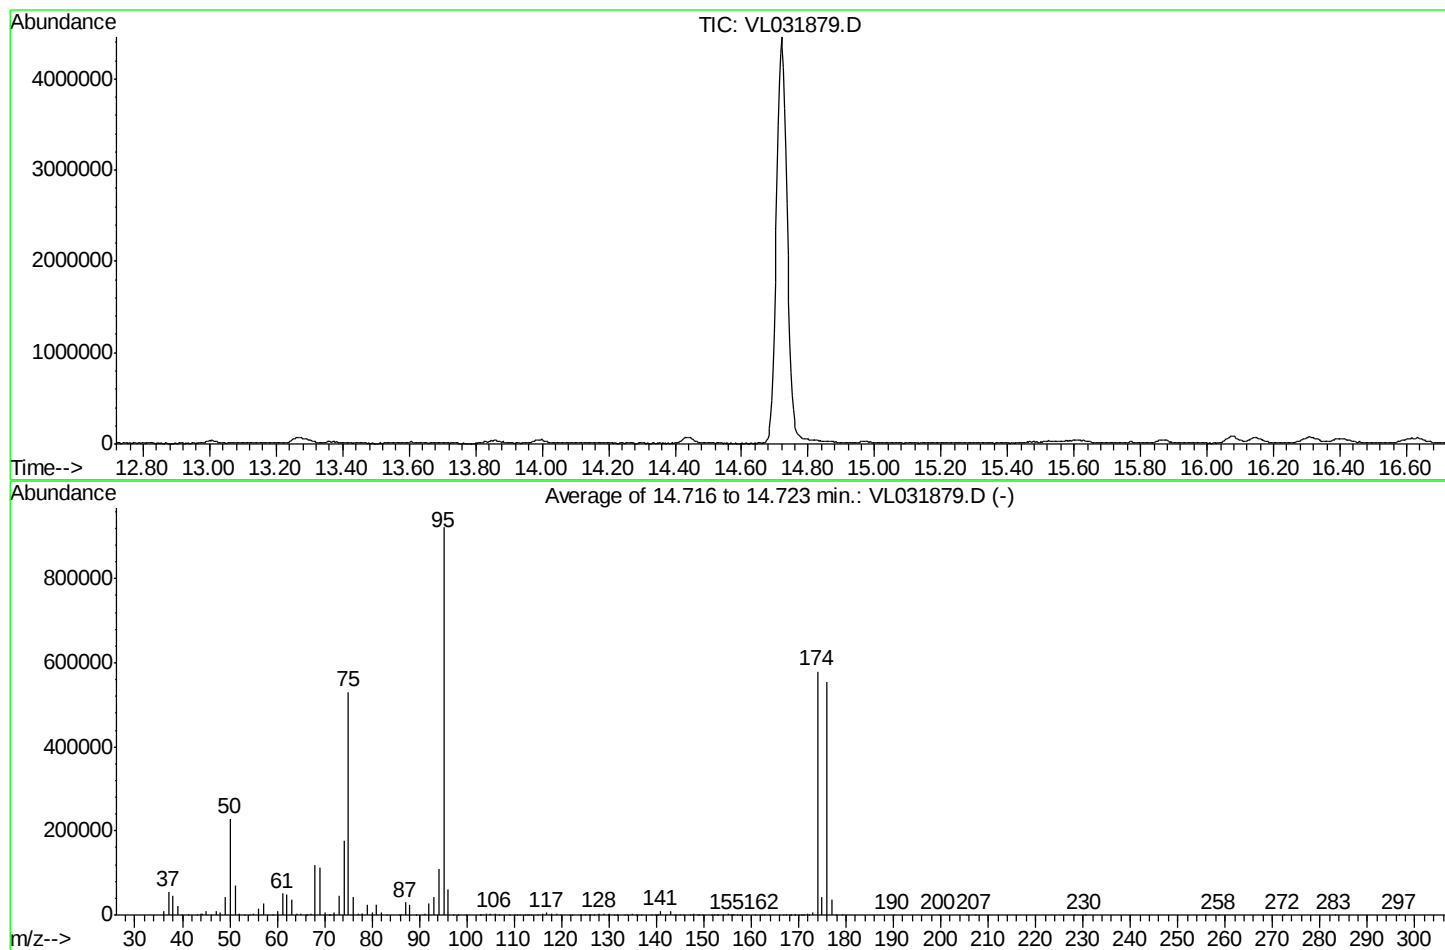

AutoFind: Scans 4239, 4240, 4241; Background Corrected with Scan 4218

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	229098	PASS
75	95	30	66	57.6	531221	PASS
95	95	100	100	100.0	922197	PASS
96	95	5	9	6.5	59850	PASS
173	174	0.00	2	0.9	5416	PASS
174	95	50	120	62.8	579584	PASS
175	174	4	9	7.3	42405	PASS
176	174	93	101	95.8	554986	PASS
177	176	5	9	6.7	37274	PASS