
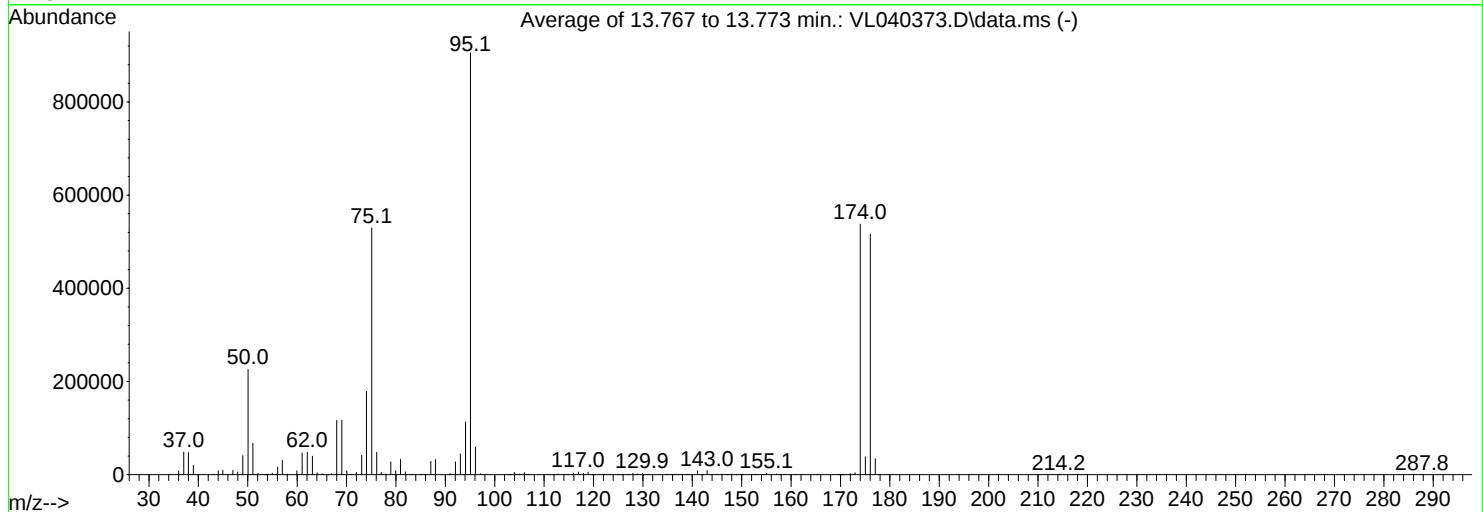


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041923\
Data File : VL040373.D
Acq On : 19 Apr 2023 9:56
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041323AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Apr 13 14:37:02 2023

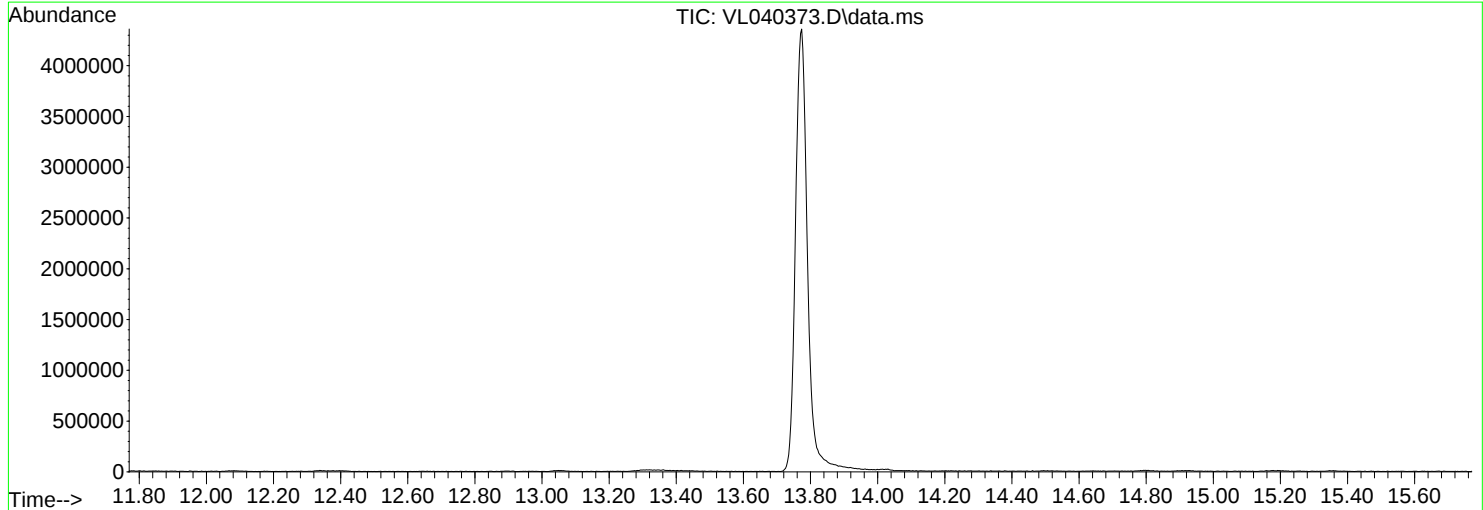

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	226112	PASS
75	95	30	66	58.5	529579	PASS
95	95	100	100	100.0	905408	PASS
96	95	5	9	6.6	59317	PASS
173	174	0.00	2	0.8	4132	PASS
174	95	50	120	59.4	537963	PASS
175	174	4	9	7.1	38360	PASS
176	174	93	101	96.0	516181	PASS
177	176	5	9	6.6	34267	PASS

Average of 13.767 to 13.773 min.: VL040373.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8053	47.95	5794	57.00	30605	68.00	11612
37.05	48461	49.00	40939	58.05	1104	69.05	11667
38.00	47469	50.05	226112	59.95	8445	70.05	842
39.00	19783	51.05	66877	61.00	46563	71.10	47
40.05	613	51.90	971	62.05	47936	72.00	4925
41.15	261	52.10	2377	63.10	39624	73.05	41272
43.00	721	53.05	291	64.05	4116	74.05	178773
44.05	8537	53.40	81	65.05	2129	75.10	529579
44.95	9510	53.80	61	65.90	194	76.10	47832
46.05	769	54.95	3377	66.20	62	77.00	4785
47.00	9264	56.05	16500	66.95	1985	77.90	1560

Average of 13.767 to 13.773 min.: VL040373.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.10	606	87.05	28597	103.20	122	112.95	1013
78.95	27621	88.00	32333	103.95	4754	114.10	159
79.95	8787	90.80	1523	104.90	508	114.85	1054
80.95	33435	91.10	1752	105.05	1208	115.95	3540
81.90	5734	92.05	27672	106.00	4505	116.95	5691
82.85	414	93.05	44419	106.85	645	118.00	2935
83.10	148	94.10	113072	107.10	770	118.90	5228
84.00	214	95.10	905408	109.90	661	119.70	85
85.00	84	96.10	59317	110.70	240	120.15	182
85.75	430	97.10	2038	111.05	507	122.00	85
86.00	218	102.80	127	112.00	875	122.70	217

Average of 13.767 to 13.773 min.: VL040373.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.20	52	131.85	260	141.05	8002	148.00	1302
123.85	443	133.95	212	141.95	506	148.95	717
124.80	111	134.80	752	142.20	278	149.80	586
125.65	286	134.95	1084	143.00	8716	150.15	660
125.90	59	135.75	266	143.90	541	151.95	381
127.00	112	136.10	64	144.10	245	152.80	349
128.00	2729	136.80	1114	145.05	989	153.00	243
128.95	1900	137.10	539	145.90	1083	154.00	525
129.90	3130	138.75	178	146.90	691	155.05	2844
130.80	445	139.20	194	147.10	140	155.75	210
131.05	1165	139.90	540	147.80	717	156.00	208

Average of 13.767 to 13.773 min.: VL040373.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.05	1841	171.80	618	287.80	53		
157.85	170	172.05	2238				
158.70	631	172.95	4132				
160.85	1031	174.00	537963				
165.20	70	175.05	38360				
167.80	156	176.05	516181				
169.50	114	177.05	34267				
169.85	354	177.80	230				
170.20	88	178.10	985				
170.50	105	214.20	110				
171.20	444	223.90	60				