

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL042021\
 Data File : VL036830.D
 Acq On : 20 Apr 2021 20:35
 Operator : SY/AP
 Sample : M2096-03
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Apr 21 06:38:49 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Mar 25 09:42:40 2021
 QLast Update : Thu Mar 25 09:42:40 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	1345943	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.18	114	3146139	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.10	117	2739990	10.00	ppbv	0.00


System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.43	95	2052752	9.40	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	94.00%


Target Compounds					Ovalue
2) Dichlorodifluoromethane	3.05	85	59896	0.273 ppbv	# 85
3) Chlorodifluoromethane	2.99	51	109338	0.435 ppbv	94
4) Chloromethane	3.14	50	70643	0.795 ppbv	95
9) Propene	3.02	41	189556	2.364 ppbv	85
10) Heptane	8.13	43	32410	0.159 ppbv	# 64
11) Trichlorofluoromethane	3.95	101	18302	0.082 ppbv	92
12) 1,1,2-Trichlorotrifluoroet	4.49	101	6464	0.045 ppbv	# 11
13) Ethanol	3.66	45	36184513	3790.269 ppbv	86
15) Acetone	3.85	43	1894199	14.299 ppbv	99
16) 1,3-Butadiene	3.33	39	6428	0.070 ppbv	# 1
19) Isopropyl Alcohol	3.66	45	36184513	496.546 ppbv	# 93
20) Methylene Chloride	4.35	84	424126	6.838 ppbv	93
21) Allyl Chloride	4.37	41	7631	0.072 ppbv	# 1
23) Vinyl Acetate	5.07	43	276452	1.220 ppbv	# 80
25) Ethyl Acetate	5.69	43	1235994	3.924 ppbv	98
26) Hexane	5.69	57	655016	4.482 ppbv	90
29) Chloroform	5.76	83	21187	0.091 ppbv	98
30) Cyclohexane	7.14	84	6307	0.053 ppbv	# 1
31) cis-1,2-Dichloroethene	5.68	61	86442	0.611 ppbv	# 29
34) 2-Butanone	5.25	43	456920	2.975 ppbv	99
35) Carbon Tetrachloride	7.02	117	16232	0.067 ppbv	97
36) Benzene	6.90	78	132044	0.455 ppbv	# 91
39) 1,2-Dichloropropane	7.19	63	841131	7.146 ppbv	# 23
41) Tetrahydrofuran	6.05	42	339517	4.795 ppbv	# 53
44) 2,2,4-Trimethylpentane	7.88	57	50236	0.098 ppbv	# 11
50) 4-Methyl-2-Pentanone	8.76	43	9602	0.043 ppbv	# 40
51) 2-Hexanone	10.15	43	3873	0.035 ppbv	# 1
53) Toluene	9.82	91	359637	1.164 ppbv	98
58) Ethyl Benzene	12.97	91	38363	0.096 ppbv	94
59) m/p-Xylene	13.01	91	36868	0.106 ppbv	# 32
60) o-Xylene	13.71	91	19116	0.057 ppbv	# 1
72) 4-Ethyltoluene	15.85	105	17231	0.047 ppbv	# 62
74) 1,2,4-Trimethylbenzene	16.78	105	61509	0.167 ppbv	# 57

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL042021\
Data File : VL036830.D
Acq On : 20 Apr 2021 20:35
Operator : SY/AP
Sample : M2096-03
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 06:38:49 2021
Quant Method : Z:\VQASRV\HPCHEM1\MSVOA L\METHODS\VL032521AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Mar 25 09:42:40 2021
QLast Update : Thu Mar 25 09:42:40 2021
Response via : Initial Calibration

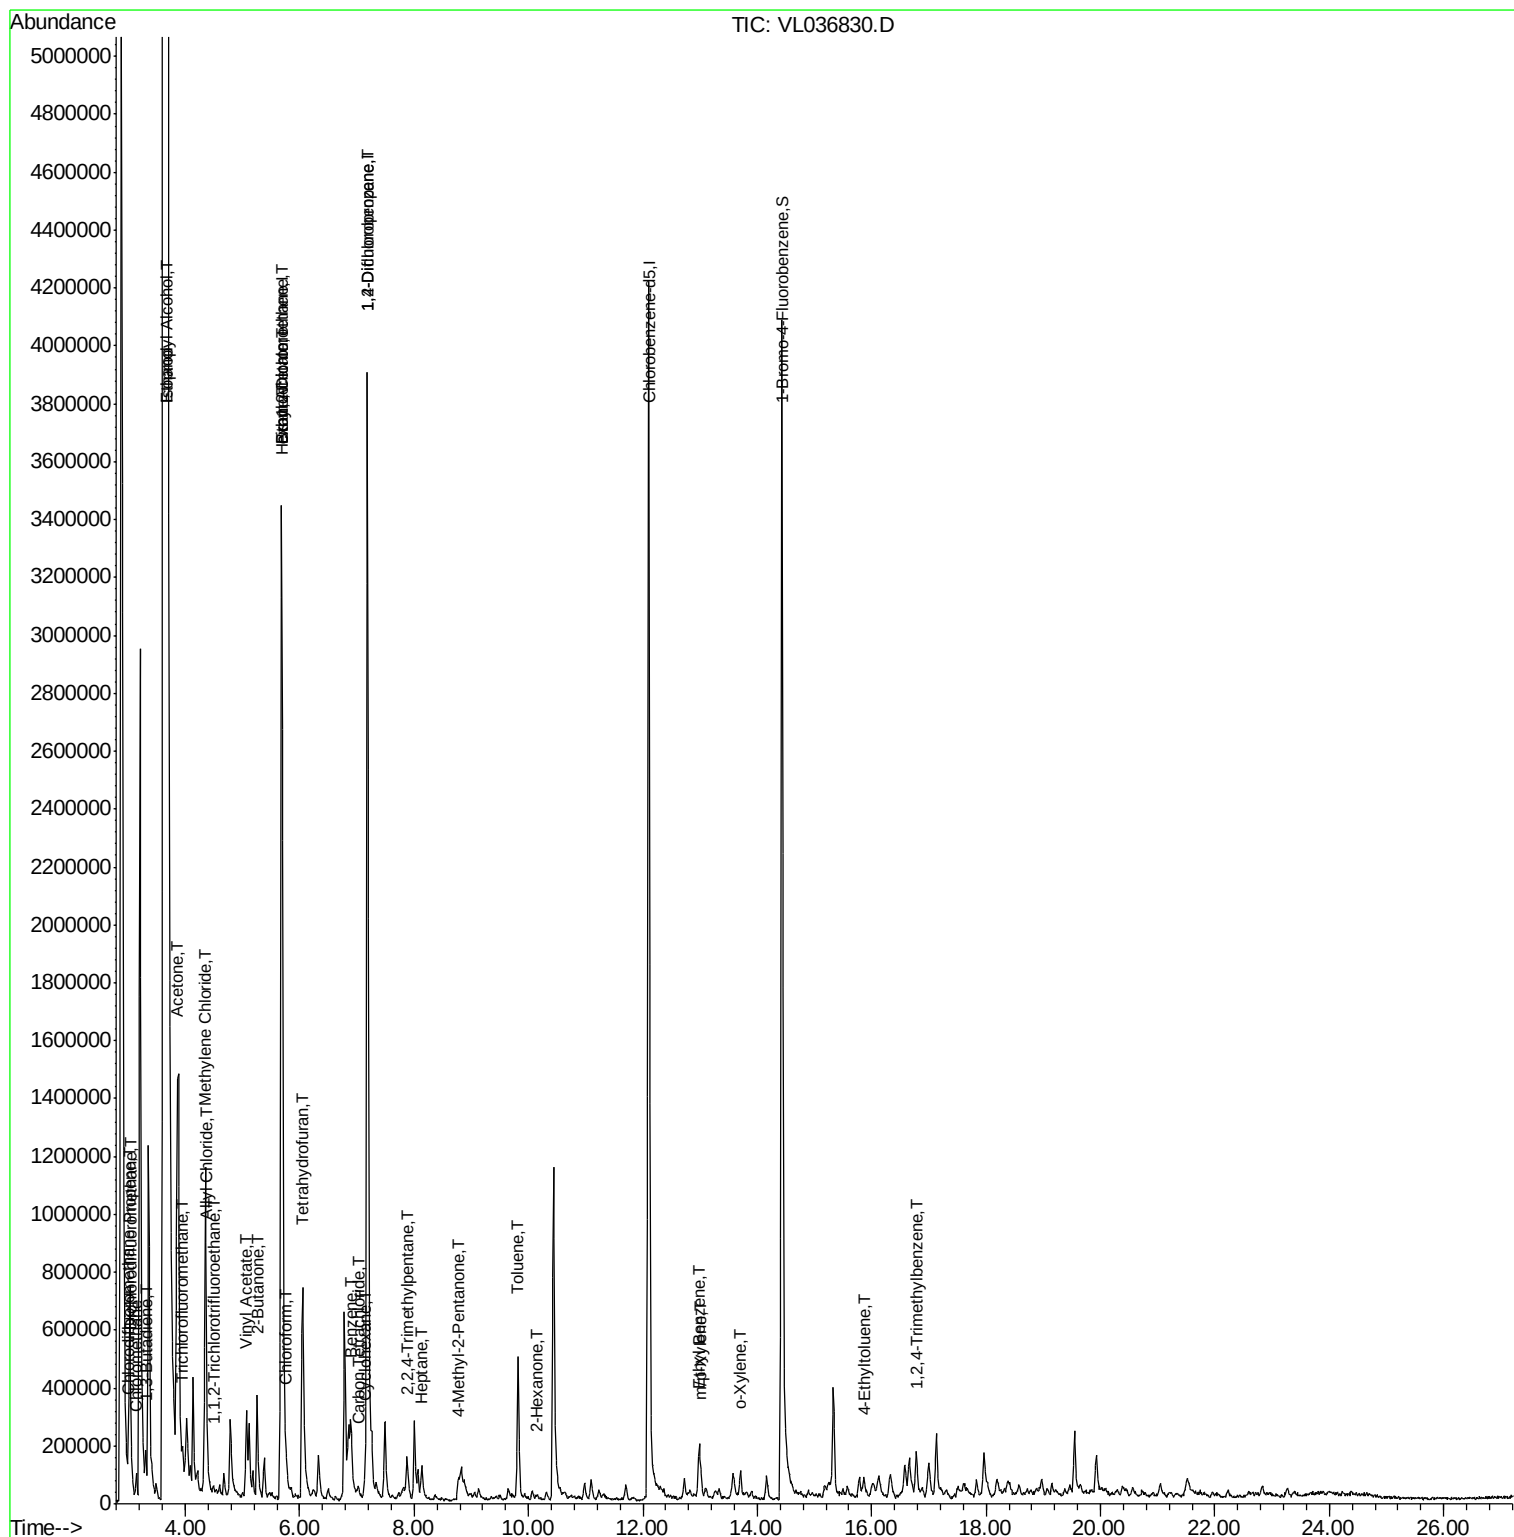

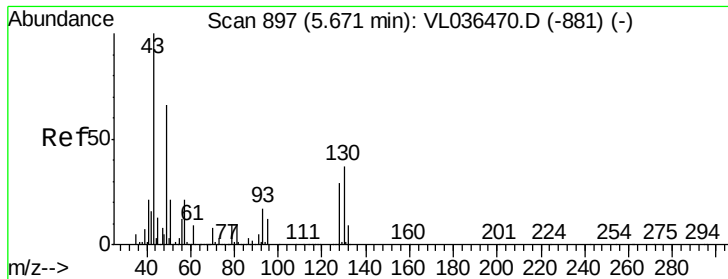

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.67 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 20 Apr 2021 20:35


Tot Ion: 49 Resp: 1345943

Ion Ratio Lower Upper

49 100

128 44.8 23.5 70.6




130 57.4 29.1 87.4

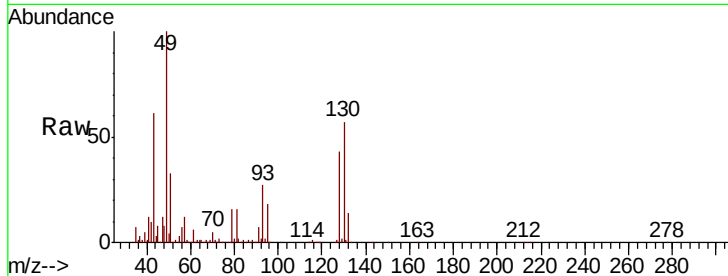

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

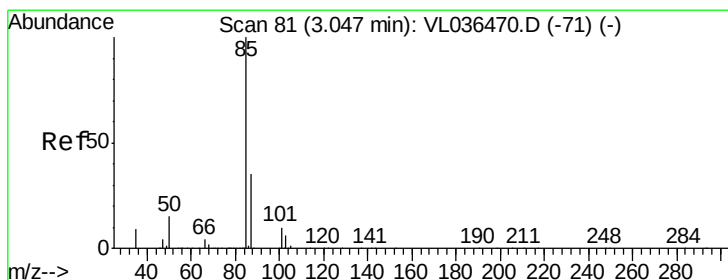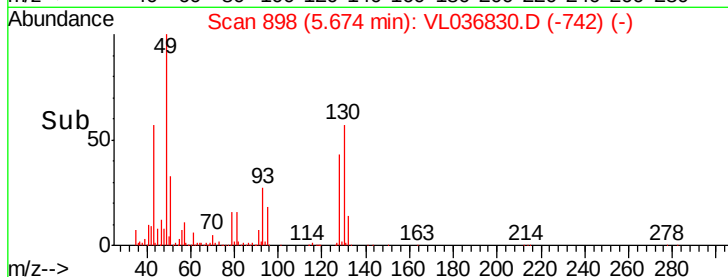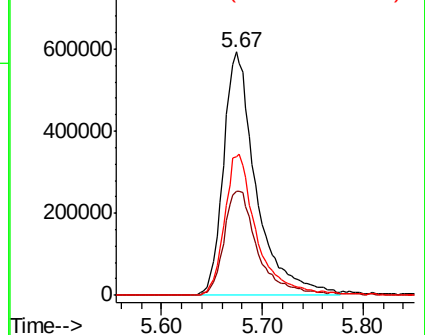

#2

Dichlorodifluoromethane

Concen: 0.273 ppbv

RT: 3.05 min Scan# 82

Delta R.T. 0.00 min

Lab File: VL036830.D


Acq: 20 Apr 2021 20:35

Tgt Ion: 85 Resp: 59896

Ion Ratio Lower Upper



85 100


87 26.3 27.8 41.8#

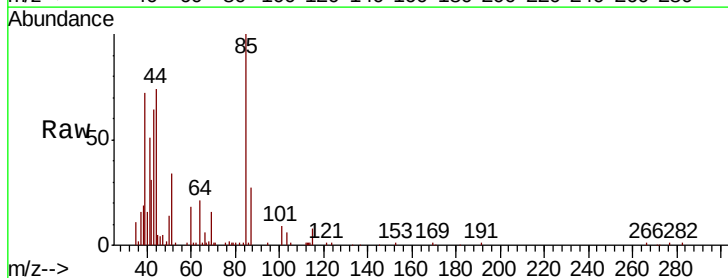

Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

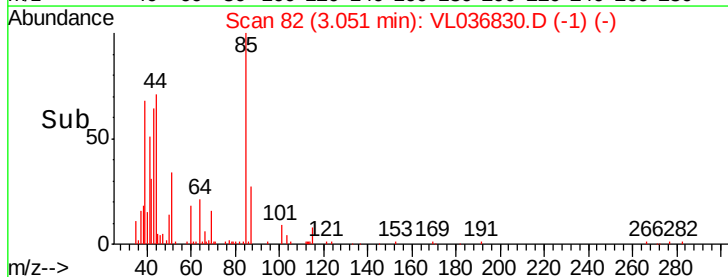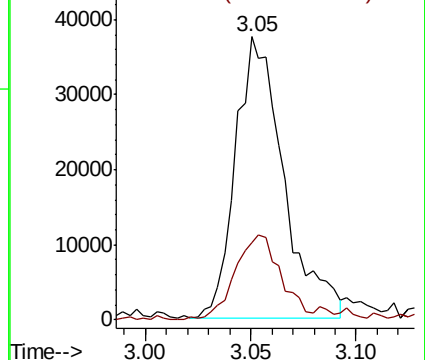

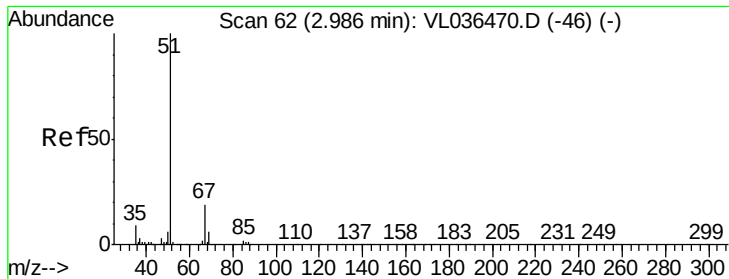

#3

Chlorodifluoromethane

Concen: 0.435 ppbv

RT: 2.99 Instrument:

Delta R.T. MSVOA.L

Lab File: ClientSampleId:





Acq: 20 Apr 2021 20:35

Tot Ion: 51 Resp: 109338

Ion Ratio Lower Upper

51 100

67 15.8 14.7 22.1

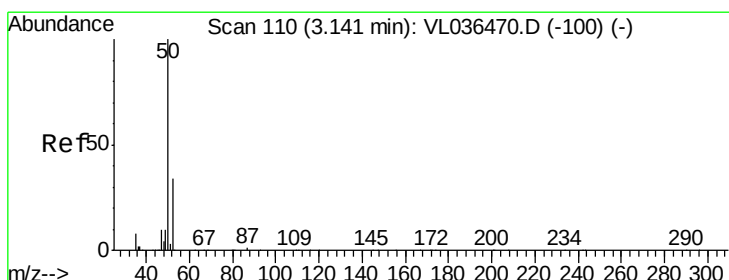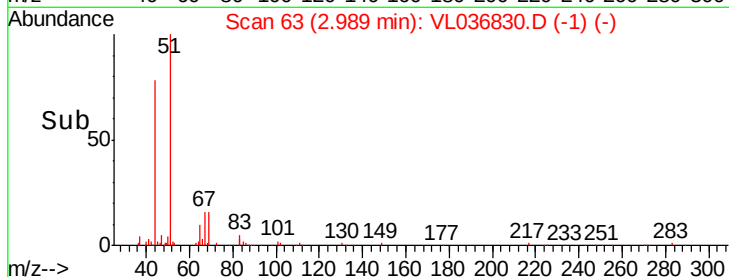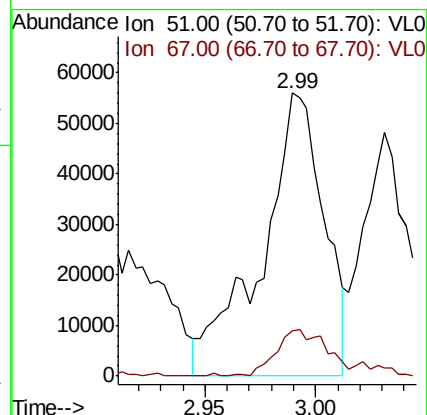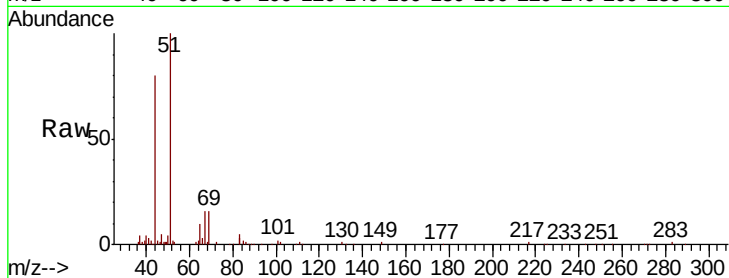

#4

Chloromethane

Concen: 0.795 ppbv

RT: 3.14 min Scan# 111

Delta R.T. 0.00 min

Lab File: VL036830.D




Acq: 20 Apr 2021 20:35


Tgt Ion: 50 Resp: 70643

Ion Ratio Lower Upper

50 100





52 31.0 27.0 40.6

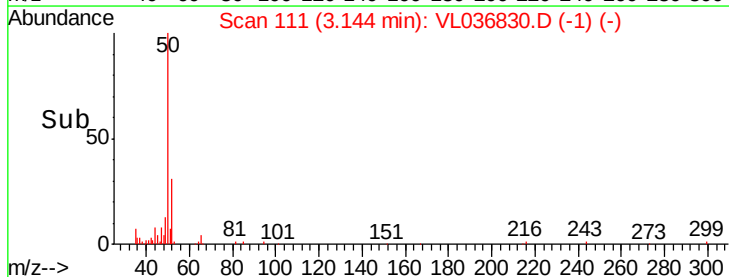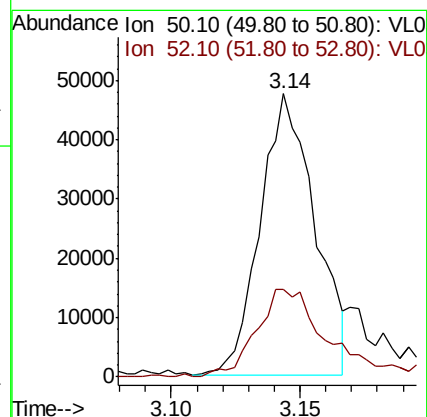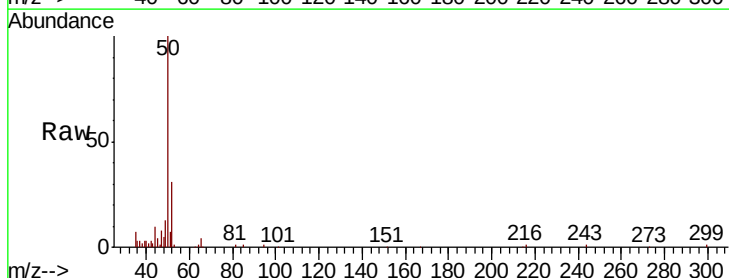

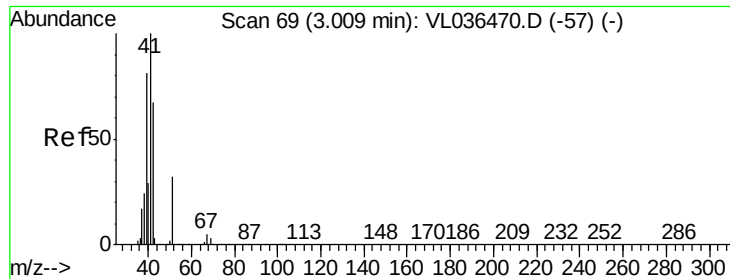




#9
 Propene
 Concen: 2.364 ppbv
 RT: 3.02
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 20 Apr 2021 20:35


Tot Ion: 41 Resp: 189556
 Ion Ratio Lower Upper
 41 100
 42 59.1 57.0 85.4

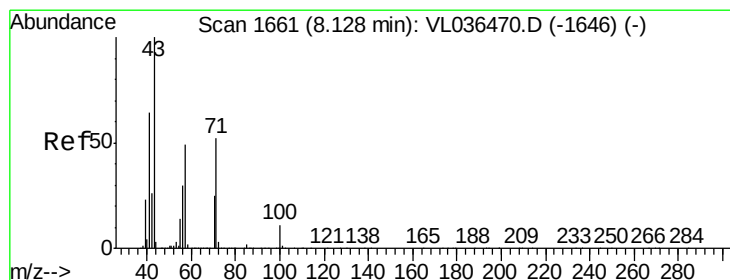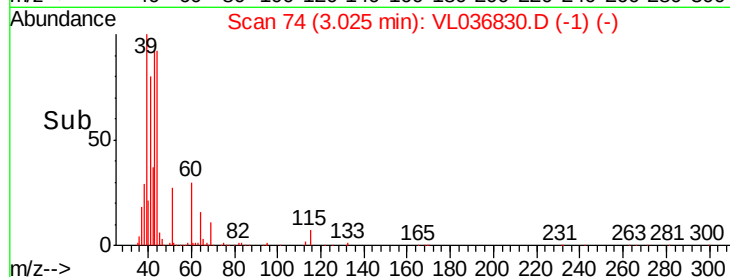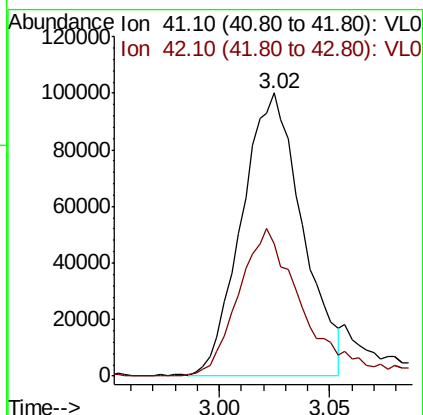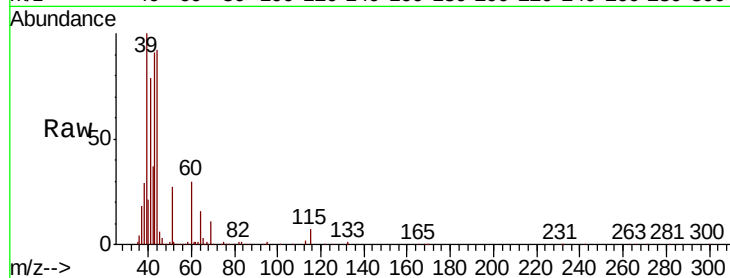

#10
 Heptane
 Concen: 0.159 ppbv
 RT: 8.13 min Scan# 1663
 Delta R.T. 0.01 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35





Tgt Ion: 43 Resp: 32410
 Ion Ratio Lower Upper
 43 100
 57 73.3 39.0 58.6#

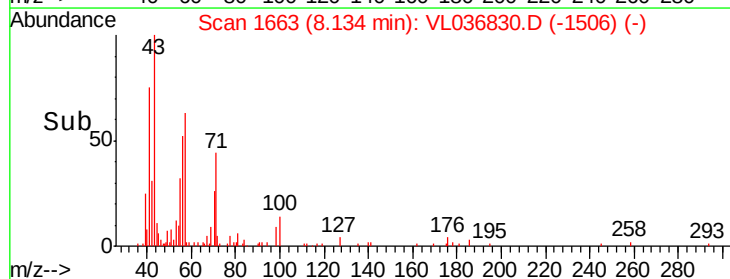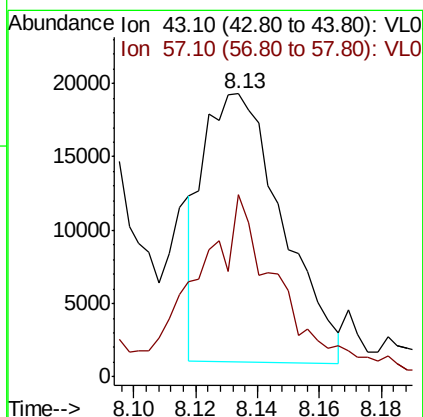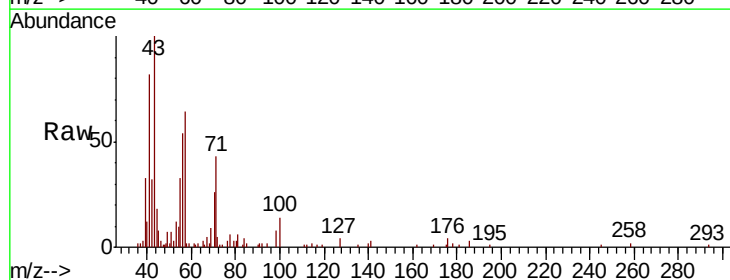

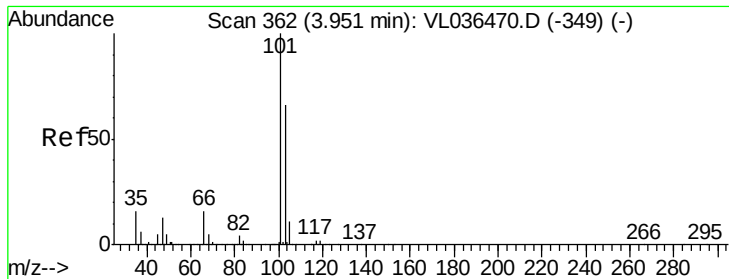




#11
 Trichlorofluoromethane
 Concen: 0.082 ppbv
 RT: 3.95 Instrument :
 Delta R.T. MSVOA_1
 Lab File: ClientSampleId :
 Acq: 20 Apr 2021 20:35


Tot Ion:101 Resp: 18302
 Ion Ratio Lower Upper
 101 100
 103 71.8 52.5 78.7

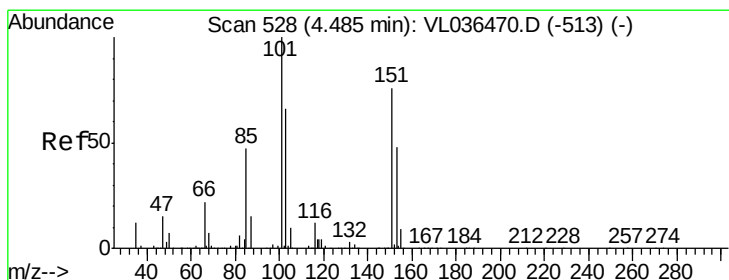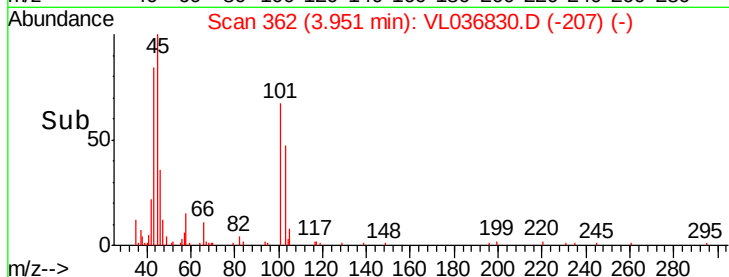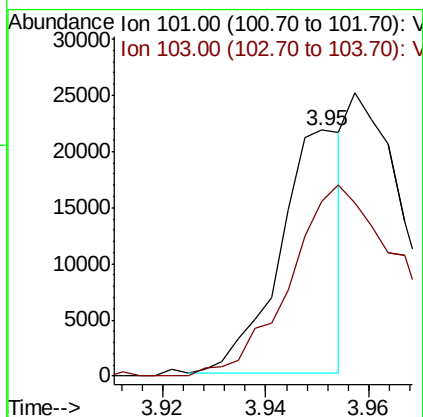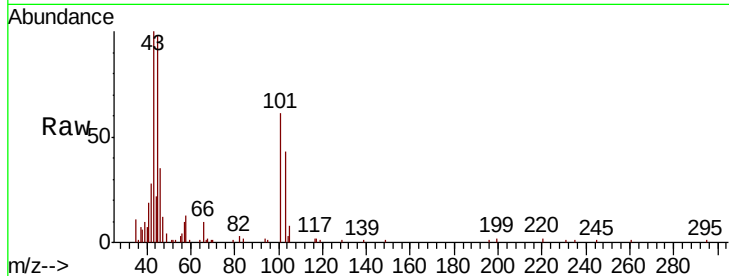

#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.045 ppbv
 RT: 4.49 min Scan# 529
 Delta R.T. 0.00 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35





Tgt Ion:101 Resp: 6464
 Ion Ratio Lower Upper
 101 100
 151 0.0 60.9 91.3#

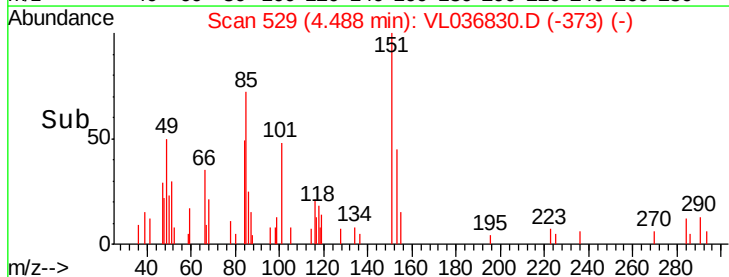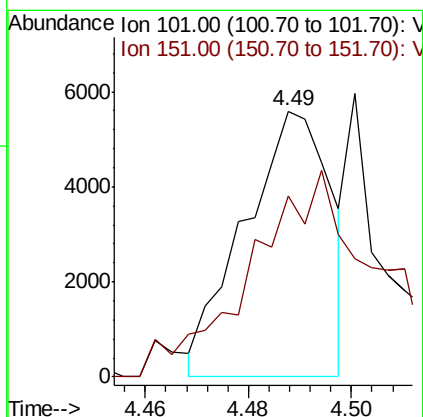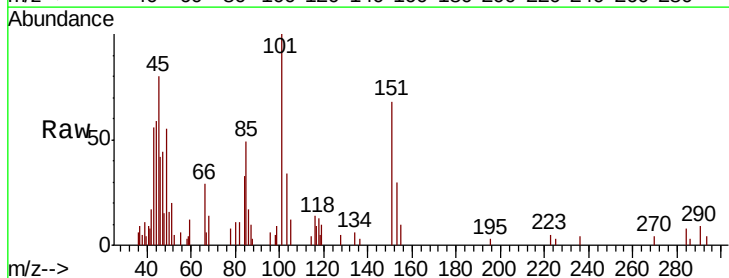

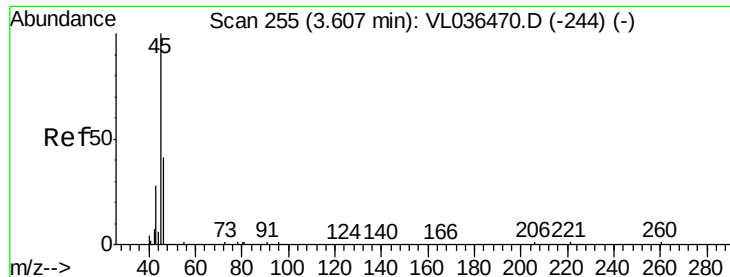




#13
 Ethanol
 Concen: 3790.269 ppbv
 RT: 3.66
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 Acq: 20 Apr 2021 20:35


Tot Ion: 45 Resp: 36184513
 Ion Ratio Lower Upper
 45 100
 46 50.3 16.6 66.2

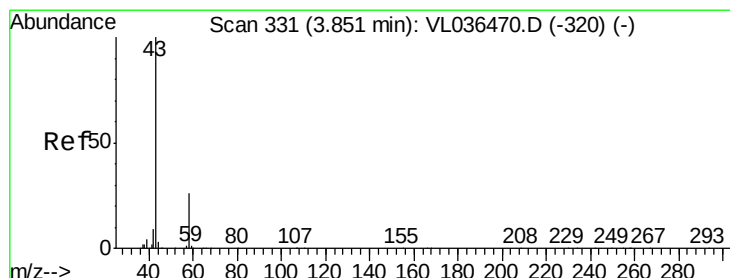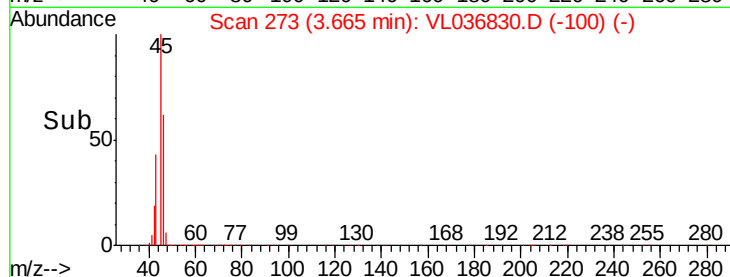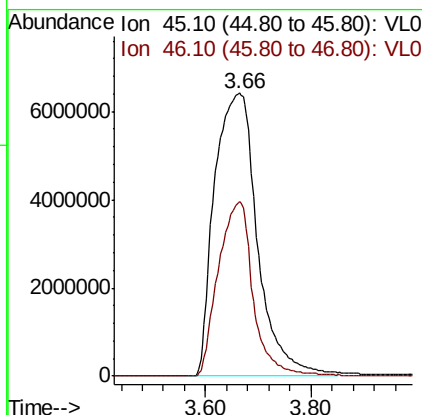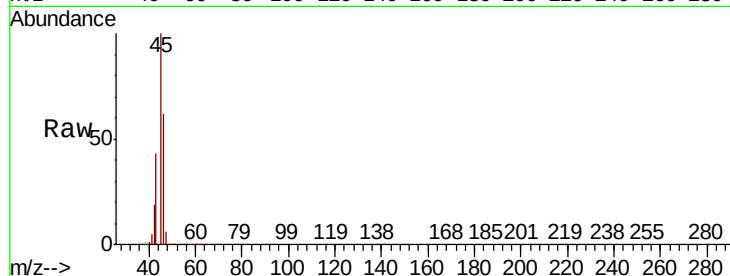

#15
 Acetone
 Concen: 14.299 ppbv
 RT: 3.85 min Scan# 332
 Delta R.T.: 0.00 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35





Tgt Ion: 43 Resp: 1894199
 Ion Ratio Lower Upper
 43 100
 58 25.7 21.2 31.8

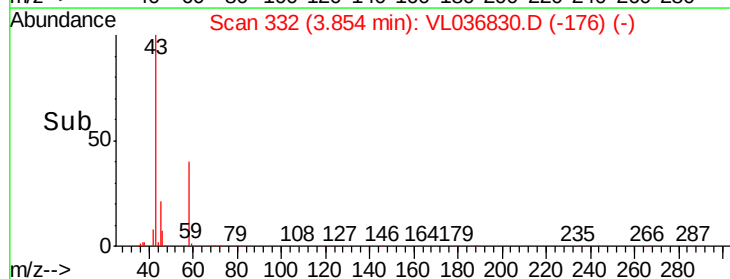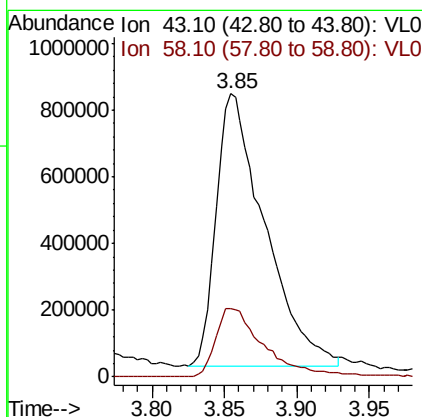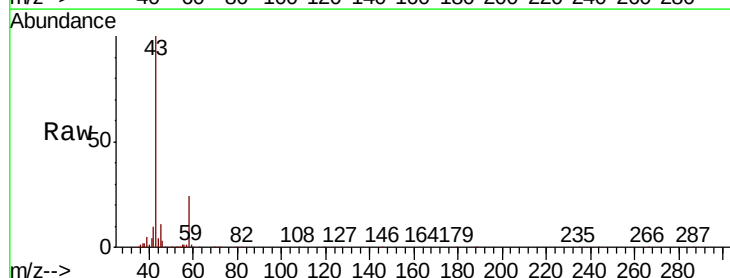

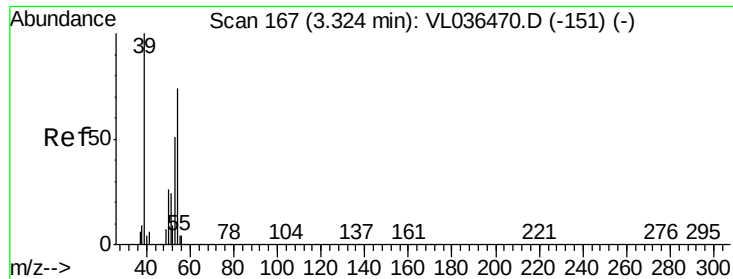




#16
 1,3-Butadiene
 Concen: 0.070 ppbv
 RT: 3.33 Instrument :
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 20 Apr 2021 20:35


Tot Ion: 39 Resp: 6428
 Ion Ratio Lower Upper
 39 100
 54 224.5 58.8 88.2#

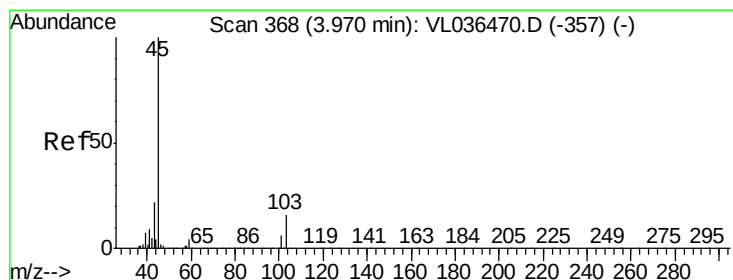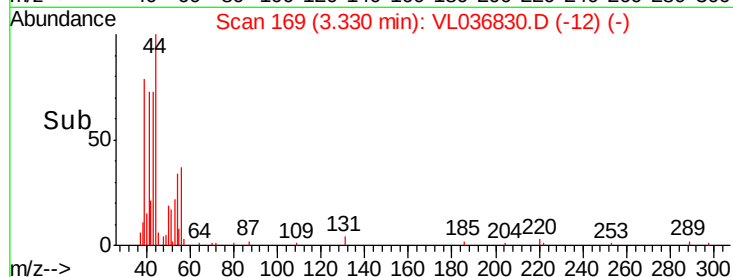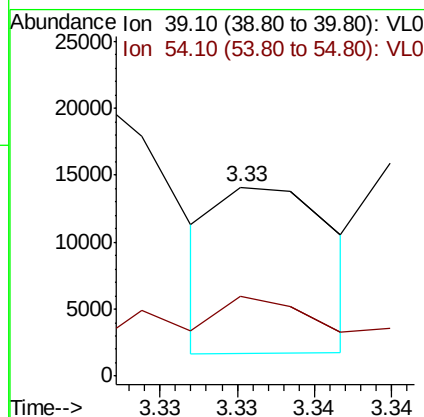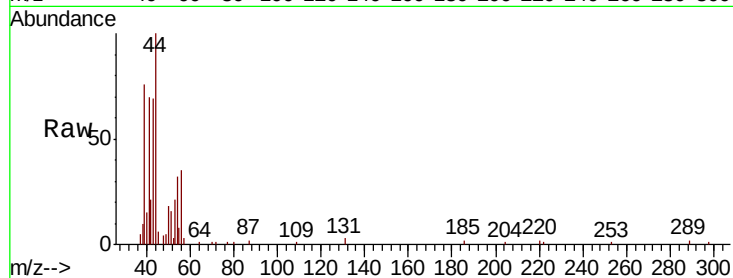

#19
 Isopropyl Alcohol
 Concen: 496.546 ppbv
 RT: 3.66 min Scan# 273
 Delta R.T. -0.31 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35





Tgt Ion: 45 Resp: 36184513
 Ion Ratio Lower Upper
 45 100
 58 1.3 2.9 4.3#

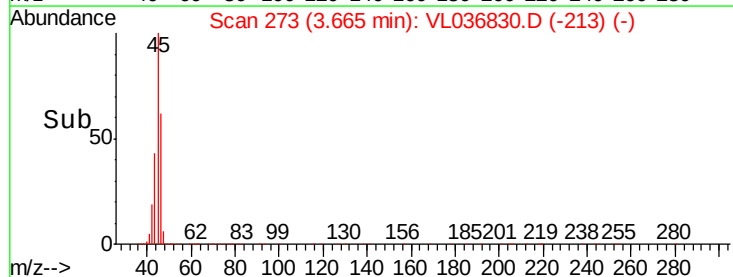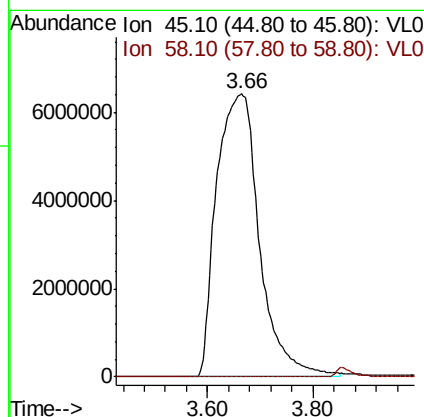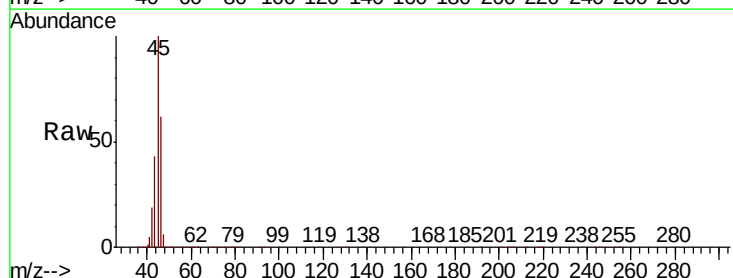

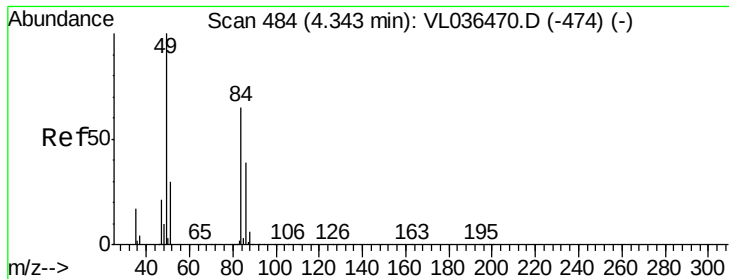




#20
Methylene Chloride
Concen: 6.838 ppbv
RT: 4.35
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
Acq: 20 Apr 2021 20:35


Tot Ion:	84	Resp:	424126
Ion	Ratio	Lower	Upper
84	100		
49	165.1	122.9	184.3
51	52.0	36.9	55.3
86	60.9	48.2	72.4

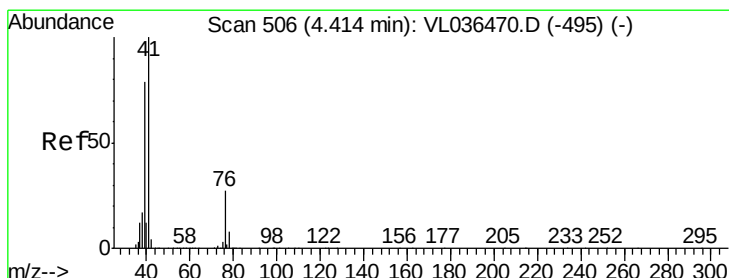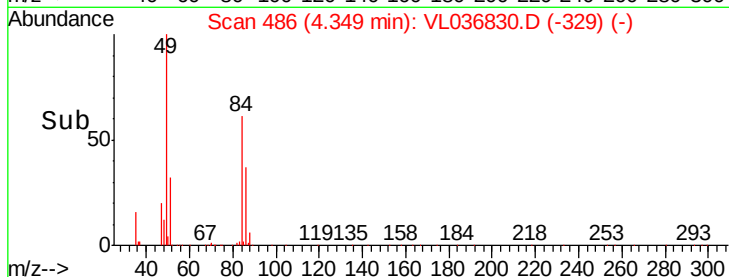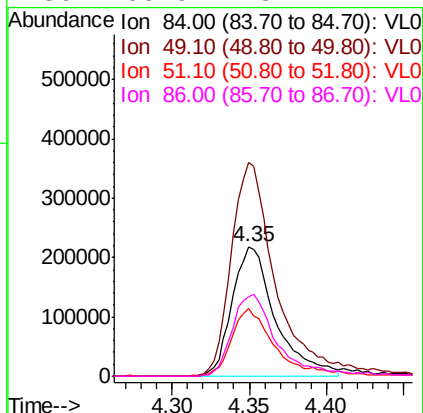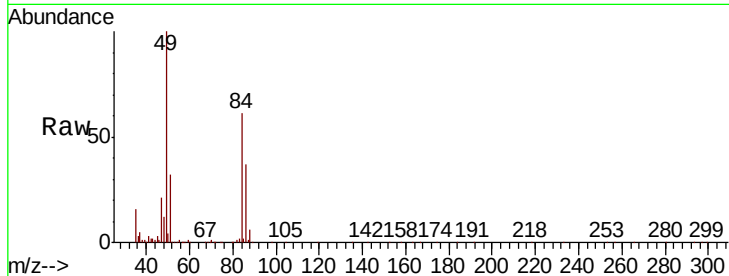

#21
Allyl Chloride
Concen: 0.072 ppbv
RT: 4.37 min Scan# 493
Delta R.T. -0.04 min
Lab File: VL036830.D
Acq: 20 Apr 2021 20:35

Tgt Ion:	41	Resp:	7631
Ion	Ratio	Lower	Upper
41	100		
76	5.6	22.9	34.3#
39	295.6	67.3	100.9#

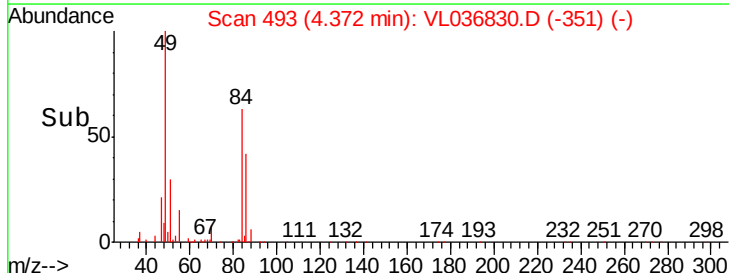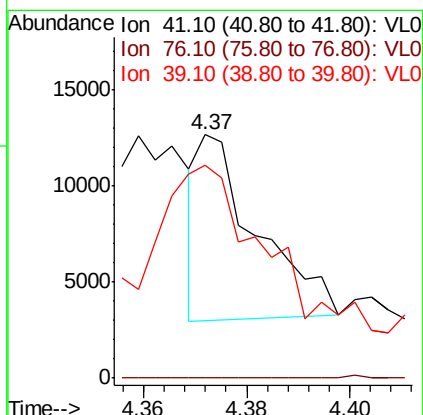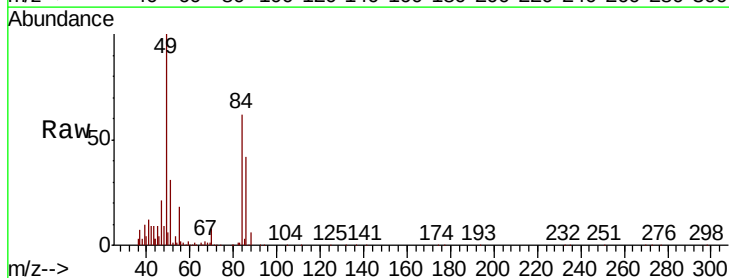

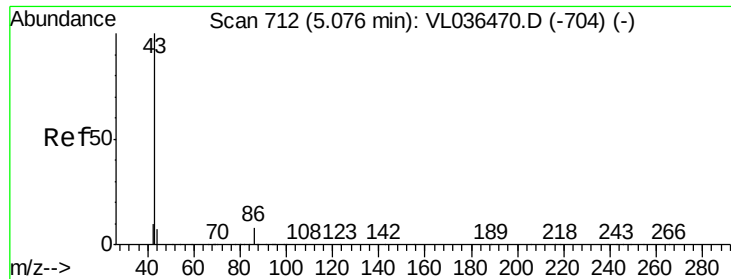

#23

Vinyl Acetate

Concen: 1.220 ppbv

RT: 5.07 Instrument:





Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 20 Apr 2021 20:35

Tot Ion: 43 Resp: 276452

Ion	Ratio	Lower	Upper
43	100		
86	9.4	5.4	8.0#
42	23.2	8.5	12.7#
44	2.6	4.6	7.0#

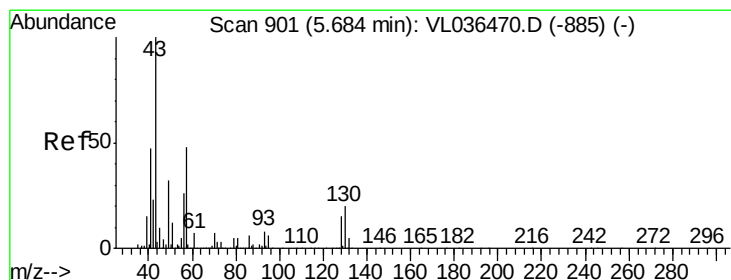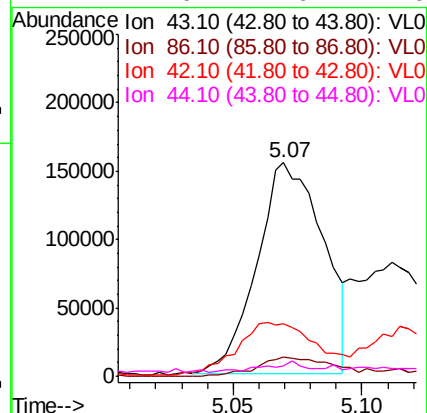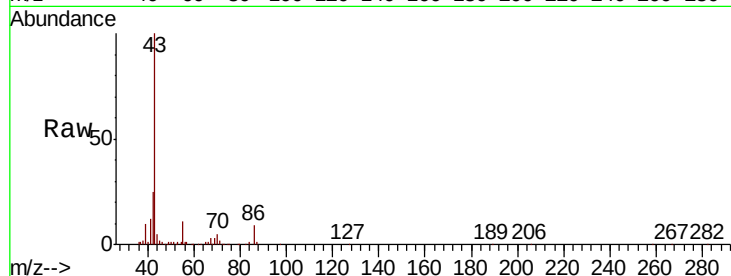

#25

Ethyl Acetate

Concen: 3.924 ppbv

RT: 5.69 min Scan# 902




Delta R.T. 0.00 min


Lab File: VL036830.D

Acq: 20 Apr 2021 20:35

Tgt Ion: 43 Resp: 1235994

Ion	Ratio	Lower	Upper
43	100		
45	9.6	7.9	11.9
61	8.1	7.4	11.2
70	6.8	5.1	7.7

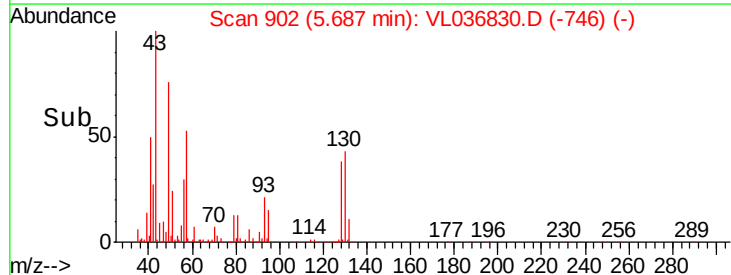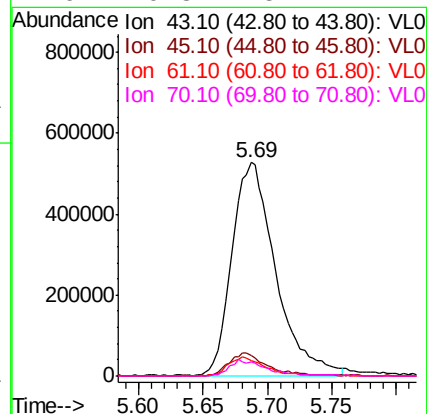

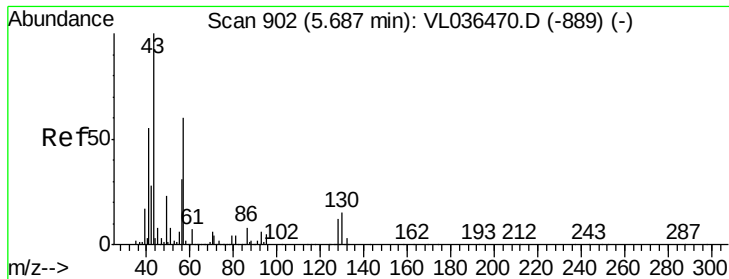

#26

Hexane

Concen: 4.482 ppbv

RT: 5.69 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 20 Apr 2021 20:35

Tot Ion: 57 Resp: 655016


Ion Ratio Lower Upper

57 100

41 97.9 77.2 115.8

43 192.8 173.8 260.6

56 57.4 43.8 65.6



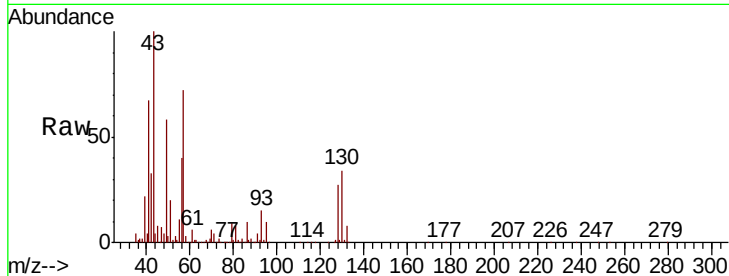


Abundance Ion 57.10 (56.80 to 57.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 43.10 (42.80 to 43.80): VL0

Ion 56.10 (55.80 to 56.80): VL0

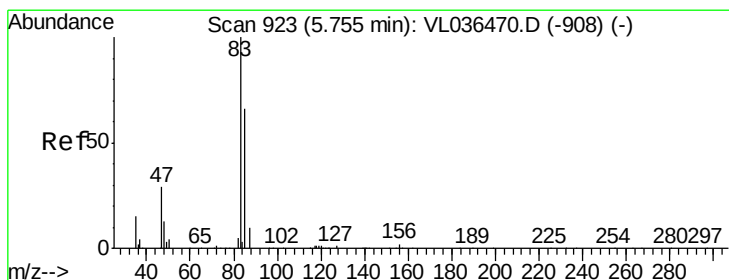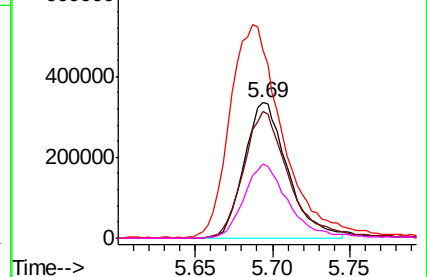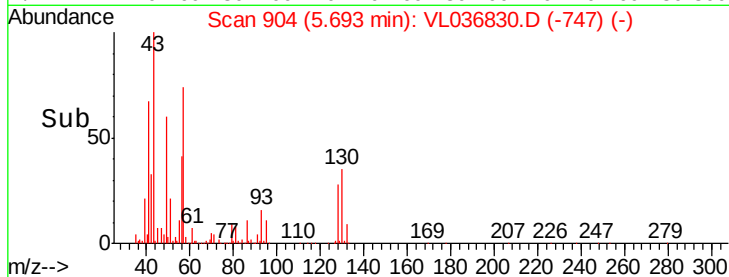

#29

Chloroform

Concen: 0.091 ppbv

RT: 5.76 min Scan# 926

Delta R.T. 0.01 min

Lab File: VL036830.D


Acq: 20 Apr 2021 20:35

Tgt Ion: 83 Resp: 21187

Ion Ratio Lower Upper



83 100


85 64.4 52.6 78.8

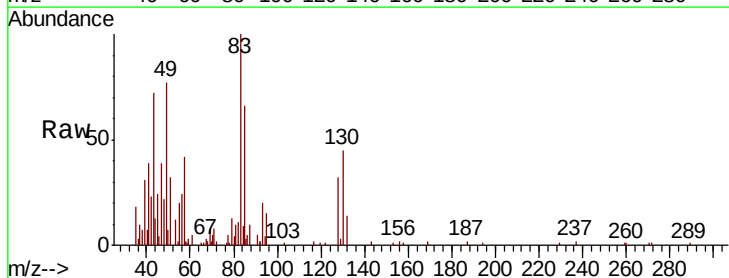

Abundance Ion 83.00 (82.70 to 83.70): VL0





Ion 85.00 (84.70 to 85.70): VL0

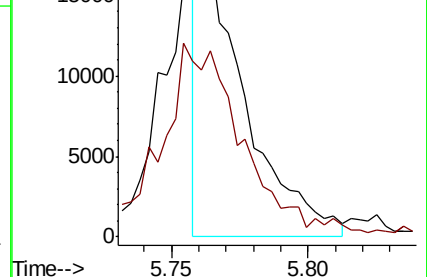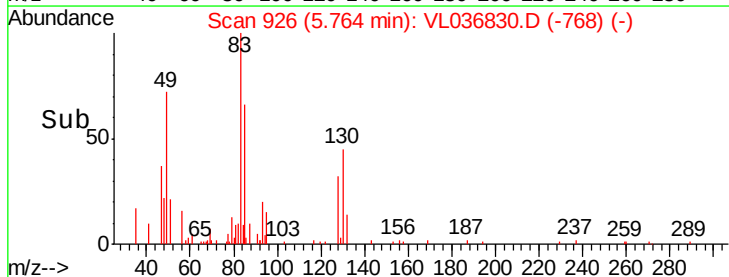






#30
Cyclohexane
Concen: 0.053 ppbv
RT: 7.14
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
Acq: 20 Apr 2021 20:35


Tot Ion	84	Resp	6307
Ion Ratio	Lower	Upper	
84	100		
56	0.0	114.6	171.8#
41	407.6	75.3	112.9#

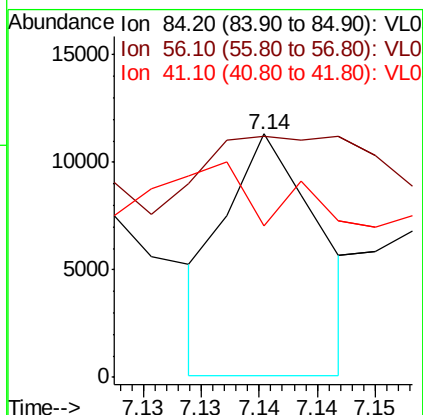

#31
cis-1,2-Dichloroethene
Concen: 0.611 ppbv
RT: 5.68 min Scan# 900
Delta R.T.: 0.13 min
Lab File: VL036830.D
Acq: 20 Apr 2021 20:35


Tgt Ion	61	Resp	86442
Ion Ratio	Lower	Upper	
61	100		
96	3.4	48.7	73.1#
98	0.0	31.4	47.0#

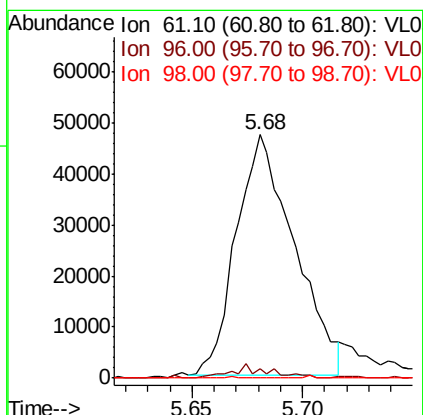






#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.18 min Instrument: MSVOA_L
 Delta R.T.:
 Lab File: ClientSampleId:
 Acq: 20 Apr 2021 20:35

Tot Ion:114 Resp: 3146139
 Ion Ratio Lower Upper
 114 100
 63 27.2 22.4 33.6
 88 18.7 15.4 23.0

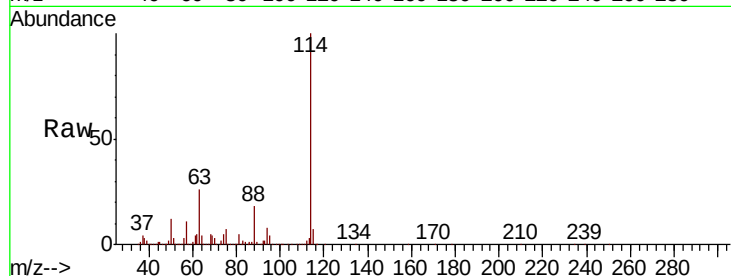


Abundance Ion 114.10 (113.80 to 114.80): VL0
 Ion 63.10 (62.80 to 63.80): VL0
 Ion 88.10 (87.80 to 88.80): VL0


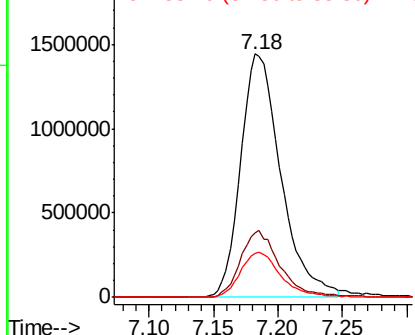



#34
 2-Butanone
 Concen: 2.975 ppbv
 RT: 5.25 min Scan# 767
 Delta R.T.: 0.00 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35

Tgt Ion: 43 Resp: 456920
 Ion Ratio Lower Upper
 43 100
 72 21.7 17.0 25.6




Abundance Ion 43.10 (42.80 to 43.80): VL0
 Ion 72.10 (71.80 to 72.80): VL0

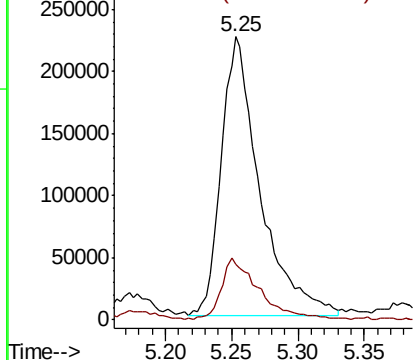



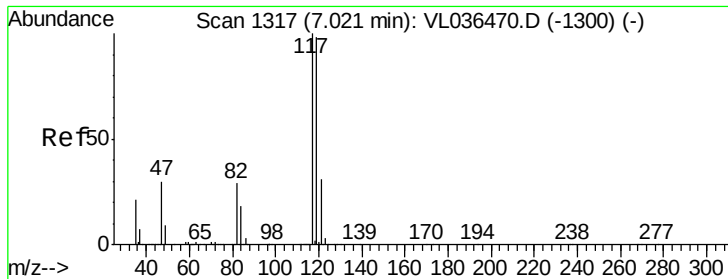


#35
 Carbon Tetrachloride
 Concen: 0.067 ppbv
 RT: 7.02 min
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 Acq: 20 Apr 2021 20:35

Tot Ion: 117 Resp: 16232
 Ion Ratio Lower Upper
 117 100
 119 95.6 78.2 117.2
 121 28.1 24.5 36.7

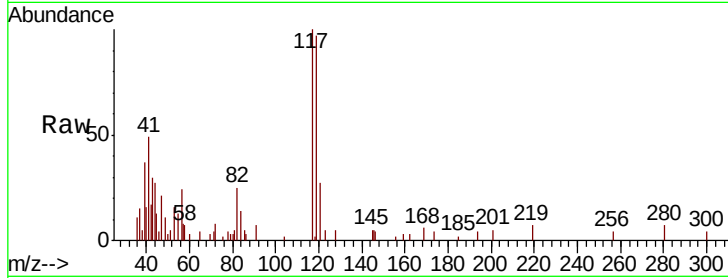


Abundance Ion 117.00 (116.70 to 117.70): V
 Ion 119.00 (118.70 to 119.70): V
 Ion 121.00 (120.70 to 121.70): V

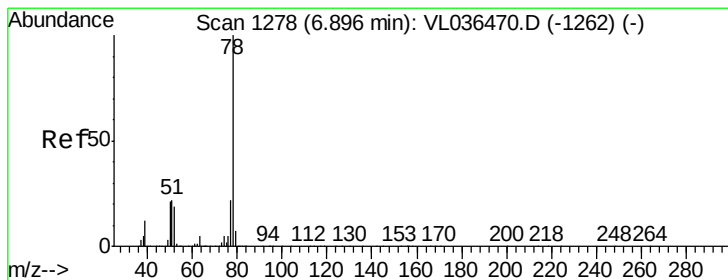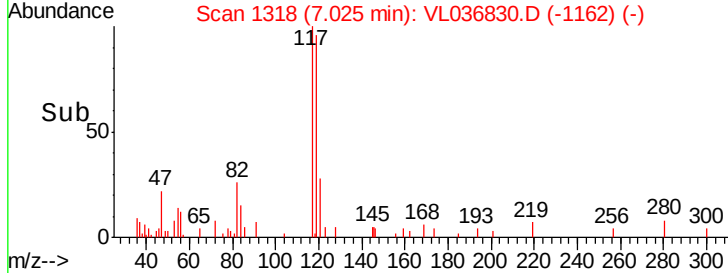
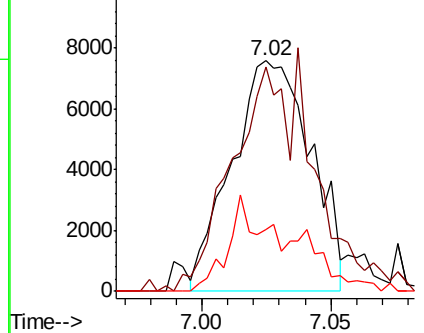



#36
 Benzene
 Concen: 0.455 ppbv
 RT: 6.90 min Scan# 1278
 Delta R.T. -0.00 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35

Tgt Ion: 78 Resp: 132044
 Ion Ratio Lower Upper
 78 100
 77 25.8 18.0 27.0
 50 15.3 16.5 24.7#

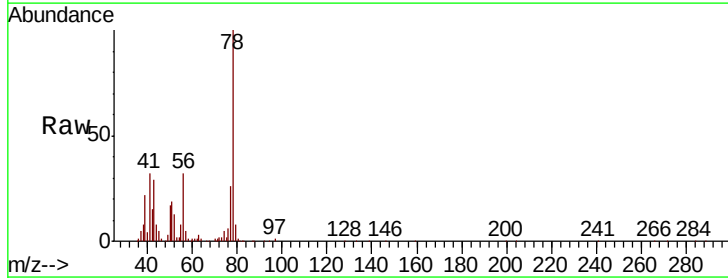

Abundance Ion 78.10 (77.80 to 78.80): VL0
 Ion 77.10 (76.80 to 77.80): VL0
 Ion 50.10 (49.80 to 50.80): VL0

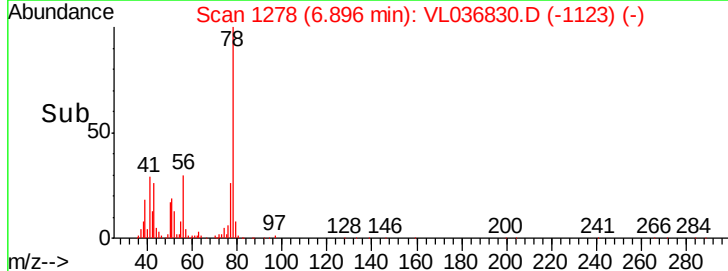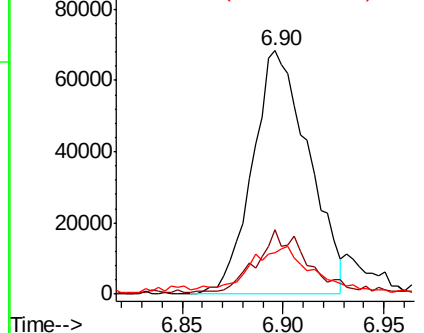



#39

1,2-Dichloropropane

Concen: 7.146 ppbv

RT: 7.19 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 20 Apr 2021 20:35





Tot Ion: 63 Resp: 841131

Ion Ratio Lower Upper

63 100

41 0.0 62.4 93.6#

62 16.7 52.8 79.2#

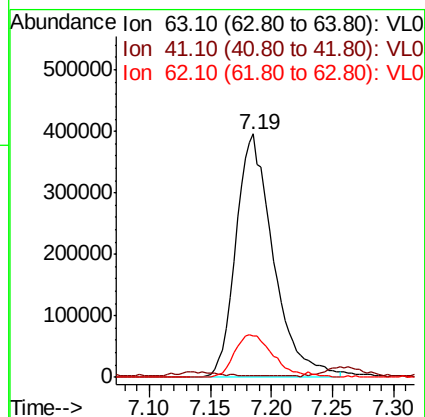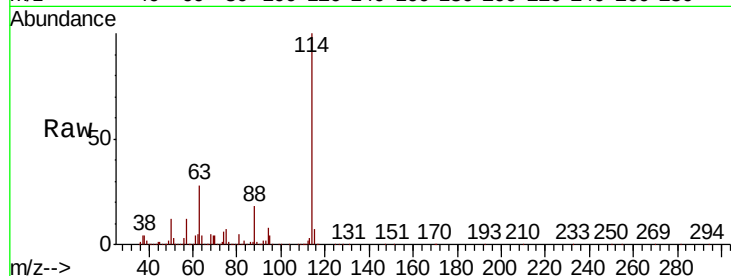

#41

Tetrahydrofuran

Concen: 4.795 ppbv

RT: 6.05 min Scan# 1014

Delta R.T. -0.01 min

Lab File: VL036830.D

Acq: 20 Apr 2021 20:35




Tgt Ion: 42 Resp: 339517


Ion Ratio Lower Upper

42 100

72 11.0 27.6 41.4#





71 2.6 27.0 40.4#

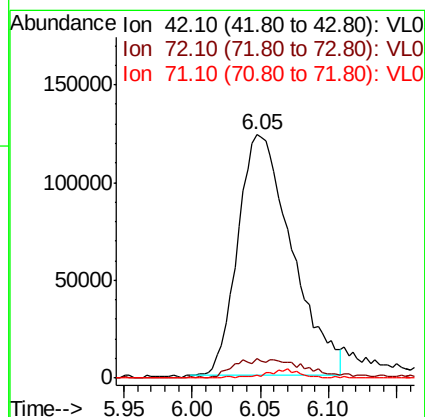

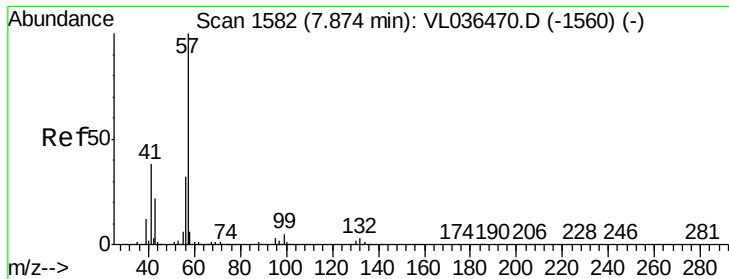




#44
 2,2,4-Trimethylpentane
 Concen: 0.098 ppbv
 RT: 7.88 Instrument:
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId:
 Acq: 20 Apr 2021 20:35


Tot Ion	57	Resp	50236
Ion	Ratio	Lower	Upper
57	100		
41	104.4	28.8	43.2#
56	0.0	26.1	39.1#

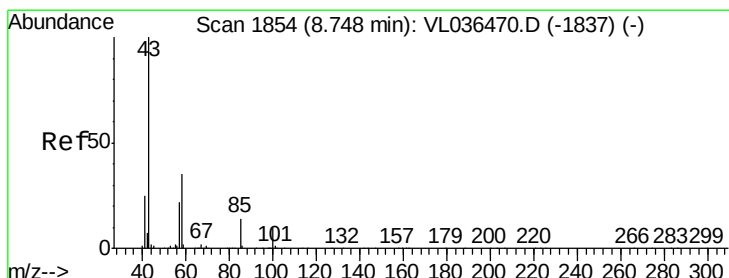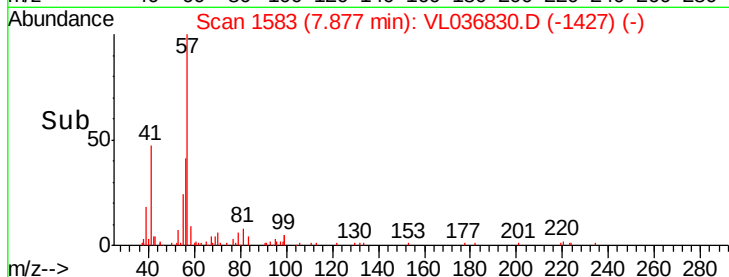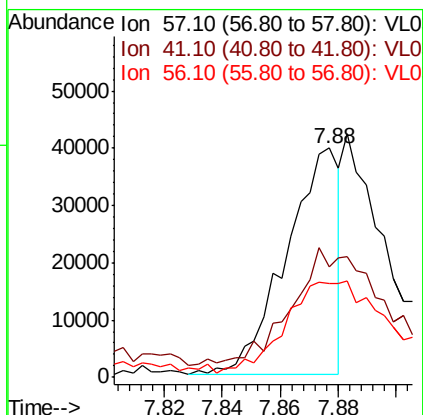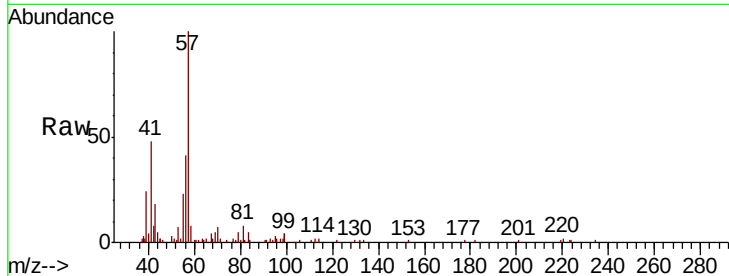

#50
 4-Methyl-2-Pentanone
 Concen: 0.043 ppbv
 RT: 8.76 min Scan# 1858
 Delta R.T. 0.01 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35





Tgt Ion	43	Resp	9602
Ion	Ratio	Lower	Upper
43	100		
58	0.0	28.2	42.2#

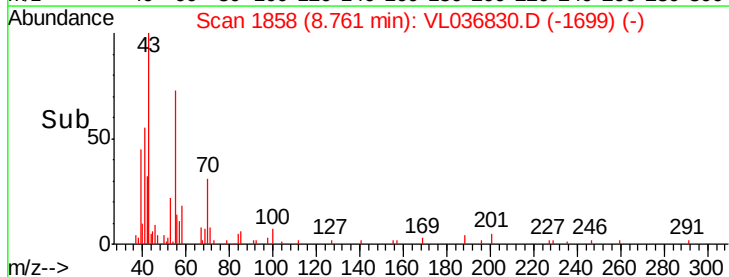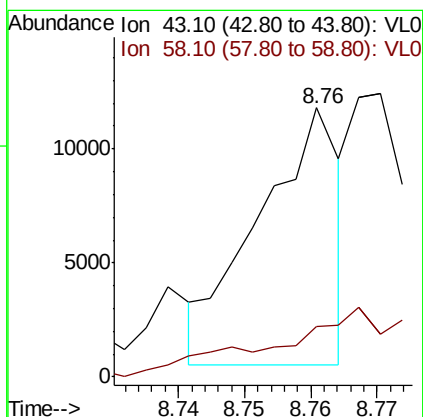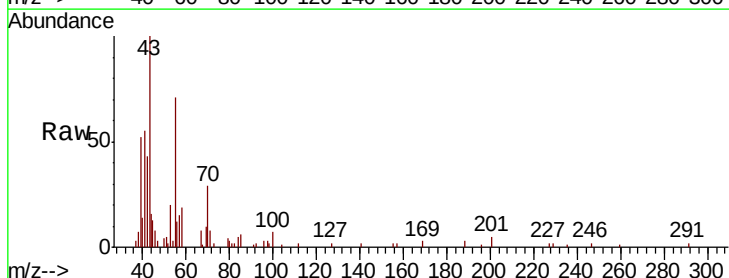

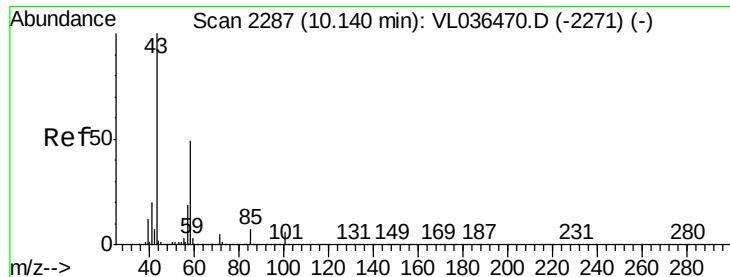




#51
 2-Hexanone
 Concen: 0.035 ppbv
 RT: 10.15
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId:
 Acq: 20 Apr 2021 20:35


Tot Ion: 43 Resp: 3873
 Ion Ratio Lower Upper
 43 100
 58 139.7 37.7 56.5#
 98 23.3 0.2 0.2#

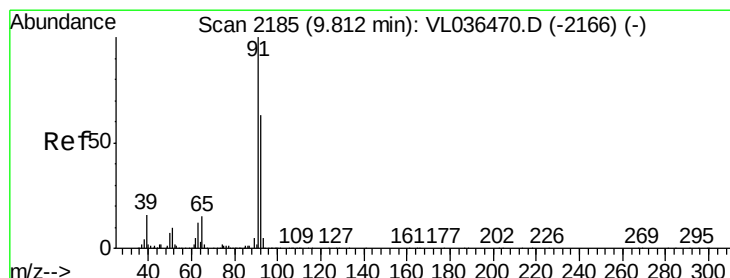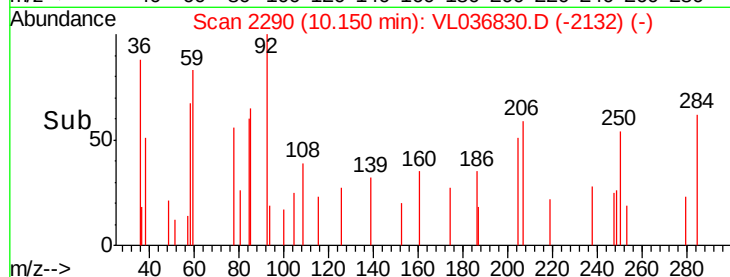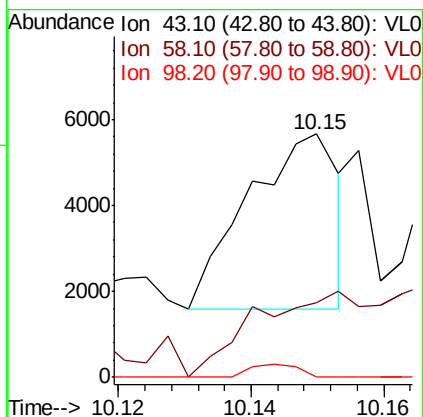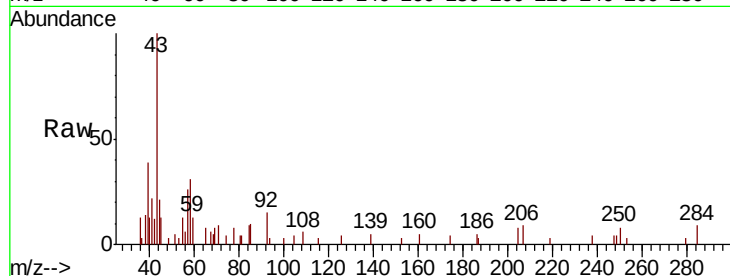

#53
 Toluene
 Concen: 1.164 ppbv
 RT: 9.82 min Scan# 2186
 Delta R.T. 0.00 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35





Tgt Ion: 91 Resp: 359637
 Ion Ratio Lower Upper
 91 100
 92 62.5 48.8 73.2

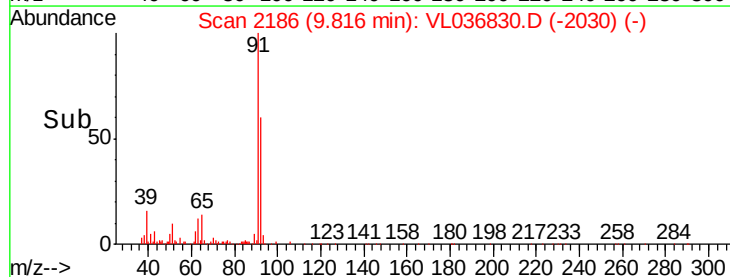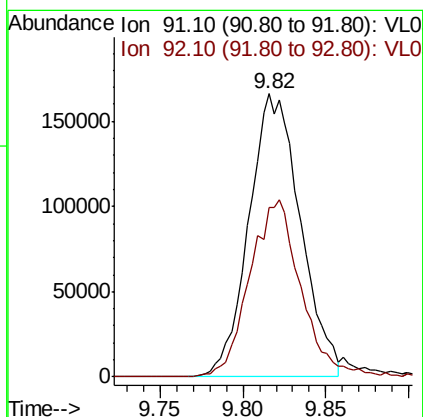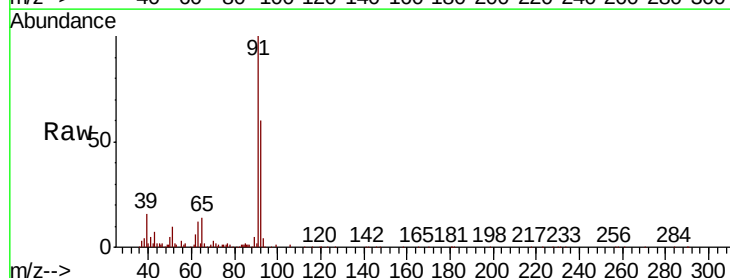

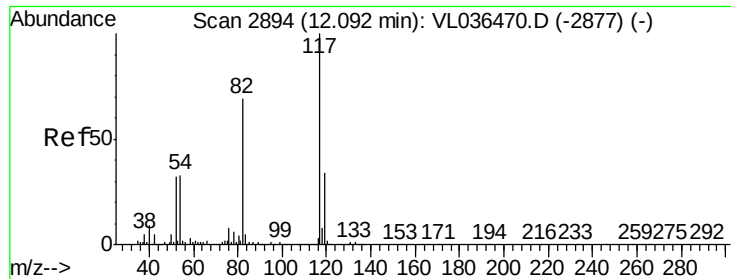




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.10 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
Acq: 20 Apr 2021 20:35


Tot Ion: 117 Resp: 2739990
Ion Ratio Lower Upper
117 100
82 69.1 57.4 86.0
119 33.5 47.4 71.0#

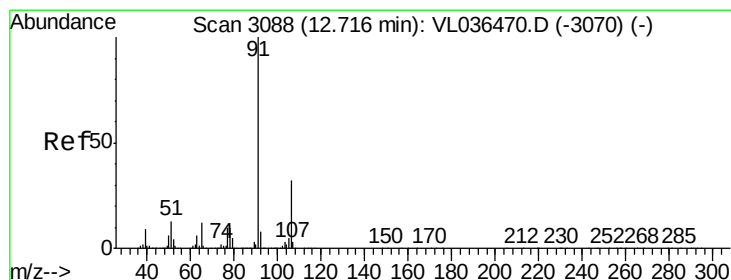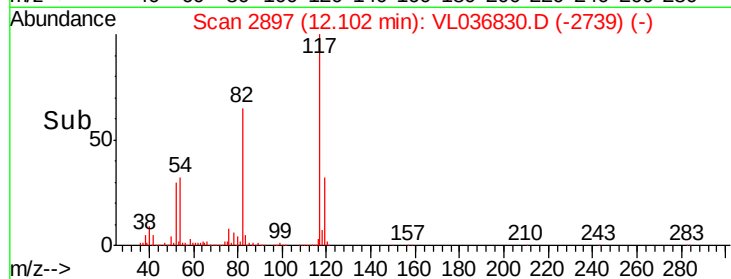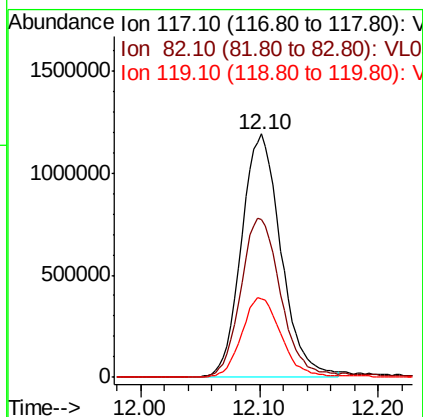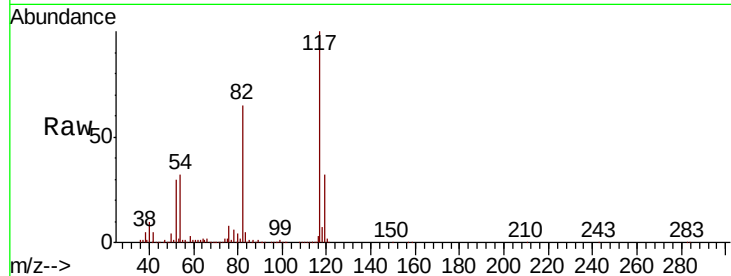

#58
Ethyl Benzene
Concen: 0.096 ppbv
RT: 12.97 min Scan# 3167
Delta R.T.: 0.25 min
Lab File: VL036830.D
Acq: 20 Apr 2021 20:35





Tgt Ion: 91 Resp: 38363
Ion Ratio Lower Upper
91 100
106 35.2 25.3 37.9

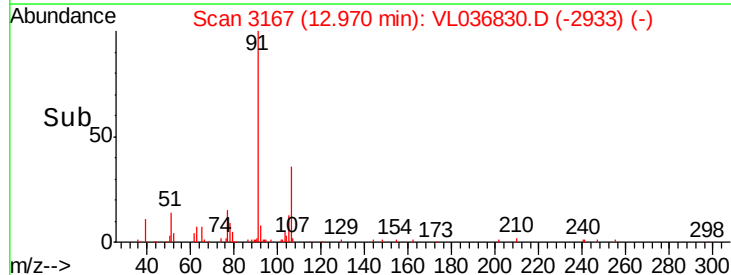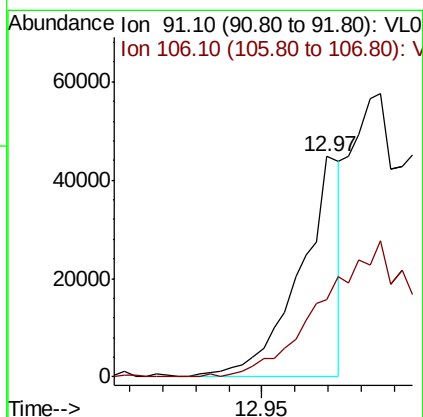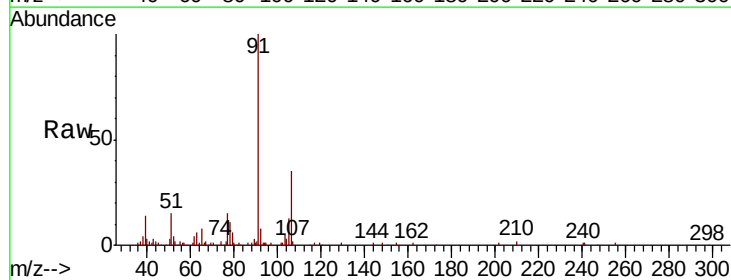






#59
m/p-Xylene
Concen: 0.106 ppbv
RT: 13.01 min
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 20 Apr 2021 20:35


Tot Ion: 91 Resp: 36868
Ion Ratio Lower Upper
91 100
106 0.0 35.3 52.9#

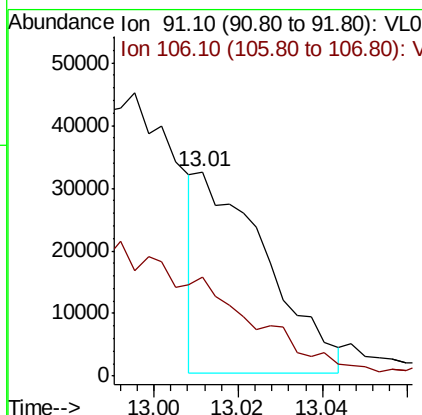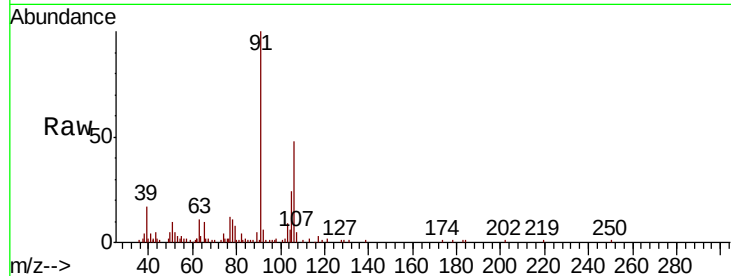

#60
o-Xylene
Concen: 0.057 ppbv
RT: 13.71 min Scan# 3396
Delta R.T. 0.01 min
Lab File: VL036830.D
Acq: 20 Apr 2021 20:35





Tgt Ion: 91 Resp: 19116
Ion Ratio Lower Upper
91 100
106 155.6 22.3 66.9#

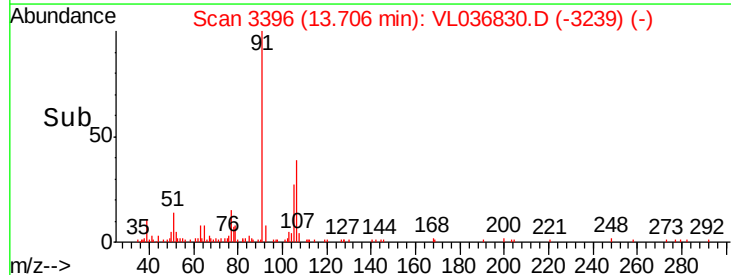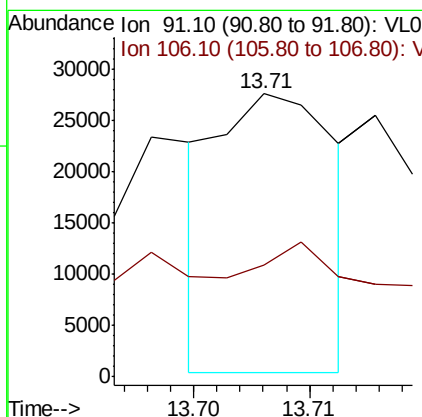






#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.400 ppbv
 RT: 14.43 min
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 20 Apr 2021 20:35


Tot Ion: 95 Resp: 2052752
 Ion Ratio Lower Upper
 95 100
 174 65.3 51.0 76.6
 175 4.8 3.9 5.9

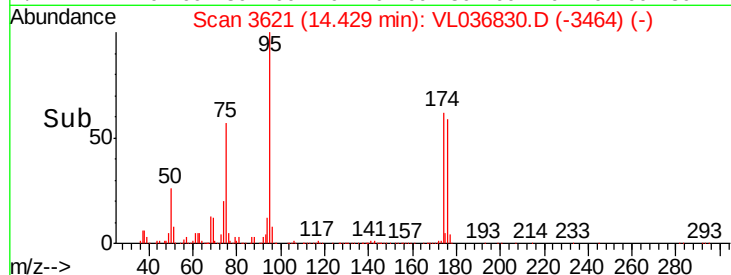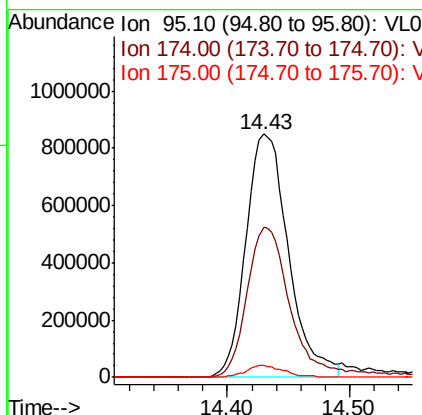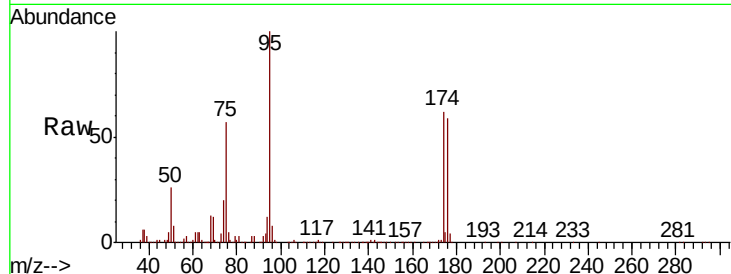

#72
 4-Ethyltoluene
 Concen: 0.047 ppbv
 RT: 15.85 min Scan# 4064
 Delta R.T. 0.01 min
 Lab File: VL036830.D
 Acq: 20 Apr 2021 20:35

Tgt Ion: 105 Resp: 17231
 Ion Ratio Lower Upper
 105 100
 120 40.8 24.0 36.0#
 91 38.4 11.0 16.4#
 77 36.7 11.7 17.5#

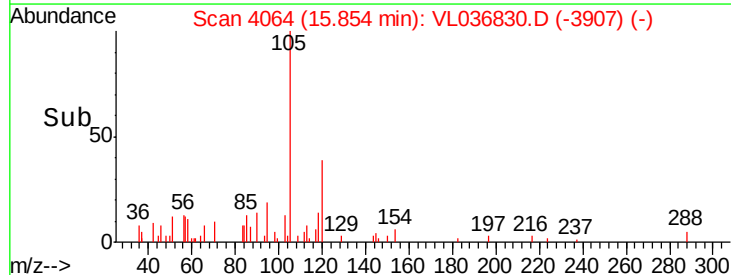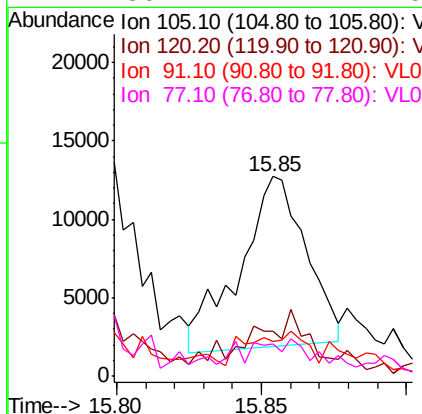

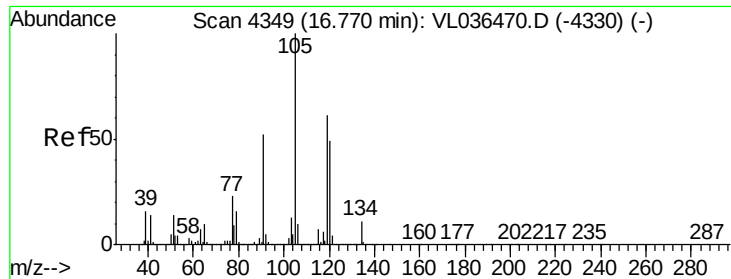

#74

1,2,4-Trimethylbenzene

Concen: 0.167 ppbv

RT: 16.78 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 20 Apr 2021 20:35

Tot Ion:	105	Resp:	61509
Ion Ratio	Lower	Upper	
105	100		
120	27.0	39.2	58.8#
91	11.2	42.6	64.0#
77	8.4	18.6	28.0#

