


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL042821\
 Data File : VL036873.D
 Acq On : 28 Apr 2021 9:04
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL042721AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Apr 27 16:56:35 2021
 Last Update : Tue Apr 27 16:56:35 2021

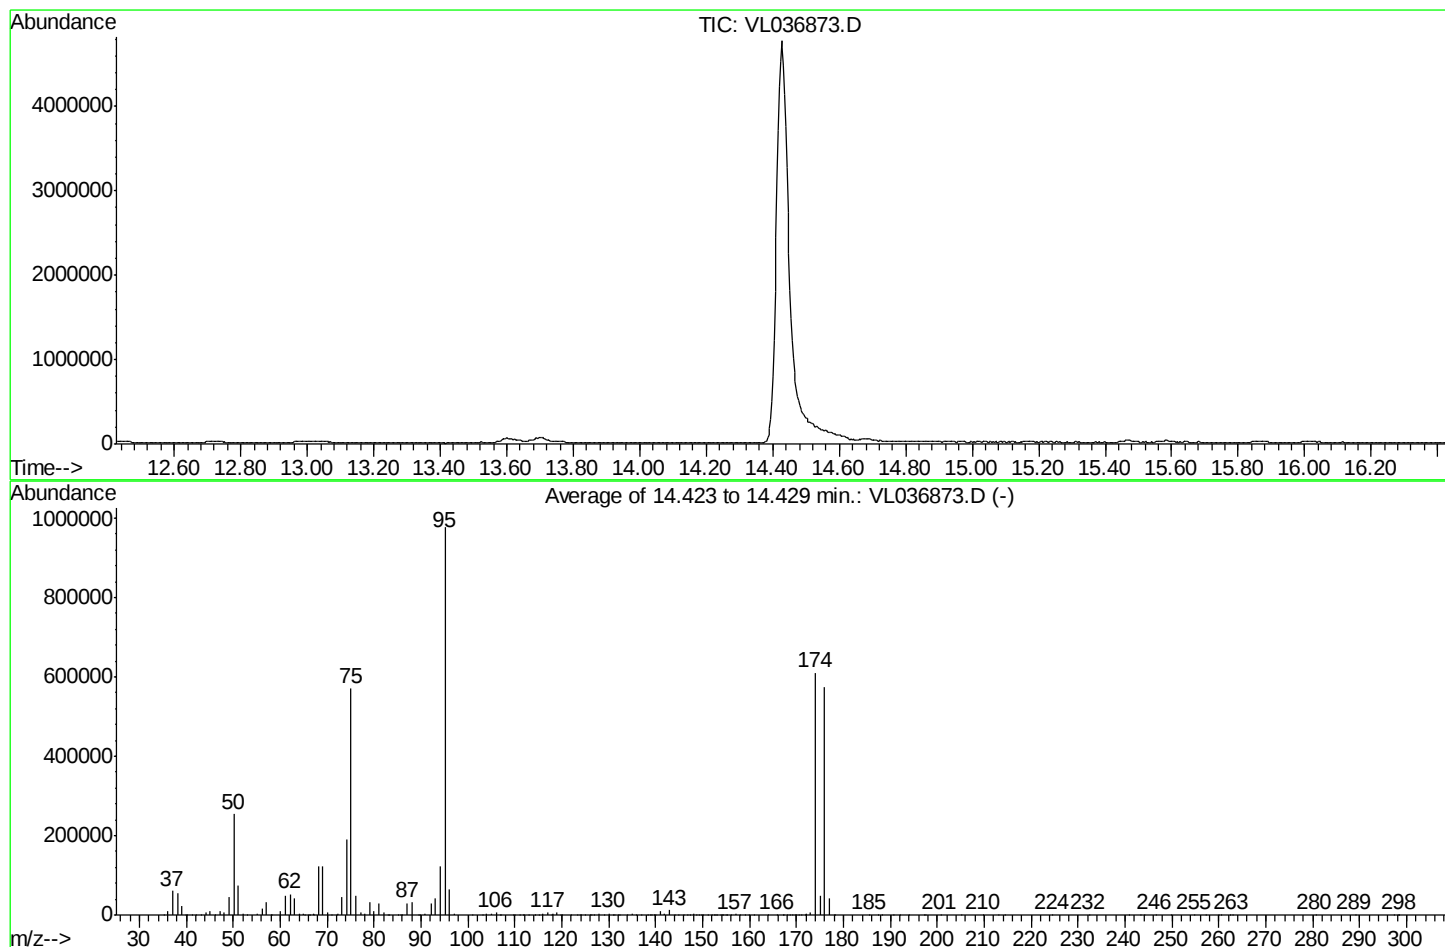

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.0	253866	PASS
75	95	30	66	58.4	570176	PASS
95	95	100	100	100.0	976618	PASS
96	95	5	9	6.7	65082	PASS
173	174	0.00	2	1.3	7782	PASS
174	95	50	120	62.5	610282	PASS
175	174	4	9	8.2	49824	PASS
176	174	93	101	94.0	573802	PASS
177	176	5	9	7.2	41562	PASS