


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL050119\
Data File : VL033613.D
Acq On : 1 May 2019 11:10
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050119AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu May 02 06:29:02 2019
Last Update : Thu May 02 06:29:02 2019

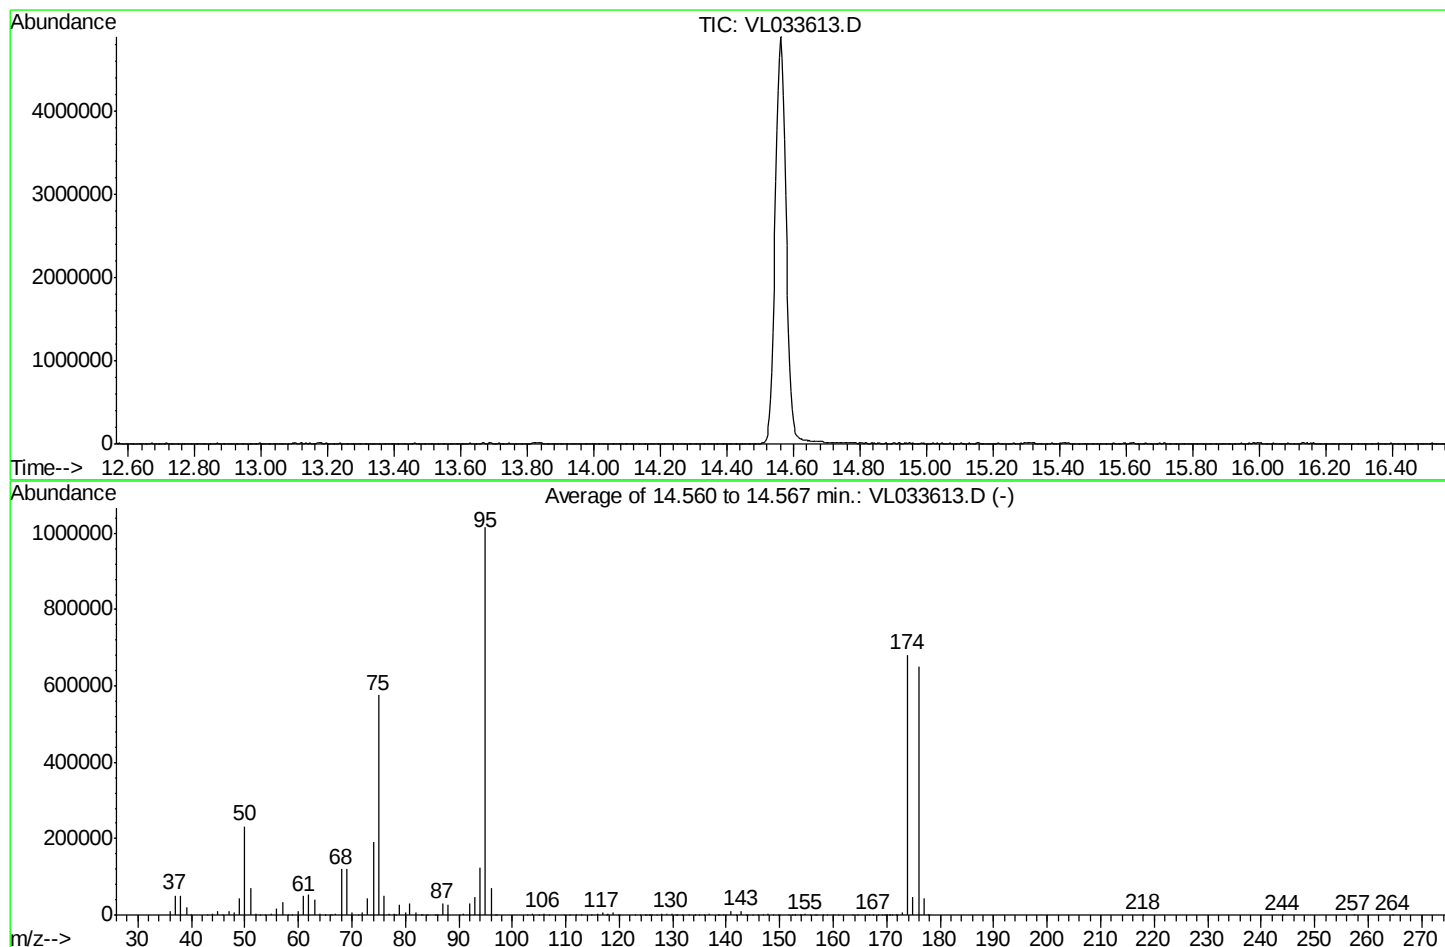

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.9	232704	PASS
75	95	30	66	56.8	576490	PASS
95	95	100	100	100.0	1015509	PASS
96	95	5	9	6.8	68986	PASS
173	174	0.00	2	0.9	6143	PASS
174	95	50	120	67.2	682133	PASS
175	174	4	9	7.1	48541	PASS
176	174	93	101	95.5	651178	PASS
177	176	5	9	6.6	43106	PASS