
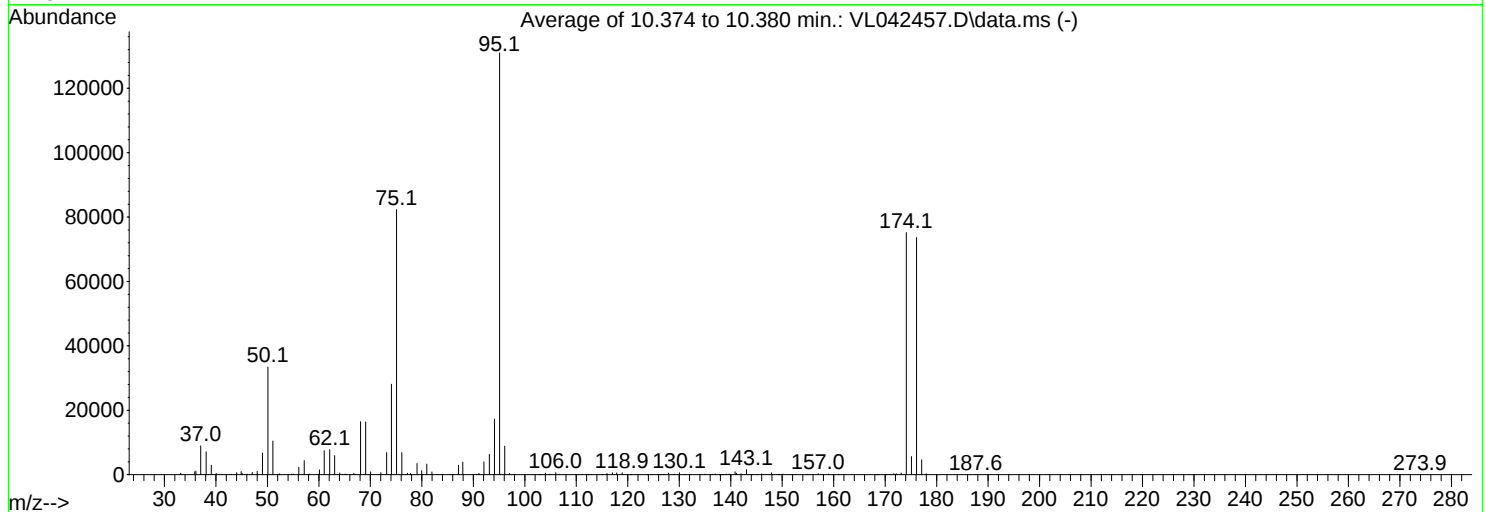


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL050125\
Data File : VL042457.D
Acq On : 01 May 2025 08:19
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL050125AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 02 03:16:31 2025

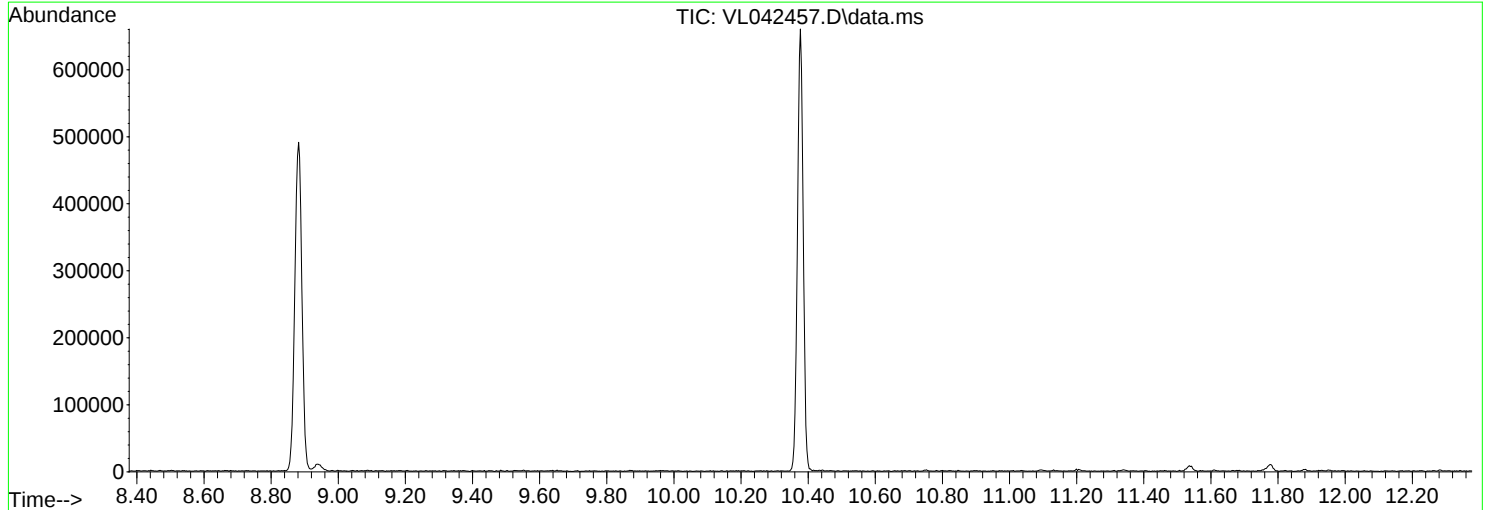

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	25.5	33424	PASS
75	95	30	66	62.8	82325	PASS
95	95	100	100	100.0	131013	PASS
96	95	5	9	6.8	8845	PASS
173	174	0.00	2	0.6	483	PASS
174	95	50	120	57.4	75195	PASS
175	174	4	9	7.5	5628	PASS
176	174	93	101	97.9	73643	PASS
177	176	5	9	6.3	4652	PASS

Average of 10.374 to 10.380 min.: VL042457.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	469	45.10	382	56.10	2274	65.30	41
35.90	906	46.10	162	57.15	4377	66.80	39
36.10	1139	47.05	684	57.90	105	67.20	15
37.05	8974	48.00	1049	58.10	226	68.10	1643
38.10	7135	49.05	6723	60.10	1472	69.10	16370
39.10	2930	50.10	33424	61.05	7465	70.05	850
40.05	356	51.05	10431	62.10	7736	72.05	662
41.10	49	51.90	98	63.05	5912	73.15	6882
43.00	119	52.30	235	64.05	486	74.10	28059
44.05	665	54.70	154	64.60	81	75.10	82325
44.90	947	55.05	208	65.10	198	76.10	6860

Average of 10.374 to 10.380 min.: VL042457.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.90	79	86.05	50	102.80	30	112.90	74
77.20	452	87.10	2929	103.35	68	115.00	24
77.80	368	87.95	3899	104.00	497	115.95	388
78.00	74	90.60	89	104.80	164	117.00	594
79.05	3488	91.10	390	105.10	83	117.85	568
79.95	1236	92.05	3969	106.00	631	118.90	604
80.95	3276	93.10	6328	106.75	75	120.60	21
81.95	827	94.10	17254	109.85	53	123.80	23
82.80	108	95.10	131013	110.95	113	124.80	51
83.00	33	96.10	8845	111.95	44	125.80	51
85.65	58	97.05	335	112.30	23	126.20	20

Average of 10.374 to 10.380 min.: VL042457.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.65	61	137.80	20	145.10	100	154.80	84
126.90	24	138.10	17	146.05	238	155.00	99
127.90	511	138.40	18	147.00	57	155.20	96
128.80	56	139.10	192	147.95	621	157.00	310
129.05	167	139.70	187	149.20	29	159.00	194
130.05	612	140.85	892	149.90	59	159.80	18
131.10	123	141.10	436	150.15	184	161.00	169
135.00	140	142.00	235	151.90	41	168.05	116
135.20	54	143.05	1602	152.10	77	168.30	27
136.45	84	143.90	37	152.70	62	168.60	59
137.00	261	144.20	62	154.00	102	168.90	50

Average of 10.374 to 10.380 min.: VL042457.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.10	26	187.60	40				
170.75	115	273.95	78				
171.10	170						
171.70	314						
172.15	321						
173.10	483						
174.10	75195						
175.10	5628						
176.10	73643						
177.10	4652						
177.95	243						