


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL050219\
 Data File : VL033622.D
 Acq On : 2 May 2019 8:47
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL050119AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu May 02 06:29:02 2019
 Last Update : Thu May 02 06:29:02 2019

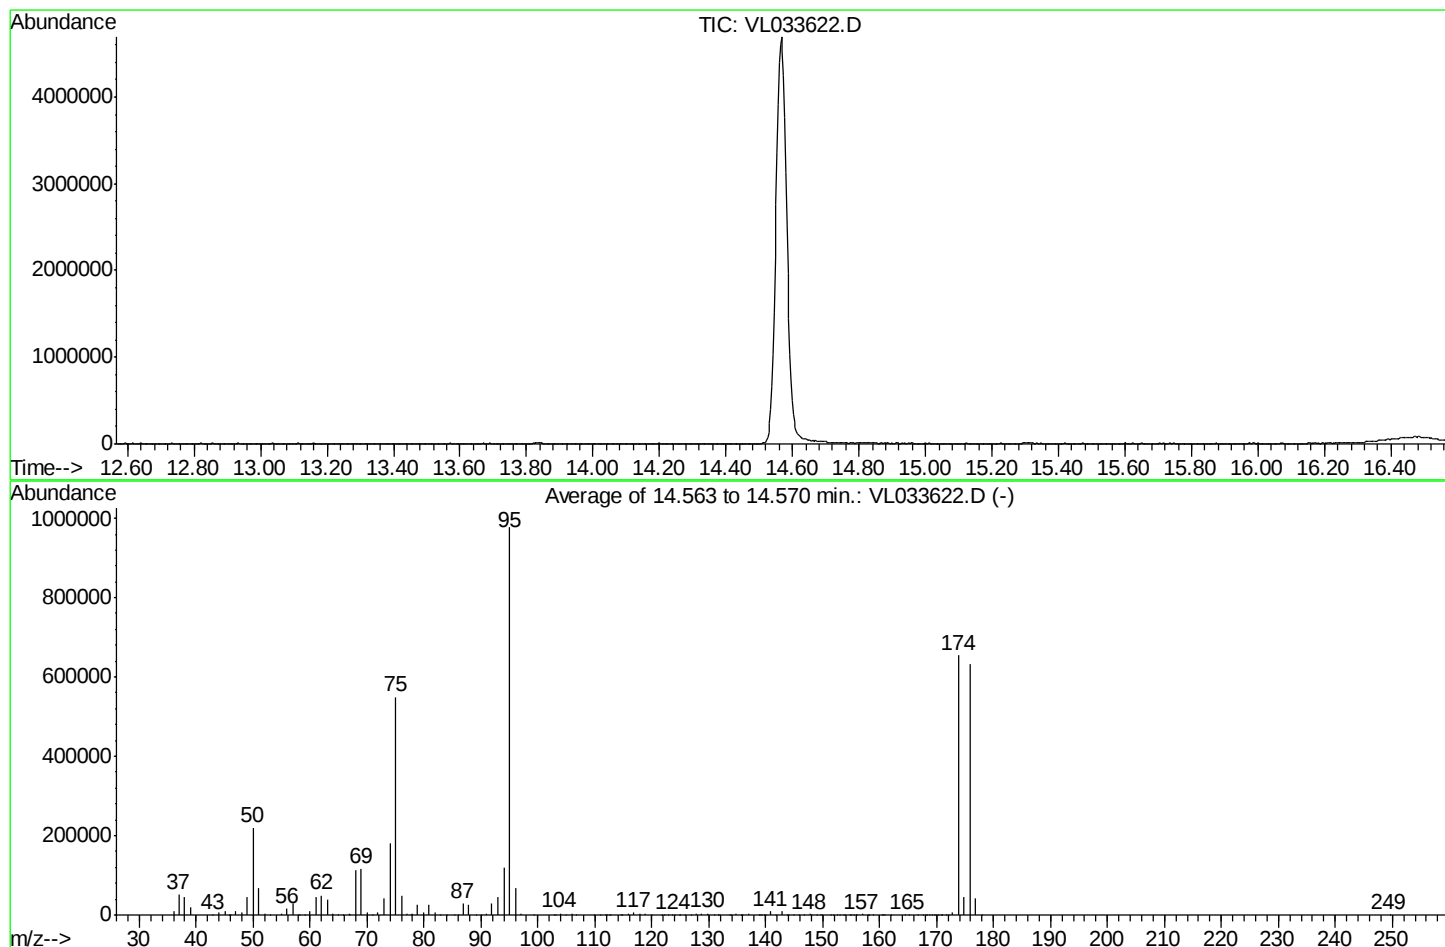

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.5	219904	PASS
75	95	30	66	56.3	550144	PASS
95	95	100	100	100.0	977216	PASS
96	95	5	9	7.0	68800	PASS
173	174	0.00	2	1.0	6625	PASS
174	95	50	120	66.9	653546	PASS
175	174	4	9	7.2	46864	PASS
176	174	93	101	96.8	632405	PASS
177	176	5	9	6.6	41626	PASS