


Data Path : W:\HPCHEM1\MSVOA L\DATA\VL050318\
Data File : VL031958.D
Acq On : 3 May 2018 9:46
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL050318AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu May 03 15:52:13 2018
Last Update : Thu May 03 15:52:13 2018

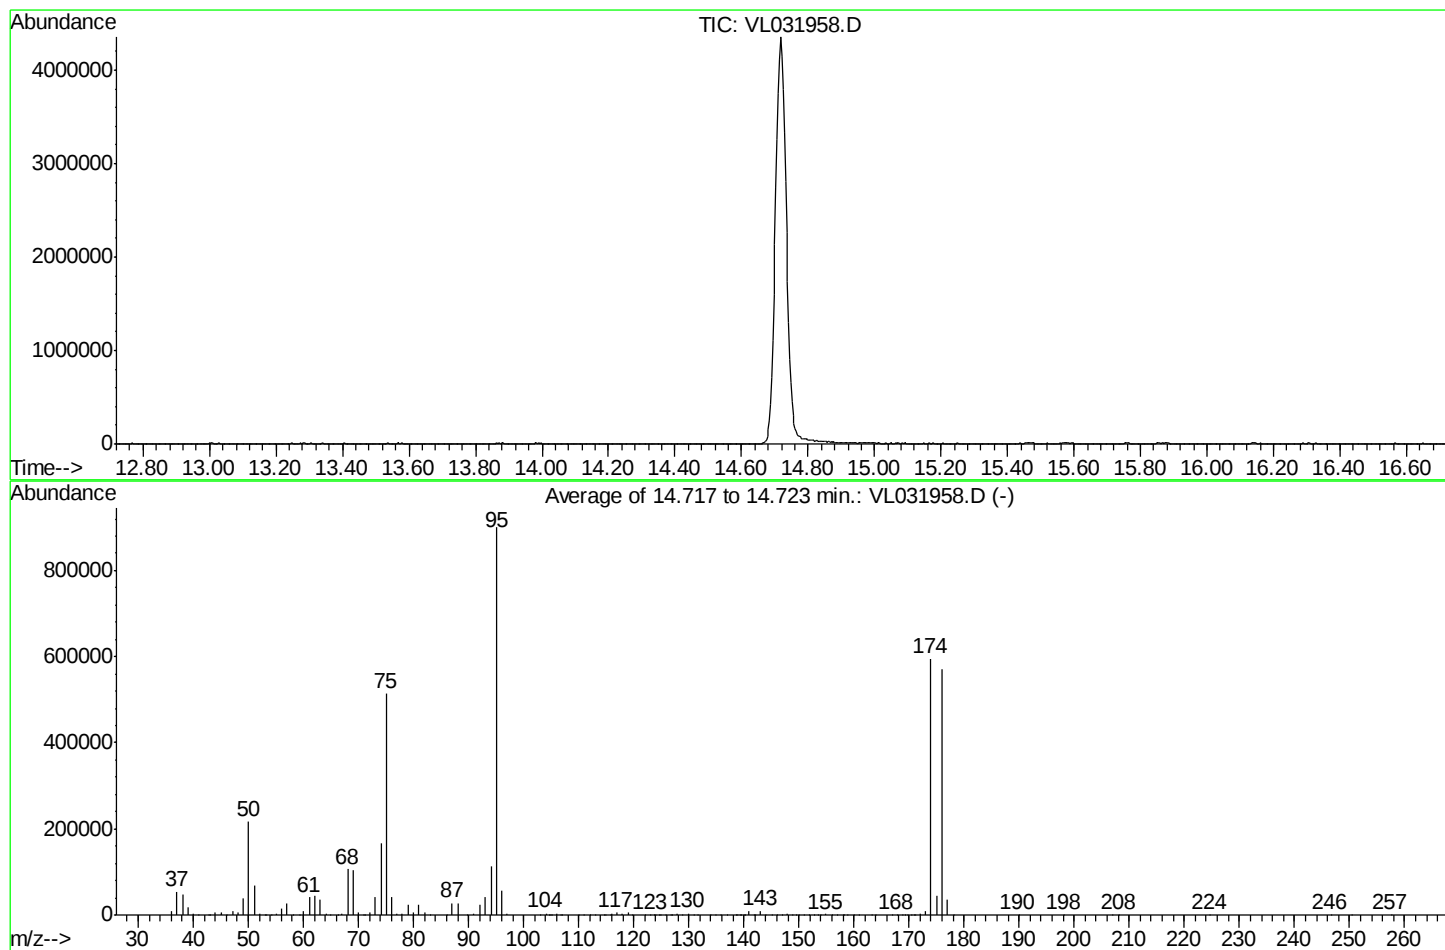

AutoFind: Scans 4239, 4240, 4241; Background Corrected with Scan 4215

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	215722	PASS
75	95	30	66	57.1	513856	PASS
95	95	100	100	100.0	900437	PASS
96	95	5	9	6.4	57664	PASS
173	174	0.00	2	1.3	7865	PASS
174	95	50	120	66.1	594901	PASS
175	174	4	9	7.5	44909	PASS
176	174	93	101	95.8	569792	PASS
177	176	5	9	6.5	36893	PASS